

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014842.D
 Acq On : 26 Apr 2023 16:03
 Operator : CG/JU
 Sample : 02418-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW8Z1

Quant Time: Apr 26 22:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 26 02:53:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.199	152	290460	20.000	ng/ul	0.00
20) Naphthalene-d8	11.034	136	1254941	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.834	164	778676	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.581	188	1623267	20.000	ng/ul	0.00
79) Chrysene-d12	21.651	240	1138873	20.000	ng/ul	0.00
88) Perylene-d12	24.251	264	999635	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.505	96	31997	4.331	ng/uL	0.00
4) Pyridine-d5	3.940	84	317283	14.808	ng/ul	0.00
7) Phenol-d5	7.340	99	683519	25.886	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.516	67	408474	25.742	ng/ul	0.00
11) 2-Chlorophenol-d4	7.722	132	520511	26.696	ng/ul	0.00
15) 4-Methylphenol-d8	8.905	113	535742	25.261	ng/ul	0.00
21) Nitrobenzene-d5	9.375	128	264073	28.111	ng/ul	0.00
24) 2-Nitrophenol-d4	10.105	143	290340	30.070	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.646	165	531962	26.506	ng/ul	0.00
31) 4-Chloroaniline-d4	11.163	131	595997	20.695	ng/ul	0.00
46) Dimethylphthalate-d6	14.234	166	1661781	27.503	ng/ul	0.00
49) Acenaphthylene-d8	14.528	160	1940528	28.014	ng/ul	0.00
54) 4-Nitrophenol-d4	15.004	143	224619	20.406	ng/ul	0.00
60) Fluorene-d10	15.822	176	1416978	27.546	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.928	200	134051	14.883	ng/ul	0.00
73) Anthracene-d10	17.681	188	2183653	28.648	ng/ul	0.00
81) Pyrene-d10	19.892	212	2343945	33.852	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.080	264	1533098	29.583	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.328	77	29204	2.303	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014842.D
Acq On : 26 Apr 2023 16:03
Operator : CG/JU
Sample : 02418-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW8Z1

Quant Time: Apr 26 22:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 26 02:53:24 2023
Response via : Initial Calibration

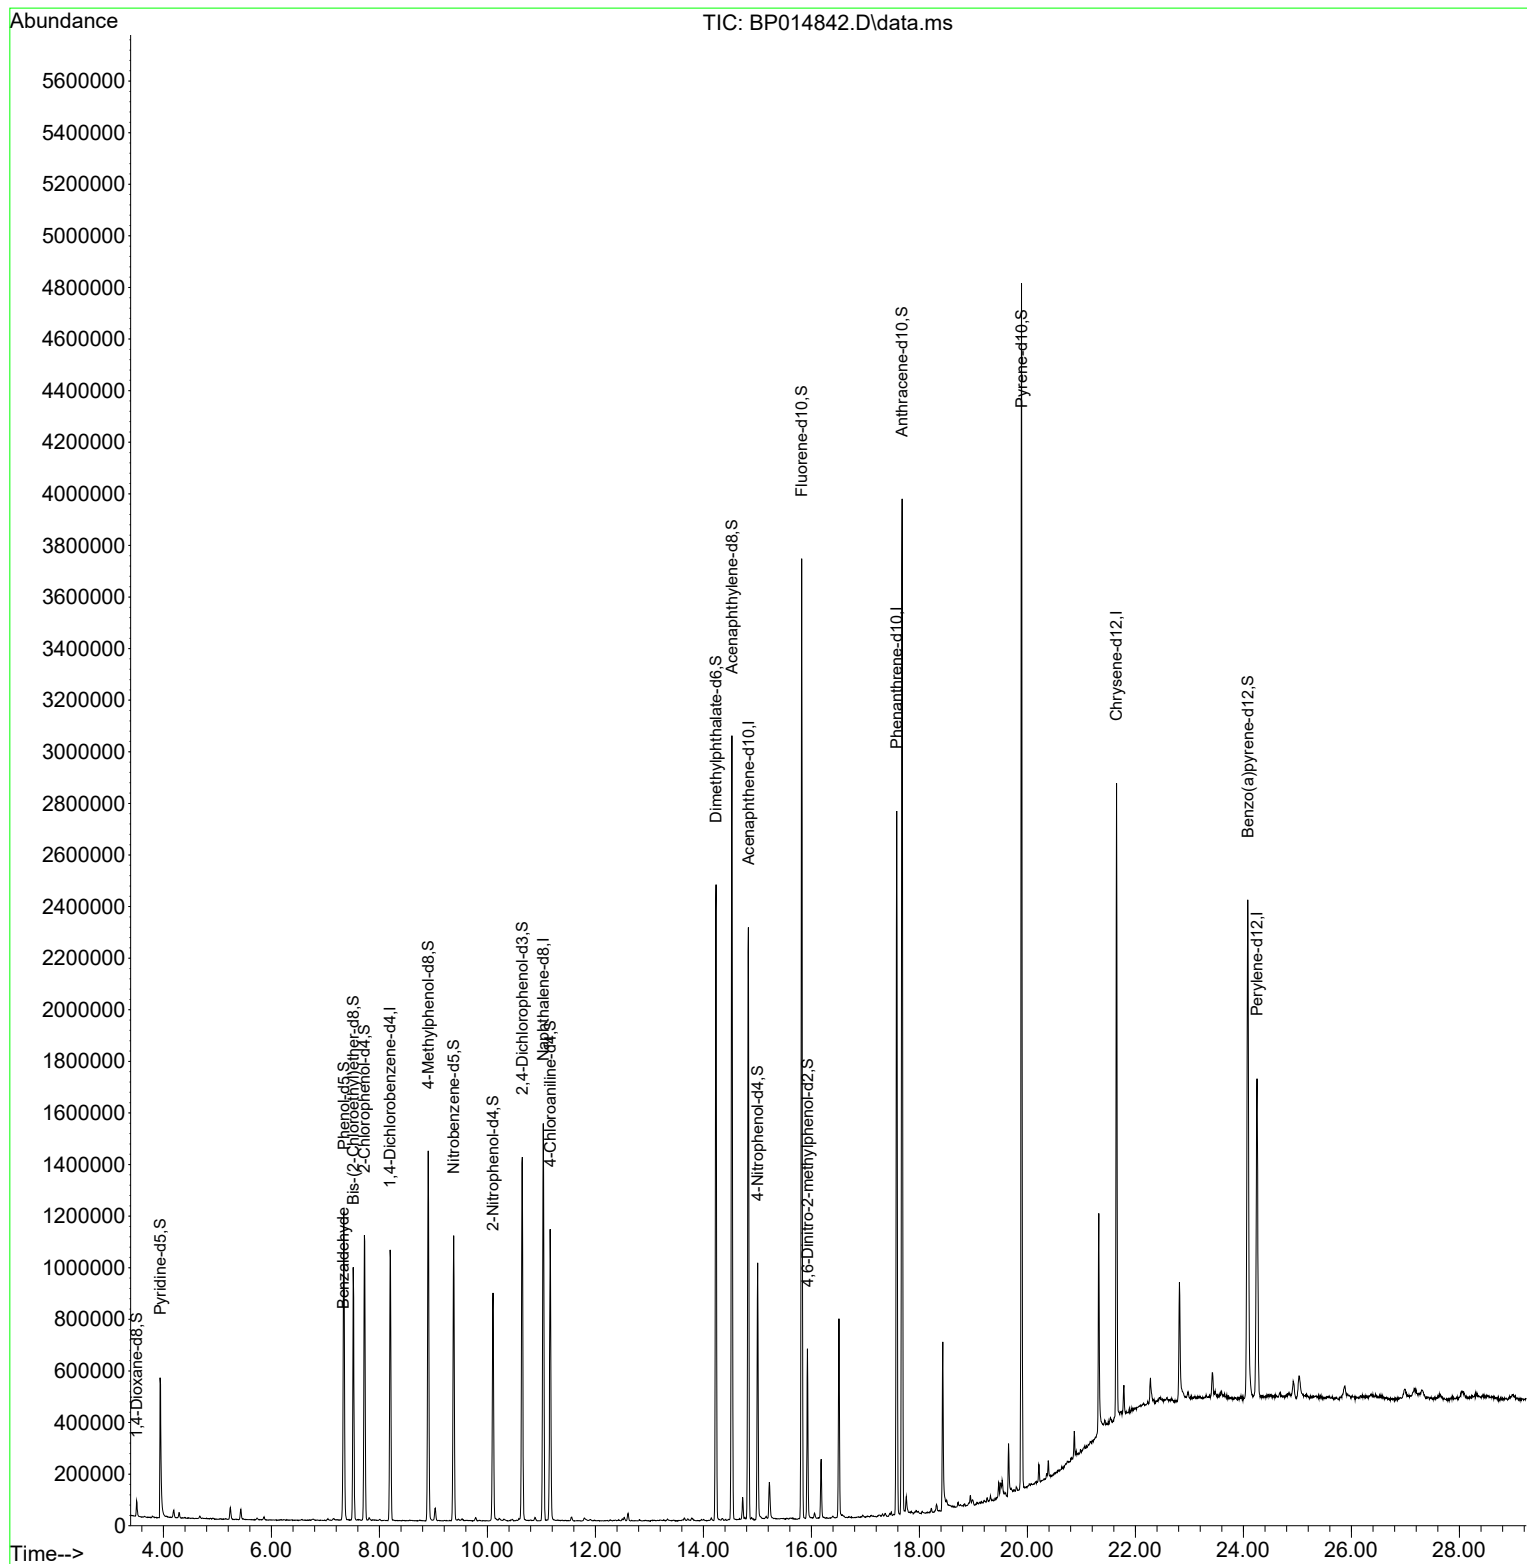

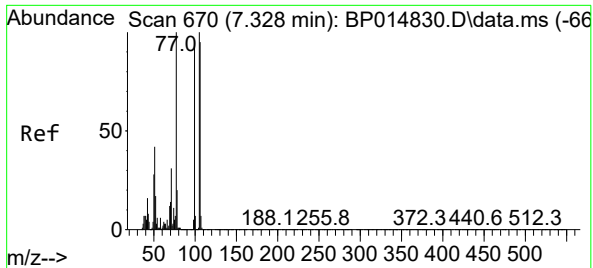

#6
Benzaldehyde
Concen: 2.303 ng/ul
RT: 7.328 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP014842.D
Acq: 26 Apr 2023 16:03

Instrument :
BNA_P
ClientSampleId :
EW8Z1

Tgt Ion:	77	Resp:	29204
Ion	Ratio	Lower	Upper
77	100		
105	99.2	79.9	119.9
106	98.2	75.2	112.8

