

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014850.D
 Acq On : 26 Apr 2023 20:32
 Operator : CG/JU
 Sample : 02488-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE66

Quant Time: Apr 26 23:32:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 26 02:53:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.199	152	295866	20.000	ng/u1	0.00
20) Naphthalene-d8	11.034	136	1305421	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.834	164	814956	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.581	188	1672851	20.000	ng/u1	0.00
79) Chrysene-d12	21.651	240	1114332	20.000	ng/u1	0.00
88) Perylene-d12	24.251	264	996737	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.505	96	35314	4.693	ng/uL	0.00
4) Pyridine-d5	3.946	84	95205	4.362	ng/u1	0.00
7) Phenol-d5	7.340	99	160066	5.951	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.516	67	477482	29.541	ng/u1	0.00
11) 2-Chlorophenol-d4	7.722	132	461877	23.256	ng/u1	0.00
15) 4-Methylphenol-d8	8.905	113	310810	14.387	ng/u1	0.00
21) Nitrobenzene-d5	9.375	128	309888	31.712	ng/u1	0.00
24) 2-Nitrophenol-d4	10.104	143	315502	31.412	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.640	165	561685	26.904	ng/u1	0.00
31) 4-Chloroaniline-d4	11.163	131	610122	20.366	ng/u1	0.00
46) Dimethylphthalate-d6	14.234	166	1960588	31.004	ng/u1	0.00
49) Acenaphthylene-d8	14.528	160	2264657	31.238	ng/u1	0.00
54) 4-Nitrophenol-d4	14.998	143	46596	4.045	ng/u1	0.00
60) Fluorene-d10	15.822	176	1685680	31.311	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.928	200	71361	7.688	ng/u1	0.00
73) Anthracene-d10	17.681	188	2653229	33.777	ng/u1	0.00
81) Pyrene-d10	19.892	212	2737882	40.412	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.080	264	1803265	34.898	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.540	88	9205	1.134	ng/uL#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014850.D
Acq On : 26 Apr 2023 20:32
Operator : CG/JU
Sample : 02488-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE66

Quant Time: Apr 26 23:32:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 26 02:53:24 2023
Response via : Initial Calibration

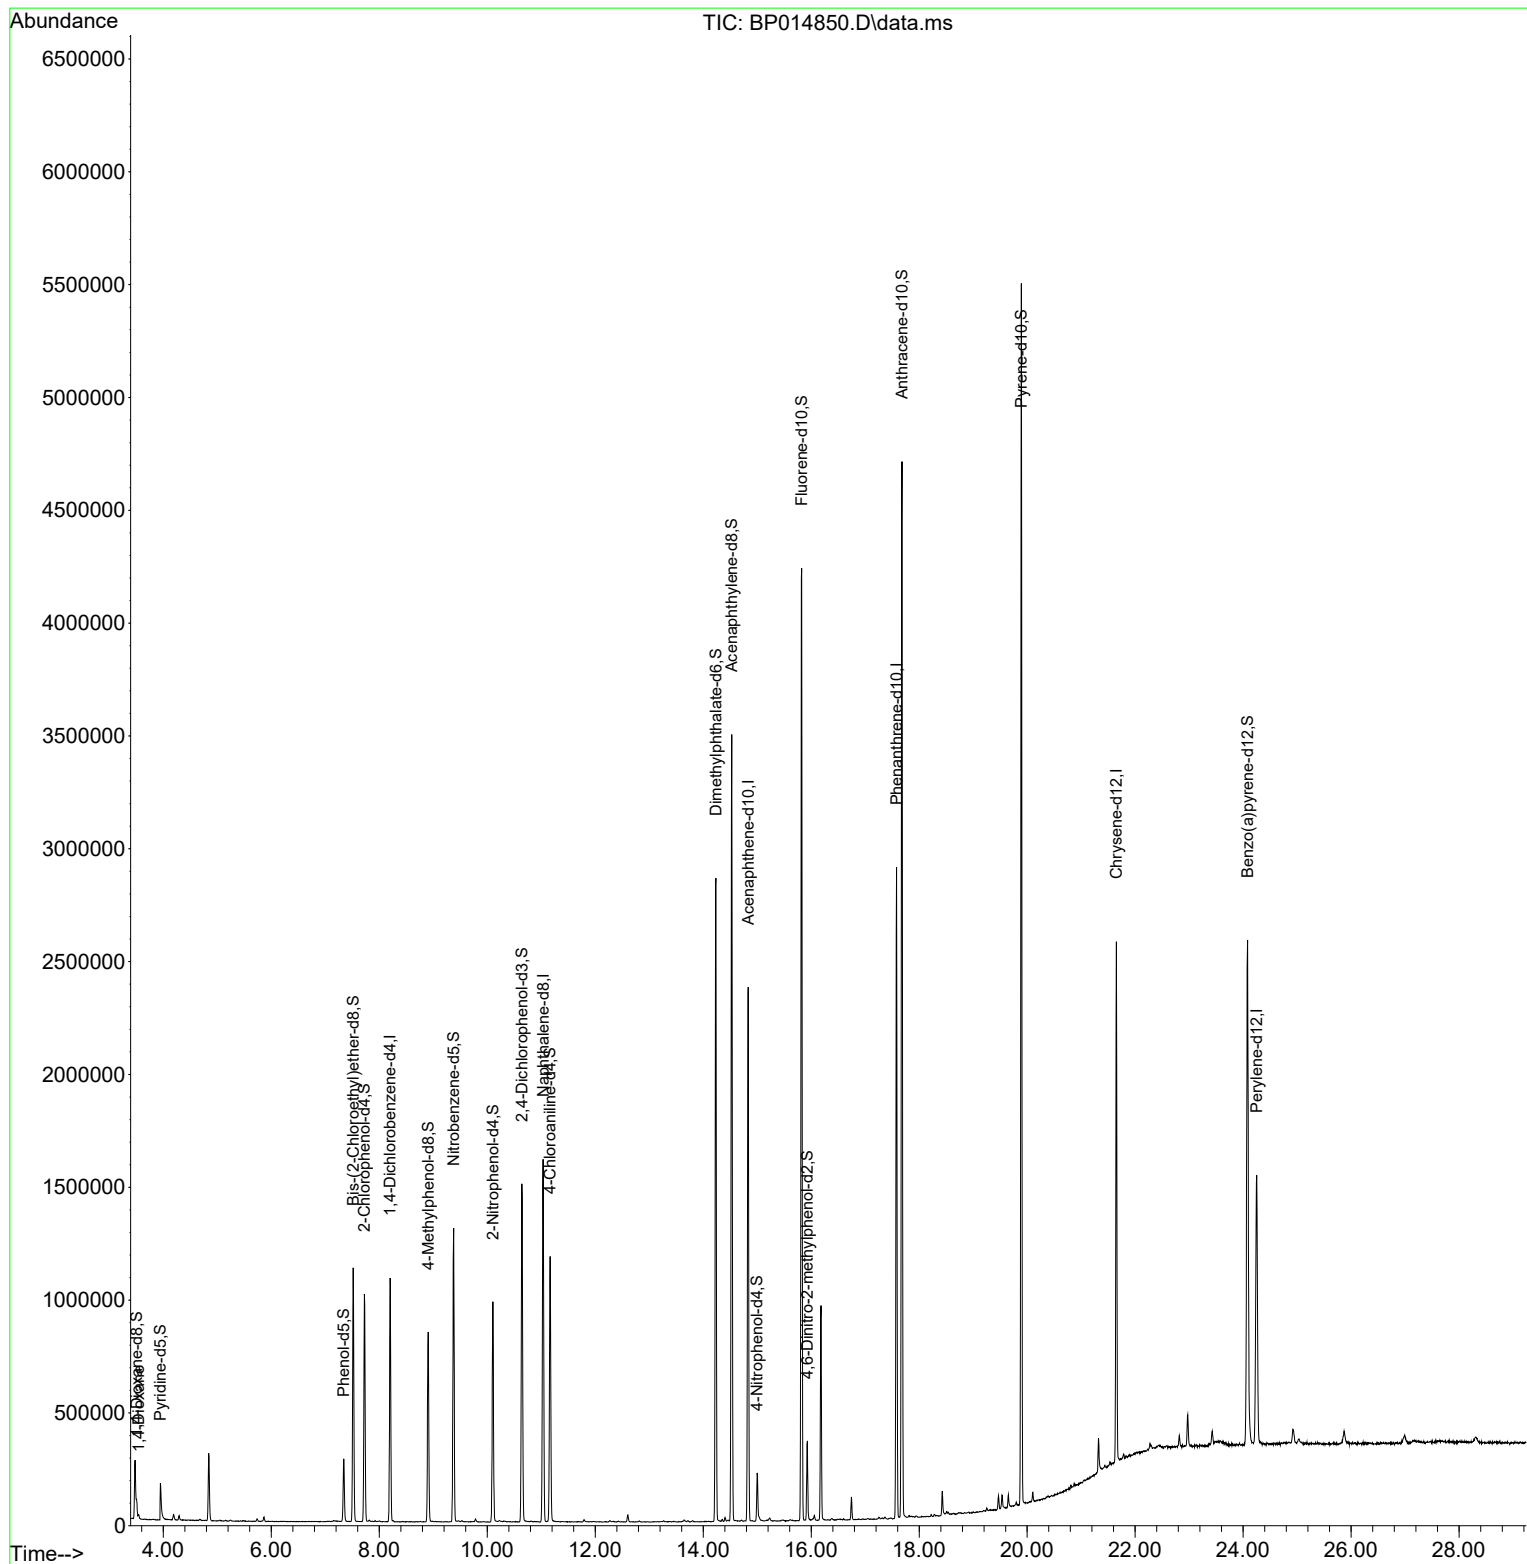

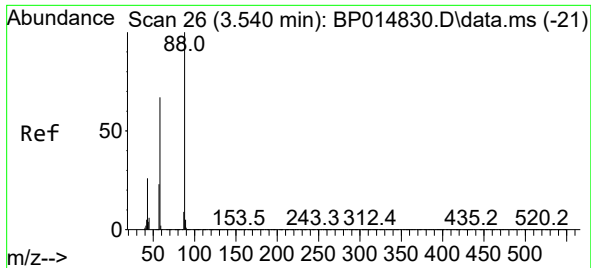

#2
1,4-Dioxane
Concen: 1.134 ng/uL
RT: 3.540 min Scan# 20
Delta R.T. 0.000 min
Lab File: BP014850.D
Acq: 26 Apr 2023 20:32

Instrument :
BNA_P
ClientSampleId :
BHE66

Tgt Ion: 88 Resp: 9205
Ion Ratio Lower Upper
88 100
43 32.0 21.3 31.9#
58 62.3 55.4 83.0

