

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014831.D
 Acq On : 26 Apr 2023 09:55
 Operator : CG/JU
 Sample : PB152344BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	15	20	27	rVB	60539	81438	1.31%	0.130%
2	3.940	90	94	112	rBV	710319	1145615	18.40%	1.825%
3	4.287	148	153	159	rVB	15869	25673	0.41%	0.041%
4	7.334	663	671	681	rBV	911534	1436667	23.08%	2.289%
5	7.516	694	702	715	rVB	809679	1262435	20.28%	2.011%
6	7.722	728	737	747	rBV	924454	1445580	23.22%	2.303%
7	8.199	809	818	825	rBV	878904	1358927	21.83%	2.165%
8	8.899	929	937	946	rBV	1184487	1891746	30.39%	3.014%
9	9.369	1009	1017	1028	rBV	890942	1442269	23.17%	2.298%
10	10.099	1129	1141	1150	rBV	696099	1117151	17.95%	1.780%
11	10.640	1225	1233	1242	rBV	1178836	1895410	30.45%	3.020%
12	11.034	1292	1300	1308	rBV	1248099	2098970	33.72%	3.344%
13	11.163	1312	1322	1337	rBV	1168977	1987772	31.93%	3.167%
14	12.598	1560	1566	1573	rVB2	22896	37362	0.60%	0.060%
15	13.804	1763	1771	1773	rBV7	4341	7493	0.12%	0.012%
16	14.228	1837	1843	1854	rBV	2417821	3358864	53.96%	5.351%
17	14.528	1885	1894	1903	rBV	2753116	4006860	64.37%	6.384%
18	14.828	1938	1945	1953	rBV	2145851	3169602	50.92%	5.050%
19	14.892	1954	1956	1964	rVB9	4537	8141	0.13%	0.013%
20	14.998	1967	1974	1991	rBV	1072722	1501031	24.11%	2.391%
21	15.228	2010	2013	2018	rVB7	4912	8564	0.14%	0.014%
22	15.816	2106	2113	2120	rBV	3510728	5002855	80.37%	7.970%
23	15.922	2125	2131	2146	rVV	869231	1187958	19.09%	1.893%
24	16.057	2151	2154	2160	rVB	17815	24996	0.40%	0.040%
25	16.386	2207	2210	2215	rVB7	3573	6488	0.10%	0.010%
26	16.598	2243	2246	2251	rVB6	4441	6459	0.10%	0.010%
27	17.363	2372	2376	2382	rBV3	6013	8066	0.13%	0.013%
28	17.581	2406	2413	2421	rBV	2684815	3881313	62.36%	6.184%
29	17.675	2423	2429	2444	rVV	3852010	5543905	89.07%	8.832%
30	18.222	2520	2522	2526	rVB5	6241	6809	0.11%	0.011%
31	18.428	2553	2557	2561	rBV7	6361	11360	0.18%	0.018%
32	19.469	2729	2734	2739	rBV2	45113	67348	1.08%	0.107%
33	19.533	2741	2745	2751	rVV	40033	59300	0.95%	0.094%
34	19.892	2800	2806	2816	rBV	4785795	6224495	100.00%	9.917%
35	21.651	3099	3105	3113	rBV	2714027	3606859	57.95%	5.746%
36	24.080	3510	3518	3533	rVB2	2235451	4734920	76.07%	7.544%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014831.D
Acq On : 26 Apr 2023 09:55
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Title : SVOA CALIBRATION

37	24.251	3539	3547	3562	rVB	1420400	3107417	49.92%	4.951%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 62768118

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014831.D
Acq On : 26 Apr 2023 09:55
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

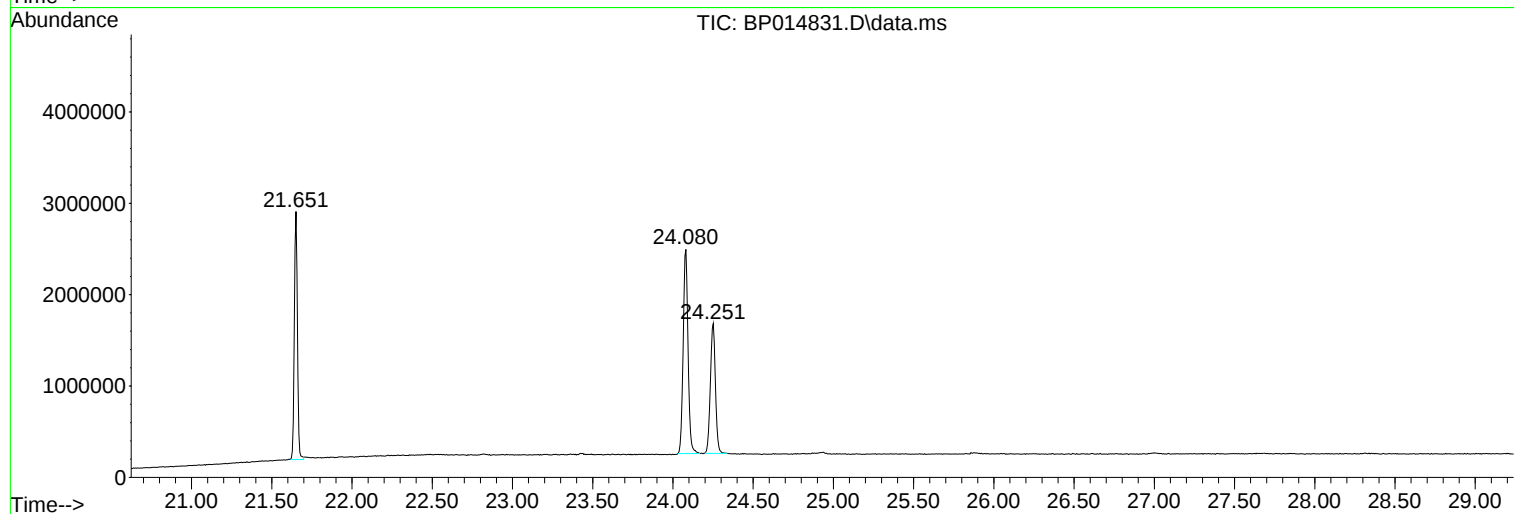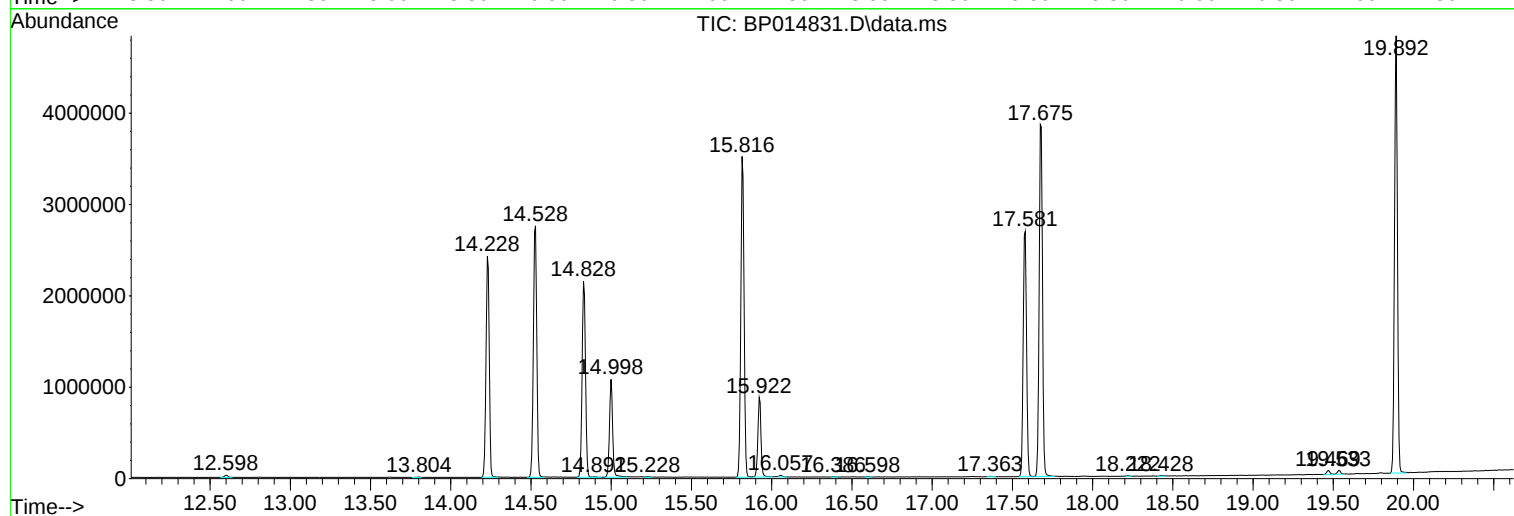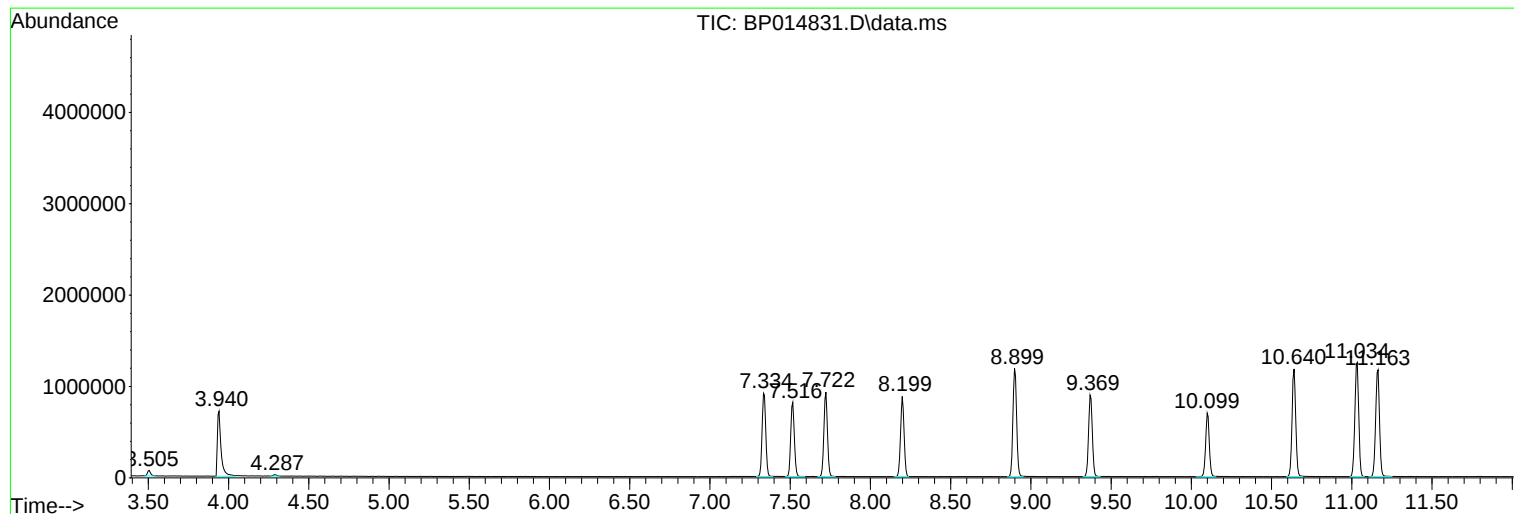

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014831.D
Acq On : 26 Apr 2023 09:55
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014831.D
Acq On : 26 Apr 2023 09:55
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------