

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014845.D
 Acq On : 26 Apr 2023 17:44
 Operator : CG/JU
 Sample : PB152344BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	16	20	26	rVB	78334	104627	1.61%	0.141%
2	3.940	90	94	114	rBV	946426	1441663	22.19%	1.949%
3	4.287	150	153	159	rVB	19772	28270	0.44%	0.038%
4	7.340	665	672	681	rBV	1279156	2045938	31.49%	2.765%
5	7.516	693	702	713	rBV	1104257	1711226	26.34%	2.313%
6	7.722	729	737	752	rBV	1277596	2089313	32.16%	2.824%
7	8.199	809	818	827	rBV	1143385	1862156	28.66%	2.517%
8	8.905	929	938	948	rBV	1711056	2705704	41.64%	3.657%
9	9.375	1008	1018	1027	rBV	1263526	2063340	31.76%	2.789%
10	9.463	1029	1033	1041	rVB	4236	9956	0.15%	0.013%
11	10.104	1134	1142	1151	rBV	1039469	1679314	25.85%	2.270%
12	10.646	1225	1234	1245	rBV	1633133	2740415	42.18%	3.704%
13	11.034	1290	1300	1310	rVB	1720689	2855913	43.95%	3.860%
14	11.163	1312	1322	1337	rBV	1568407	2608826	40.15%	3.526%
15	11.787	1424	1428	1435	rBV5	6784	12539	0.19%	0.017%
16	12.604	1561	1567	1574	rVB	30898	54073	0.83%	0.073%
17	13.810	1766	1772	1779	rVB9	5652	11191	0.17%	0.015%
18	14.234	1837	1844	1856	rBV	2820042	3927040	60.44%	5.308%
19	14.528	1885	1894	1905	rBV	3482554	5014530	77.18%	6.778%
20	14.834	1937	1946	1954	rBV	2605795	3873208	59.61%	5.235%
21	15.004	1967	1975	1991	rBV	1307528	1866804	28.73%	2.523%
22	15.822	2106	2114	2123	rBV	4039120	5907108	90.91%	7.984%
23	15.928	2126	2132	2147	rVV	1032407	1390009	21.39%	1.879%
24	16.057	2150	2154	2159	rVB3	18493	28799	0.44%	0.039%
25	16.604	2243	2247	2252	rVB8	5753	7371	0.11%	0.010%
26	17.251	2353	2357	2361	rVB6	6395	9337	0.14%	0.013%
27	17.363	2372	2376	2385	rVB2	8139	12697	0.20%	0.017%
28	17.581	2406	2413	2421	rBV	3190246	4349647	66.94%	5.879%
29	17.681	2423	2430	2440	rBV	4301939	6172956	95.00%	8.343%
30	17.816	2448	2453	2458	rBV7	12124	22666	0.35%	0.031%
31	18.428	2554	2557	2560	rBV5	7321	8854	0.14%	0.012%
32	19.469	2730	2734	2739	rVB3	53067	70815	1.09%	0.096%
33	19.539	2741	2746	2749	rVV	48086	68103	1.05%	0.092%
34	19.892	2800	2806	2813	rBV	5091498	6497598	100.00%	8.782%
35	21.651	3100	3105	3116	rVB	2490552	3346854	51.51%	4.524%
36	24.080	3510	3518	3533	rVB	2142779	4508300	69.38%	6.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014845.D
Acq On : 26 Apr 2023 17:44
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Title : SVOA CALIBRATION

37	24.251	3540	3547	3558	rVB2	1324015	2879267	44.31%	3.892%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 73986427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014845.D
Acq On : 26 Apr 2023 17:44
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

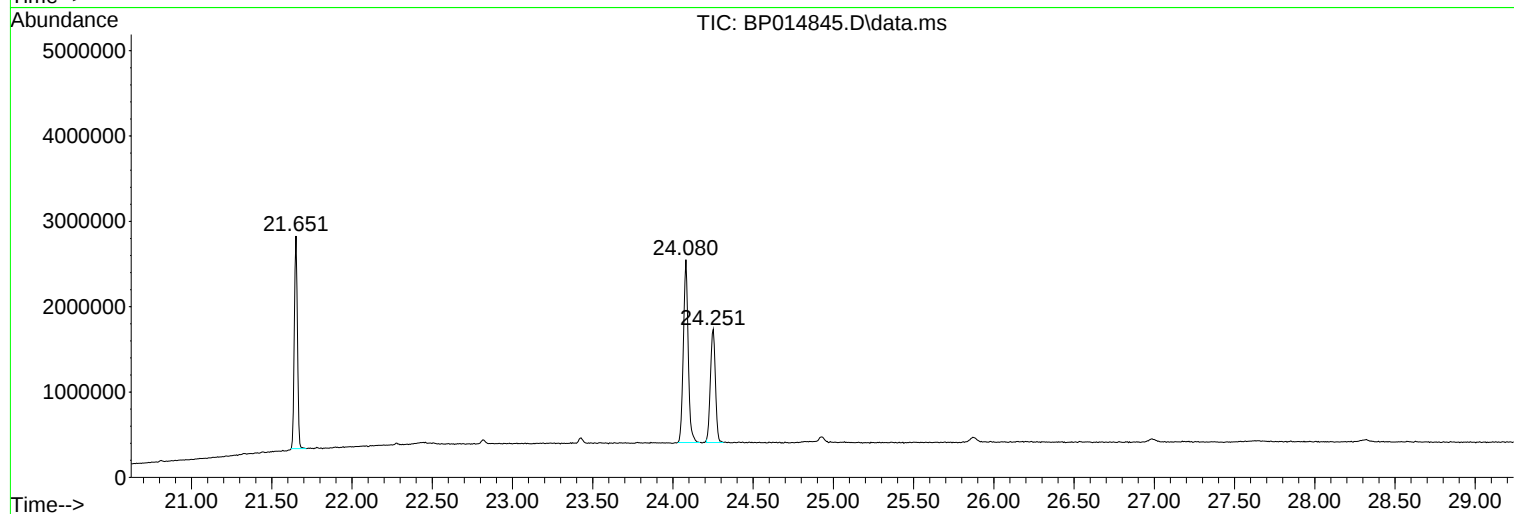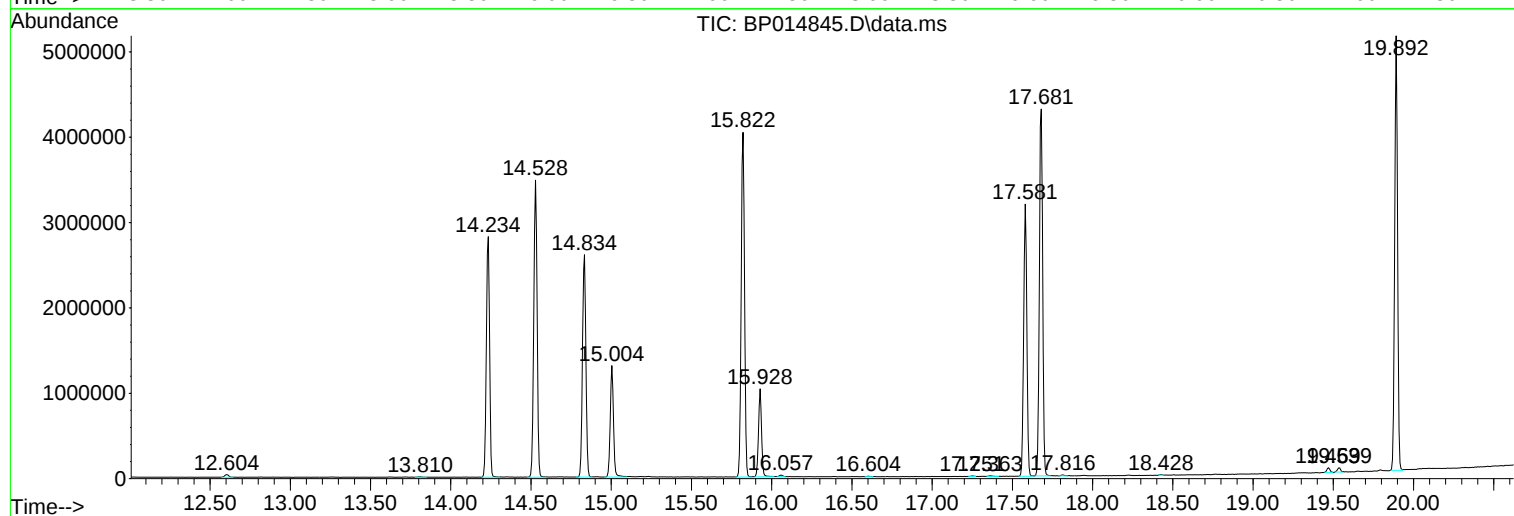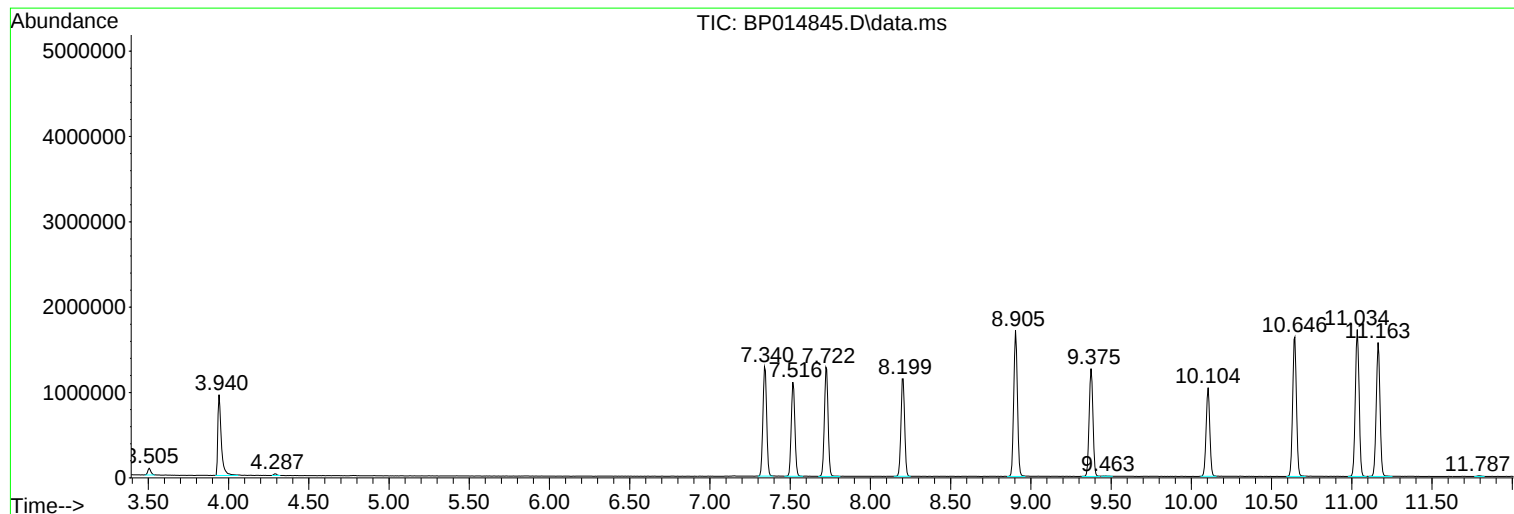

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014845.D
Acq On : 26 Apr 2023 17:44
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014845.D
Acq On : 26 Apr 2023 17:44
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------