

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014846.D
 Acq On : 26 Apr 2023 18:18
 Operator : CG/JU
 Sample : PB152426BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	16	20	30	rVB	81265	114077	1.82%	0.153%
2	3.940	91	94	123	rBV	1114741	1685008	26.89%	2.253%
3	4.293	149	154	163	rVB	20944	35294	0.56%	0.047%
4	7.340	664	672	680	rBV	1317257	2092797	33.40%	2.798%
5	7.516	693	702	712	rBV	1135141	1744516	27.84%	2.332%
6	7.722	730	737	745	rBV	1305272	2096204	33.45%	2.803%
7	8.204	809	819	829	rBV	1196519	1942271	31.00%	2.597%
8	8.904	930	938	949	rBV	1712008	2730927	43.58%	3.651%
9	9.375	1009	1018	1027	rBV	1281133	2082327	33.23%	2.784%
10	9.463	1030	1033	1042	rVB	3404	7581	0.12%	0.010%
11	10.104	1132	1142	1150	rBV	1044561	1695060	27.05%	2.266%
12	10.646	1225	1234	1246	rBV	1637810	2761531	44.07%	3.692%
13	11.034	1289	1300	1309	rBV	1780104	2967484	47.36%	3.967%
14	11.163	1314	1322	1331	rBV	1721358	2842432	45.36%	3.800%
15	11.798	1425	1430	1433	rBV7	4362	6763	0.11%	0.009%
16	12.604	1561	1567	1576	rBV	33532	58017	0.93%	0.078%
17	13.810	1765	1772	1779	rVB8	5323	12110	0.19%	0.016%
18	14.234	1837	1844	1854	rBV	2912204	3907877	62.37%	5.225%
19	14.528	1886	1894	1907	rBV2	3466553	5010130	79.96%	6.698%
20	14.834	1938	1946	1955	rBV	2663606	3983262	63.57%	5.325%
21	14.904	1955	1958	1964	rVB7	4088	7052	0.11%	0.009%
22	15.004	1968	1975	1988	rBV	1255839	1799114	28.71%	2.405%
23	15.234	2010	2014	2020	rVB7	9160	13930	0.22%	0.019%
24	15.822	2107	2114	2123	rBV	4033786	5929876	94.64%	7.928%
25	15.928	2125	2132	2142	rBV	1005398	1355475	21.63%	1.812%
26	16.057	2150	2154	2159	rVB2	20761	29892	0.48%	0.040%
27	16.392	2205	2211	2217	rBV8	3620	6607	0.11%	0.009%
28	17.369	2373	2377	2383	rVB4	7672	12840	0.20%	0.017%
29	17.580	2406	2413	2422	rBV	3254266	4466993	71.29%	5.972%
30	17.680	2423	2430	2445	rVV	4394133	6159319	98.30%	8.235%
31	17.810	2449	2452	2457	rVV7	7983	13023	0.21%	0.017%
32	17.945	2472	2475	2480	rVB5	5098	6769	0.11%	0.009%
33	18.427	2554	2557	2565	rBV9	5676	13505	0.22%	0.018%
34	19.469	2730	2734	2739	rBV	52369	66670	1.06%	0.089%
35	19.533	2741	2745	2751	rBV2	49853	76086	1.21%	0.102%
36	19.892	2800	2806	2812	rBV	4816769	6265774	100.00%	8.377%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014846.D
Acq On : 26 Apr 2023 18:18
Operator : CG/JU
Sample : PB152426BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Title : SVOA CALIBRATION

37	21.651	3099	3105	3112	rBV	2507466	3292420	52.55%	4.402%
38	24.080	3510	3518	3536	rVB2	2099561	4566698	72.88%	6.106%
39	24.251	3539	3547	3556	rVB2	1342236	2938722	46.90%	3.929%




Sum of corrected areas: 74796433

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014846.D
Acq On : 26 Apr 2023 18:18
Operator : CG/JU
Sample : PB152426BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

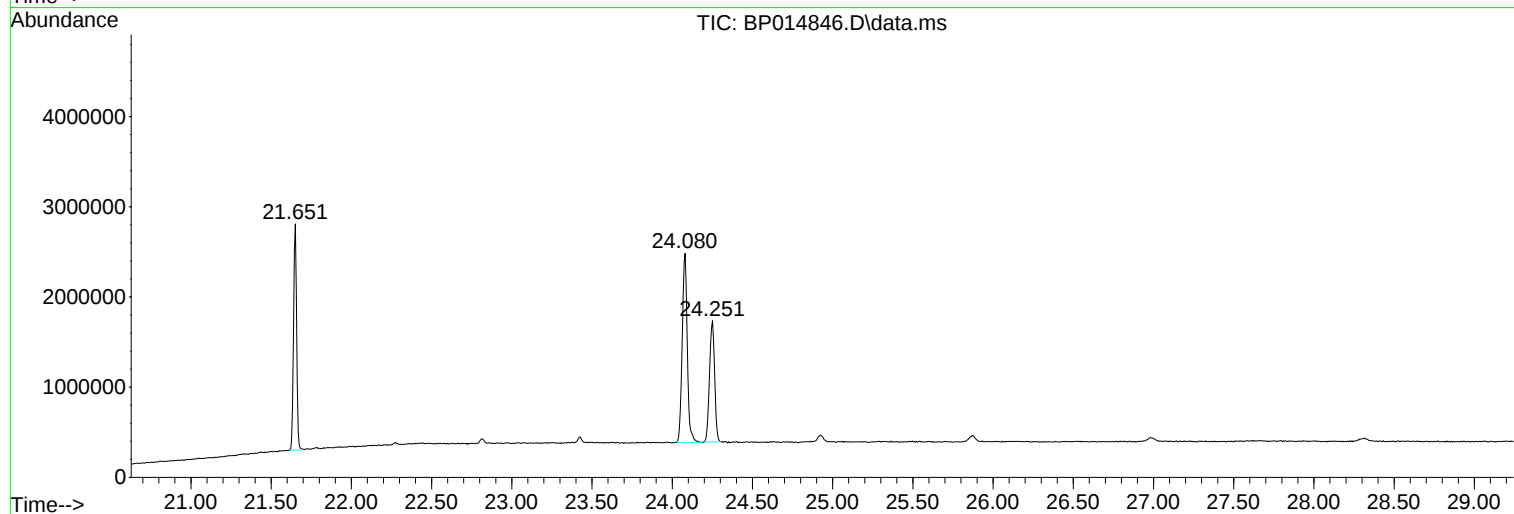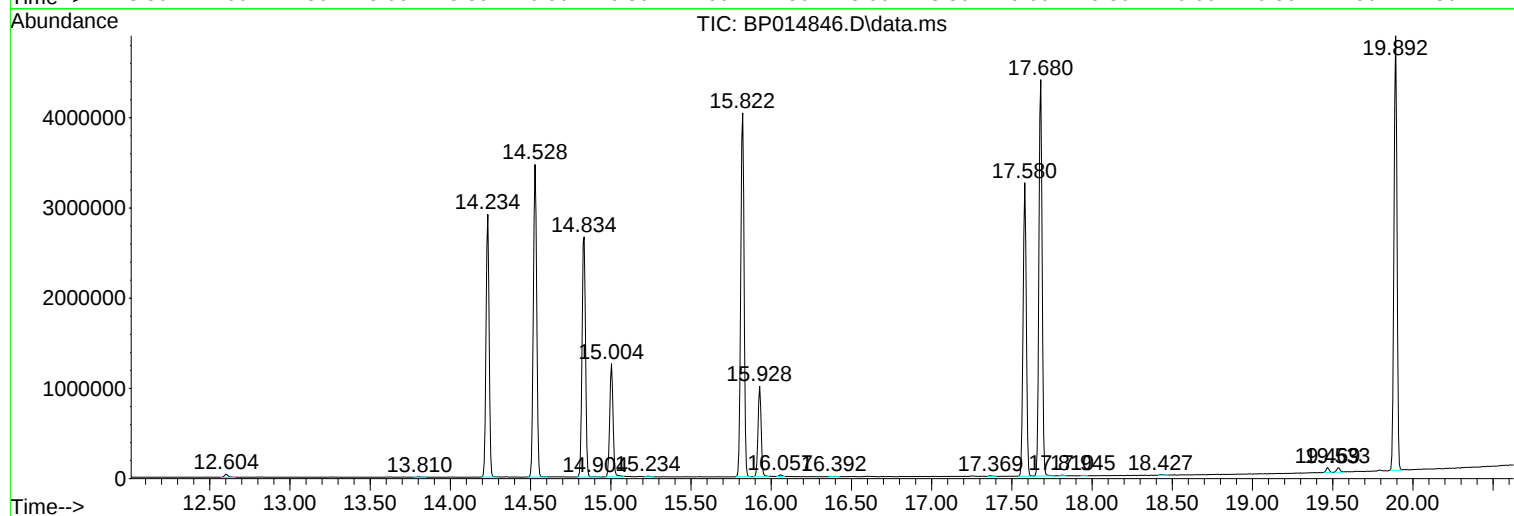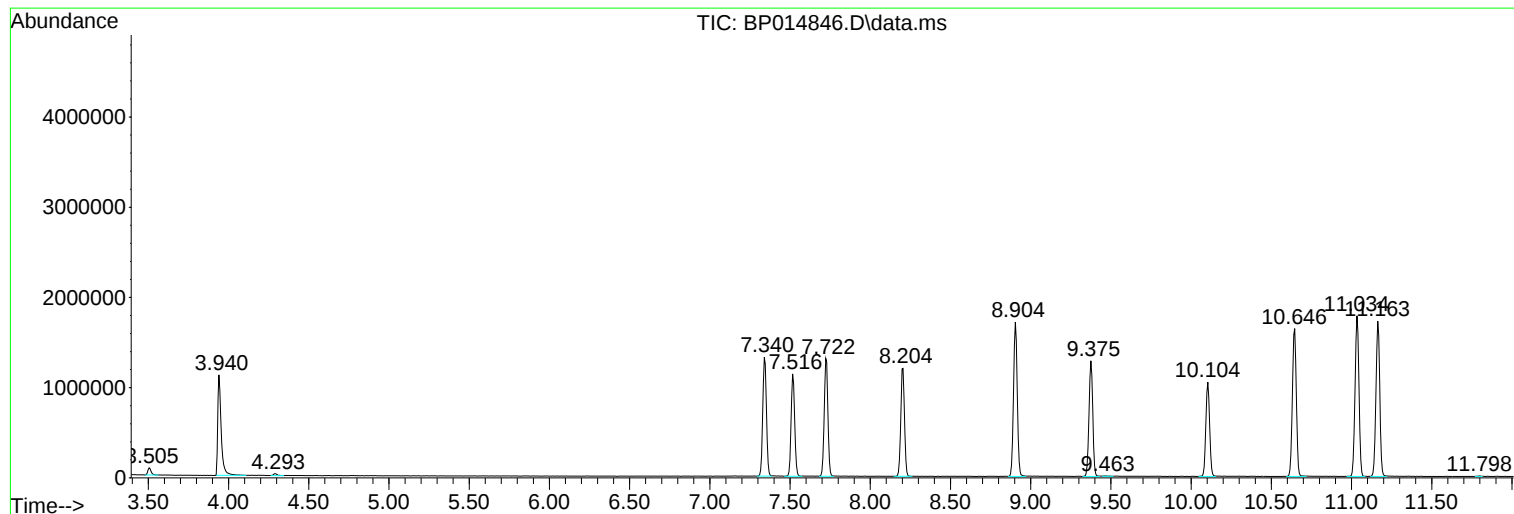

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014846.D
Acq On : 26 Apr 2023 18:18
Operator : CG/JU
Sample : PB152426BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014846.D
Acq On : 26 Apr 2023 18:18
Operator : CG/JU
Sample : PB152426BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------