

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014849.D
 Acq On : 26 Apr 2023 19:59
 Operator : CG/JU
 Sample : 02488-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	17	20	28	rVB	62576	84069	1.22%	0.124%
2	3.946	92	95	112	rBV	391280	576307	8.33%	0.853%
3	4.187	132	136	142	rVB	24009	37285	0.54%	0.055%
4	4.293	150	154	159	rVB	25757	35912	0.52%	0.053%
5	4.675	216	219	225	rVB6	7844	12917	0.19%	0.019%
6	4.764	230	234	247	rBV	37945	146217	2.11%	0.216%
7	5.240	311	315	321	rVB4	5380	9755	0.14%	0.014%
8	5.734	393	399	404	rBV2	11402	20816	0.30%	0.031%
9	5.864	416	421	428	rVB	19967	31017	0.45%	0.046%
10	6.081	454	458	461	rVB	5529	6957	0.10%	0.010%
11	6.222	478	482	487	rBV4	10717	16357	0.24%	0.024%
12	7.346	663	673	690	rBV3	127082	460831	6.66%	0.682%
13	7.517	692	702	715	rVB	1194766	1876086	27.11%	2.777%
14	7.734	731	739	769	rBV2	164834	916585	13.25%	1.357%
15	8.199	812	818	826	rBV	1328839	2159073	31.20%	3.196%
16	8.258	826	828	833	rVB4	12987	16161	0.23%	0.024%
17	8.911	931	939	955	rBV	446514	944291	13.65%	1.398%
18	9.034	955	960	964	rVV4	10421	18722	0.27%	0.028%
19	9.116	968	974	978	rBV5	5427	11326	0.16%	0.017%
20	9.281	995	1002	1006	rBV5	7570	14792	0.21%	0.022%
21	9.375	1010	1018	1029	rVV	1259278	2043015	29.53%	3.024%
22	9.528	1038	1044	1049	rBV3	17094	27780	0.40%	0.041%
23	9.787	1080	1088	1101	rBV	72483	154767	2.24%	0.229%
24	10.128	1139	1146	1151	rBV9	6939	19327	0.28%	0.029%
25	10.169	1151	1153	1161	rVB9	5205	8944	0.13%	0.013%
26	10.652	1227	1235	1258	rBV	237010	805188	11.64%	1.192%
27	11.034	1292	1300	1307	rBV	1993558	3314690	47.91%	4.907%
28	11.087	1307	1309	1315	rVB7	6995	8679	0.13%	0.013%
29	11.163	1315	1322	1340	rVB	1586801	2694214	38.94%	3.988%
30	11.687	1405	1411	1417	rVB2	17345	28839	0.42%	0.043%
31	11.816	1427	1433	1440	rVB7	15014	34917	0.50%	0.052%
32	11.940	1449	1454	1457	rBV6	4535	7344	0.11%	0.011%
33	11.969	1457	1459	1467	rVB9	3521	7221	0.10%	0.011%
34	12.281	1506	1512	1521	rBV	178841	324717	4.69%	0.481%
35	12.410	1530	1534	1540	rVB4	12998	21156	0.31%	0.031%
36	12.599	1561	1566	1572	rVB	33933	54837	0.79%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
 Data File : BP014849.D
 Acq On : 26 Apr 2023 19:59
 Operator : CG/JU
 Sample : 02488-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Title : SVOA CALIBRATION

37	13.110	1648	1653	1656	rBV3	17241	25062	0.36%	0.037%
38	13.140	1656	1658	1664	rVB7	8618	10733	0.16%	0.016%
39	14.146	1824	1829	1836	rBV4	23165	39630	0.57%	0.059%
40	14.228	1836	1843	1856	rBV	2323860	3279042	47.39%	4.854%
41	14.475	1879	1885	1887	rBV7	8986	14645	0.21%	0.022%
42	14.528	1887	1894	1905	rVB	3621213	5377271	77.72%	7.960%
43	14.834	1935	1946	1953	rBV	2959837	4559819	65.90%	6.750%
44	15.034	1976	1980	1984	rBV2	8753	12566	0.18%	0.019%
45	15.610	2072	2078	2084	rBV4	10676	17811	0.26%	0.026%
46	15.822	2104	2114	2124	rBV	4405273	6541836	94.55%	9.684%
47	15.945	2129	2135	2140	rBV6	4485	8504	0.12%	0.013%
48	16.057	2148	2154	2158	rBV	20825	30652	0.44%	0.045%
49	16.175	2170	2174	2180	rBV4	6612	10921	0.16%	0.016%
50	17.040	2317	2321	2326	rBV4	7659	11835	0.17%	0.018%
51	17.169	2336	2343	2345	rBV6	5080	9801	0.14%	0.015%
52	17.257	2353	2358	2362	rVB6	6990	8866	0.13%	0.013%
53	17.363	2372	2376	2380	rBV3	8281	13101	0.19%	0.019%
54	17.581	2406	2413	2422	rBV	3353916	4810980	69.53%	7.122%
55	17.675	2423	2429	2444	rVB2	4693268	6919092	100.00%	10.242%
56	17.951	2472	2476	2479	rBV4	6018	9511	0.14%	0.014%
57	18.222	2518	2522	2528	rBV5	32434	44978	0.65%	0.067%
58	18.281	2530	2532	2535	rBV4	5928	7208	0.10%	0.011%
59	18.504	2566	2570	2575	rBV	22296	28232	0.41%	0.042%
60	19.251	2694	2697	2703	rBV7	13447	19033	0.28%	0.028%
61	19.469	2730	2734	2738	rBV2	58590	79413	1.15%	0.118%
62	19.534	2741	2745	2749	rBV	55459	74801	1.08%	0.111%
63	19.892	2800	2806	2815	rBV	4945109	6624611	95.74%	9.806%
64	21.651	3099	3105	3111	rBV	2494444	3371286	48.72%	4.990%
65	24.080	3510	3518	3530	rVB2	2418922	5215825	75.38%	7.721%
66	24.245	3539	3546	3560	rVB2	1608081	3426273	49.52%	5.072%


Sum of corrected areas: 67554449

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014849.D
Acq On : 26 Apr 2023 19:59
Operator : CG/JU
Sample : 02488-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

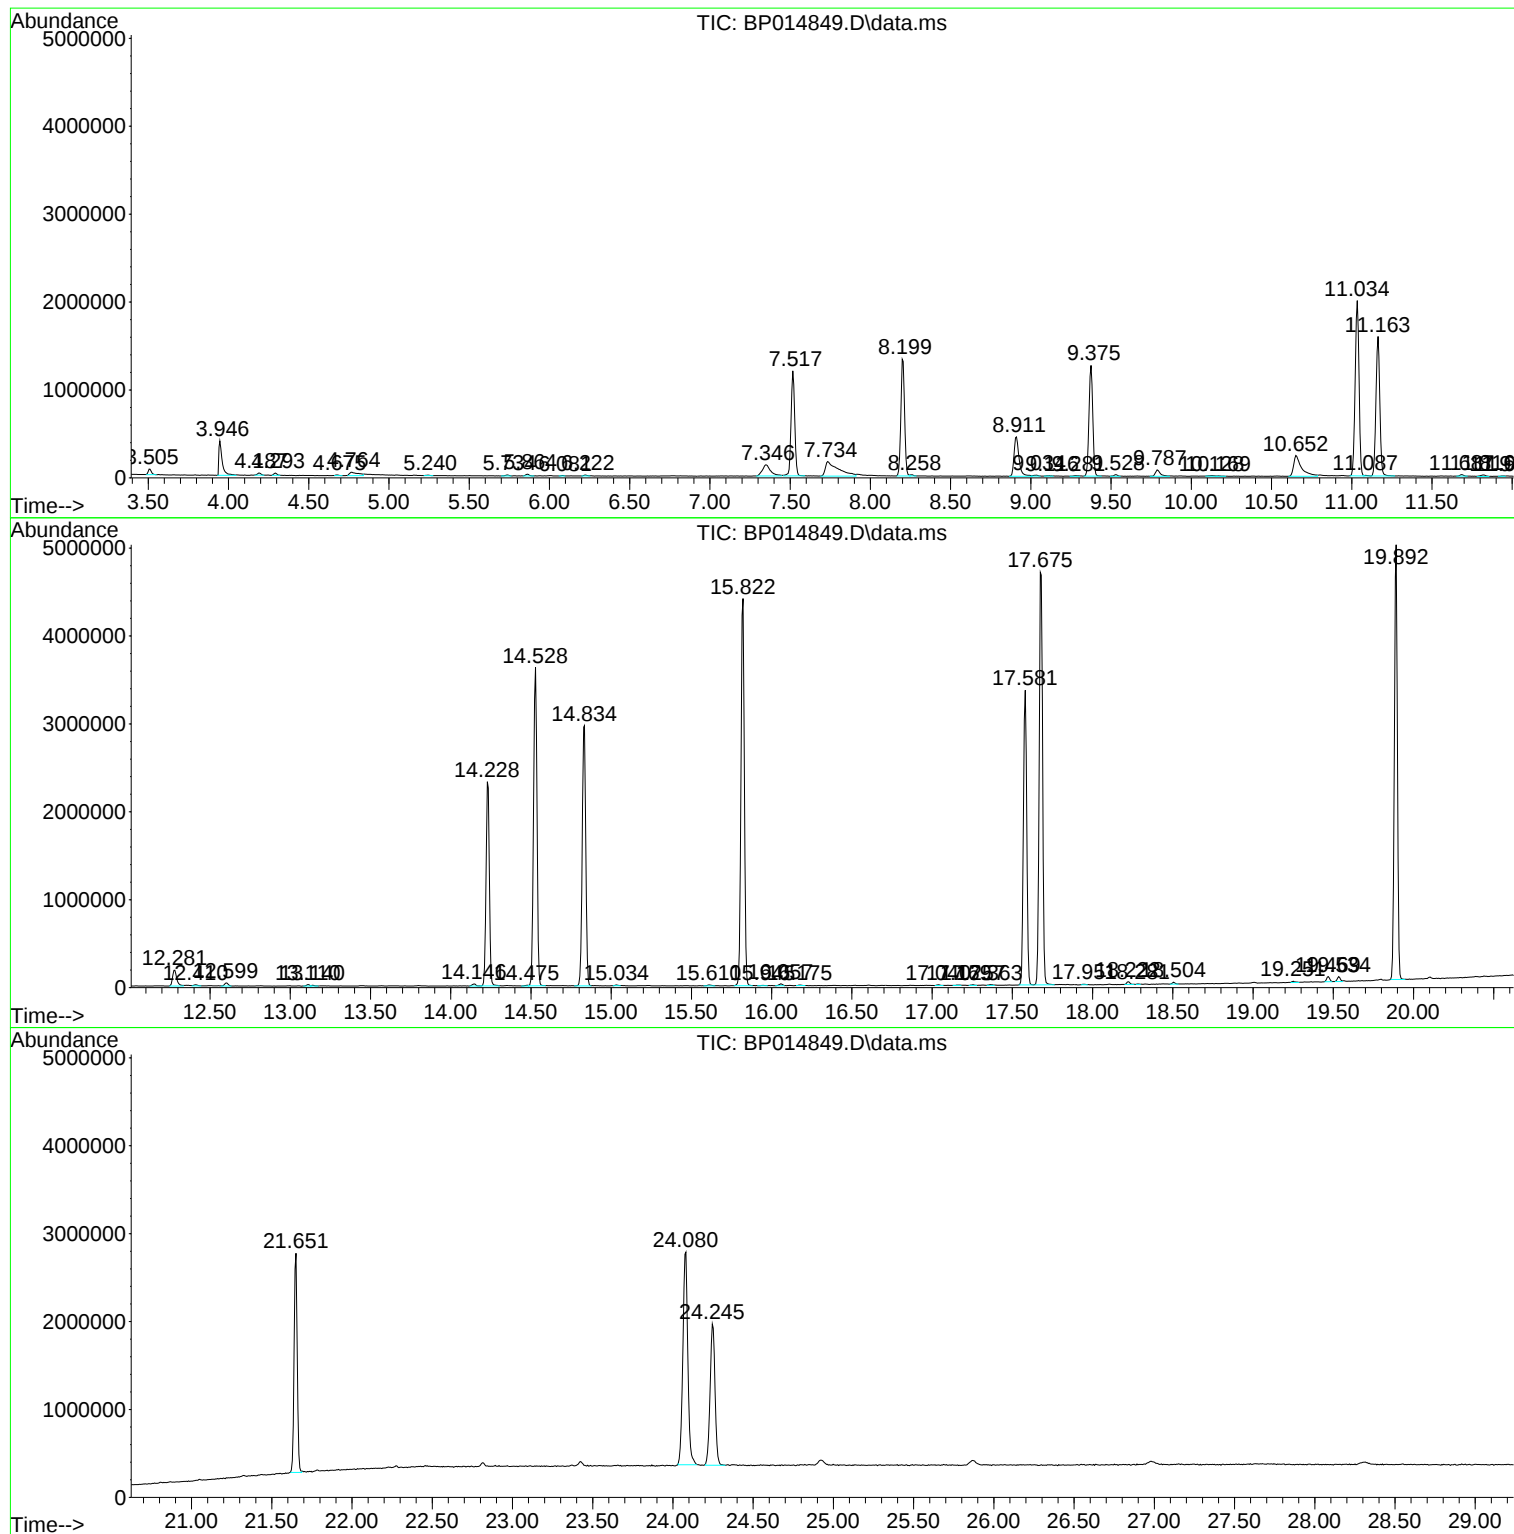

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014849.D
Acq On : 26 Apr 2023 19:59
Operator : CG/JU
Sample : 02488-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042623\
Data File : BP014849.D
Acq On : 26 Apr 2023 19:59
Operator : CG/JU
Sample : 02488-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc