

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014920.D
 Acq On : 01 May 2023 18:05
 Operator : CG/JU
 Sample : 02528-10DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA40DL

Quant Time: May 02 00:22:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.169	152	200463	20.000	ng/u1	0.00
20) Naphthalene-d8	11.004	136	803986	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.816	164	461922	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.575	188	907936	20.000	ng/u1	0.00
79) Chrysene-d12	21.657	240	759893	20.000	ng/u1	0.00
88) Perylene-d12	24.262	264	866311	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	3595	0.646	ng/uL	0.00
4) Pyridine-d5	3.928	84	20263	1.515	ng/u1	0.02
7) Phenol-d5	7.310	99	16208	1.033	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.487	67	69010	7.013	ng/u1	0.00
11) 2-Chlorophenol-d4	7.693	132	56097	4.722	ng/u1	0.00
15) 4-Methylphenol-d8	8.875	113	28182	2.357	ng/u1	0.00
21) Nitrobenzene-d5	9.346	128	30643	5.308	ng/u1	0.00
24) 2-Nitrophenol-d4	10.075	143	25887	4.885	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.616	165	54271	4.769	ng/u1	0.00
31) 4-Chloroaniline-d4	11.140	131	65024	3.952	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	264330	7.985	ng/u1	0.00
49) Acenaphthylene-d8	14.510	160	271384	6.863	ng/u1	0.00
54) 4-Nitrophenol-d4	15.010	143	495	0.100	ng/u1	0.01
60) Fluorene-d10	15.810	176	212454	7.362	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	13939	3.630	ng/u1	0.00
73) Anthracene-d10	17.669	188	330469	7.970	ng/u1	0.00
81) Pyrene-d10	19.886	212	390647	9.256	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.086	264	336750	7.870	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.505	88	96157	16.235	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014920.D
Acq On : 01 May 2023 18:05
Operator : CG/JU
Sample : 02528-10DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA40DL


Quant Time: May 02 00:22:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

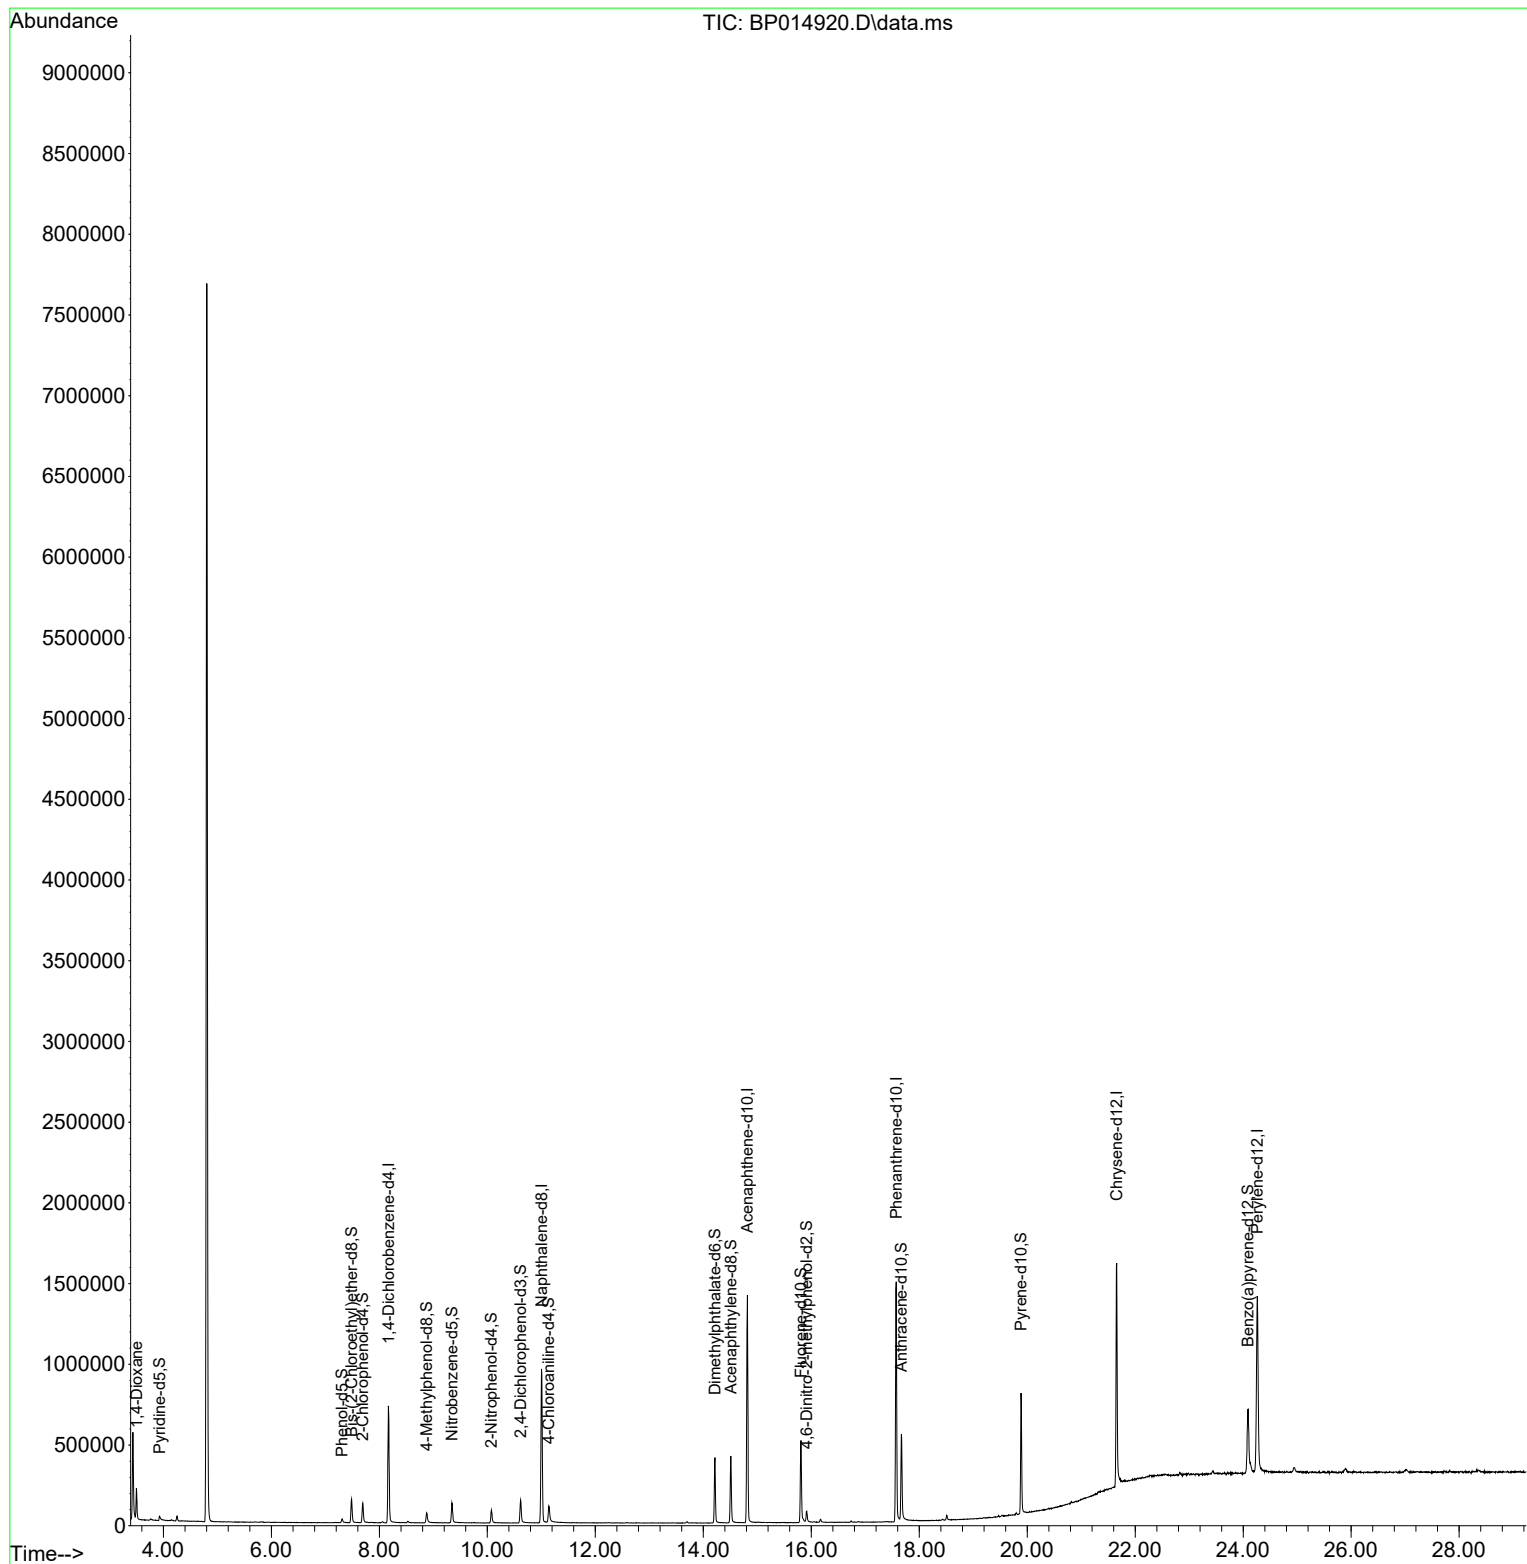

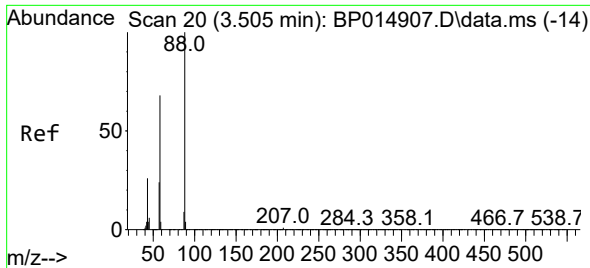

#2
 1,4-Dioxane
 Concen: 16.235 ng/uL
 RT: 3.505 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BP014920.D
 Acq: 01 May 2023 18:05

Instrument :
 BNA_P
 ClientSampleId :
 HOA40DL

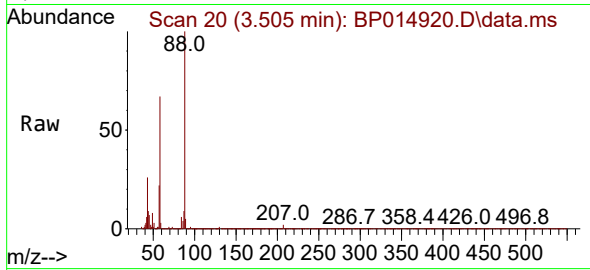

Tgt Ion: 88 Resp: 96157
 Ion Ratio Lower Upper
 88 100
 43 25.9 22.2 33.4
 58 66.5 55.1 82.7

