

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014921.D
 Acq On : 01 May 2023 18:38
 Operator : CG/JU
 Sample : 02528-04DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA36DL

Quant Time: May 02 00:22:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.169	152	202954	20.000	ng/u1	0.00
20) Naphthalene-d8	11.005	136	836231	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.816	164	500674	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.575	188	1040259	20.000	ng/u1	0.00
79) Chrysene-d12	21.651	240	904276	20.000	ng/u1	-0.01
88) Perylene-d12	24.263	264	974584	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	6818	1.211	ng/uL	0.00
4) Pyridine-d5	3.917	84	57163	4.223	ng/u1	0.01
7) Phenol-d5	7.311	99	42610	2.682	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.487	67	178037	17.870	ng/u1	0.00
11) 2-Chlorophenol-d4	7.693	132	150709	12.531	ng/u1	0.00
15) 4-Methylphenol-d8	8.875	113	71639	5.919	ng/u1	0.00
21) Nitrobenzene-d5	9.346	128	88783	14.787	ng/u1	0.00
24) 2-Nitrophenol-d4	10.075	143	91604	16.620	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.616	165	167464	14.147	ng/u1	0.00
31) 4-Chloroaniline-d4	11.140	131	74887	4.376	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	720456	20.079	ng/u1	0.00
49) Acenaphthylene-d8	14.510	160	725071	16.917	ng/u1	0.00
54) 4-Nitrophenol-d4	14.993	143	8146	1.526	ng/u1	0.00
60) Fluorene-d10	15.804	176	610440	19.517	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	69337	15.758	ng/u1	0.00
73) Anthracene-d10	17.669	188	975887	20.541	ng/u1	0.00
81) Pyrene-d10	19.886	212	1208575	24.063	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.092	264	1074520	22.322	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.505	88	142581	23.778	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014921.D
Acq On : 01 May 2023 18:38
Operator : CG/JU
Sample : 02528-04DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA36DL


Quant Time: May 02 00:22:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

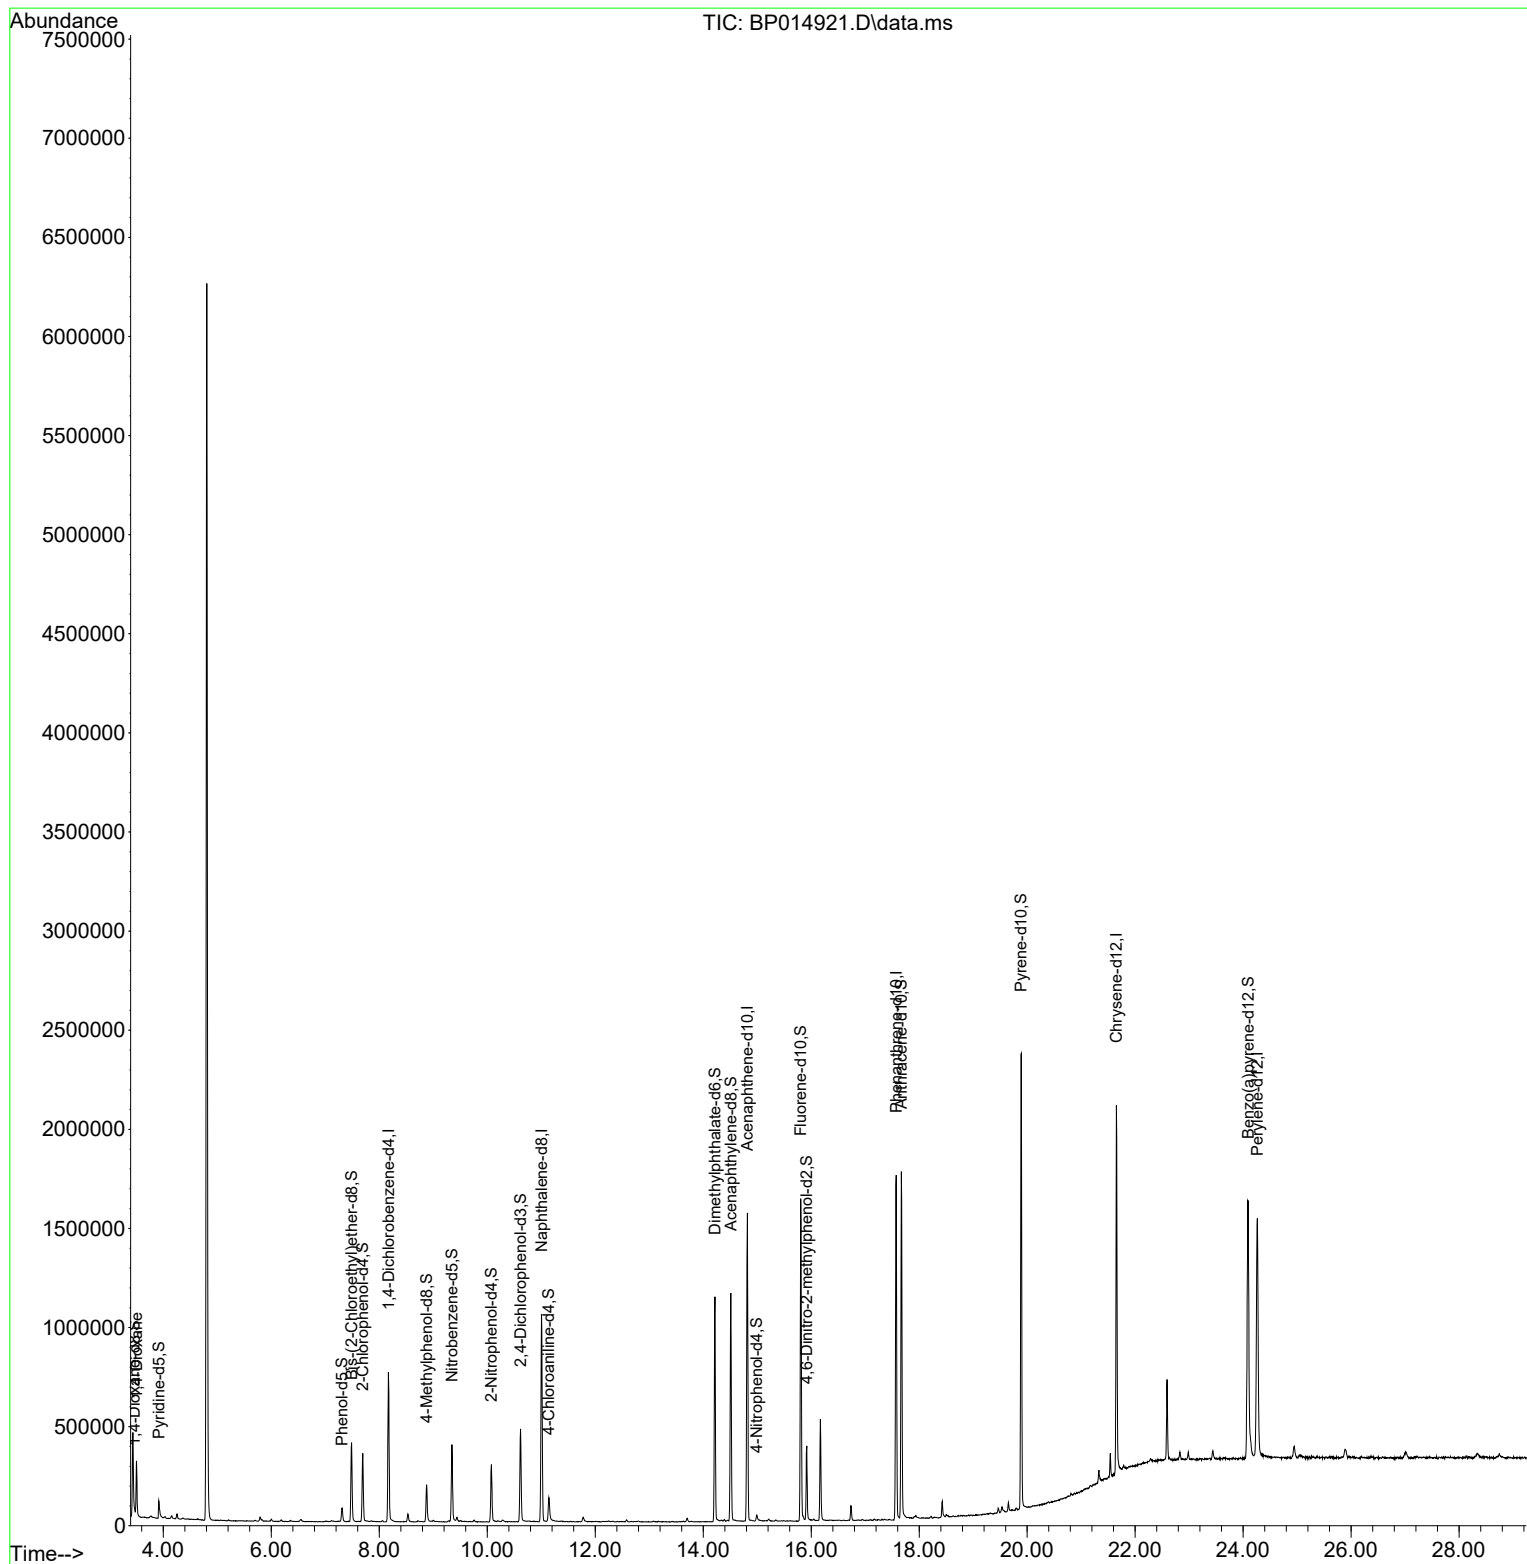

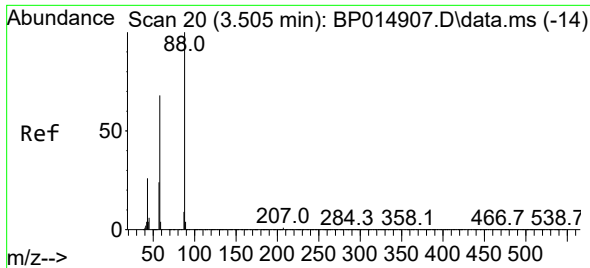

#2
 1,4-Dioxane
 Concen: 23.778 ng/uL
 RT: 3.505 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BP014921.D
 Acq: 01 May 2023 18:38

Instrument :
 BNA_P
 ClientSampleId :
 HOA36DL

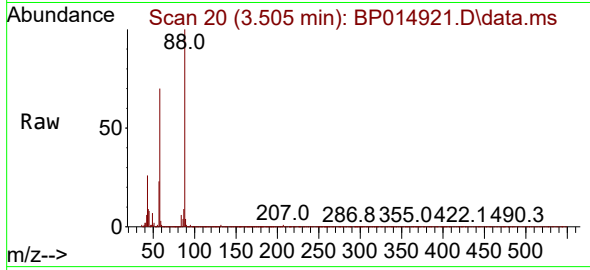

Tgt Ion: 88 Resp: 142581

Ion	Ratio	Lower	Upper
88	100		
43	26.5	22.2	33.4
58	69.7	55.1	82.7

