




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014909.D
Acq On : 01 May 2023 11:53
Operator : CG/JU
Sample : 02551-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE77

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: May 02 00:19:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

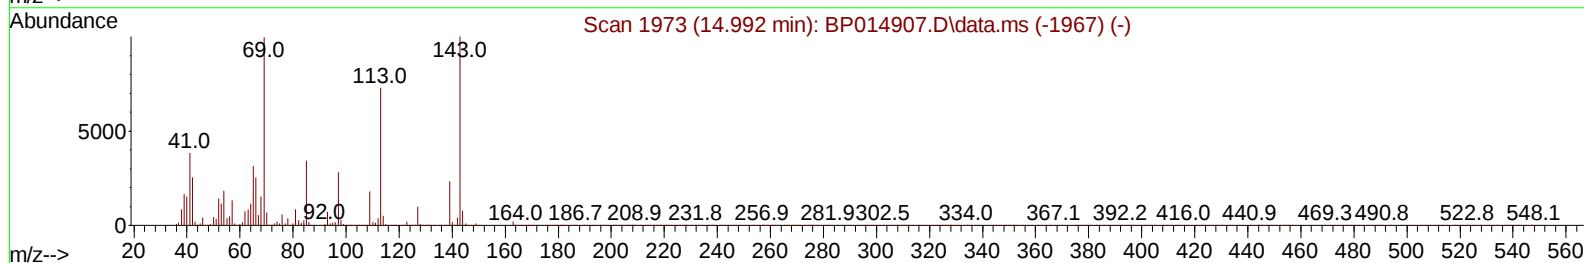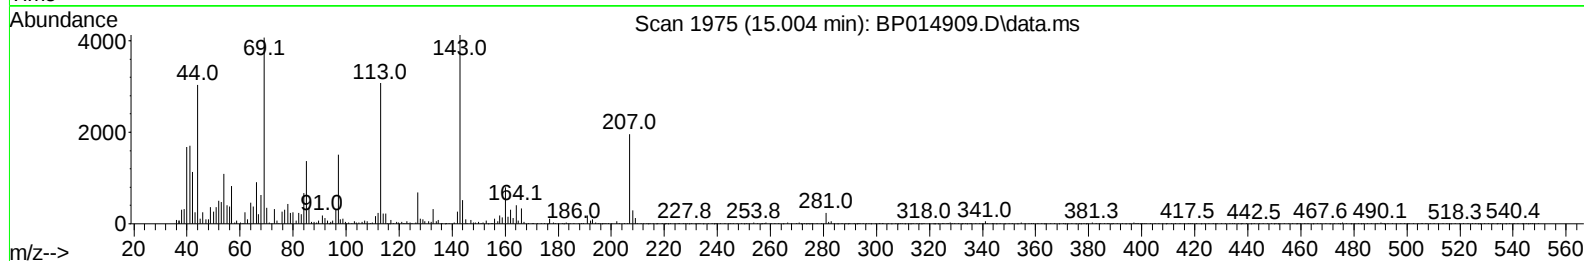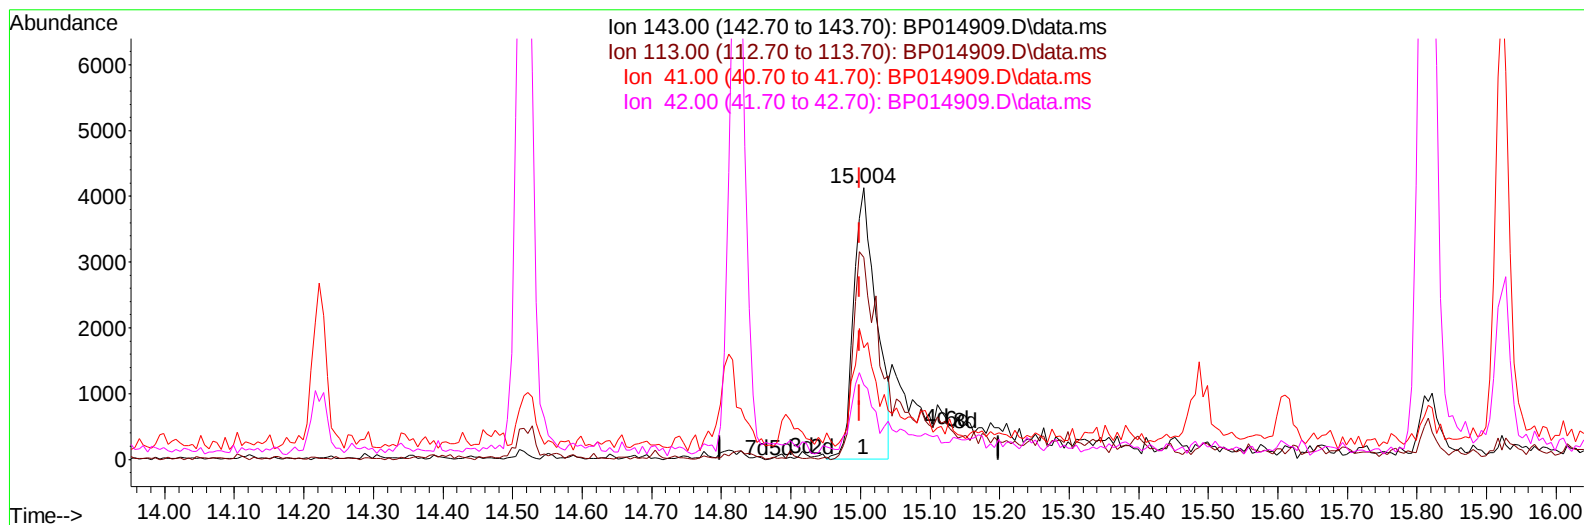

TIC: BP014909.D\data.ms

(54) 4-Nitrophenol-d4 (S)**15.004min (+ 0.006) 1.88 ng/u1****response 9284**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	68.20	74.44
41.00	36.10	41.24
42.00	26.80	27.38




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014909.D
Acq On : 01 May 2023 11:53
Operator : CG/JU
Sample : 02551-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE77

Manual IntegrationsAPPROVED

Quant Time: May 02 00:19:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

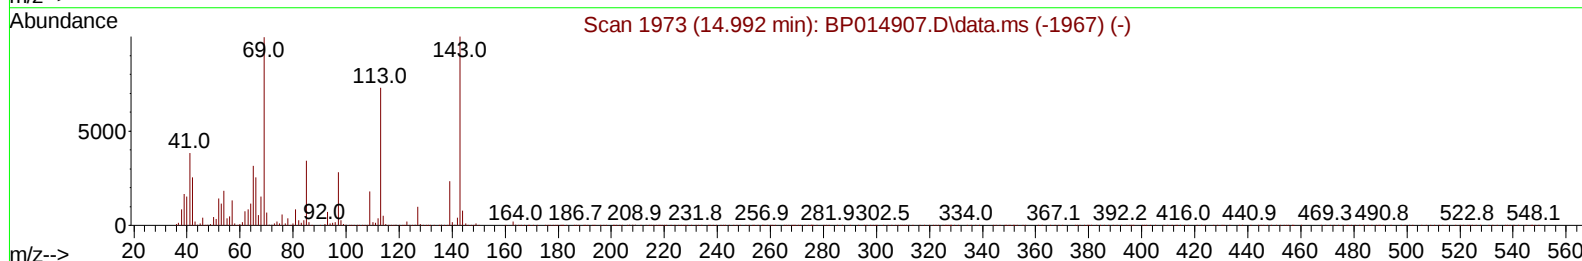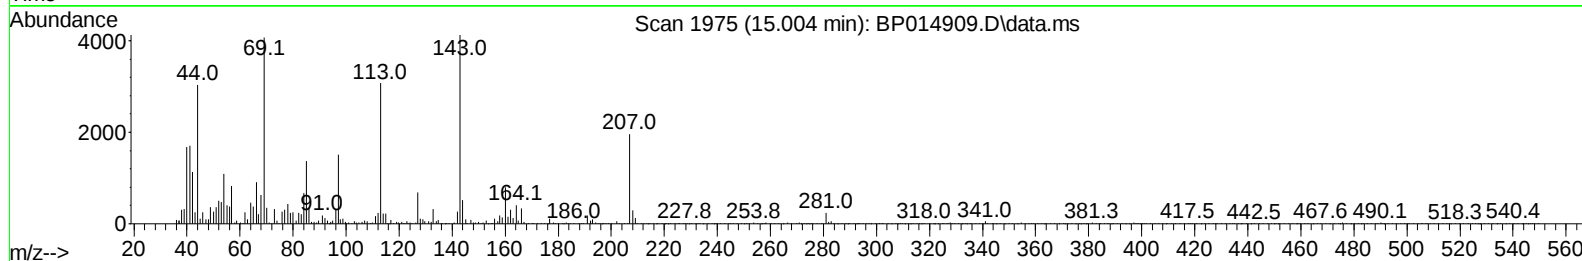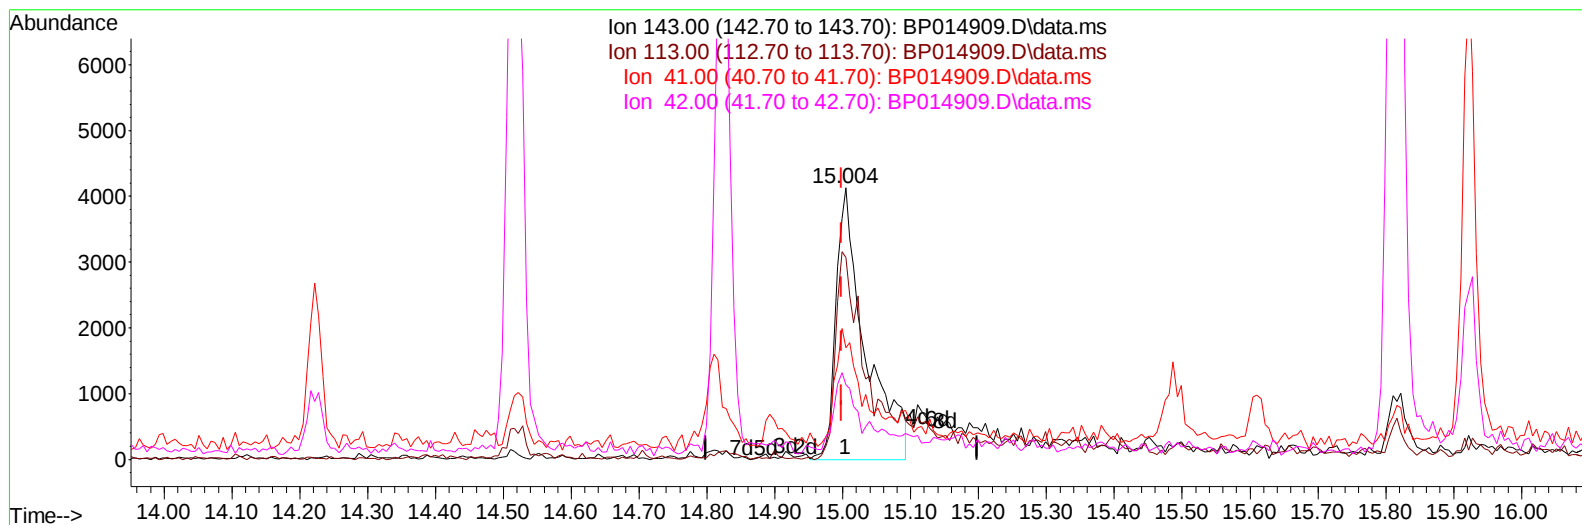

TIC: BP014909.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.004min (+ 0.006) 2.51 ng/ul m

response 12397

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	68.20	74.44
41.00	36.10	41.24
42.00	26.80	27.38

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014909.D
 Acq On : 01 May 2023 11:53
 Operator : CG/JU
 Sample : 02551-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE77

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
 Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: May 02 00:29:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.175	152	197907	20.000	ng/ul	0.00
20) Naphthalene-d8	11.016	136	802466	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.822	164	463882	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.581	188	913321	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	778612	20.000	ng/ul	0.00
88) Perylene-d12	24.274	264	908967	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.470	96	28045	5.107	ng/uL	0.00
4) Pyridine-d5	3.911	84	129067	9.778	ng/ul	0.00
7) Phenol-d5	7.317	99	107876	6.964	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.493	67	322691	33.216	ng/ul	0.00
11) 2-Chlorophenol-d4	7.699	132	308614	26.314	ng/ul	0.00
15) 4-Methylphenol-d8	8.881	113	189661	16.069	ng/ul	0.00
21) Nitrobenzene-d5	9.352	128	176975	30.716	ng/ul	0.00
24) 2-Nitrophenol-d4	10.081	143	170236	32.186	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.622	165	310279	27.314	ng/ul	0.00
31) 4-Chloroaniline-d4	11.146	131	436031	26.549	ng/ul	0.00
46) Dimethylphthalate-d6	14.222	166	1170919	35.222	ng/ul	0.00
49) Acenaphthylene-d8	14.516	160	1350849	34.017	ng/ul	0.00
54) 4-Nitrophenol-d4	15.004	143	12397m	2.506	ng/ul	0.00
60) Fluorene-d10	15.816	176	1017231	35.102	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.922	200	109549	28.357	ng/ul	0.00
73) Anthracene-d10	17.681	188	1663904	39.891	ng/ul	0.00
81) Pyrene-d10	19.898	212	1900593	43.949	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.104	264	1770395	39.434	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014909.D
Acq On : 01 May 2023 11:53
Operator : CG/JU
Sample : 02551-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE77

Manual IntegrationsAPPROVED

Quant Time: May 02 00:29:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

