

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014922.D
 Acq On : 01 May 2023 19:12
 Operator : CG/JU
 Sample : 02528-08DL 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA38DL

Quant Time: May 02 00:55:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.169	152	211469	20.000	ng/u1	0.00
20) Naphthalene-d8	11.005	136	875536	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.816	164	514246	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.569	188	1071973	20.000	ng/u1	-0.01
79) Chrysene-d12	21.651	240	943117	20.000	ng/u1	-0.01
88) Perylene-d12	24.263	264	1045507	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	11641	1.984	ng/uL	0.00
4) Pyridine-d5	3.911	84	107709	7.636	ng/u1	0.00
7) Phenol-d5	7.311	99	130615	7.892	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.487	67	165986	15.990	ng/u1	0.00
11) 2-Chlorophenol-d4	7.693	132	181608	14.492	ng/u1	0.00
15) 4-Methylphenol-d8	8.875	113	130869	10.377	ng/u1	0.00
21) Nitrobenzene-d5	9.346	128	84857	13.499	ng/u1	0.00
24) 2-Nitrophenol-d4	10.075	143	87104	15.094	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.616	165	179980	14.522	ng/u1	0.00
31) 4-Chloroaniline-d4	11.140	131	98773	5.512	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	666734	18.091	ng/u1	0.00
49) Acenaphthylene-d8	14.510	160	764368	17.363	ng/u1	0.00
54) 4-Nitrophenol-d4	14.993	143	26110	4.761	ng/u1	0.00
60) Fluorene-d10	15.804	176	570219	17.750	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	62362	13.753	ng/u1	0.00
73) Anthracene-d10	17.669	188	848119	17.324	ng/u1	0.00
81) Pyrene-d10	19.886	212	1039766	19.850	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.086	264	939893	18.201	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.499	88	112257	17.967	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014922.D
Acq On : 01 May 2023 19:12
Operator : CG/JU
Sample : 02528-08DL 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA38DL


Quant Time: May 02 00:55:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

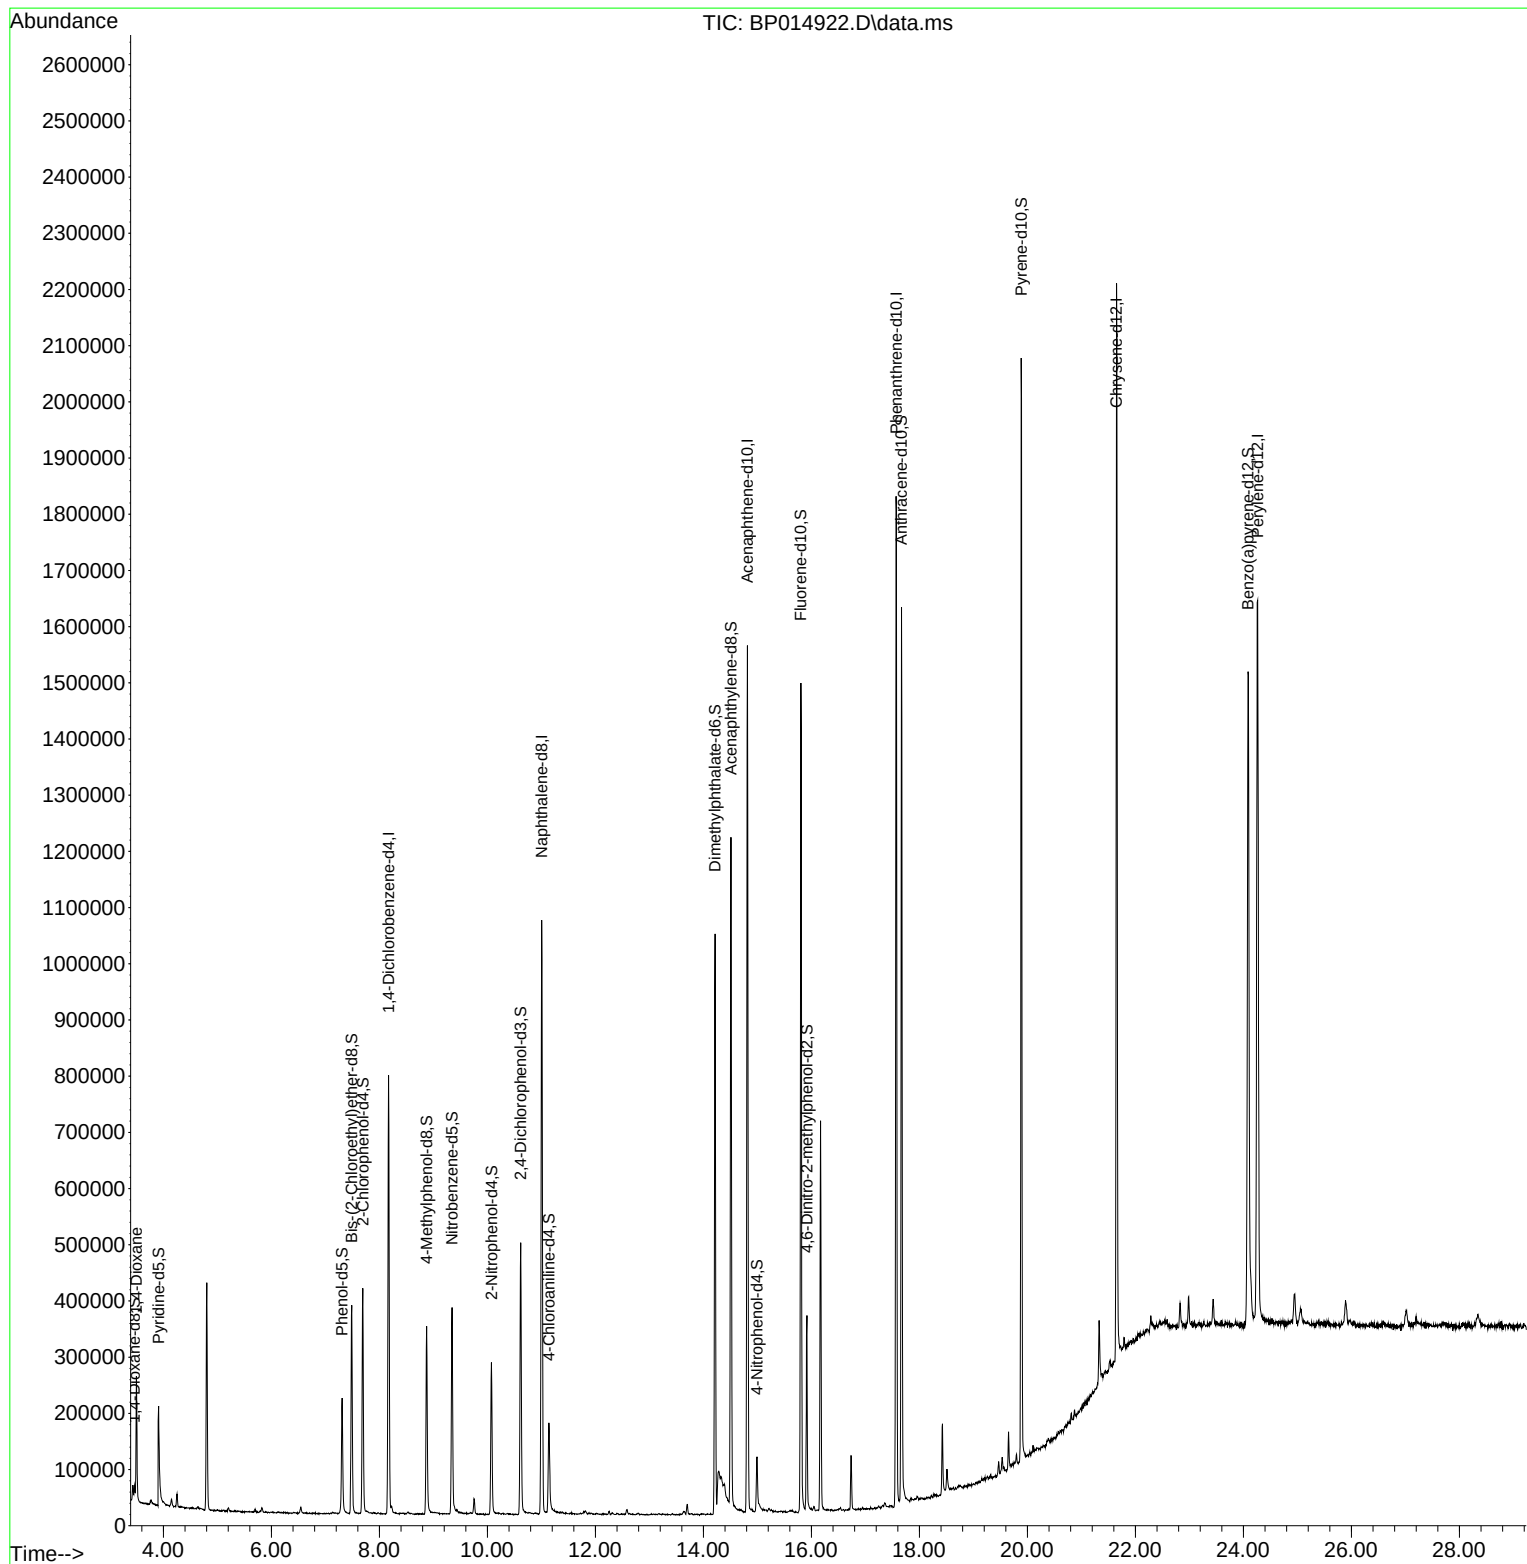

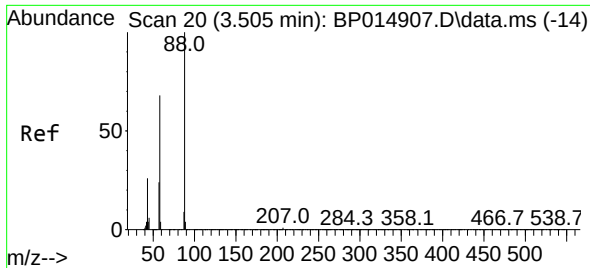

#2
 1,4-Dioxane
 Concen: 17.967 ng/uL
 RT: 3.499 min Scan# 19
 Delta R.T. -0.006 min
 Lab File: BP014922.D
 Acq: 01 May 2023 19:12

Instrument :
 BNA_P
 ClientSampleId :
 HOA38DL

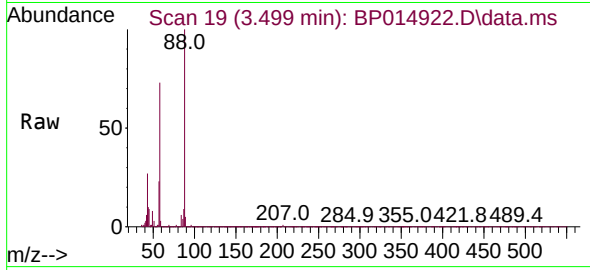

Tgt Ion: 88 Resp: 112257

Ion	Ratio	Lower	Upper
88	100		
43	26.7	22.2	33.4
58	73.1	55.1	82.7

