

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014914.D
 Acq On : 01 May 2023 14:43
 Operator : CG/JU
 Sample : 02528-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	3	8	16	rBV	2267842	3206668	10.44%	3.942%
2	3.499	16	19	34	rVB	801570	1109185	3.61%	1.364%
3	3.911	86	89	109	rBV	220003	360769	1.17%	0.444%
4	4.811	234	242	264	rBV	15520521	30720481	100.00%	37.769%
5	7.311	660	667	681	rBV	131572	227181	0.74%	0.279%
6	7.487	691	697	716	rBV	713083	1140561	3.71%	1.402%
7	7.693	725	732	744	rBV	615793	1021621	3.33%	1.256%
8	8.058	789	794	802	rVB2	28851	50940	0.17%	0.063%
9	8.175	805	814	827	rBV	703107	1195900	3.89%	1.470%
10	8.534	868	875	884	rBV	37918	66239	0.22%	0.081%
11	8.881	926	934	948	rBV	412672	745855	2.43%	0.917%
12	9.346	1006	1013	1027	rBV	707906	1228164	4.00%	1.510%
13	10.081	1130	1138	1150	rBV	520598	893183	2.91%	1.098%
14	10.616	1220	1229	1246	rBV	823583	1467543	4.78%	1.804%
15	11.010	1286	1296	1309	rBV	992834	1647379	5.36%	2.025%
16	11.140	1311	1318	1340	rBV	703841	1344113	4.38%	1.653%
17	14.216	1834	1841	1856	rBV	1894732	2678557	8.72%	3.293%
18	14.516	1885	1892	1905	rBV	2058435	3146454	10.24%	3.868%
19	14.822	1937	1944	1954	rBV	1367781	2053637	6.68%	2.525%
20	14.998	1968	1974	1984	rBV3	33058	76230	0.25%	0.094%
21	15.810	2101	2112	2124	rBV	2710521	3990107	12.99%	4.906%
22	15.916	2125	2130	2140	rVB	653412	925020	3.01%	1.137%
23	16.175	2168	2174	2185	rVB	121286	180499	0.59%	0.222%
24	16.740	2265	2270	2275	rBV	41850	58634	0.19%	0.072%
25	16.875	2286	2293	2300	rBV	27215	47335	0.15%	0.058%
26	17.575	2405	2412	2422	rBV	1562667	2250111	7.32%	2.766%
27	17.675	2422	2429	2449	rVV	2908809	4272892	13.91%	5.253%
28	18.428	2553	2557	2564	rBV4	37024	57199	0.19%	0.070%
29	18.522	2567	2573	2580	rBV	225299	323448	1.05%	0.398%
30	19.469	2730	2734	2740	rBV3	39399	59133	0.19%	0.073%
31	19.539	2742	2746	2754	rVB2	34919	59328	0.19%	0.073%
32	19.657	2762	2766	2769	rBV4	22593	31725	0.10%	0.039%
33	19.892	2800	2806	2824	rBV	3905270	5079850	16.54%	6.245%
34	21.657	3101	3106	3119	rBV	1471365	2258306	7.35%	2.776%
35	24.098	3513	3521	3540	rBV2	2208406	4933742	16.06%	6.066%
36	24.269	3543	3550	3564	rVB2	1097090	2429161	7.91%	2.987%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014914.D
Acq On : 01 May 2023 14:43
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA37

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 81337150

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014914.D
Acq On : 01 May 2023 14:43
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

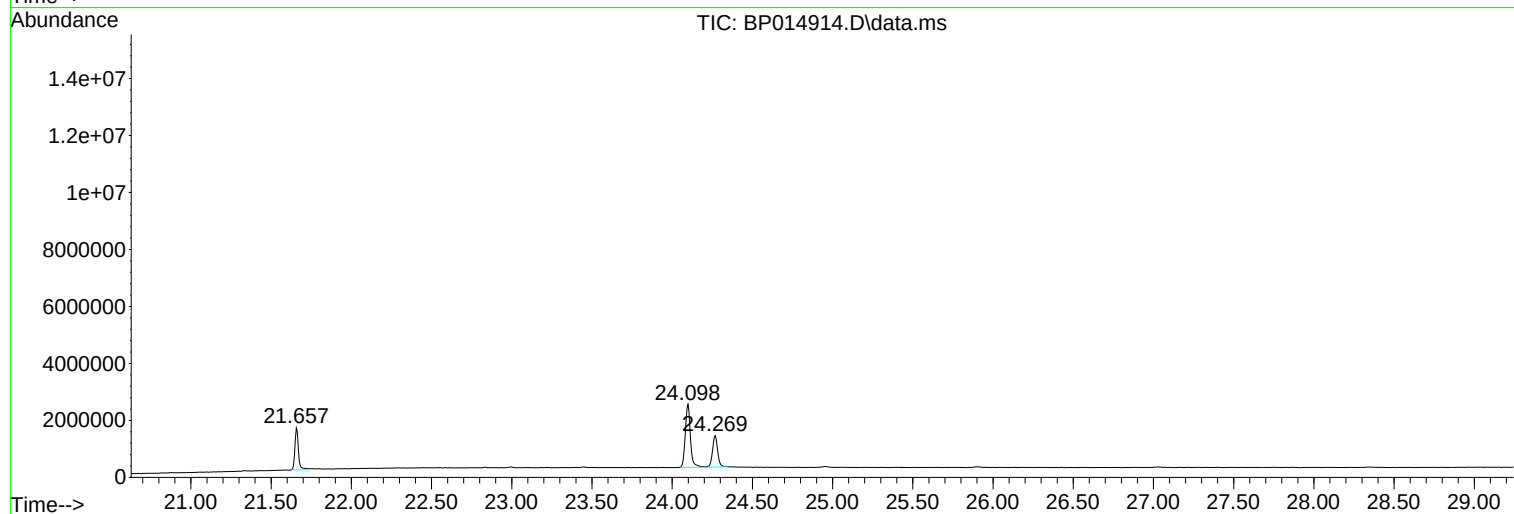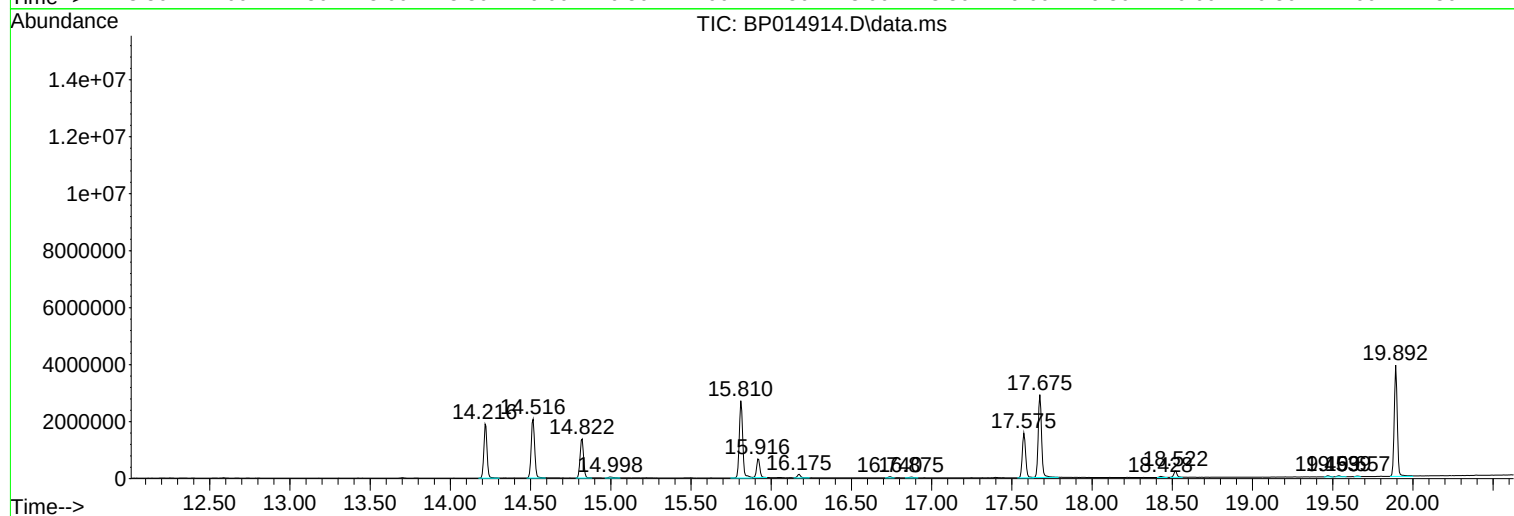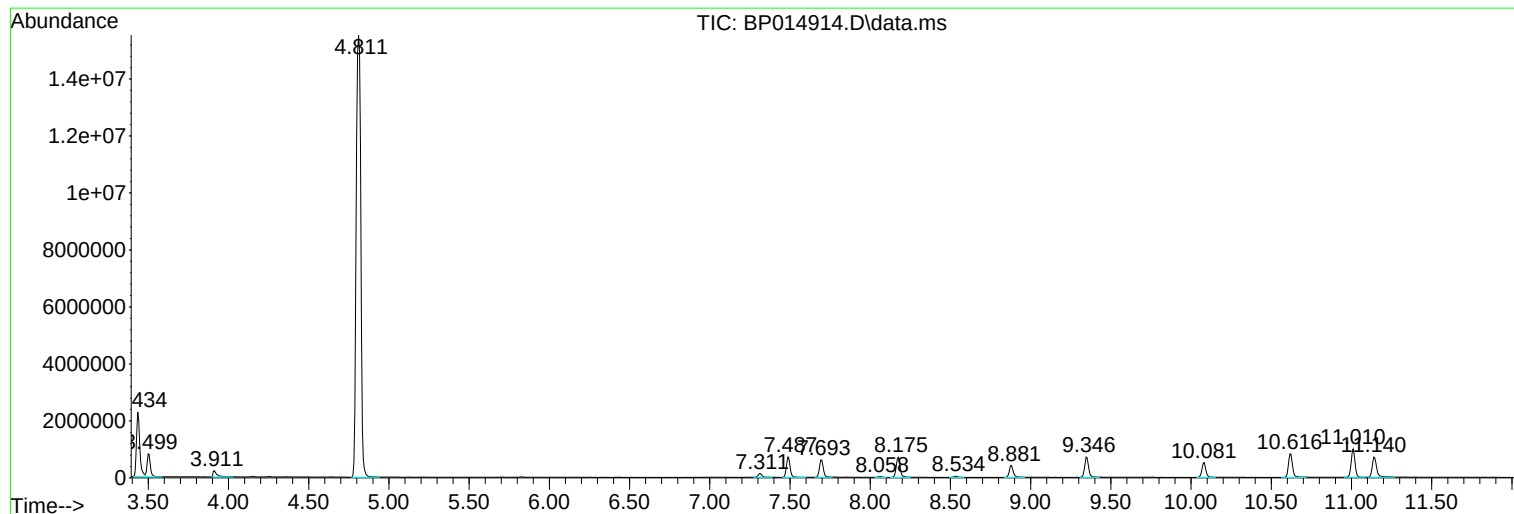

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014914.D
Acq On : 01 May 2023 14:43
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA37










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Bromacil Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.522	2.87 ng/ul	323448	Phenanthrene-d10	17.575

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bromacil	260	C9H13BrN2O2	000314-40-9	91
2			Bromacil	260	C9H13BrN2O2	000314-40-9	91
3			Bromacil	260	C9H13BrN2O2	000314-40-9	78
4			5-Acetamido-2,4-dichlorobenzoic ...	247	C9H7Cl2NO3	050602-49-8	59
5			5-Chloro-2,3-dihydrofuro(2,3-b)q...	205	C11H8ClNO	064124-92-1	38

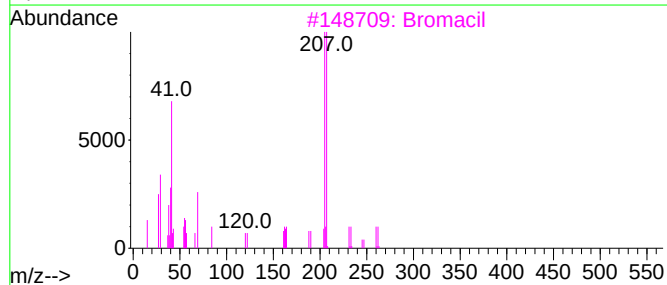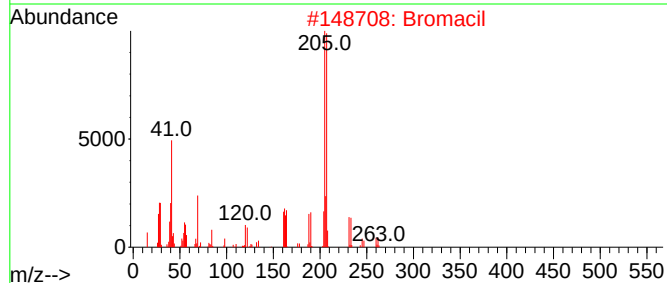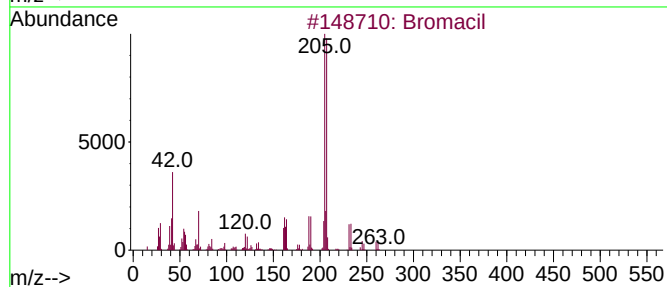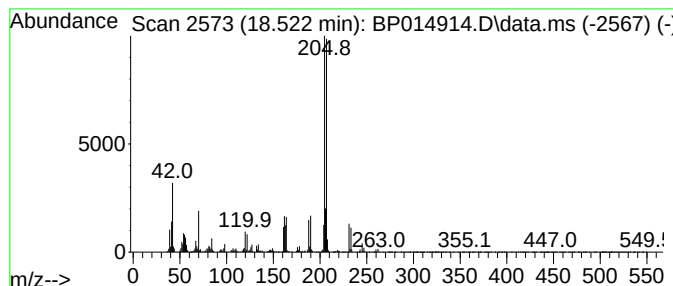

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014914.D
Acq On : 01 May 2023 14:43
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Bromacil	18.522	2.9	ng/u1	323448	4	17.575	2250110	20.0