

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014917.D
 Acq On : 01 May 2023 16:24
 Operator : CG/JU
 Sample : 02528-02DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	3	8	15	rBV	411248	560253	5.73%	1.911%
2	3.499	15	19	28	rVB	234958	309077	3.16%	1.054%
3	3.923	90	91	106	rBV	29786	65994	0.67%	0.225%
4	4.252	143	147	152	rVB	31195	41122	0.42%	0.140%
5	4.805	234	241	257	rBV	6512201	9782901	100.00%	33.362%
6	7.311	661	667	674	rBV	24646	42895	0.44%	0.146%
7	7.487	691	697	709	rBV	151669	249167	2.55%	0.850%
8	7.693	724	732	743	rBV	123046	211329	2.16%	0.721%
9	8.169	805	813	828	rBV	785420	1318140	13.47%	4.495%
10	8.875	926	933	941	rBV2	63285	125344	1.28%	0.427%
11	9.346	1006	1013	1025	rBV	124423	234427	2.40%	0.799%
12	10.075	1129	1137	1151	rBV	80205	154437	1.58%	0.527%
13	10.616	1222	1229	1241	rBV	132172	256101	2.62%	0.873%
14	11.005	1288	1295	1310	rBV	1053004	1815288	18.56%	6.191%
15	11.140	1312	1318	1331	rVV	93775	200424	2.05%	0.684%
16	13.699	1749	1753	1761	rVB3	10708	17367	0.18%	0.059%
17	14.216	1833	1841	1855	rBV	360985	536401	5.48%	1.829%
18	14.510	1882	1891	1903	rBV	378903	596011	6.09%	2.033%
19	14.816	1936	1943	1959	rBV	1517700	2231478	22.81%	7.610%
20	15.804	2105	2111	2124	rBV	470392	749115	7.66%	2.555%
21	15.916	2124	2130	2146	rVB2	68411	130250	1.33%	0.444%
22	16.169	2169	2173	2179	rBV	39080	58672	0.60%	0.200%
23	16.734	2265	2269	2273	rBV4	8205	12767	0.13%	0.044%
24	17.569	2404	2411	2422	rBV	1603840	2376491	24.29%	8.104%
25	17.669	2423	2428	2438	rVB	511478	744053	7.61%	2.537%
26	18.510	2567	2571	2580	rBV	27622	46111	0.47%	0.157%
27	19.886	2800	2805	2816	rBV	676487	970502	9.92%	3.310%
28	21.657	3100	3106	3118	rBV	1493160	2357360	24.10%	8.039%
29	24.086	3514	3519	3526	rBV	349901	708127	7.24%	2.415%
30	24.263	3542	3549	3560	rVB2	1129808	2421551	24.75%	8.258%




Sum of corrected areas: 29323155

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014917.D
Acq On : 01 May 2023 16:24
Operator : CG/JU
Sample : 02528-02DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA34DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

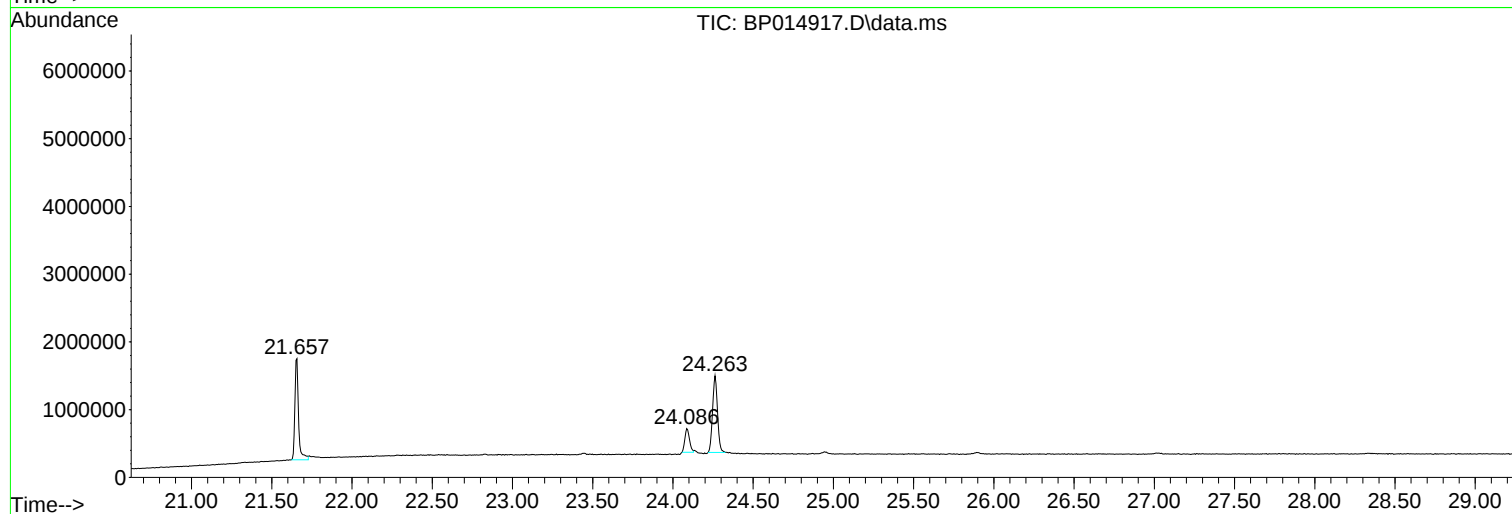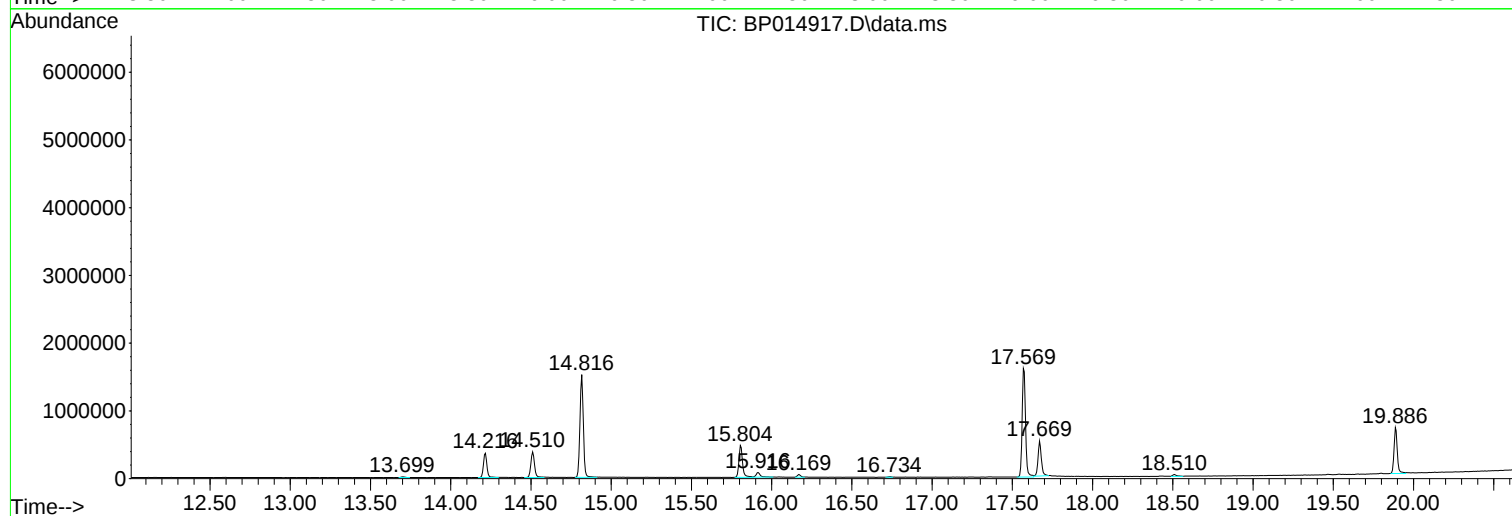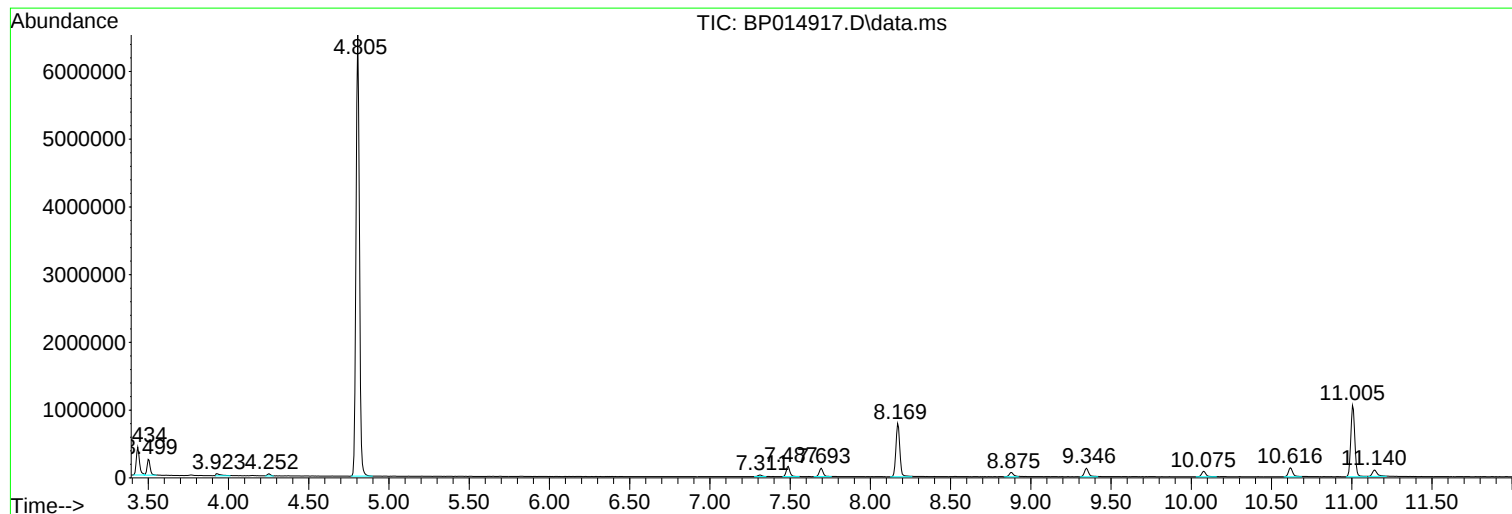

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014917.D
Acq On : 01 May 2023 16:24
Operator : CG/JU
Sample : 02528-02DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA34DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014917.D
Acq On : 01 May 2023 16:24
Operator : CG/JU
Sample : 02528-02DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA34DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
