

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014918.D
 Acq On : 01 May 2023 16:58
 Operator : CG/JU
 Sample : 02528-03DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA35DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	3	8	16	rBV	438305	602686	6.26%	2.141%
2	3.499	16	19	28	rVB	151941	203177	2.11%	0.722%
3	3.764	61	64	73	rVB7	6799	14365	0.15%	0.051%
4	3.928	91	92	104	rBV	23381	44875	0.47%	0.159%
5	4.252	142	147	152	rVB	31385	42617	0.44%	0.151%
6	4.805	234	241	260	rBV	6414903	9628875	100.00%	34.211%
7	7.311	662	667	677	rVB2	19298	34534	0.36%	0.123%
8	7.487	691	697	705	rBV	123496	206005	2.14%	0.732%
9	7.693	725	732	741	rBV	101872	171838	1.78%	0.611%
10	8.169	805	813	830	rBV	746672	1245318	12.93%	4.425%
11	8.875	926	933	945	rBV2	50741	109189	1.13%	0.388%
12	9.346	1006	1013	1023	rBV	103061	192949	2.00%	0.686%
13	10.075	1131	1137	1147	rBV2	62331	117905	1.22%	0.419%
14	10.616	1222	1229	1238	rBV	111751	200703	2.08%	0.713%
15	11.005	1287	1295	1304	rBV	973646	1699447	17.65%	6.038%
16	11.140	1312	1318	1332	rBV	65083	145614	1.51%	0.517%
17	13.699	1748	1753	1761	rVB	20019	31991	0.33%	0.114%
18	14.216	1835	1841	1857	rBV	323023	473953	4.92%	1.684%
19	14.510	1884	1891	1912	rBV	339726	514636	5.34%	1.828%
20	14.816	1935	1943	1963	rBV	1486577	2184286	22.68%	7.761%
21	15.804	2105	2111	2125	rBV	415491	671216	6.97%	2.385%
22	15.916	2125	2130	2137	rVB	52644	86956	0.90%	0.309%
23	16.169	2168	2173	2182	rBV	77461	122621	1.27%	0.436%
24	16.740	2264	2270	2277	rBV3	15449	23751	0.25%	0.084%
25	17.575	2404	2412	2422	rBV	1550621	2328030	24.18%	8.271%
26	17.669	2423	2428	2445	rVB2	460520	737347	7.66%	2.620%
27	18.428	2554	2557	2562	rBV7	8336	11857	0.12%	0.042%
28	18.510	2567	2571	2578	rVV2	26123	37657	0.39%	0.134%
29	19.886	2800	2805	2814	rBV	625352	889852	9.24%	3.162%
30	21.657	3101	3106	3121	rBV	1511559	2284094	23.72%	8.115%
31	24.092	3514	3520	3526	rBV2	330298	685891	7.12%	2.437%
32	24.263	3542	3549	3561	rBV2	1095449	2401455	24.94%	8.532%




Sum of corrected areas: 28145690

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014918.D
Acq On : 01 May 2023 16:58
Operator : CG/JU
Sample : 02528-03DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA35DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

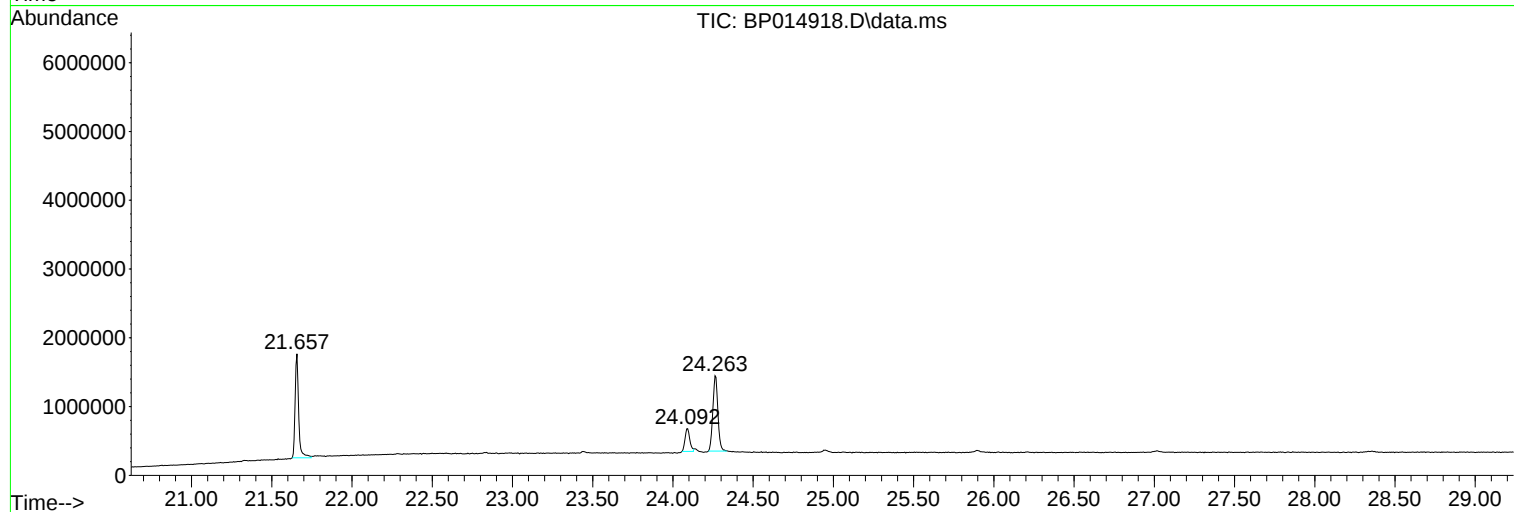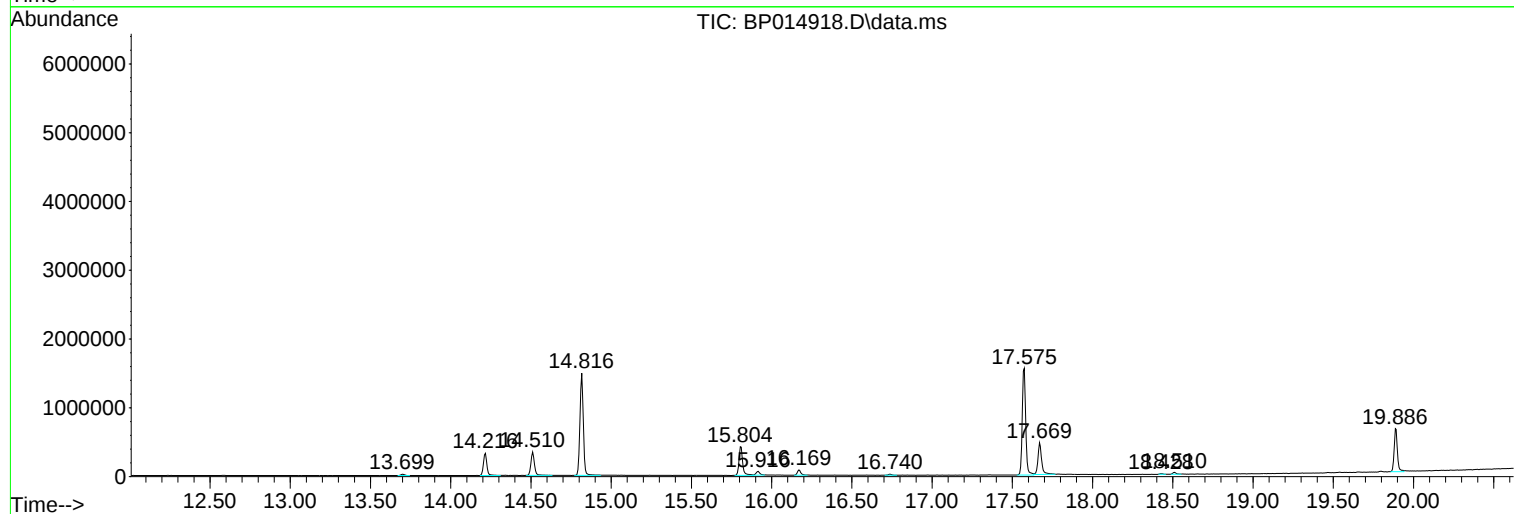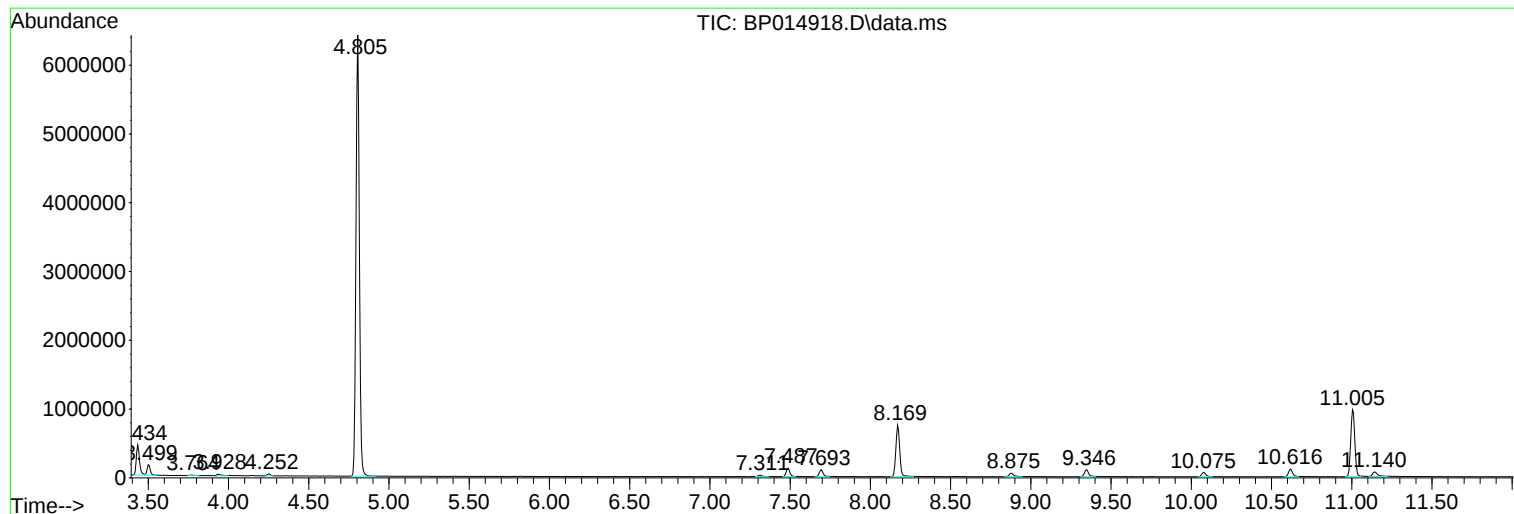

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014918.D
Acq On : 01 May 2023 16:58
Operator : CG/JU
Sample : 02528-03DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA35DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014918.D
Acq On : 01 May 2023 16:58
Operator : CG/JU
Sample : 02528-03DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA35DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------