

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
 Data File : BP014920.D
 Acq On : 01 May 2023 18:05
 Operator : CG/JU
 Sample : 02528-10DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	3	8	15	rBV	537848	741953	6.33%	2.396%
2	3.499	15	19	31	rVB	195848	270503	2.31%	0.874%
3	3.928	89	92	101	rBV	27327	56143	0.48%	0.181%
4	4.152	127	130	140	rVB6	7597	14185	0.12%	0.046%
5	4.252	142	147	152	rVB	29523	40823	0.35%	0.132%
6	4.805	234	241	261	rBV	7669797	11727688	100.00%	37.873%
7	7.310	661	667	678	rBV2	24378	45679	0.39%	0.148%
8	7.487	688	697	706	rBV	148539	252012	2.15%	0.814%
9	7.693	725	732	740	rBV	119647	204535	1.74%	0.661%
10	8.057	790	794	803	rVB7	7661	14642	0.12%	0.047%
11	8.169	806	813	827	rBV	724238	1198297	10.22%	3.870%
12	8.528	868	874	879	rBV2	10204	17648	0.15%	0.057%
13	8.875	926	933	944	rBV	62363	127786	1.09%	0.413%
14	9.346	1003	1013	1024	rBV	124474	235618	2.01%	0.761%
15	10.075	1131	1137	1150	rBV	79880	149848	1.28%	0.484%
16	10.616	1221	1229	1238	rBV	142691	259840	2.22%	0.839%
17	11.004	1286	1295	1305	rBV	954927	1657700	14.13%	5.353%
18	11.140	1312	1318	1334	rBV	98607	206439	1.76%	0.667%
19	13.698	1747	1753	1759	rBV4	8808	15636	0.13%	0.050%
20	14.216	1834	1841	1849	rBV	405057	570797	4.87%	1.843%
21	14.510	1884	1891	1904	rBV	414454	625199	5.33%	2.019%
22	14.816	1936	1943	1958	rBV	1410119	2070605	17.66%	6.687%
23	15.810	2104	2112	2124	rBV	509204	821157	7.00%	2.652%
24	15.916	2124	2130	2140	rVB	66177	117890	1.01%	0.381%
25	16.175	2169	2174	2181	rBV	17743	31287	0.27%	0.101%
26	16.739	2265	2270	2275	rBV3	8980	12208	0.10%	0.039%
27	17.575	2405	2412	2423	rBV	1487025	2225382	18.98%	7.187%
28	17.669	2423	2428	2445	rVB2	532377	853253	7.28%	2.756%
29	18.510	2567	2571	2577	rBV2	28209	41677	0.36%	0.135%
30	19.886	2800	2805	2815	rBV	747603	1019961	8.70%	3.294%
31	21.657	3100	3106	3116	rBV	1386973	2179841	18.59%	7.040%
32	24.092	3514	3520	3534	rVB	385493	907272	7.74%	2.930%
33	24.263	3542	3549	3560	rVB2	1068724	2251923	19.20%	7.272%




Sum of corrected areas: 30965427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014920.D
Acq On : 01 May 2023 18:05
Operator : CG/JU
Sample : 02528-10DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA40DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

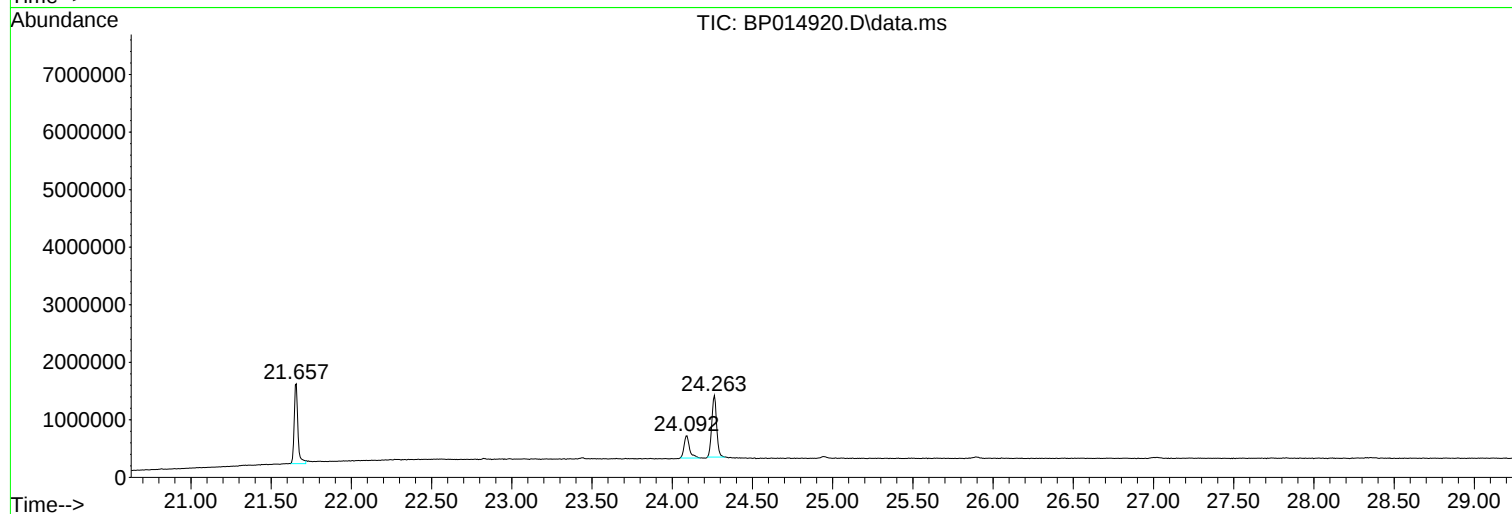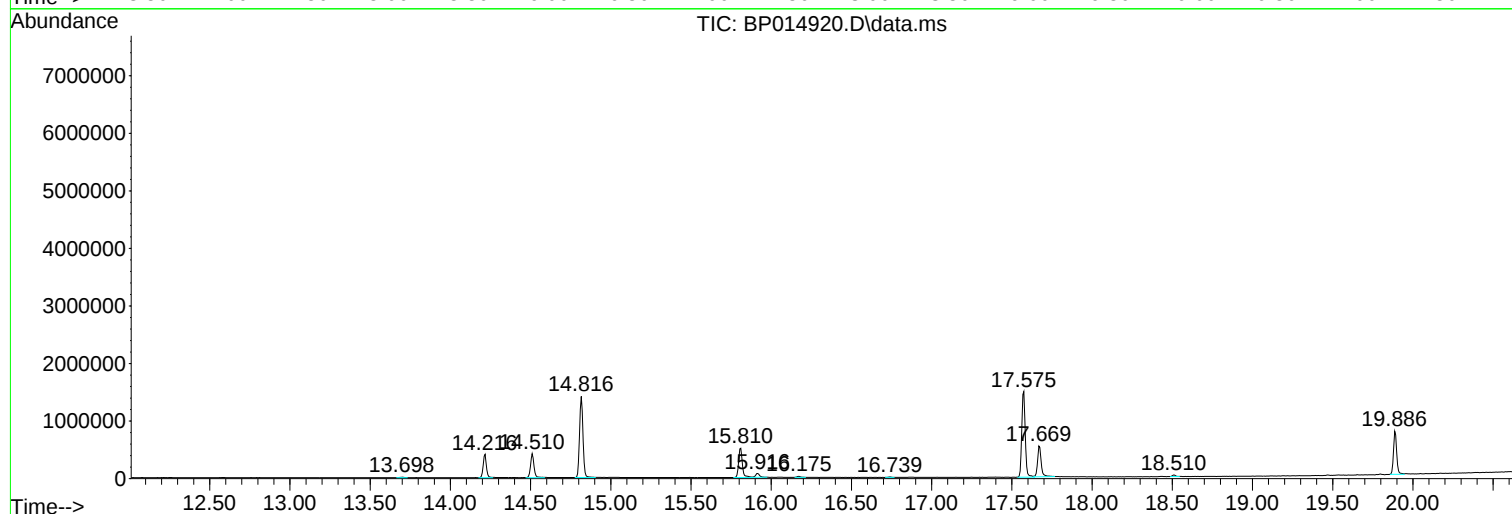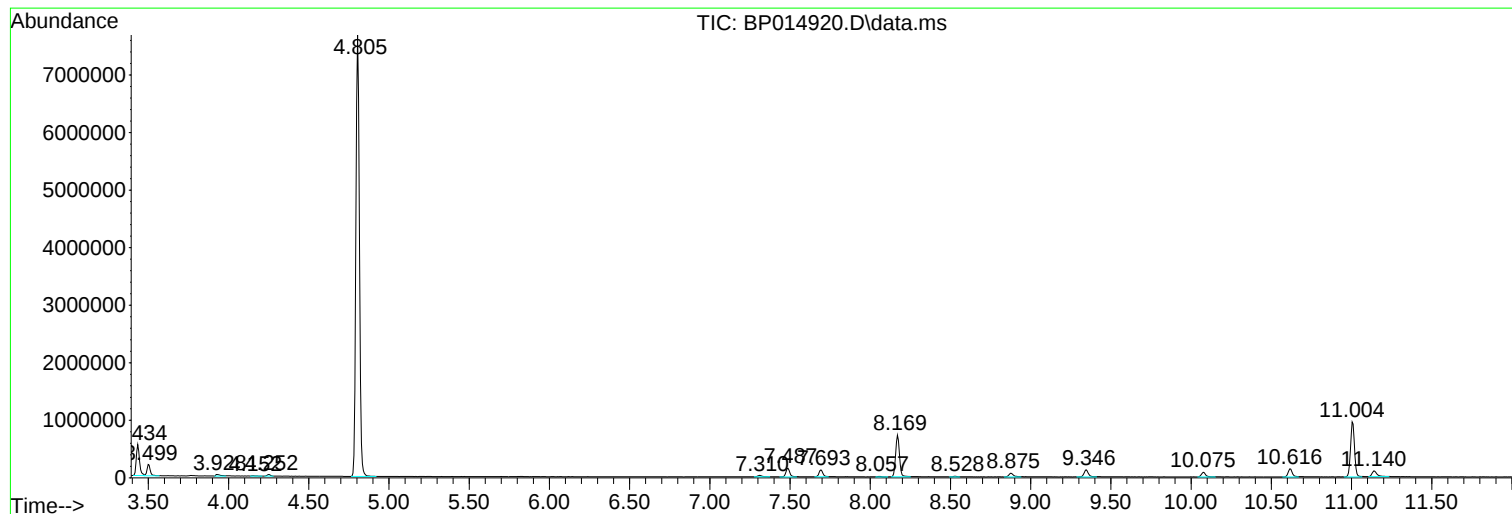

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014920.D
Acq On : 01 May 2023 18:05
Operator : CG/JU
Sample : 02528-10DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA40DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050123\
Data File : BP014920.D
Acq On : 01 May 2023 18:05
Operator : CG/JU
Sample : 02528-10DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA40DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------