




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010230.D
Acq On : 04 May 2022 19:07
Operator : CG/JU
Sample : N2668-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL69

Manual IntegrationsAPPROVED

Quant Time: May 05 02:40:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :mohammad ahmed 05/09/2022

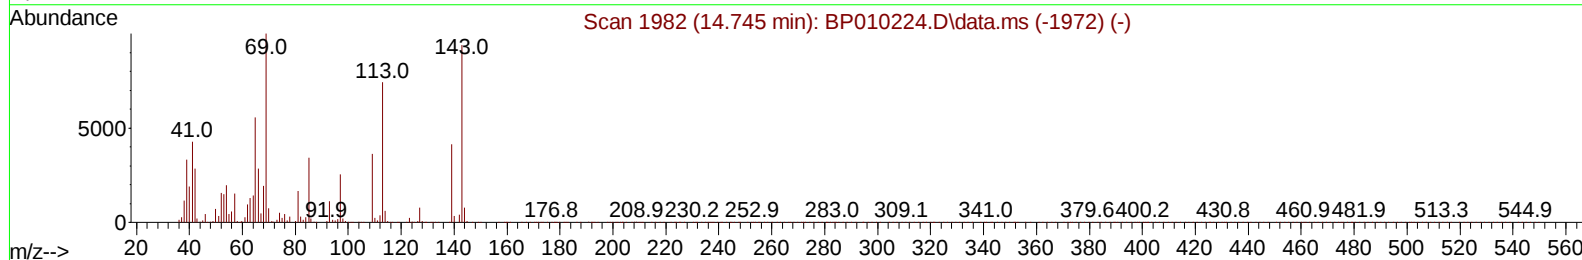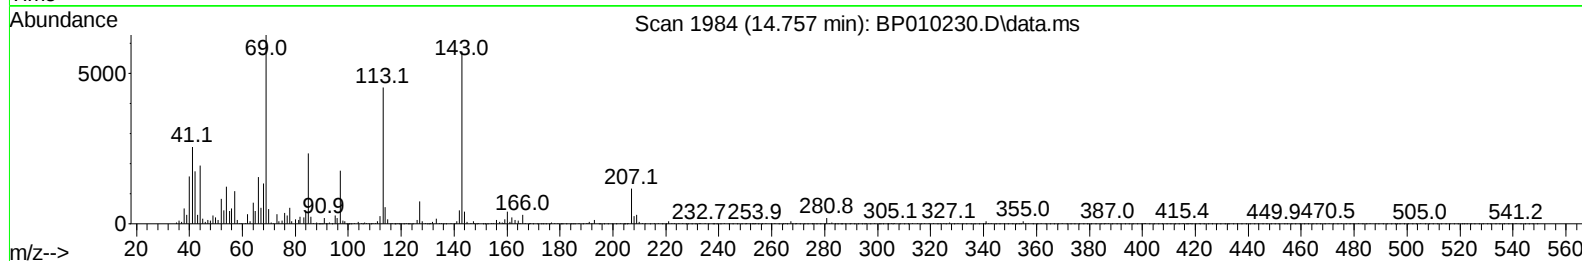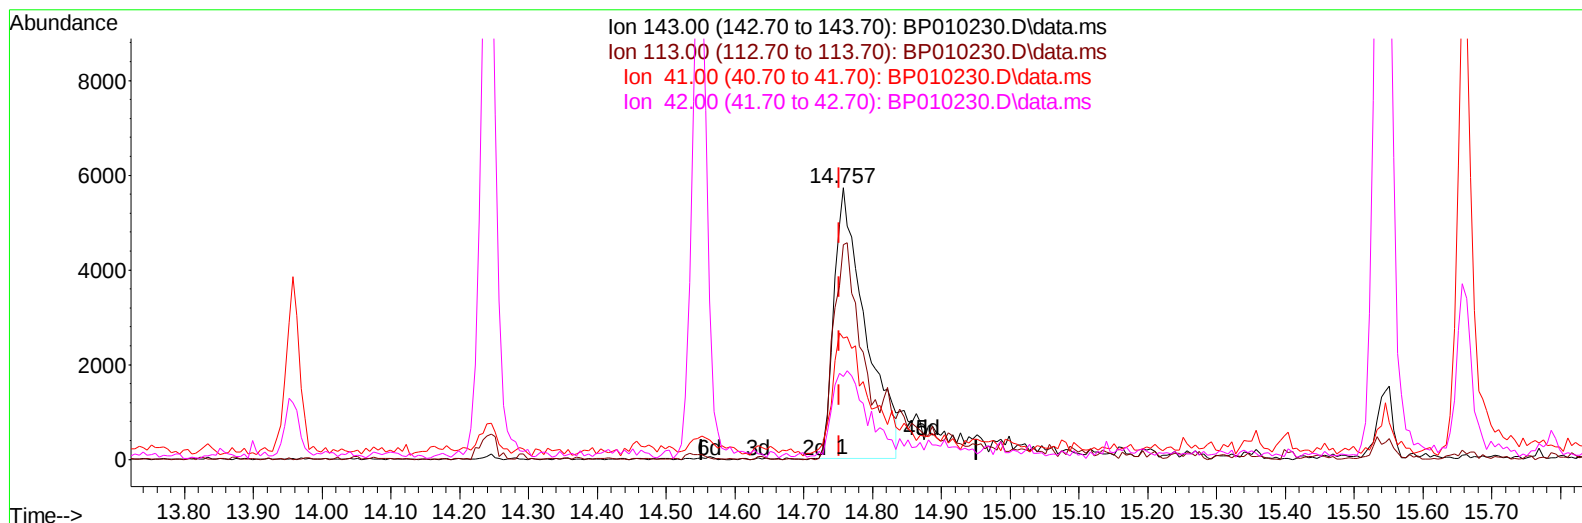

TIC: BP010230.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 2.53 ng/u1

response 18058

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.00#
41.00	23.20	44.74#
42.00	18.00	30.58#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010230.D
 Acq On : 04 May 2022 19:07
 Operator : CG/JU
 Sample : N2668-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL69

Manual IntegrationsAPPROVED

Quant Time: May 05 02:40:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :mohammad ahmed 05/09/2022

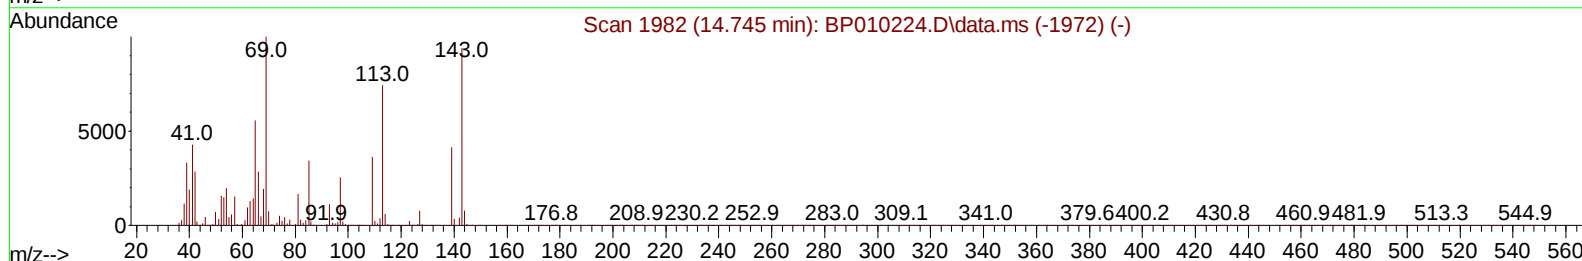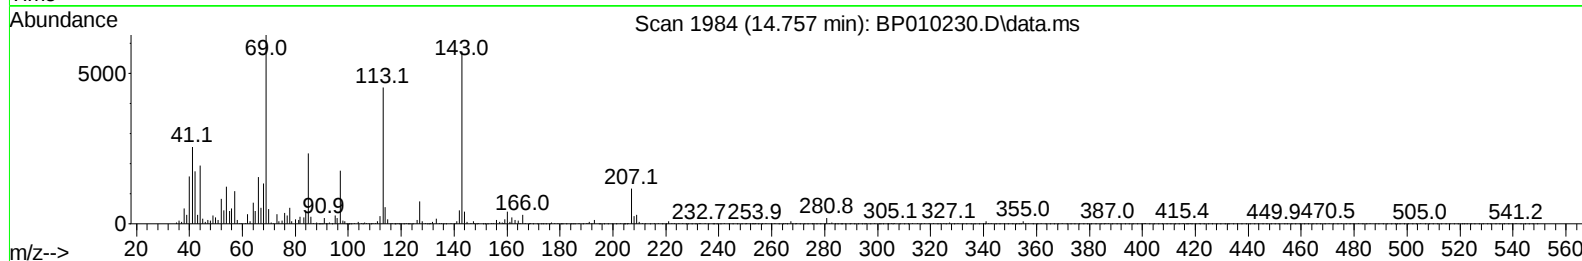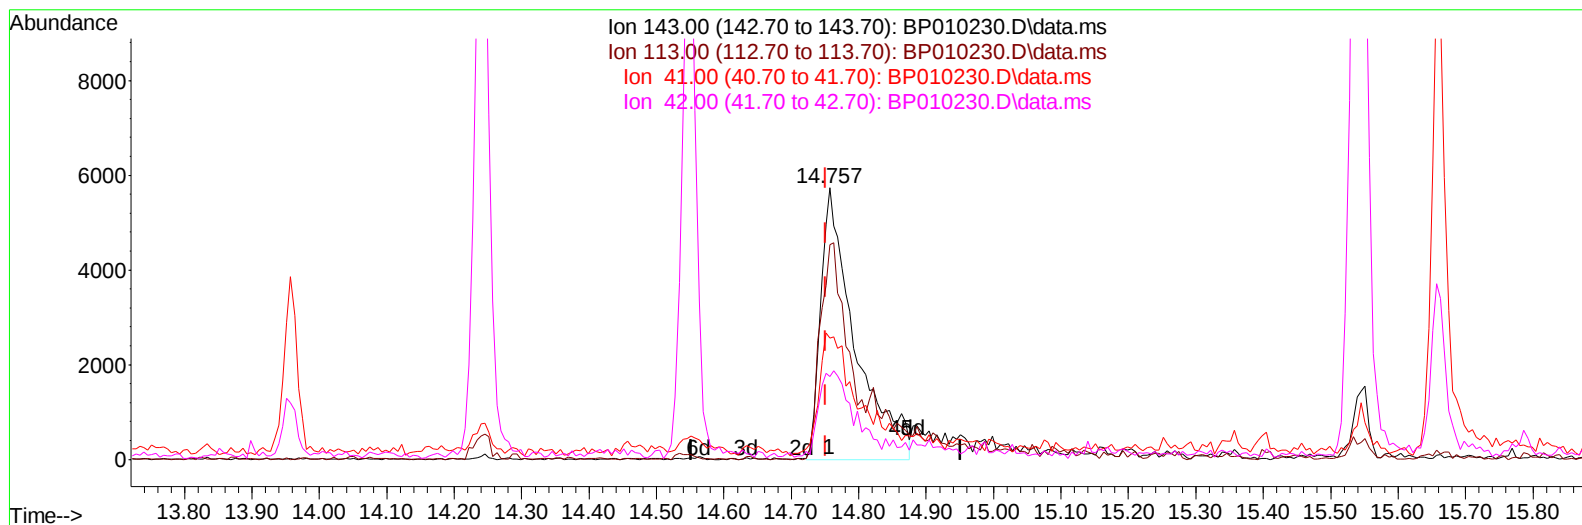

TIC: BP010230.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 2.83 ng/ul m

response 2022

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.00#
41.00	23.20	44.74#
42.00	18.00	30.58#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010230.D
 Acq On : 04 May 2022 19:07
 Operator : CG/JU
 Sample : N2668-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL69

Manual IntegrationsAPPROVED

Quant Time: May 05 02:40:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :mohammad ahmed 05/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	166861	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	740046	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	498353	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	1001175	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	685456	20.000	ng/ul	0.00
88) Perylene-d12	23.827	264	617248	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	16106	4.209	ng/uL	0.00
4) Pyridine-d5	3.781	84	62953	5.848	ng/ul	0.00
7) Phenol-d5	7.081	99	78683	5.184	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	325881	35.783	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	274502	24.421	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	167333	13.307	ng/ul	-0.01
21) Nitrobenzene-d5	9.075	128	207569	35.265	ng/ul	0.00
24) 2-Nitrophenol-d4	9.799	143	211804	32.949	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	333025	26.612	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.857	131	354902	19.779	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1388068	35.806	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	1560994	33.271	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.757	143	20222m	2.834	ng/ul	0.00
60) Fluorene-d10	15.545	176	1193685	35.796	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	165274	26.107	ng/ul	0.00
73) Anthracene-d10	17.398	188	1710189	35.308	ng/ul	-0.01
81) Pyrene-d10	19.633	212	1783040	45.740	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1230807	38.035	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010230.D
Acq On : 04 May 2022 19:07
Operator : CG/JU
Sample : N2668-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL69

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :mohammad ahmed 05/09/2022

Quant Time: May 05 02:40:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

