

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010227.D
 Acq On : 04 May 2022 17:26
 Operator : CG/JU
 Sample : N2668-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	52	rVB2	33561	46669	1.10%	0.114%
2	3.787	115	119	133	rBV	82304	159749	3.75%	0.389%
3	4.005	154	156	160	rVB5	5694	6569	0.15%	0.016%
4	4.099	169	172	177	rBV	16499	22014	0.52%	0.054%
5	4.634	258	263	272	rVB	53408	83925	1.97%	0.204%
6	7.081	673	679	695	rVB	120866	211957	4.97%	0.516%
7	7.246	699	707	721	rBV	600578	986063	23.14%	2.402%
8	7.452	734	742	755	rBV	541640	911427	21.39%	2.221%
9	7.546	755	758	761	rVB4	3429	4596	0.11%	0.011%
10	7.916	812	821	829	rBV	637805	1023520	24.02%	2.494%
11	8.622	934	941	956	rBV	391002	680941	15.98%	1.659%
12	9.075	1009	1018	1028	rBV	787648	1348005	31.63%	3.284%
13	9.140	1028	1029	1035	rVB6	5347	5093	0.12%	0.012%
14	9.257	1045	1049	1056	rVB10	2558	6147	0.14%	0.015%
15	9.522	1088	1094	1102	rVB2	9763	16477	0.39%	0.040%
16	9.799	1134	1141	1156	rBV	613755	1054039	24.74%	2.568%
17	10.340	1226	1233	1249	rBV	761292	1396666	32.78%	3.403%
18	10.722	1290	1298	1313	rBV	906822	1571136	36.87%	3.828%
19	10.857	1313	1321	1345	rBV	583200	1179472	27.68%	2.874%
20	12.010	1514	1517	1525	rBV10	2514	4334	0.10%	0.011%
21	12.157	1537	1542	1551	rVB10	3662	7368	0.17%	0.018%
22	12.316	1562	1569	1576	rBV	14620	30736	0.72%	0.075%
23	12.528	1600	1605	1608	rBV6	2213	4562	0.11%	0.011%
24	13.169	1710	1714	1718	rBV7	2762	4459	0.10%	0.011%
25	13.381	1746	1750	1755	rVB5	6504	10336	0.24%	0.025%
26	13.834	1823	1827	1833	rBV9	2939	6386	0.15%	0.016%
27	13.957	1840	1848	1861	rBV	1849527	2604666	61.13%	6.346%
28	14.239	1889	1896	1914	rBV	1914297	2920784	68.54%	7.116%
29	14.551	1941	1949	1963	rBV	1404888	2141132	50.25%	5.216%
30	14.751	1978	1983	2004	rBV3	33491	117559	2.76%	0.286%
31	15.304	2072	2077	2079	rVB6	2894	4704	0.11%	0.011%
32	15.369	2081	2088	2093	rVV4	12264	19756	0.46%	0.048%
33	15.545	2106	2118	2132	rBV	2416508	3787641	88.89%	9.228%
34	15.663	2132	2138	2153	rVV	696716	1088882	25.55%	2.653%
35	15.786	2155	2159	2164	rVB	31510	49049	1.15%	0.119%
36	16.328	2246	2251	2259	rVB5	11173	18981	0.45%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010227.D
 Acq On : 04 May 2022 17:26
 Operator : CG/JU
 Sample : N2668-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	16.980	2356	2362	2367	rBV9	6520	12493	0.29%	0.030%
38	17.304	2409	2417	2427	rBV	1645779	2441710	57.30%	5.949%
39	17.398	2427	2433	2456	rVB2	2703347	4261189	100.00%	10.382%
40	17.886	2508	2516	2518	rBV9	3083	7233	0.17%	0.018%
41	18.192	2564	2568	2573	rBV8	5121	11302	0.27%	0.028%
42	18.663	2644	2648	2651	rBV6	4237	5990	0.14%	0.015%
43	19.210	2737	2741	2746	rBV4	35253	49599	1.16%	0.121%
44	19.280	2749	2753	2759	rVB2	28679	40326	0.95%	0.098%
45	19.633	2807	2813	2827	rBV	3198912	4246643	99.66%	10.346%
46	21.092	3058	3061	3067	rBV5	38458	59579	1.40%	0.145%
47	21.386	3106	3111	3117	rBV	1287661	1733849	40.69%	4.224%
48	23.668	3492	3499	3517	rVB2	1446699	3034713	71.22%	7.394%
49	23.827	3520	3526	3538	rVB2	756758	1604961	37.66%	3.910%


Sum of corrected areas: 41045387

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010227.D
Acq On : 04 May 2022 17:26
Operator : CG/JU
Sample : N2668-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL67

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

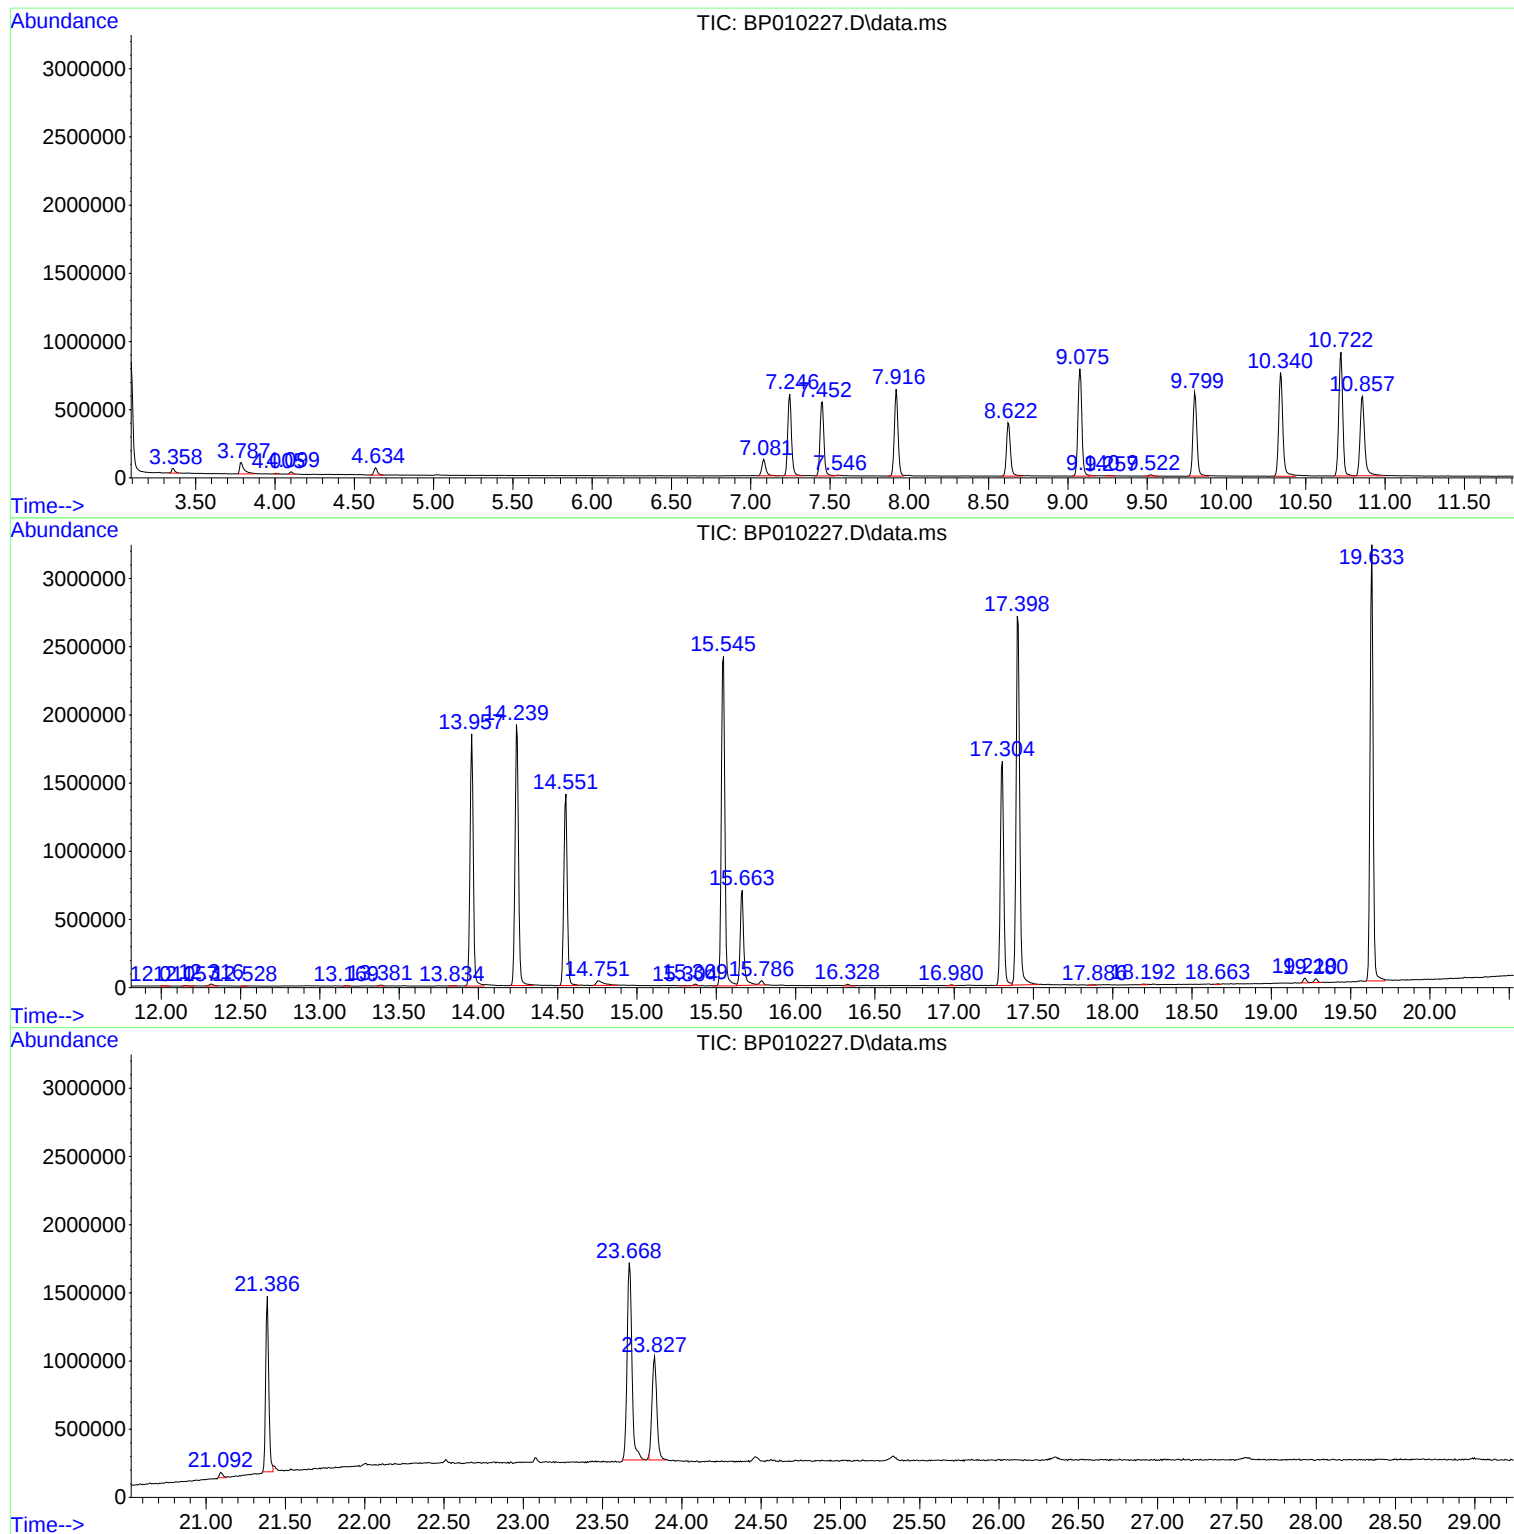

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010227.D
Acq On : 04 May 2022 17:26
Operator : CG/JU
Sample : N2668-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL67

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010227.D
Acq On : 04 May 2022 17:26
Operator : CG/JU
Sample : N2668-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL67

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc