

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010230.D
 Acq On : 04 May 2022 19:07
 Operator : CG/JU
 Sample : N2668-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	56	rVB	35502	58948	1.29%	0.132%
2	3.781	115	118	133	rBV	110207	198521	4.34%	0.443%
3	4.105	169	173	178	rVB	13273	18935	0.41%	0.042%
4	5.022	327	329	331	rBV2	4398	4767	0.10%	0.011%
5	7.081	672	679	692	rBV	136905	242403	5.30%	0.541%
6	7.246	700	707	720	rBV	705913	1146812	25.08%	2.560%
7	7.340	721	723	730	rVB8	4550	7112	0.16%	0.016%
8	7.446	735	741	755	rVV	618427	1041223	22.77%	2.324%
9	7.546	757	758	766	rVB8	5644	8306	0.18%	0.019%
10	7.916	812	821	831	rBV	631686	1028609	22.49%	2.296%
11	7.993	831	834	842	rVB6	6033	11888	0.26%	0.027%
12	8.622	933	941	955	rBV	442594	762221	16.67%	1.702%
13	9.075	1009	1018	1035	rBV	912114	1569849	34.33%	3.504%
14	9.522	1089	1094	1102	rVB3	15443	26750	0.58%	0.060%
15	9.799	1132	1141	1157	rBV	698495	1217375	26.62%	2.718%
16	10.340	1225	1233	1250	rBV	890484	1611986	35.25%	3.598%
17	10.446	1250	1251	1258	rVB7	4936	9509	0.21%	0.021%
18	10.722	1288	1298	1312	rBV	888862	1579818	34.55%	3.527%
19	10.857	1312	1321	1346	rBV	626624	1266428	27.69%	2.827%
20	12.157	1540	1542	1549	rVB8	4235	6478	0.14%	0.014%
21	12.310	1562	1568	1578	rVB2	16729	38142	0.83%	0.085%
22	13.163	1710	1713	1718	rVB6	3780	5101	0.11%	0.011%
23	13.281	1729	1733	1740	rBV9	2270	5185	0.11%	0.012%
24	13.387	1746	1751	1759	rVB5	11284	18482	0.40%	0.041%
25	13.957	1841	1848	1860	rBV	2188252	3037417	66.42%	6.781%
26	14.045	1860	1863	1872	rVB7	7019	20919	0.46%	0.047%
27	14.240	1888	1896	1918	rBV	2220478	3451892	75.48%	7.706%
28	14.457	1929	1933	1940	rVB8	3864	8876	0.19%	0.020%
29	14.551	1941	1949	1958	rBV	1397399	2148204	46.98%	4.795%
30	14.757	1978	1984	1998	rBV2	39290	128976	2.82%	0.288%
31	15.363	2083	2087	2095	rBV4	17777	30578	0.67%	0.068%
32	15.545	2110	2118	2131	rBV	2805562	4426620	96.80%	9.882%
33	15.657	2131	2137	2153	rVV	778795	1226069	26.81%	2.737%
34	15.787	2153	2159	2164	rVB2	36688	60403	1.32%	0.135%
35	15.904	2176	2179	2188	rVB4	10422	19293	0.42%	0.043%
36	16.239	2233	2236	2239	rBV5	3109	4654	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010230.D
 Acq On : 04 May 2022 19:07
 Operator : CG/JU
 Sample : N2668-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	16.334	2247	2252	2257	rVB5	11975	18683	0.41%	0.042%
38	16.645	2300	2305	2309	rVB7	3913	7668	0.17%	0.017%
39	16.981	2357	2362	2368	rVB9	7056	10098	0.22%	0.023%
40	17.086	2374	2380	2382	rBV7	4941	8368	0.18%	0.019%
41	17.304	2409	2417	2427	rBV	1564904	2443002	53.42%	5.454%
42	17.398	2427	2433	2452	rVB	2929104	4467416	97.69%	9.973%
43	17.969	2526	2530	2535	rVB8	6535	10936	0.24%	0.024%
44	18.186	2564	2567	2573	rBV8	8106	10773	0.24%	0.024%
45	18.469	2611	2615	2616	rBV4	4324	5112	0.11%	0.011%
46	18.792	2667	2670	2672	rBV4	4626	6461	0.14%	0.014%
47	19.210	2737	2741	2746	rBV	36452	47217	1.03%	0.105%
48	19.280	2749	2753	2759	rBV	33538	45843	1.00%	0.102%
49	19.633	2807	2813	2830	rBV	3406976	4573042	100.00%	10.209%
50	21.092	3058	3061	3068	rBV6	51422	71770	1.57%	0.160%
51	21.386	3106	3111	3126	rBV	1247289	1841948	40.28%	4.112%
52	23.668	3492	3499	3507	rBV	1577216	3185211	69.65%	7.110%
53	23.827	3519	3526	3537	rVB2	745028	1594012	34.86%	3.558%


Sum of corrected areas: 44796309

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010230.D
Acq On : 04 May 2022 19:07
Operator : CG/JU
Sample : N2668-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

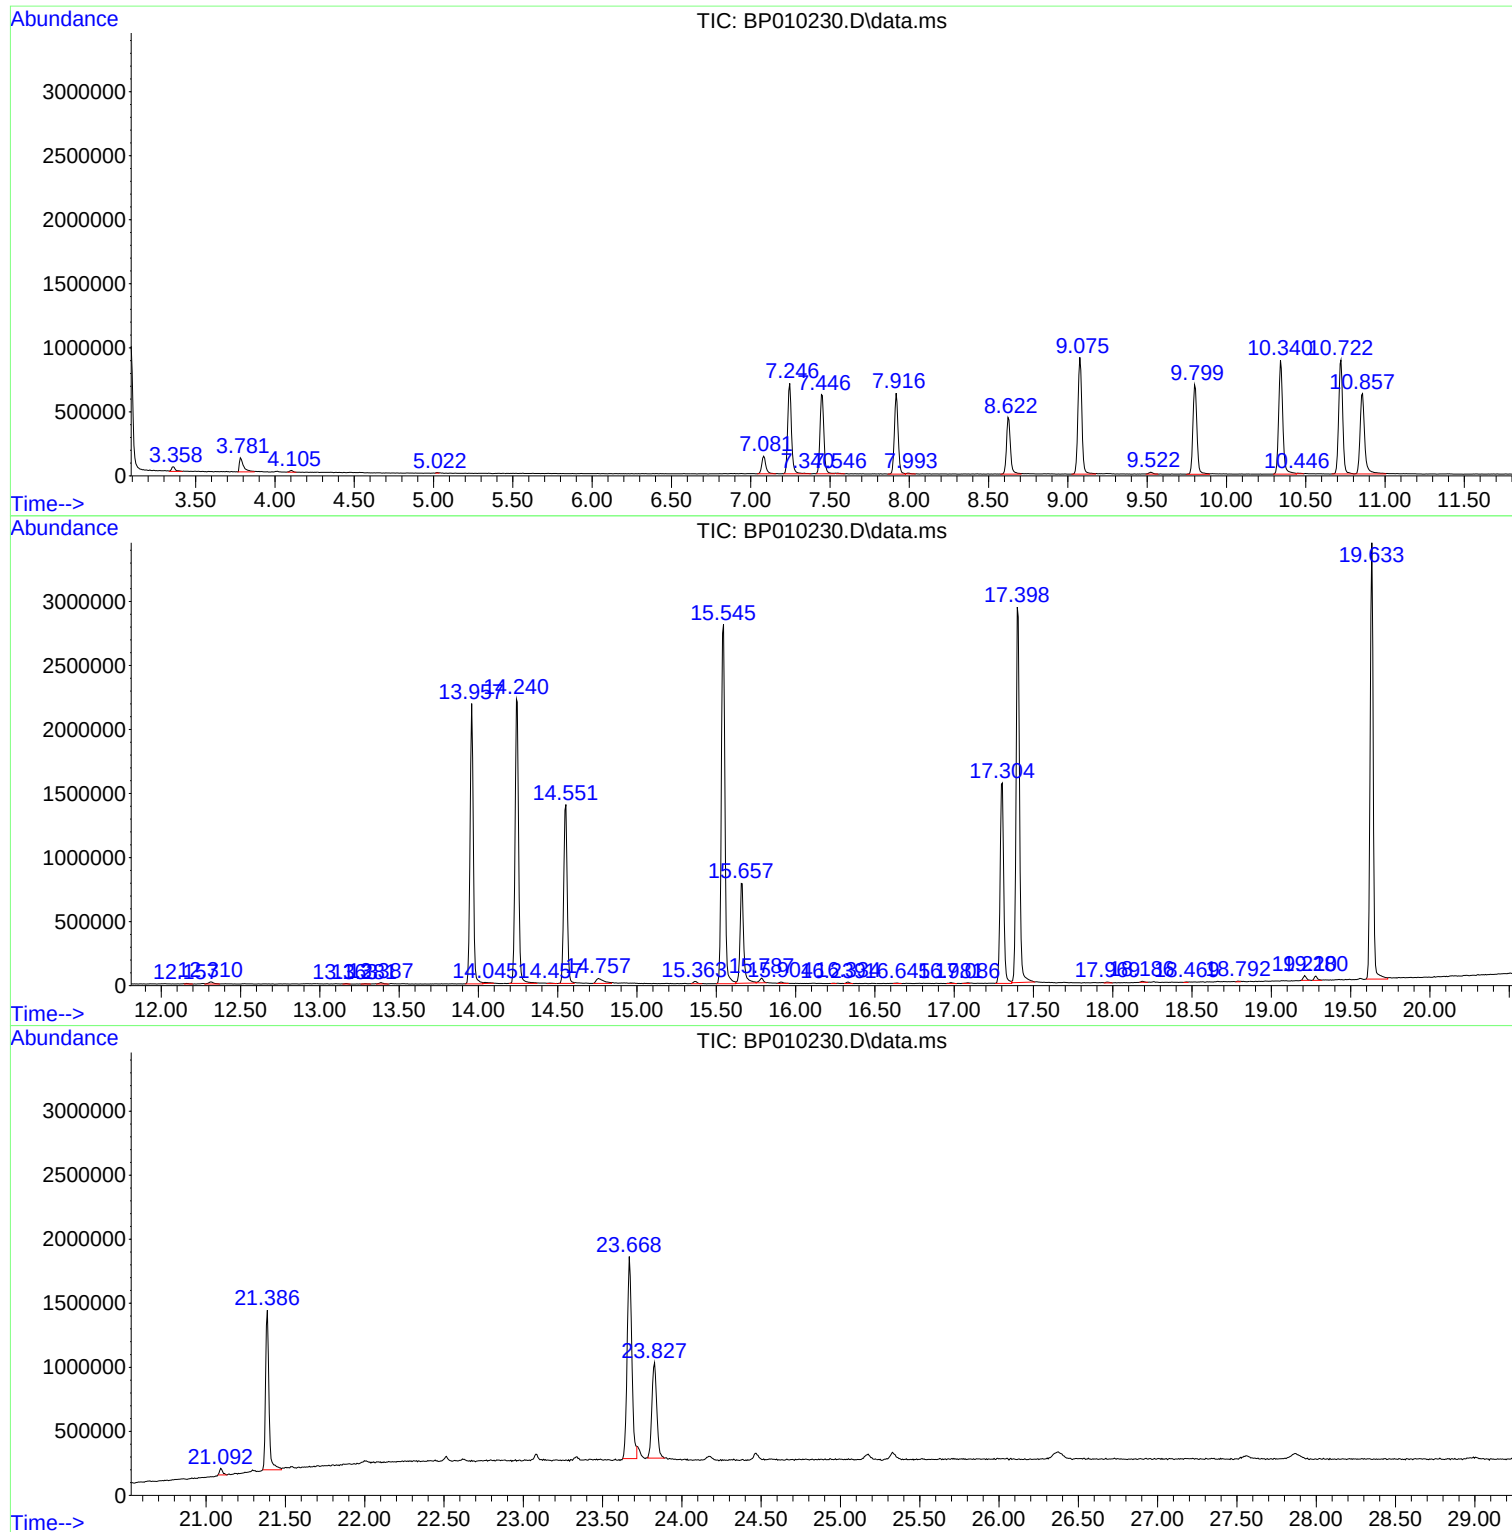

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010230.D
Acq On : 04 May 2022 19:07
Operator : CG/JU
Sample : N2668-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010230.D
Acq On : 04 May 2022 19:07
Operator : CG/JU
Sample : N2668-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc