

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010233.D
 Acq On : 04 May 2022 20:48
 Operator : CG/JU
 Sample : N2668-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	54	rBV	35590	49212	1.21%	0.119%
2	3.781	115	118	133	rBV	119611	212603	5.23%	0.513%
3	4.099	168	172	177	rBV2	12684	20378	0.50%	0.049%
4	5.022	326	329	334	rBV4	4203	5982	0.15%	0.014%
5	6.934	650	654	659	rBV7	4203	8355	0.21%	0.020%
6	7.081	673	679	689	rBV	117925	199185	4.90%	0.481%
7	7.246	699	707	719	rBV	582300	980162	24.13%	2.367%
8	7.340	721	723	728	rVB5	3381	4976	0.12%	0.012%
9	7.446	734	741	753	rBV	532085	883105	21.74%	2.133%
10	7.546	756	758	766	rVB9	5790	9453	0.23%	0.023%
11	7.916	814	821	830	rBV	689909	1106087	27.23%	2.671%
12	8.622	934	941	955	rBV	369352	626967	15.44%	1.514%
13	9.075	1010	1018	1033	rBV	788108	1328117	32.70%	3.207%
14	9.205	1036	1040	1045	rVV6	8412	12954	0.32%	0.031%
15	9.522	1089	1094	1101	rVB2	17260	28145	0.69%	0.068%
16	9.799	1131	1141	1155	rBV	583965	1011830	24.91%	2.444%
17	10.075	1185	1188	1194	rVB8	2183	4234	0.10%	0.010%
18	10.340	1223	1233	1252	rBV	749450	1336386	32.90%	3.227%
19	10.499	1258	1260	1266	rVB7	2999	4523	0.11%	0.011%
20	10.722	1290	1298	1310	rBV	955977	1641023	40.40%	3.963%
21	10.857	1313	1321	1341	rBV	640267	1250994	30.80%	3.021%
22	11.669	1451	1459	1468	rBV5	12368	35571	0.88%	0.086%
23	12.157	1534	1542	1545	rBV10	4548	8427	0.21%	0.020%
24	12.316	1562	1569	1574	rBV2	12636	24309	0.60%	0.059%
25	13.381	1741	1750	1755	rBV2	12260	21009	0.52%	0.051%
26	13.522	1772	1774	1781	rVB8	3119	4930	0.12%	0.012%
27	13.957	1841	1848	1861	rBV	1783164	2526711	62.21%	6.102%
28	14.240	1886	1896	1911	rBV	1830608	2793955	68.79%	6.747%
29	14.457	1930	1933	1937	rVB5	3455	4210	0.10%	0.010%
30	14.545	1941	1948	1958	rBV	1431903	2184073	53.77%	5.275%
31	14.757	1977	1984	1995	rBV3	35782	109622	2.70%	0.265%
32	14.969	2016	2020	2026	rBV8	9284	16878	0.42%	0.041%
33	15.363	2083	2087	2093	rVB5	5223	8996	0.22%	0.022%
34	15.540	2110	2117	2132	rBV	2367912	3720956	91.62%	8.986%
35	15.657	2132	2137	2153	rVV	681263	1105199	27.21%	2.669%
36	15.787	2154	2159	2166	rVB3	30872	58943	1.45%	0.142%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010233.D
 Acq On : 04 May 2022 20:48
 Operator : CG/JU
 Sample : N2668-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	16.104	2209	2213	2219	rBV8	2785	5722	0.14%	0.014%
38	16.239	2229	2236	2239	rBV9	4129	7636	0.19%	0.018%
39	16.328	2247	2251	2256	rVB5	8793	11993	0.30%	0.029%
40	16.439	2264	2270	2271	rBV5	4302	6571	0.16%	0.016%
41	16.845	2336	2339	2342	rVB5	4122	5176	0.13%	0.012%
42	16.981	2356	2362	2364	rBV7	5192	8470	0.21%	0.020%
43	17.063	2373	2376	2379	rBV4	4114	6221	0.15%	0.015%
44	17.298	2410	2416	2426	rBV	1500527	2287106	56.31%	5.523%
45	17.398	2427	2433	2453	rVB	2562850	3978732	97.96%	9.609%
46	17.592	2460	2466	2472	rVB	191890	248754	6.12%	0.601%
47	17.804	2500	2502	2508	rVB7	2567	4181	0.10%	0.010%
48	17.934	2519	2524	2528	rBV7	4476	9095	0.22%	0.022%
49	18.186	2563	2567	2573	rBV6	21013	34069	0.84%	0.082%
50	18.257	2574	2579	2584	rVB	112447	139864	3.44%	0.338%
51	18.475	2612	2616	2622	rVB8	5009	8326	0.20%	0.020%
52	19.210	2737	2741	2748	rBV2	32892	44486	1.10%	0.107%
53	19.280	2749	2753	2760	rVV2	24681	39728	0.98%	0.096%
54	19.633	2806	2813	2824	rBV	2926239	4061506	100.00%	9.808%
55	21.092	3057	3061	3070	rBV3	89846	143402	3.53%	0.346%
56	21.380	3105	3110	3125	rBV	1256716	1905683	46.92%	4.602%
57	23.668	3492	3499	3514	rBV2	1595010	3329852	81.99%	8.042%
58	23.821	3519	3525	3540	rVB2	839802	1773018	43.65%	4.282%




Sum of corrected areas: 41408051

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010233.D
Acq On : 04 May 2022 20:48
Operator : CG/JU
Sample : N2668-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

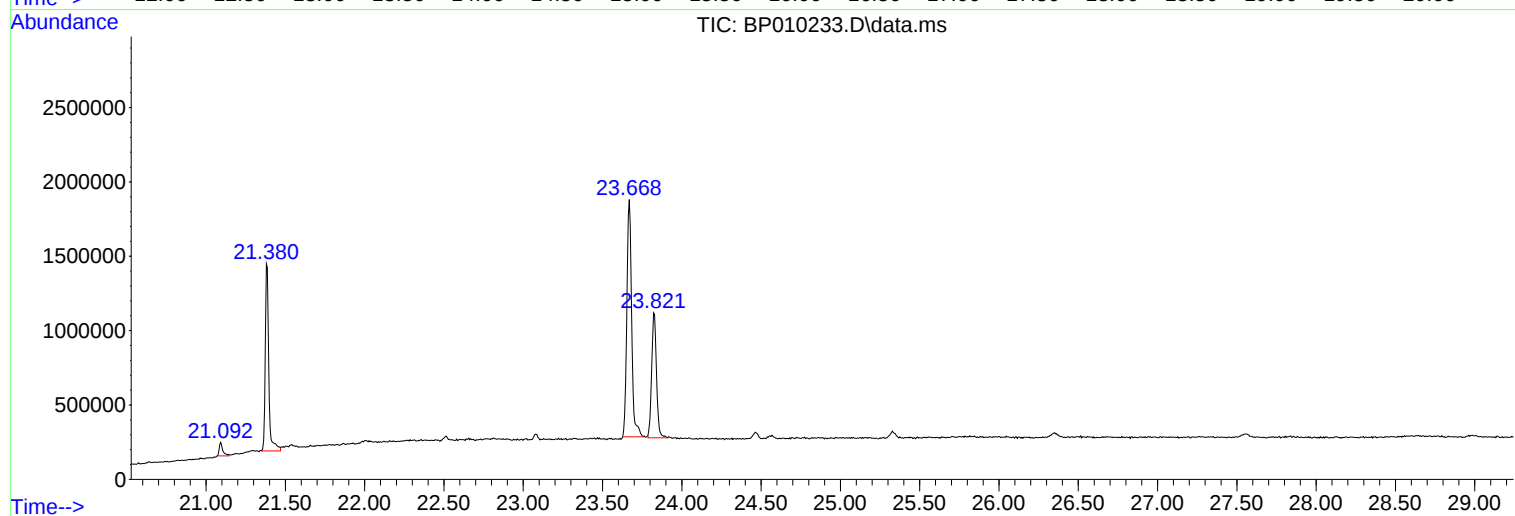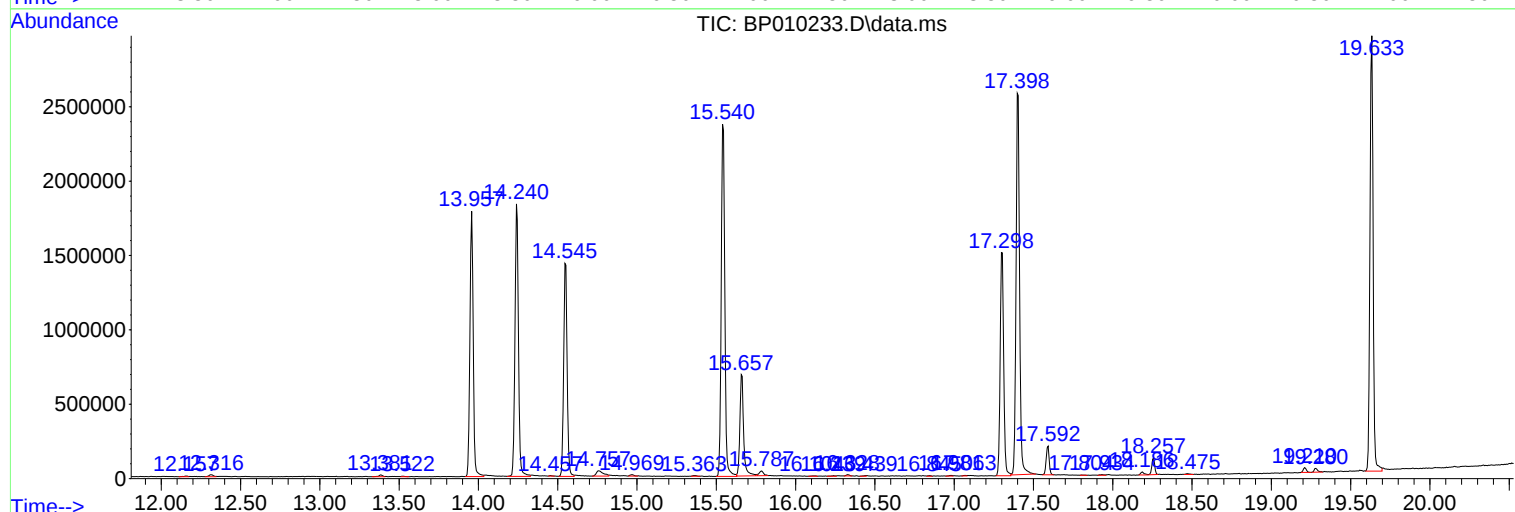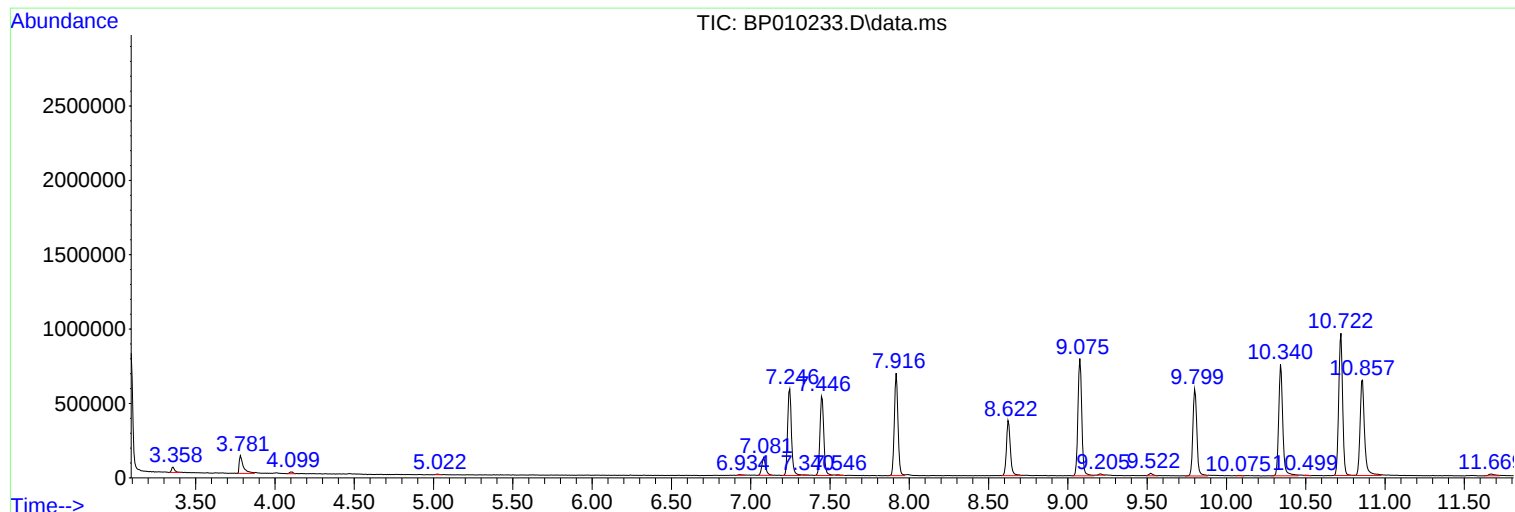

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010233.D
Acq On : 04 May 2022 20:48
Operator : CG/JU
Sample : N2668-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010233.D
Acq On : 04 May 2022 20:48
Operator : CG/JU
Sample : N2668-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc