

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010234.D
 Acq On : 04 May 2022 21:22
 Operator : CG/JU
 Sample : N2668-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	43	46	52	rVB	30681	38906	0.54%	0.091%
2	3.781	115	118	132	rBV	123112	210797	2.94%	0.491%
3	4.104	169	173	180	rVB3	11431	19281	0.27%	0.045%
4	4.634	258	263	272	rVB	80942	117341	1.64%	0.273%
5	7.081	673	679	692	rVB	118317	212978	2.97%	0.496%
6	7.246	700	707	718	rBV	550375	896960	12.51%	2.091%
7	7.445	733	741	755	rBV	505944	845899	11.80%	1.972%
8	7.545	757	758	766	rVB8	4585	7197	0.10%	0.017%
9	7.916	814	821	830	rBV	597173	965792	13.47%	2.251%
10	7.987	830	833	838	rVB6	5610	9579	0.13%	0.022%
11	8.622	934	941	960	rBV	378615	659728	9.20%	1.538%
12	9.075	1006	1018	1032	rBV	712415	1202642	16.78%	2.803%
13	9.198	1035	1039	1045	rBV4	11357	20478	0.29%	0.048%
14	9.522	1089	1094	1102	rVB2	18302	29462	0.41%	0.069%
15	9.798	1134	1141	1160	rBV	535957	929605	12.97%	2.167%
16	10.051	1178	1184	1191	rBV	7671	21195	0.30%	0.049%
17	10.339	1225	1233	1252	rBV	757653	1356623	18.93%	3.162%
18	10.722	1288	1298	1306	rBV	812320	1429313	19.94%	3.331%
19	10.857	1312	1321	1340	rBV	632262	1247346	17.40%	2.907%
20	12.151	1537	1541	1547	rVB5	5154	8562	0.12%	0.020%
21	12.310	1561	1568	1575	rBV2	13300	26560	0.37%	0.062%
22	12.833	1652	1657	1664	rBV2	18905	39024	0.54%	0.091%
23	13.386	1747	1751	1754	rBV2	13317	17938	0.25%	0.042%
24	13.957	1841	1848	1861	rBV	1604354	2337141	32.61%	5.447%
25	14.239	1886	1896	1909	rBV	1660691	2554766	35.64%	5.954%
26	14.457	1928	1933	1940	rVB10	5361	10244	0.14%	0.024%
27	14.551	1940	1949	1963	rBV	1205014	1844423	25.73%	4.299%
28	14.751	1978	1983	1994	rBV4	34016	94933	1.32%	0.221%
29	15.010	2014	2027	2053	rBV	3523486	7167543	100.00%	16.705%
30	15.357	2082	2086	2091	rVB7	6602	13203	0.18%	0.031%
31	15.539	2111	2117	2132	rBV	2157856	3188146	44.48%	7.431%
32	15.657	2132	2137	2153	rVV	578404	892536	12.45%	2.080%
33	15.786	2154	2159	2163	rVB2	24542	38317	0.53%	0.089%
34	16.327	2247	2251	2258	rVB7	8786	14070	0.20%	0.033%
35	16.445	2267	2271	2274	rBV5	7460	11097	0.15%	0.026%
36	16.704	2310	2315	2326	rBV3	47720	75841	1.06%	0.177%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
 Data File : BP010234.D
 Acq On : 04 May 2022 21:22
 Operator : CG/JU
 Sample : N2668-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	17.298	2410	2416	2426	rVV	1257056	1864483	26.01%	4.346%
38	17.398	2427	2433	2450	rVB	2122366	3140422	43.81%	7.319%
39	17.968	2527	2530	2537	rVB9	10012	16248	0.23%	0.038%
40	18.186	2562	2567	2574	rBV	81994	129500	1.81%	0.302%
41	18.463	2611	2614	2621	rVB8	10842	16431	0.23%	0.038%
42	19.210	2737	2741	2746	rBV3	26085	35193	0.49%	0.082%
43	19.280	2749	2753	2760	rBV2	21173	38615	0.54%	0.090%
44	19.415	2772	2776	2781	rBV4	24853	36531	0.51%	0.085%
45	19.633	2807	2813	2824	rBV	2277796	3185209	44.44%	7.424%
46	21.092	3057	3061	3067	rBV5	101155	151935	2.12%	0.354%
47	21.292	3093	3095	3098	rBV2	34666	28204	0.39%	0.066%
48	21.380	3105	3110	3117	rBV	1064811	1544518	21.55%	3.600%
49	23.668	3492	3499	3506	rBV2	1341857	2686556	37.48%	6.262%
50	23.827	3519	3526	3535	rVB2	703791	1476594	20.60%	3.441%




Sum of corrected areas: 42905905

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010234.D
Acq On : 04 May 2022 21:22
Operator : CG/JU
Sample : N2668-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

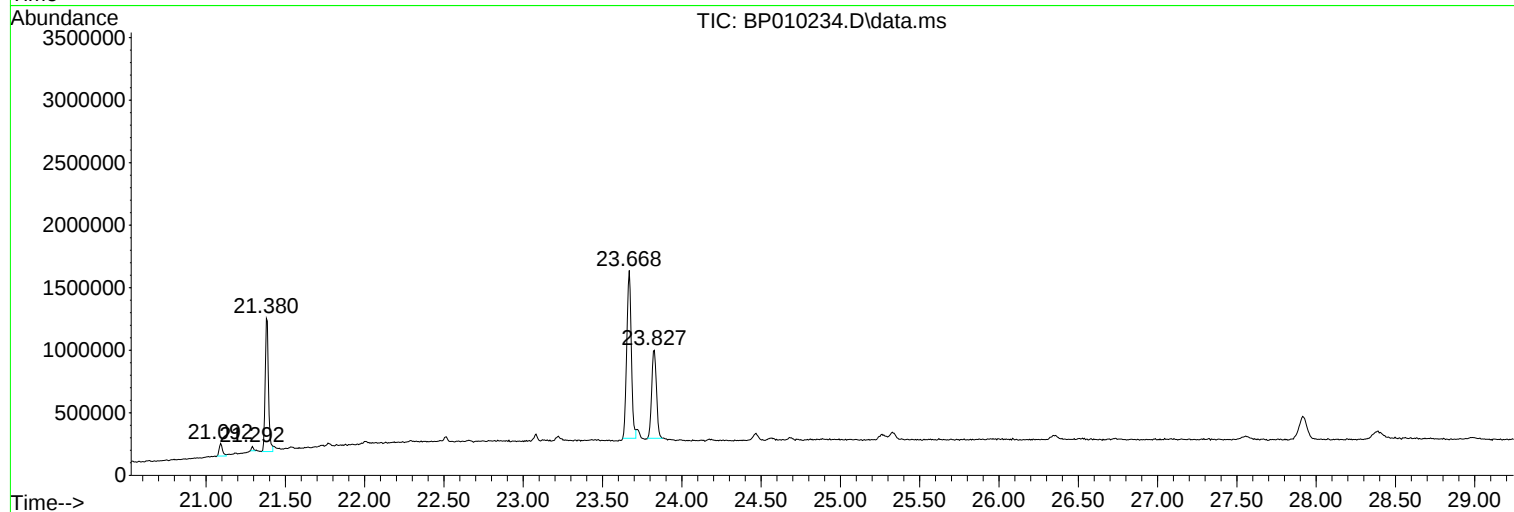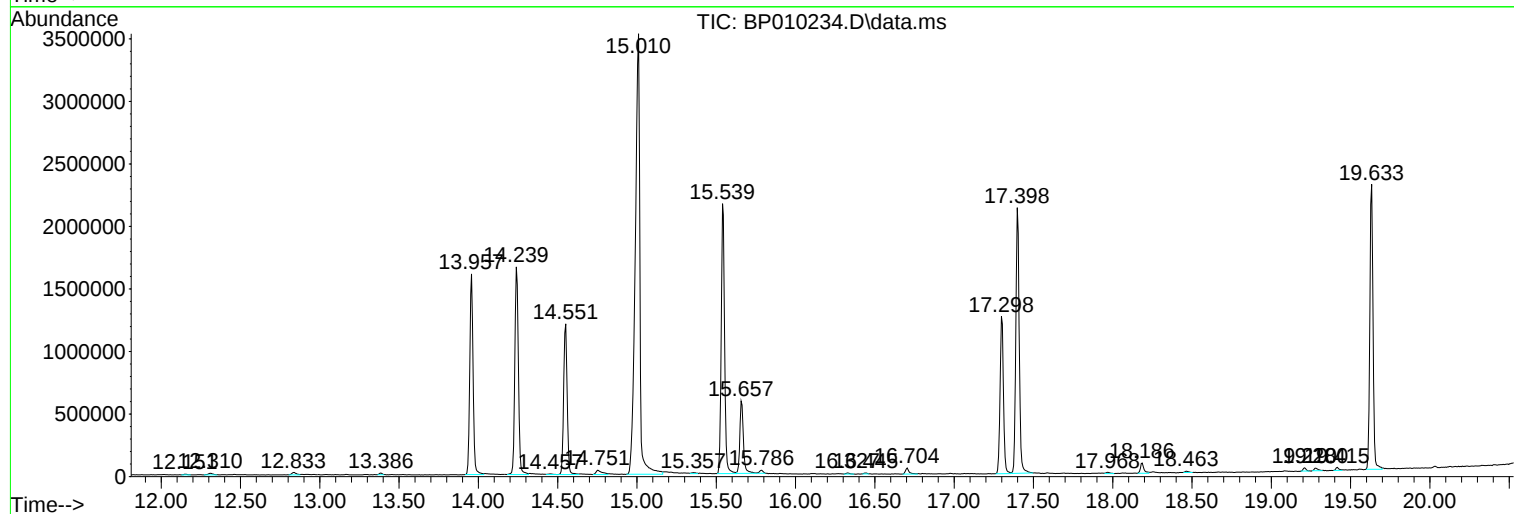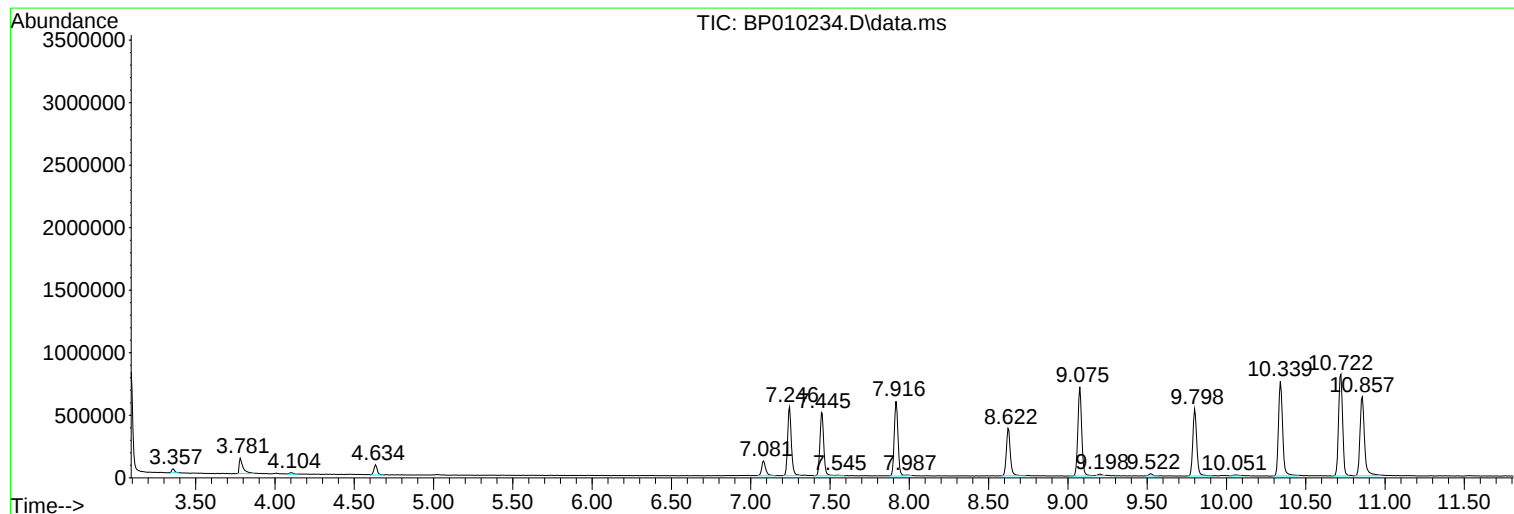

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010234.D
Acq On : 04 May 2022 21:22
Operator : CG/JU
Sample : N2668-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050422\
Data File : BP010234.D
Acq On : 04 May 2022 21:22
Operator : CG/JU
Sample : N2668-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc