
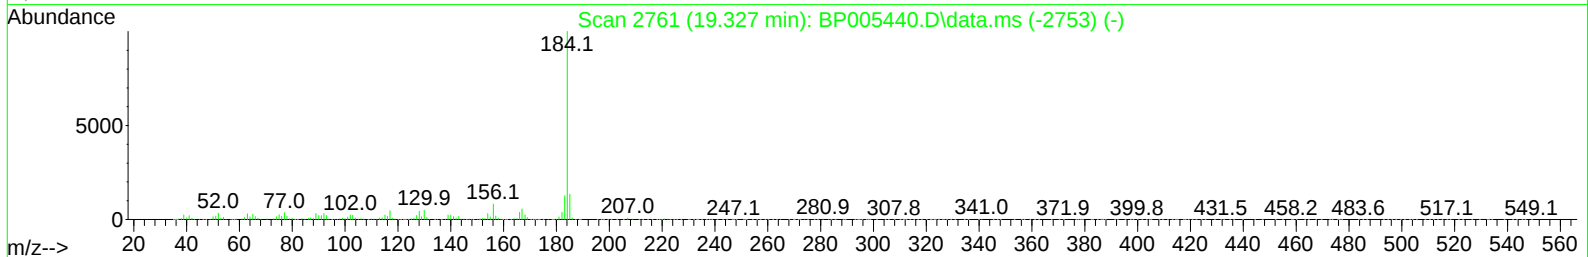
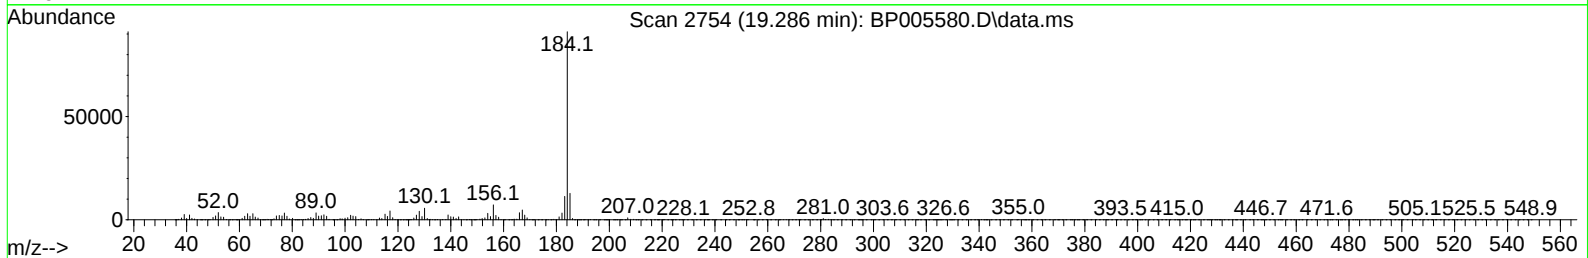


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051721\
 Data File : BP005580.D
 Acq On : 17 May 2021 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 15:25:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 12:01:17 2021
 Response via : Initial Calibration

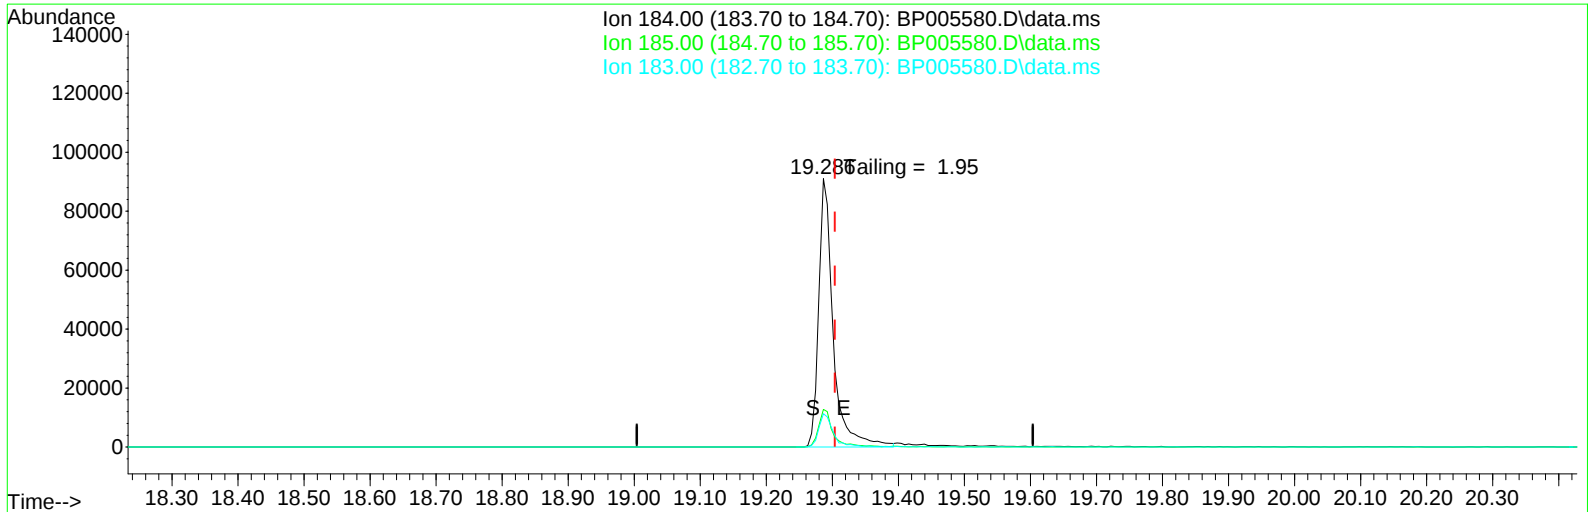




TIC: BP005580.D\data.ms

(77) Benzidine**19.286min (-0.018) 535811.08 ng****response 140993**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.02
183.00	12.30	12.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051721\
Data File : BP005580.D
Acq On : 17 May 2021 14:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 15:25:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 12:01:17 2021
Response via : Initial Calibration

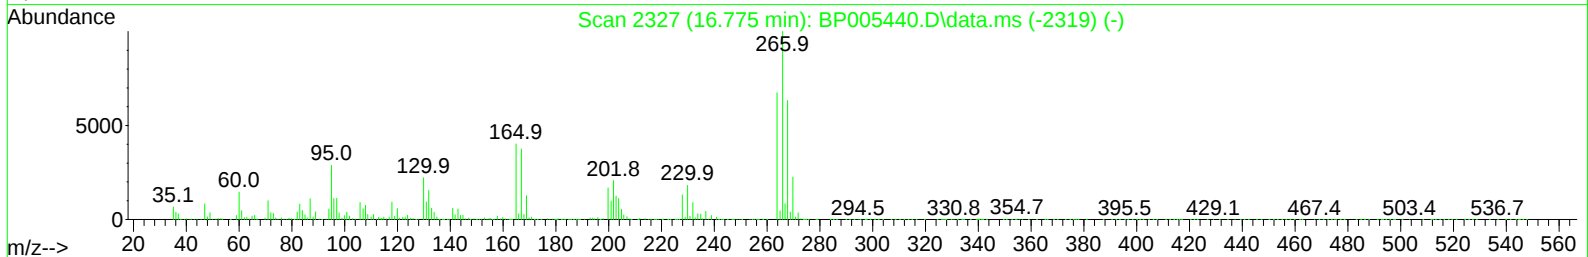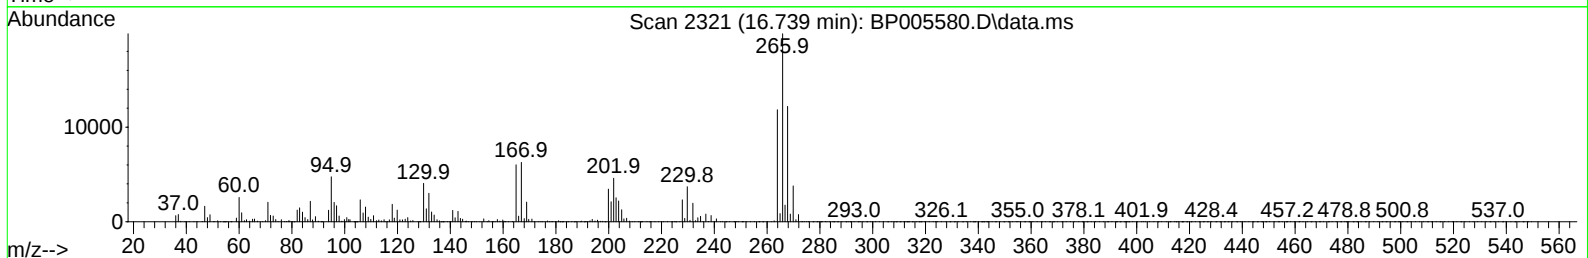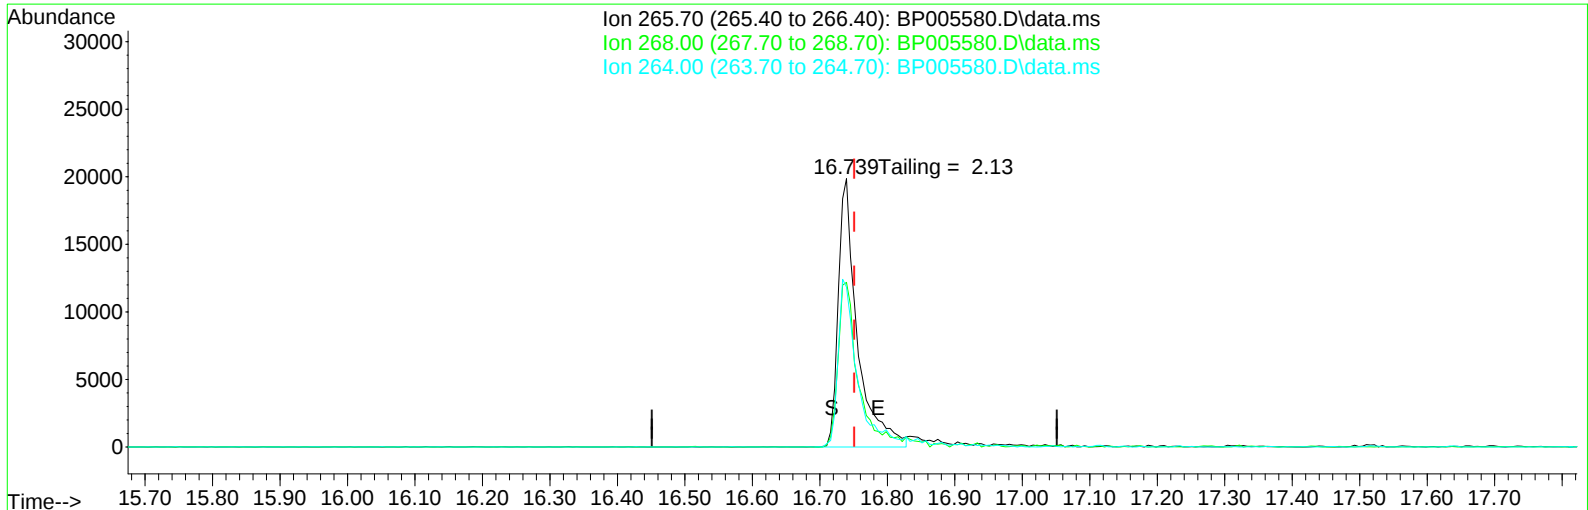

TIC: BP005580.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 127677.70 ng

response 38891

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.35
264.00	67.10	59.61
0.00	0.00	0.00