
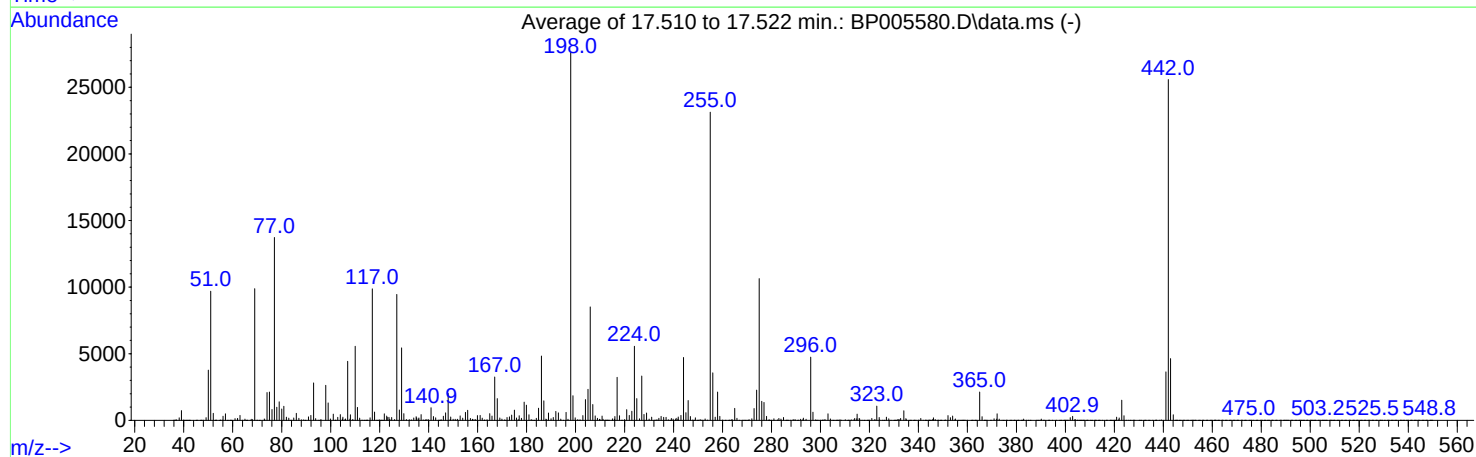


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051721\
 Data File : BP005580.D
 Acq On : 17 May 2021 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 17 15:35:47 2021

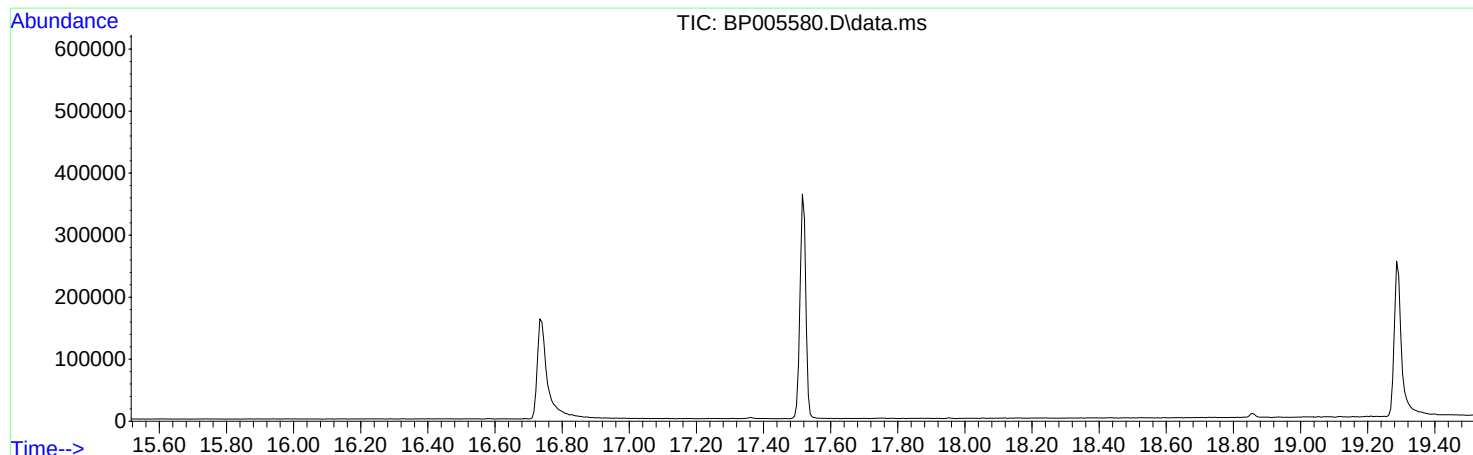




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	9688	PASS
68	69	0.00	2	0.9	89	PASS
69	198	0.00	100	35.8	9888	PASS
70	69	0.00	2	0.2	17	PASS
127	198	10	80	34.2	9455	PASS
197	198	0.00	2	0.3	80	PASS
198	198	100	100	100.0	27611	PASS
199	198	5	9	6.7	1848	PASS
275	198	10	60	38.5	10642	PASS
365	198	1	100	7.7	2121	PASS
441	198	0.01	100	13.2	3636	PASS
442	442	100	100	100.0	25580	PASS
443	442	15	24	18.1	4640	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051721\
 Data File : BP005580.D
 Acq On : 17 May 2021 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 17 15:25:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 12:01:17 2021
 Response via : Initial Calibration

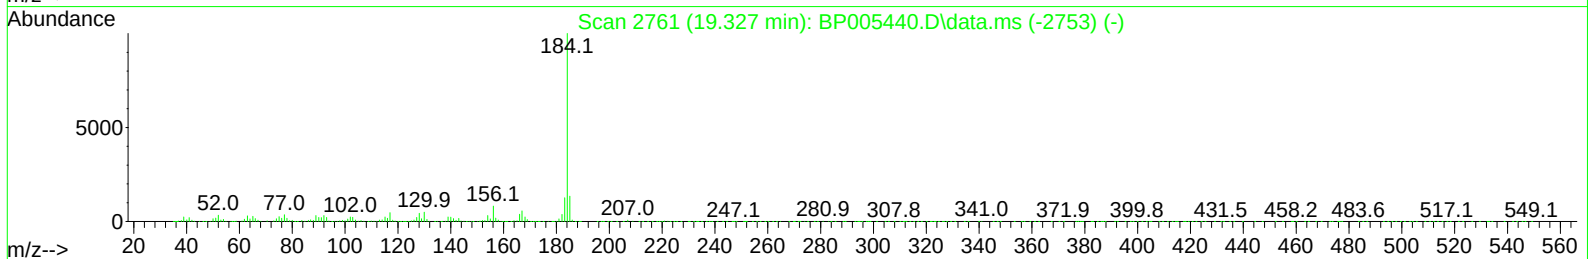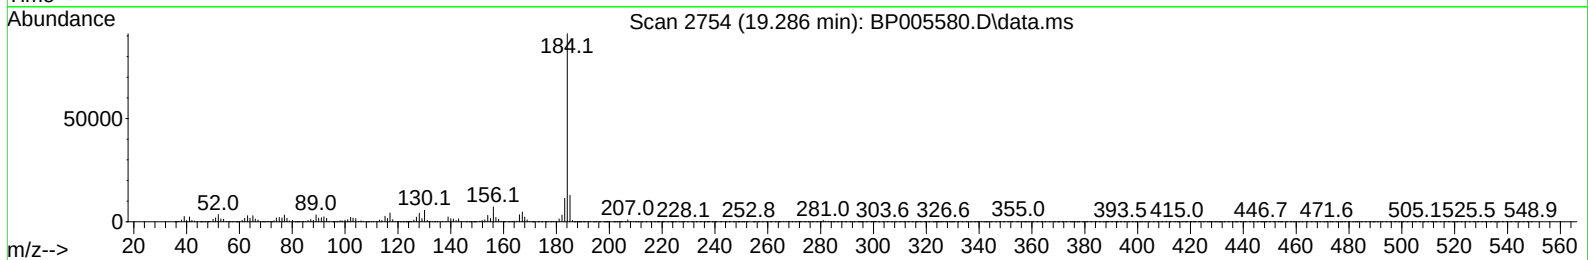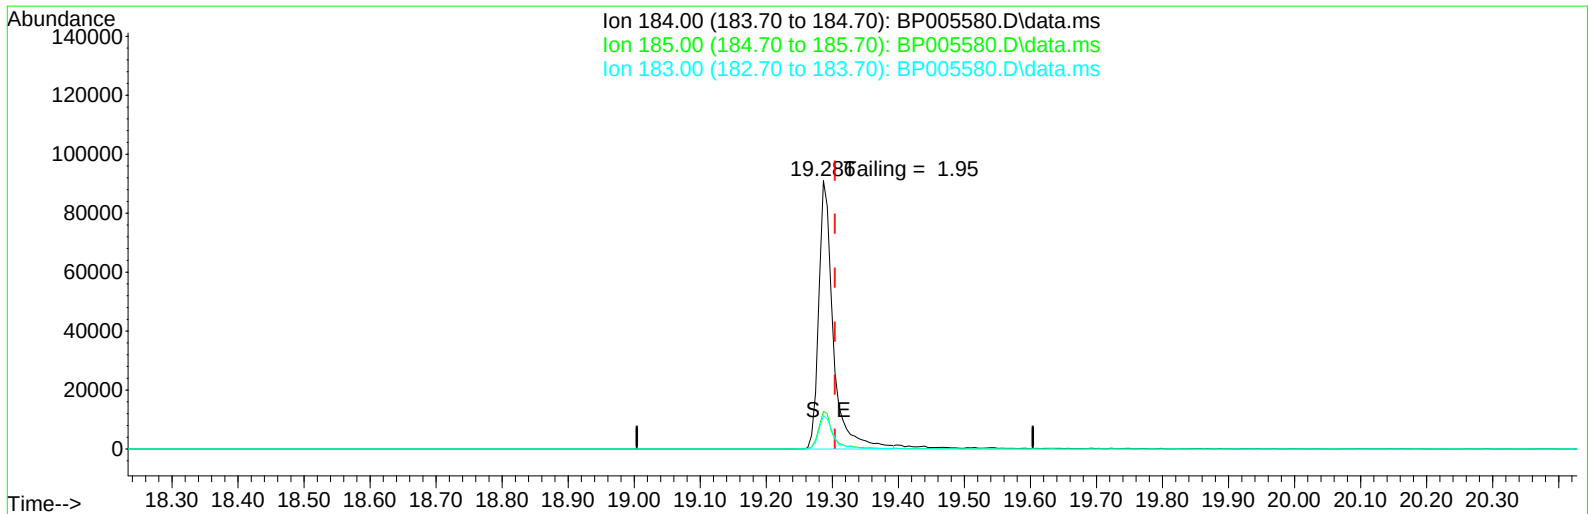

TIC: BP005580.D\data.ms

(77) Benzidine

19.286min (-0.018) 535811.08 ng




response 140993

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.02
183.00	12.30	12.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051721\
Data File : BP005580.D
Acq On : 17 May 2021 14:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 17 15:25:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 12:01:17 2021
Response via : Initial Calibration

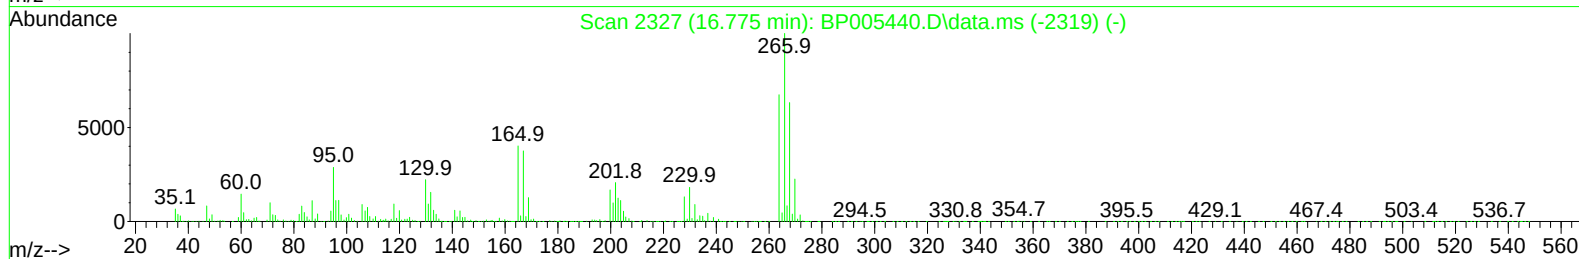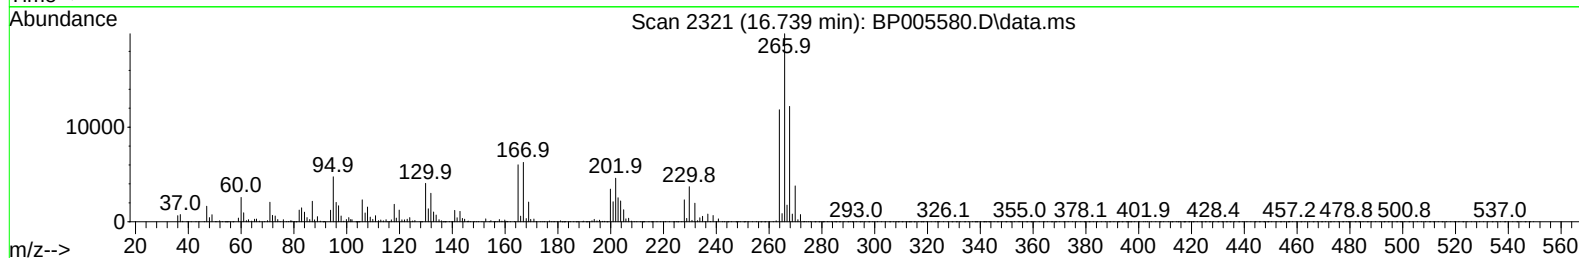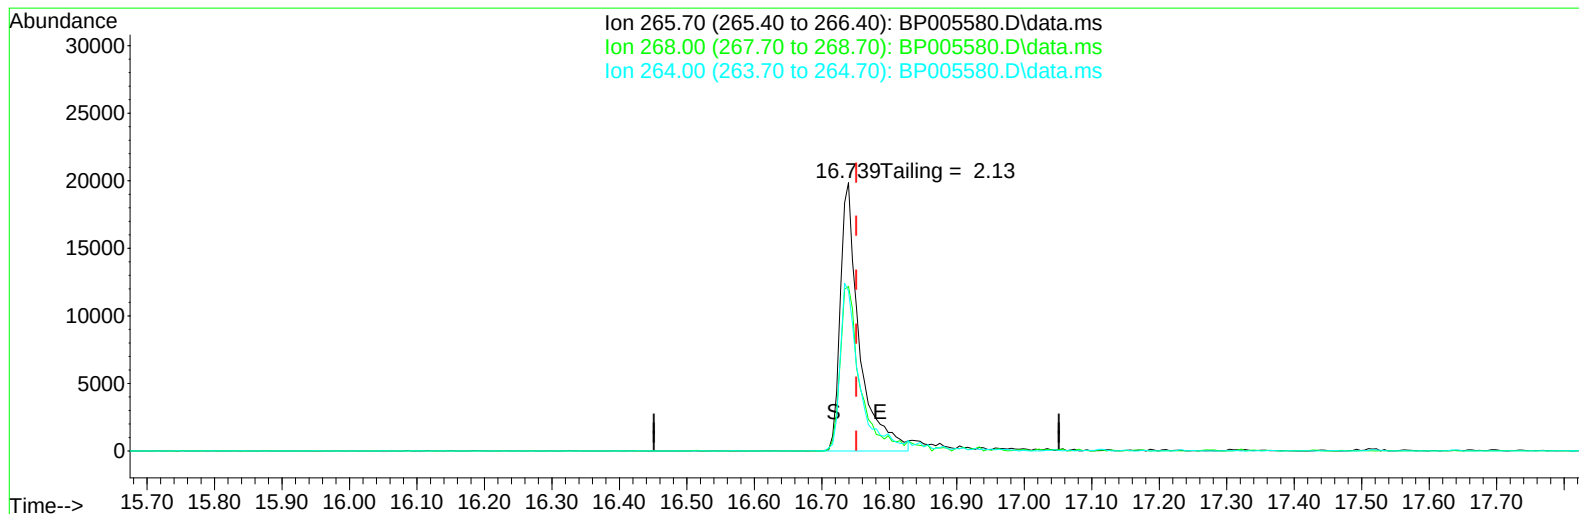

TIC: BP005580.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 127677.70 ng

response 38891

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.35
264.00	67.10	59.61
0.00	0.00	0.00

[

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/17/2021	BNA_P	<u>BP005580.D</u>
Compound Name	Response	Retention Time
DDT	110705	20.48
DDD	448	20.05
DDE	285	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
733	111438	0.66

Instrument :
BNA_P
ClientSampleId :
DFTPP