




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010394.D
 Acq On : 18 May 2022 11:24
 Operator : CG/JU
 Sample : N2766-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:57:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

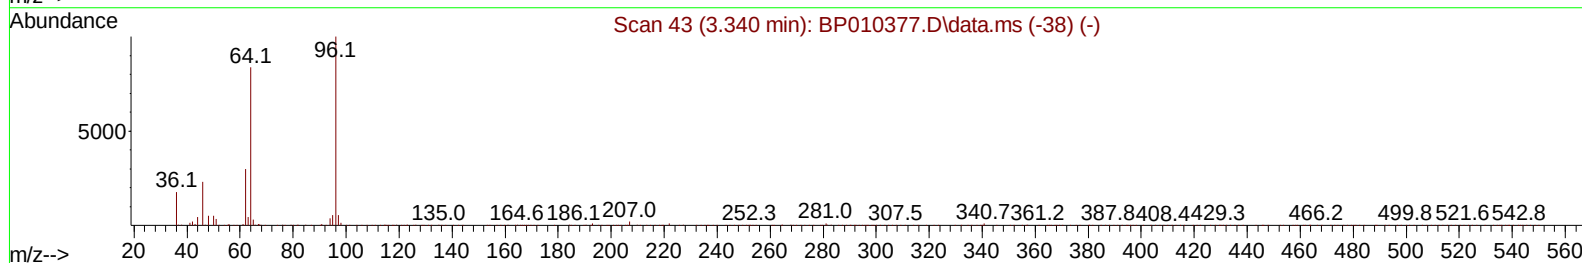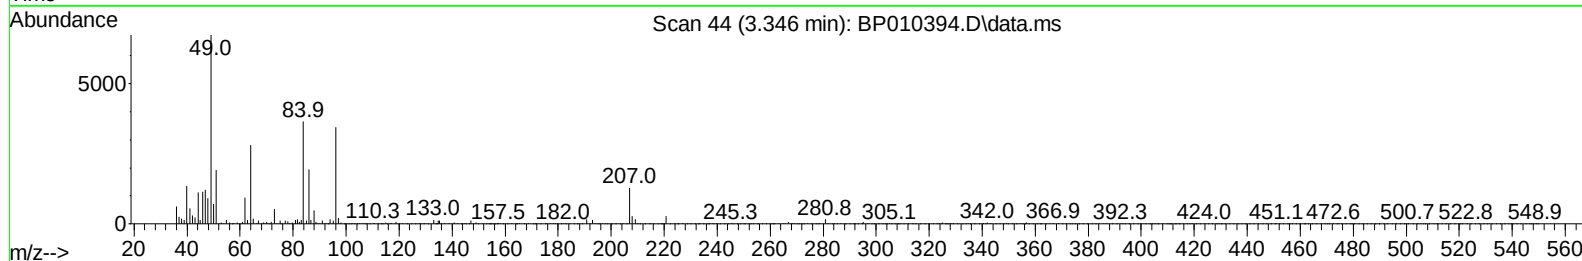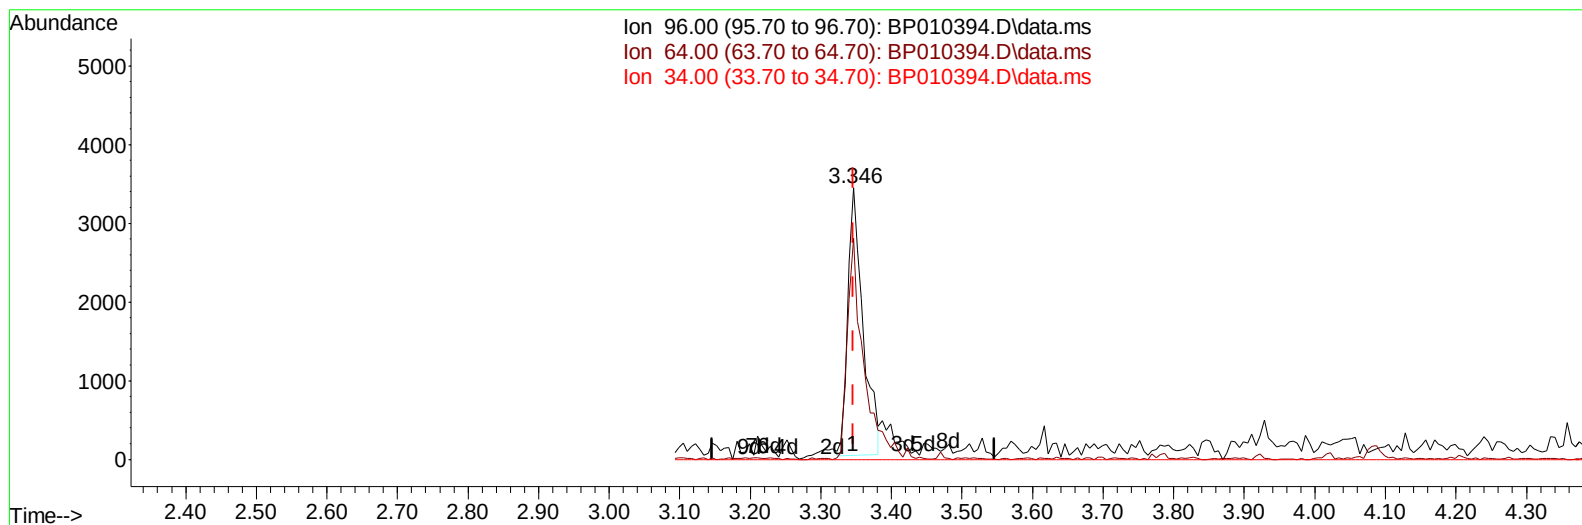

TIC: BP010394.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (-0.000) 1.85 ng/uL

response 5149

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	81.56#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010394.D
 Acq On : 18 May 2022 11:24
 Operator : CG/JU
 Sample : N2766-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:57:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

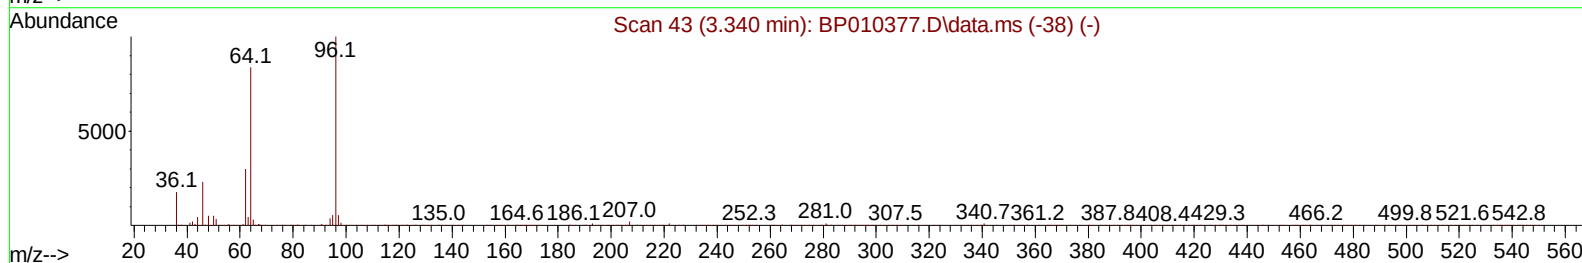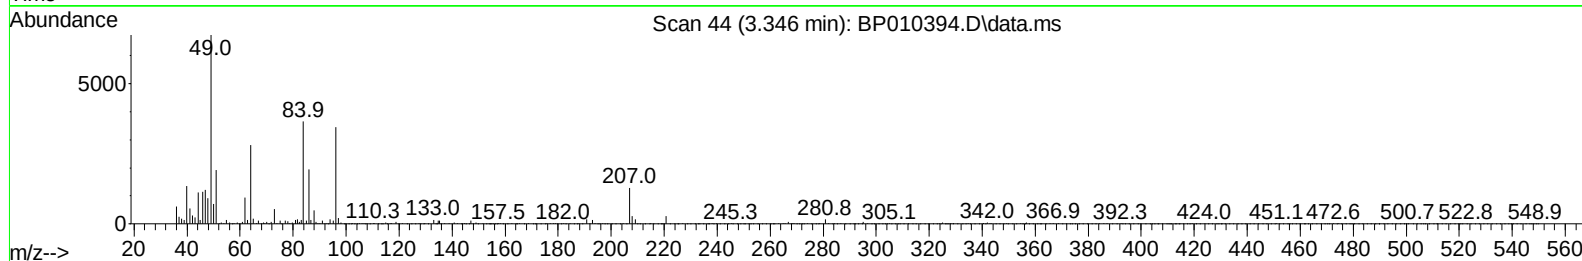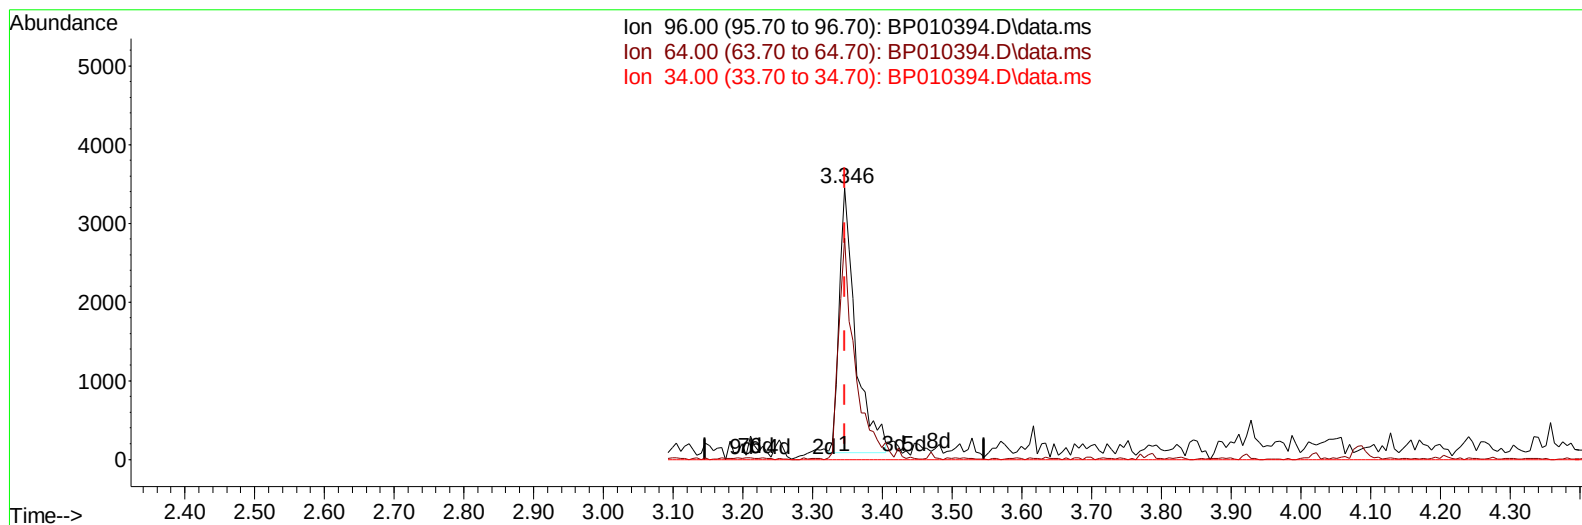

TIC: BP010394.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (-0.000) 1.96 ng/uL m

response 5462

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	81.56#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010394.D
 Acq On : 18 May 2022 11:24
 Operator : CG/JU
 Sample : N2766-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:57:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

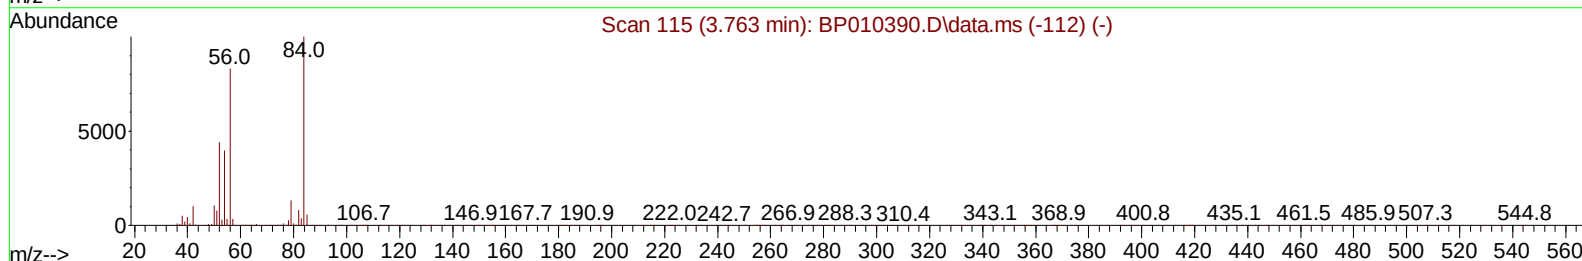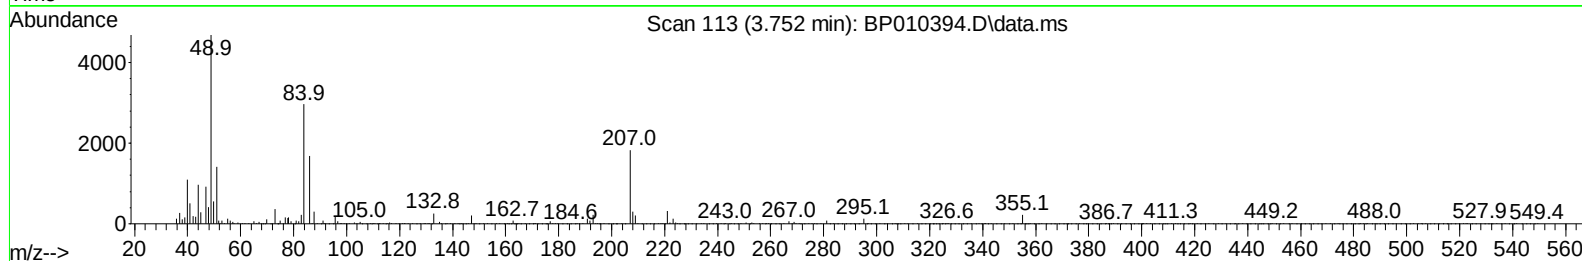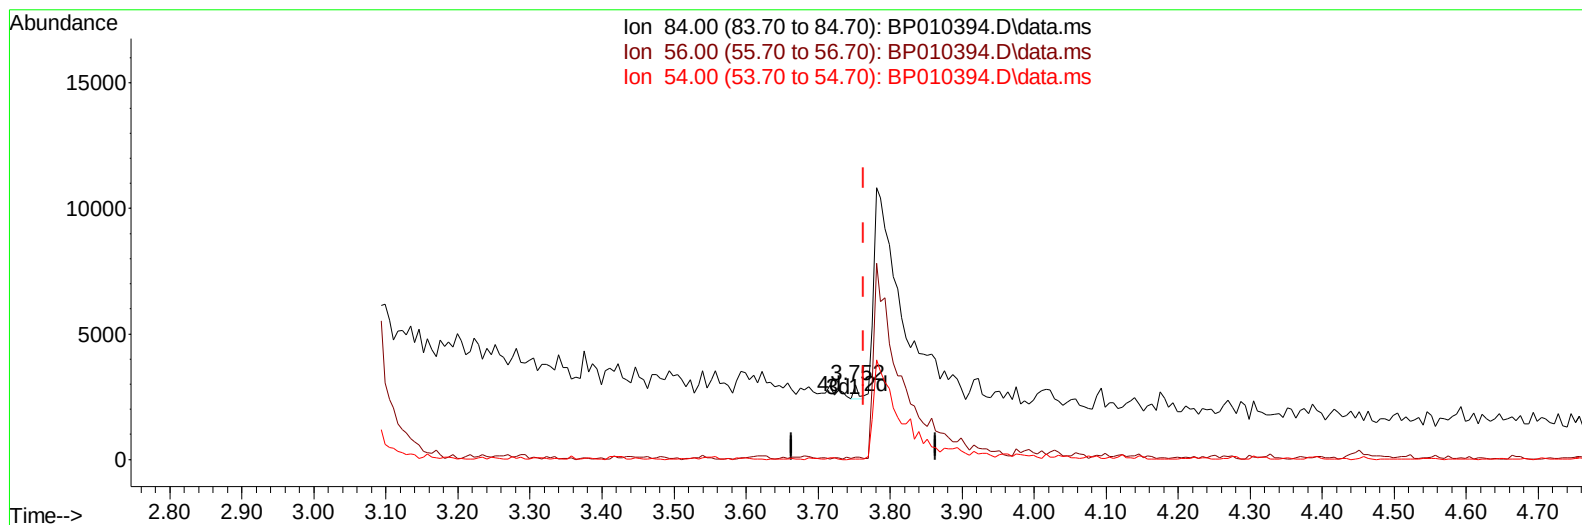

TIC: BP010394.D\data.ms

(4) Pyridine-d5 (S)

3.752min (-0.012) 0.03 ng/ul

response 268

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	2.80#
54.00	24.80	0.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010394.D
Acq On : 18 May 2022 11:24
Operator : CG/JU
Sample : N2766-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:57:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

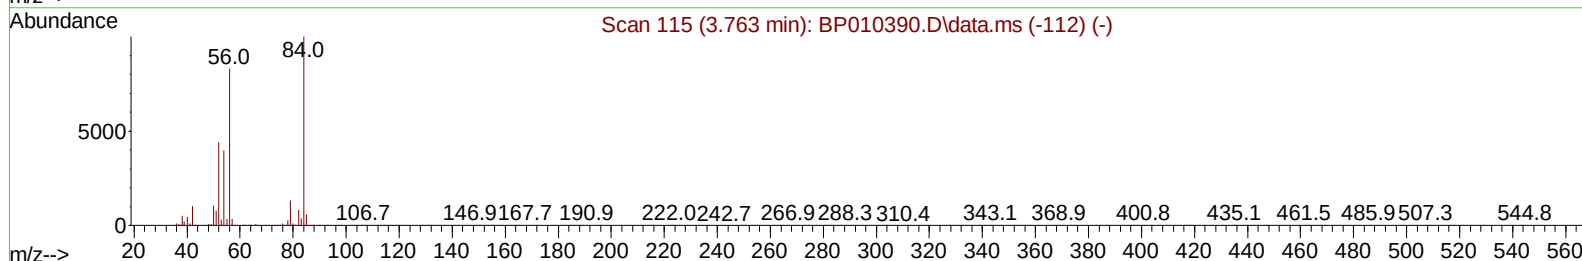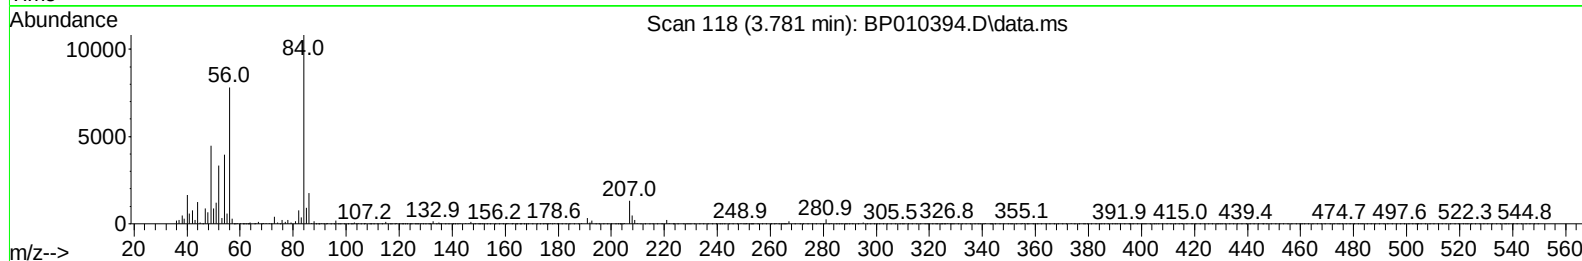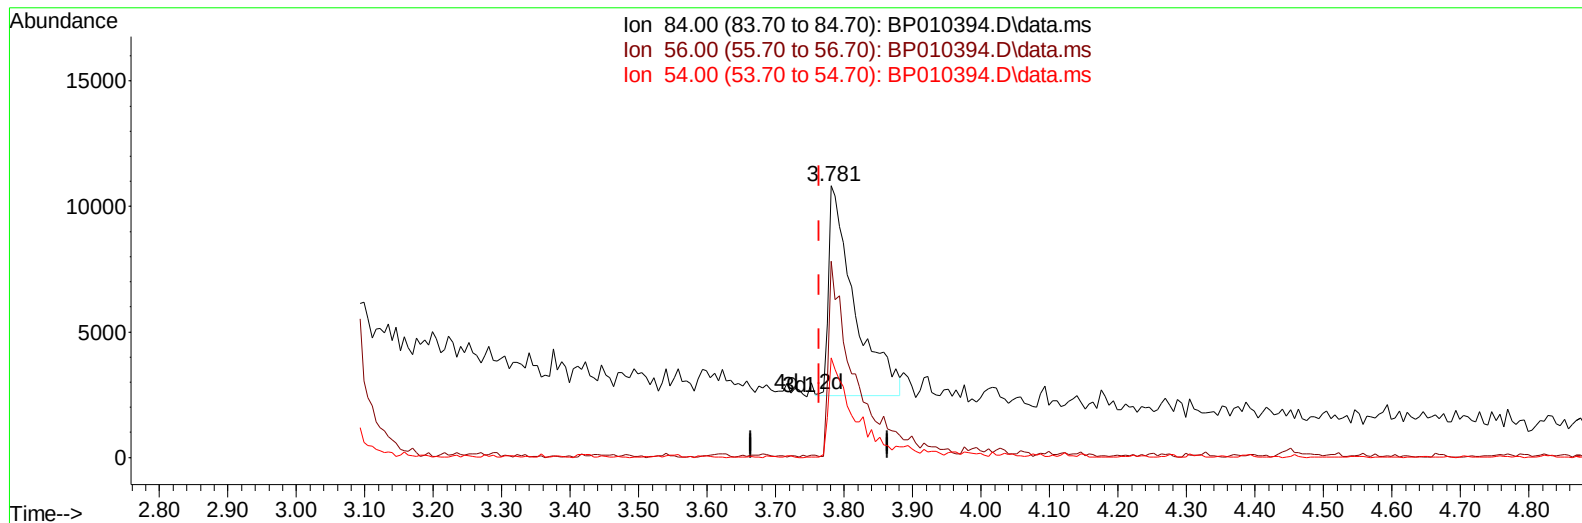

TIC: BP010394.D\data.ms

(4) Pyridine-d5 (S)

3.781min (+ 0.018) 2.76 ng/ul m

response 21862

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	72.37#
54.00	24.80	36.64#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010394.D
Acq On : 18 May 2022 11:24
Operator : CG/JU
Sample : N2766-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:57:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

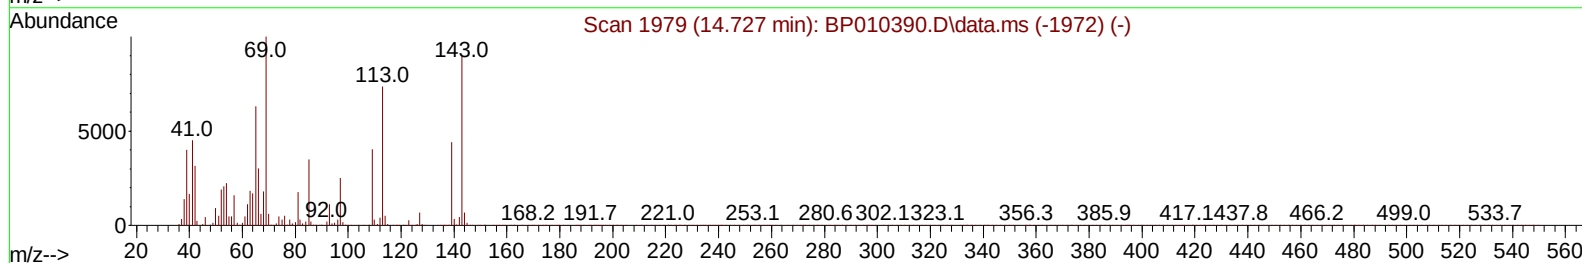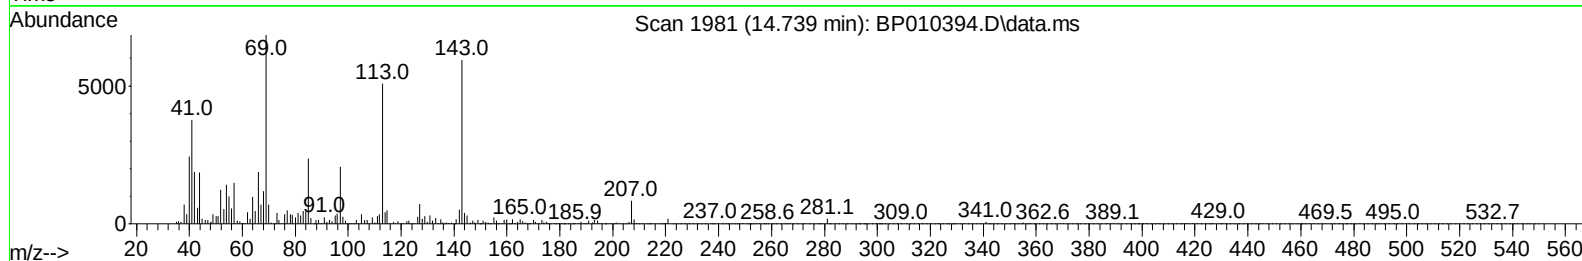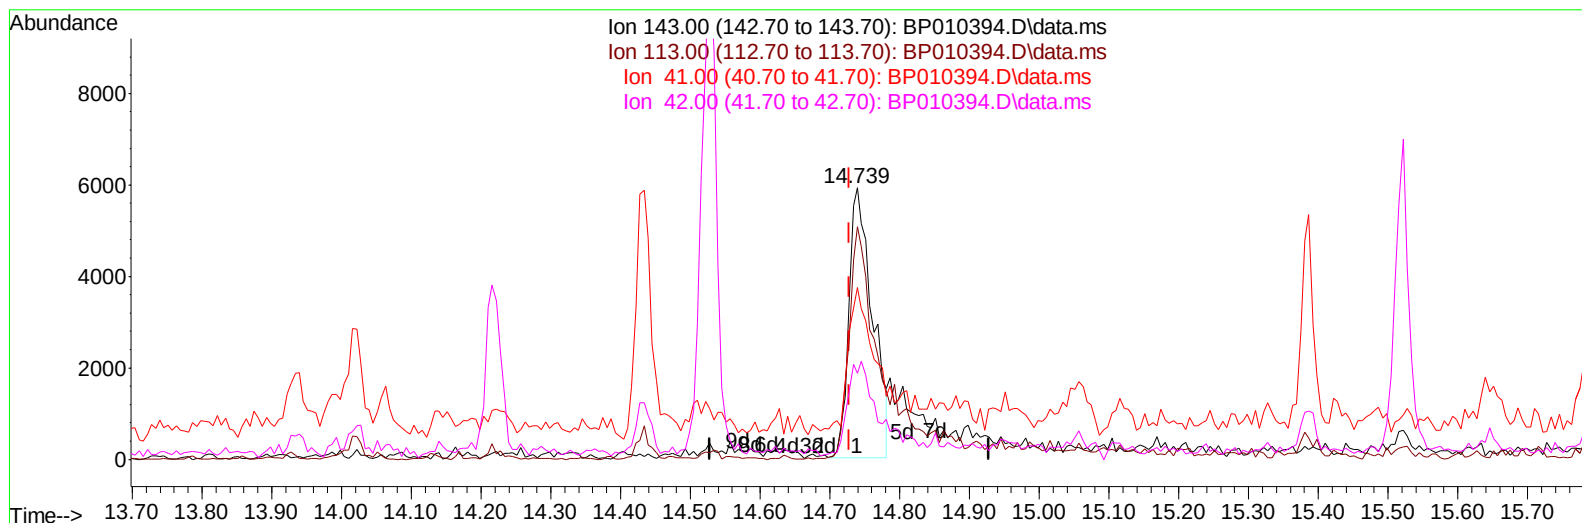

TIC: BP010394.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.012) 2.86 ng/ul

response 13792

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.78#
41.00	23.20	63.42#
42.00	18.00	31.69#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010394.D
 Acq On : 18 May 2022 11:24
 Operator : CG/JU
 Sample : N2766-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:57:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

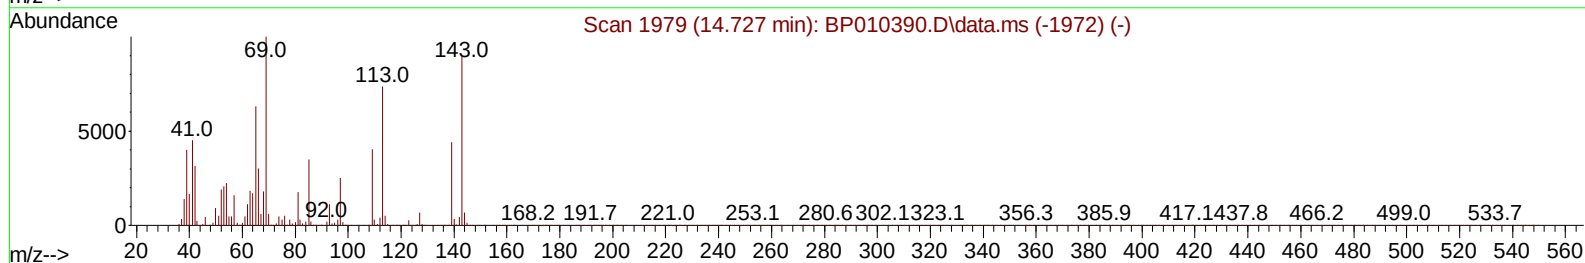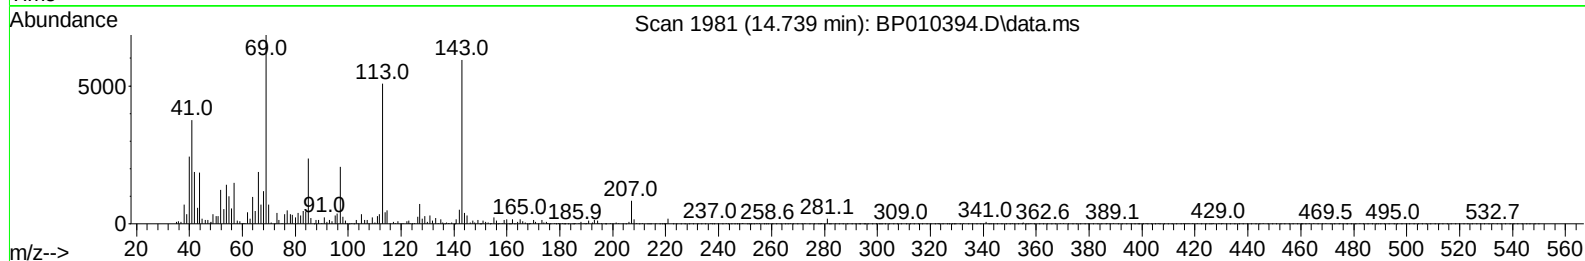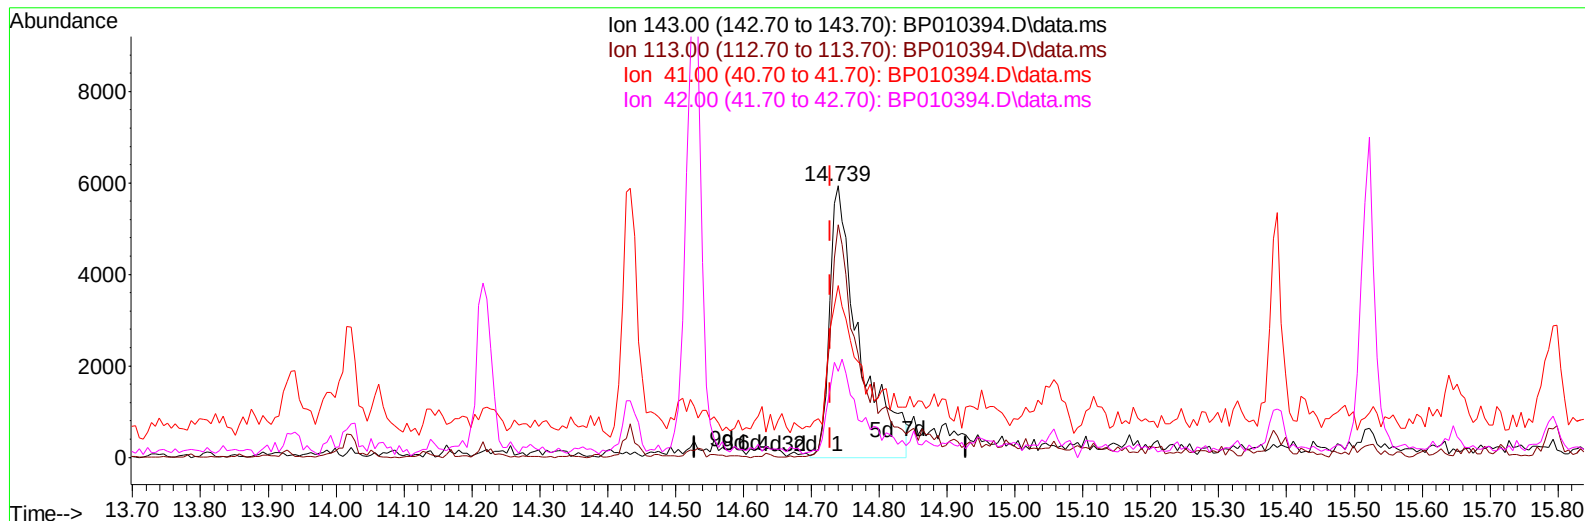

TIC: BP010394.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.012) 3.76 ng/ul m

response 18117

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.78#
41.00	23.20	63.42#
42.00	18.00	31.69#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010394.D
 Acq On : 18 May 2022 11:24
 Operator : CG/JU
 Sample : N2766-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:57:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	118857	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136	528991	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	367448	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	821983	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.363	240	881343	20.000	ng/ul	# 0.00
88) Perylene-d12	23.792	264	847305	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	5462m	1.959	ng/uL	0.00
4) Pyridine-d5	3.781	84	21862m	2.761	ng/ul	0.02
7) Phenol-d5	7.063	99	95299	9.553	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	73523	10.969	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	77808	10.193	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	71520	8.436	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128	42992	10.501	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	41186	9.493	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	71952	8.770	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	98414	8.068	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	299260	11.054	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	324704	10.398	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	18117m	3.760	ng/ul	0.01
60) Fluorene-d10	15.522	176	264330	11.223	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	16753	3.485	ng/ul	0.00
73) Anthracene-d10	17.380	188	428237	11.505	ng/ul	0.00
81) Pyrene-d10	19.610	212	606982	12.968	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	542575	12.753	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.722	105	20281	1.523	ng/ul#	Qvalue 72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010394.D
Acq On : 18 May 2022 11:24
Operator : CG/JU
Sample : N2766-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:57:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

