




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

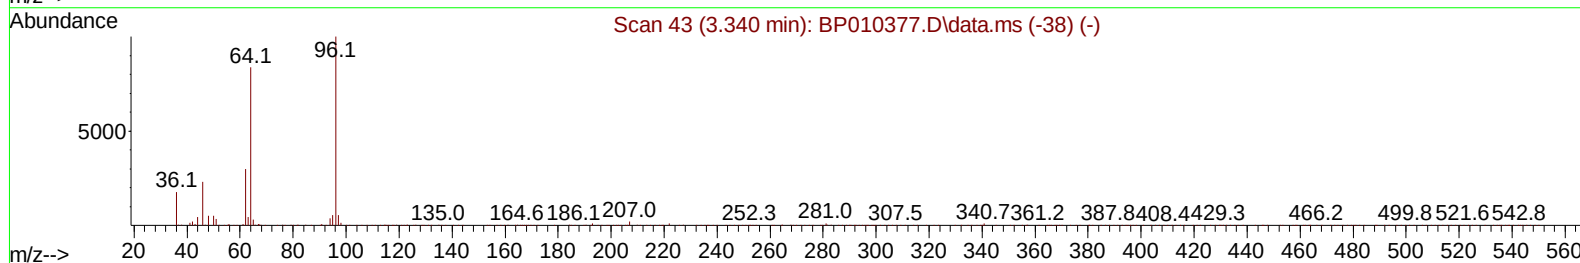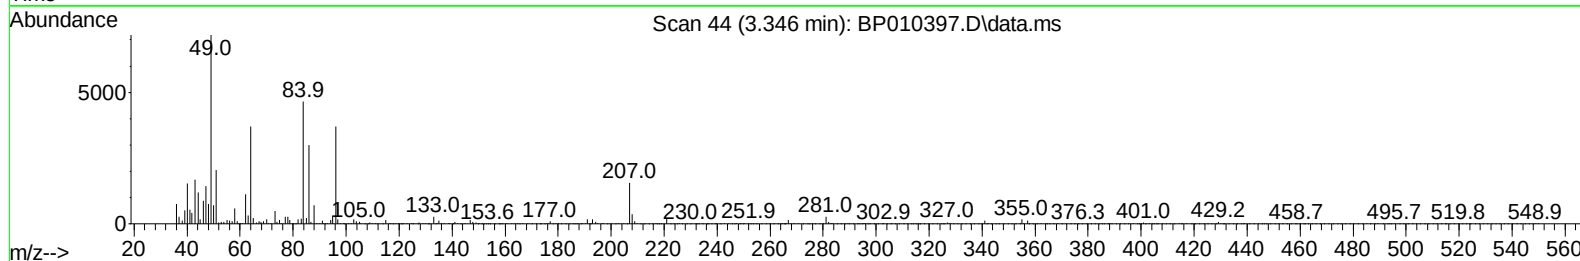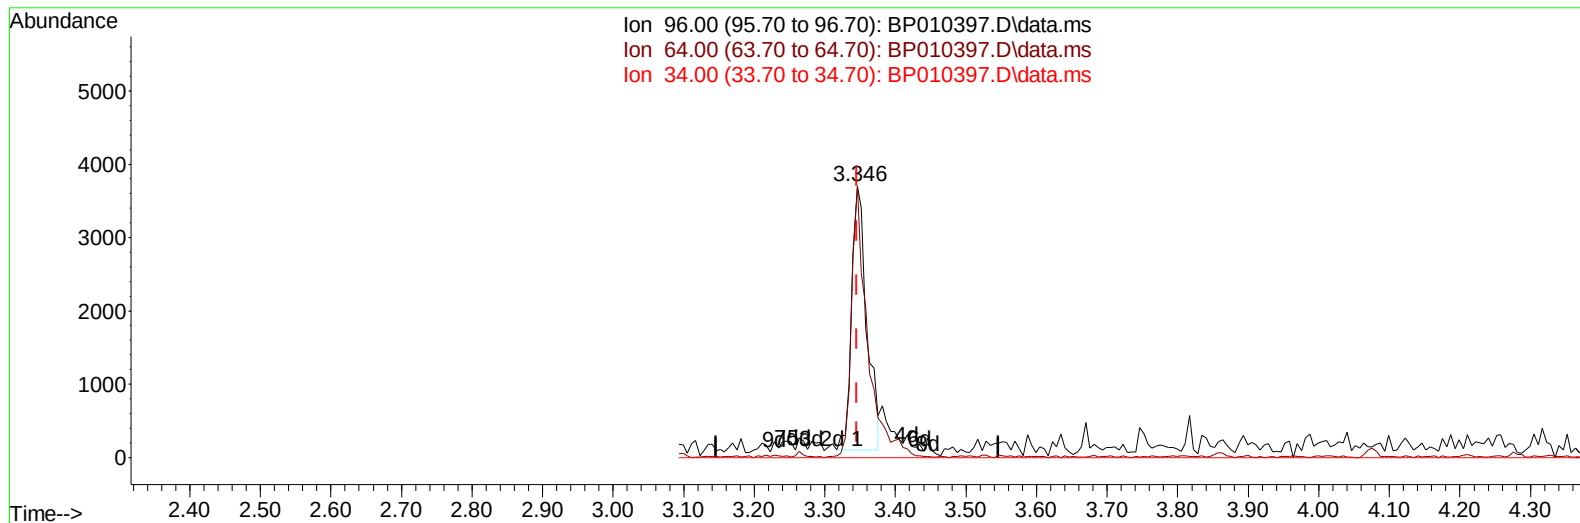

TIC: BP010397.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (+ 0.000) 1.55 ng/uL

response 5410

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	100.08#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

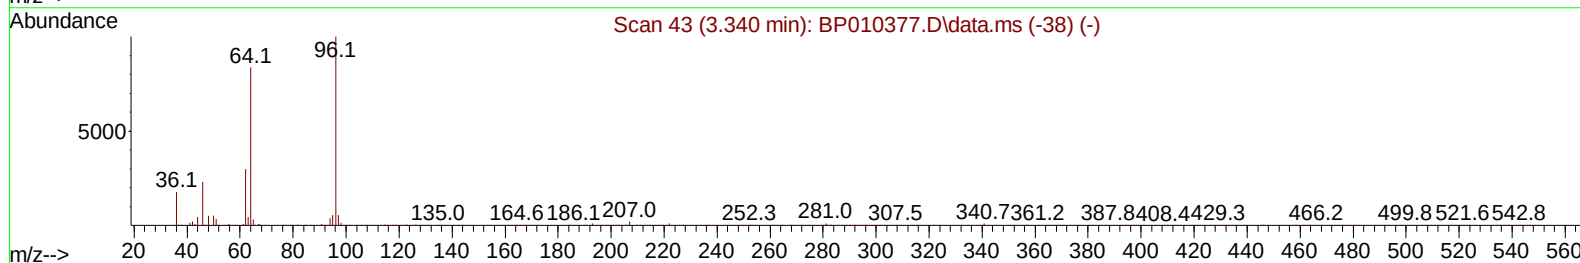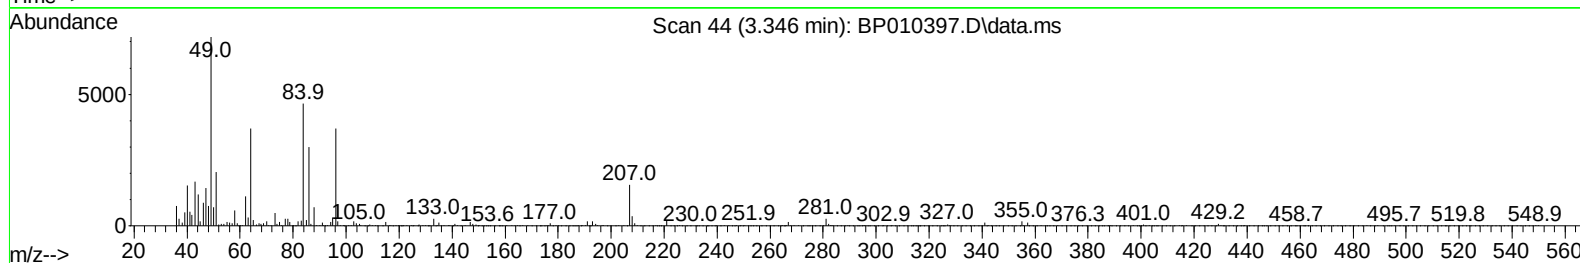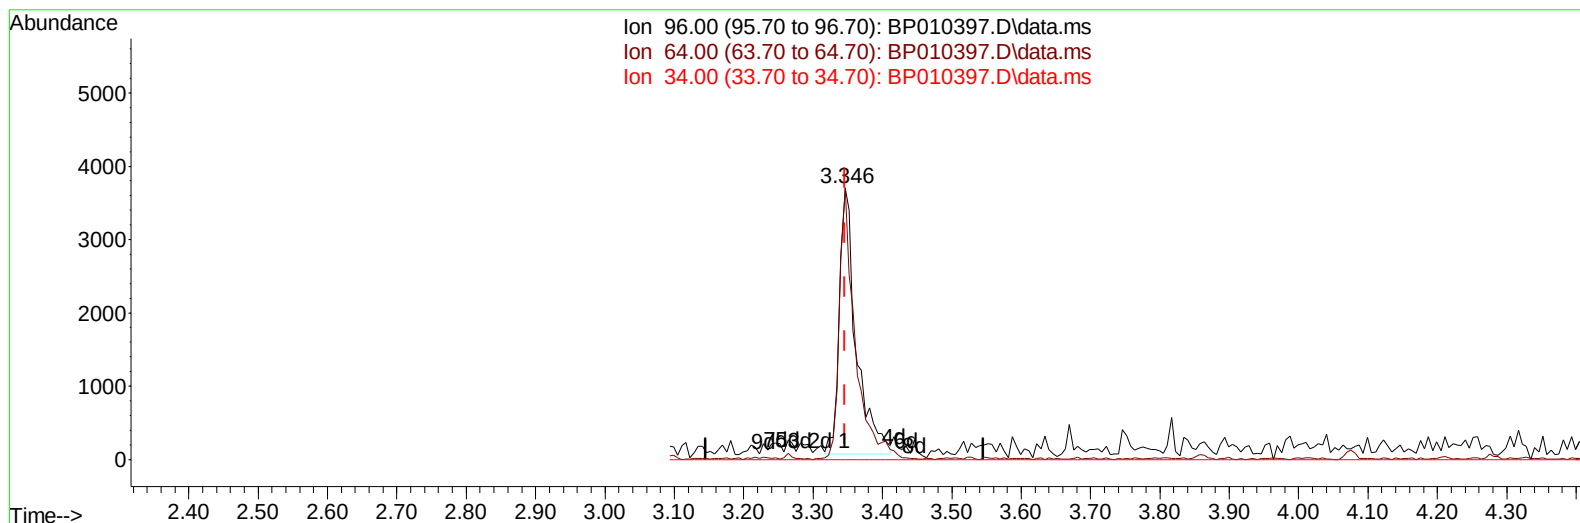

TIC: BP010397.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (+ 0.000) 1.76 ng/uL m

response 6150

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	100.08#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

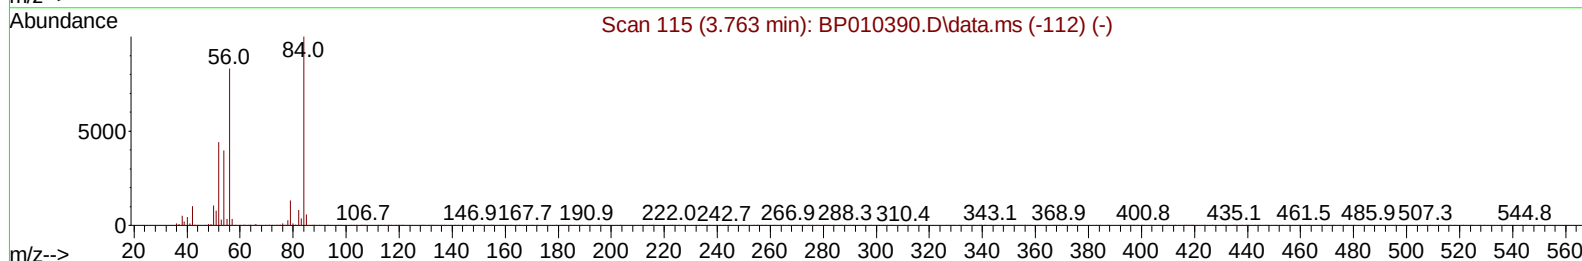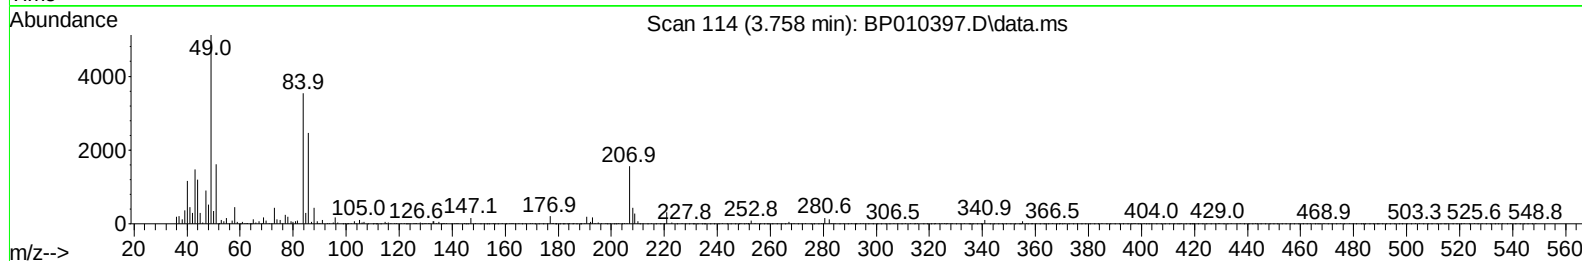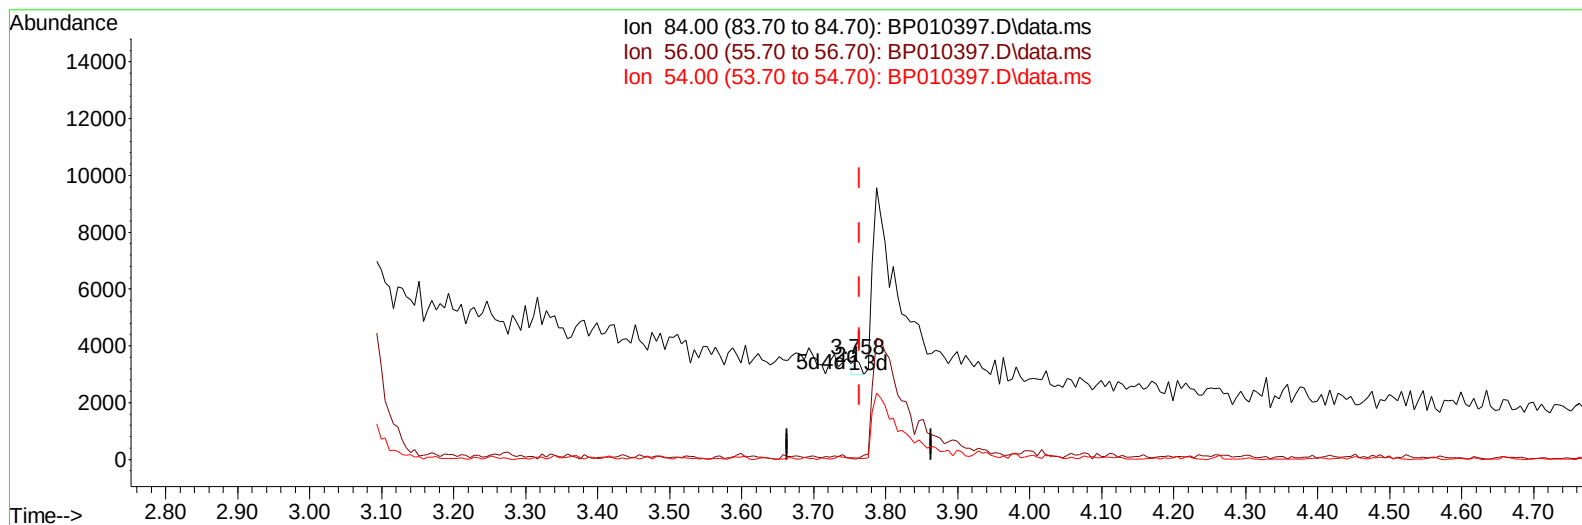

TIC: BP010397.D\data.ms

(4) Pyridine-d5 (S)

3.758min (-0.006) 0.03 ng/uI

response 340

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	0.51#
54.00	24.80	1.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

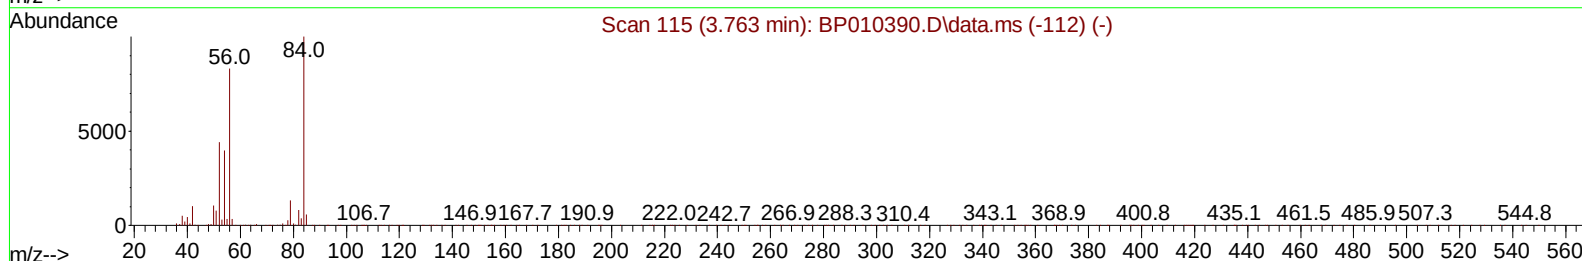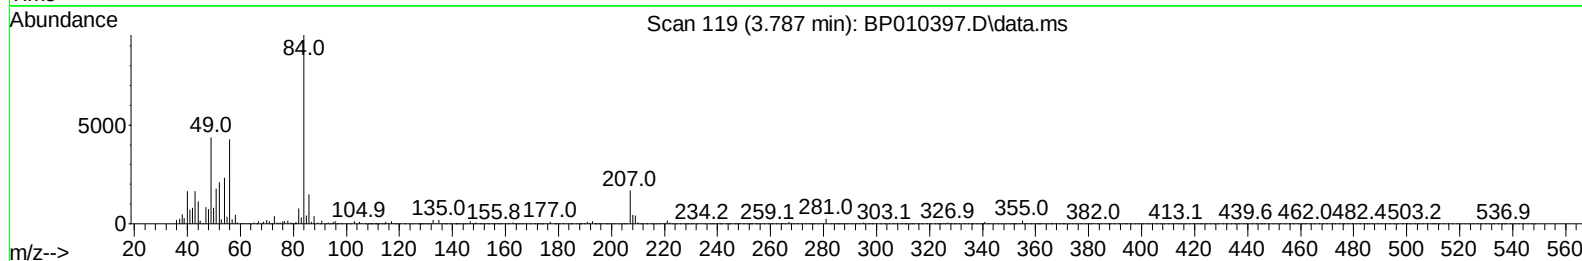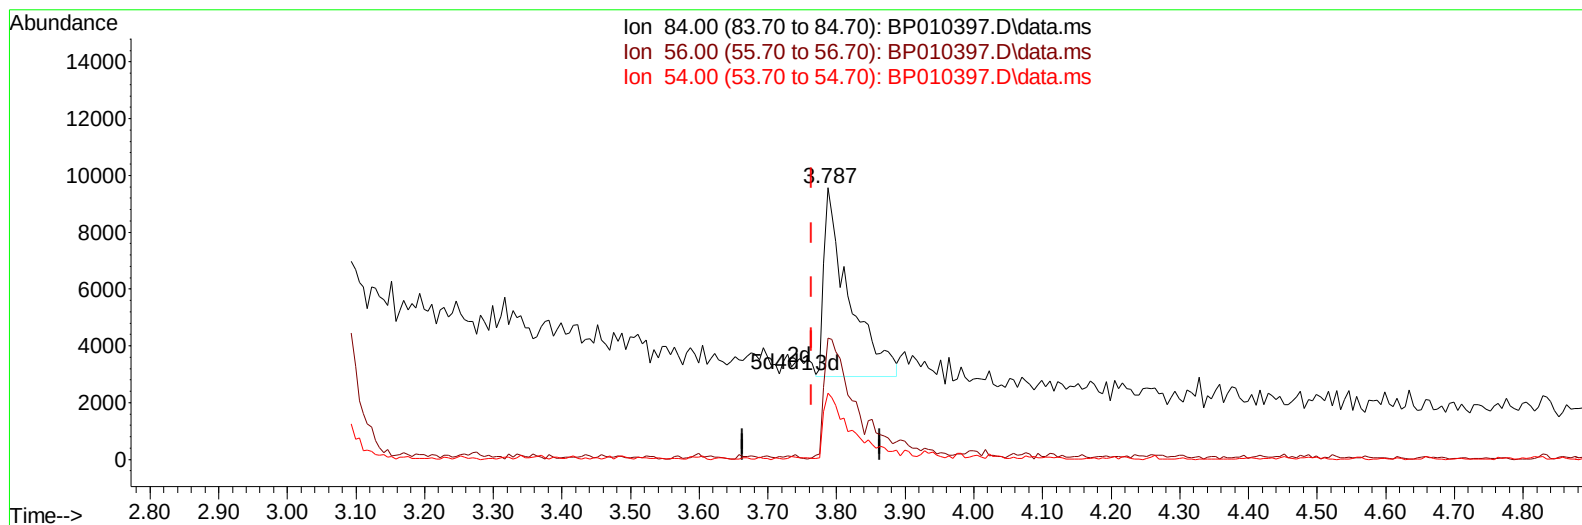

TIC: BP010397.D\data.ms

(4) Pyridine-d5 (S)

3.787min (+ 0.024) 1.67 ng/ul m

response 16493

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	44.66#
54.00	24.80	24.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

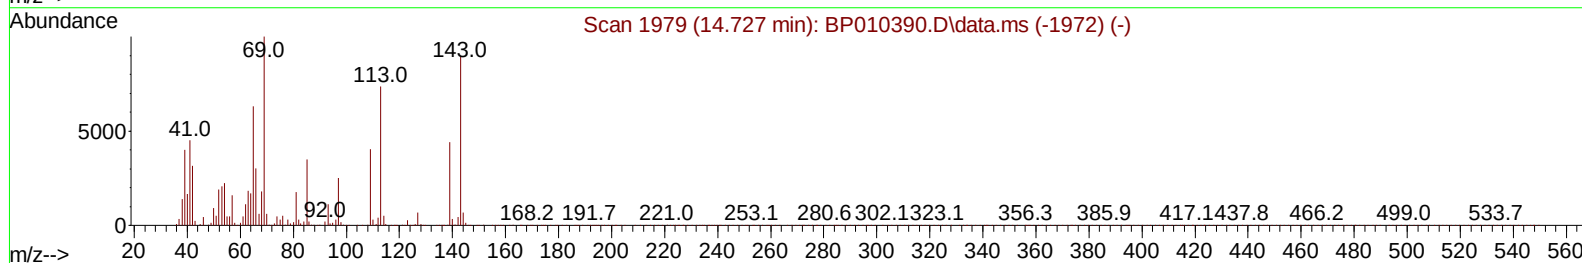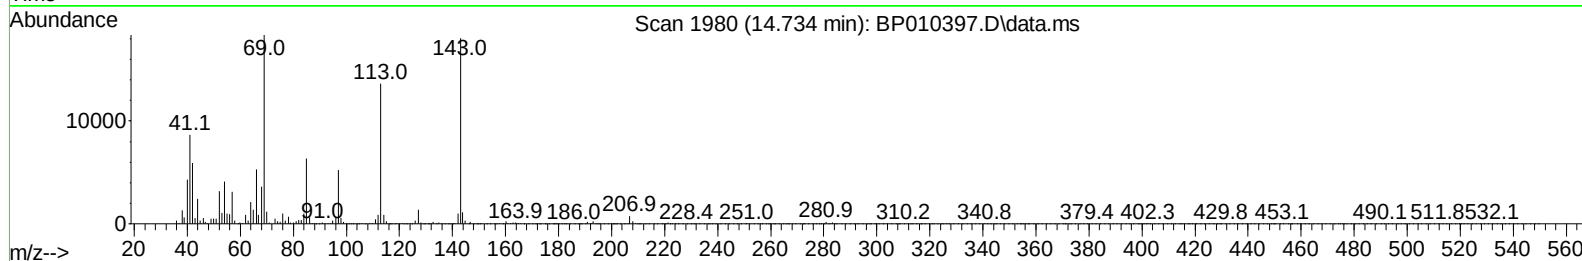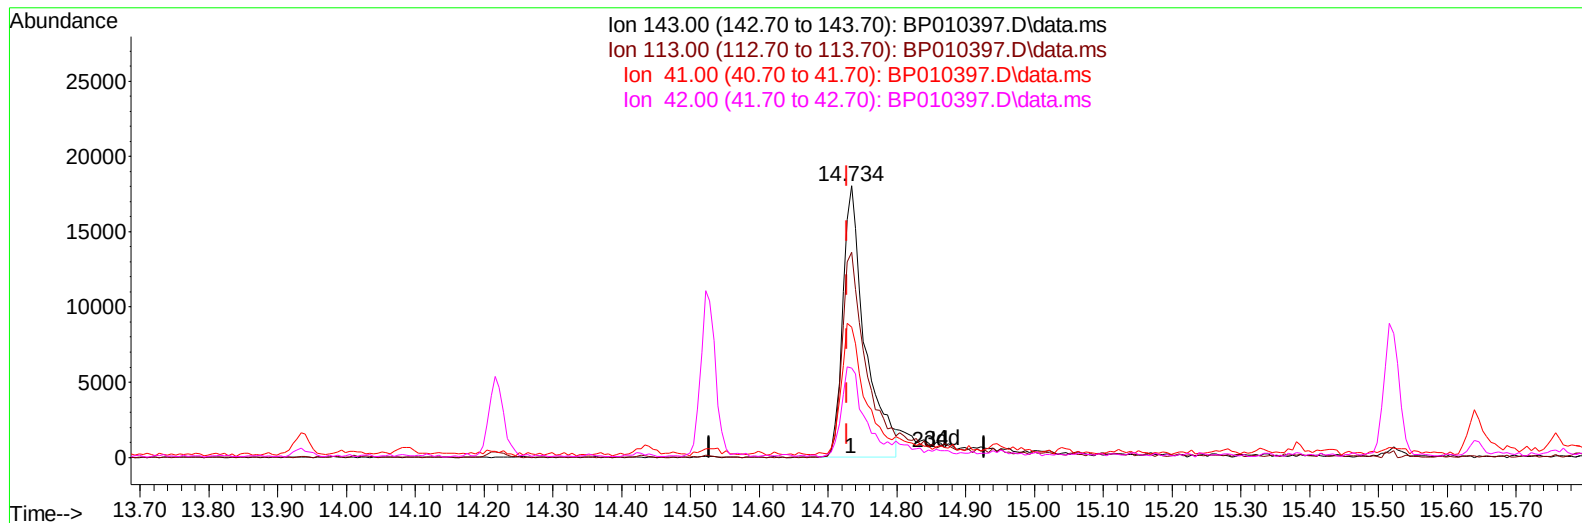

TIC: BP010397.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.006) 7.04 ng/ul

response 40695

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.54#
41.00	23.20	48.03#
42.00	18.00	32.95#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:58:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

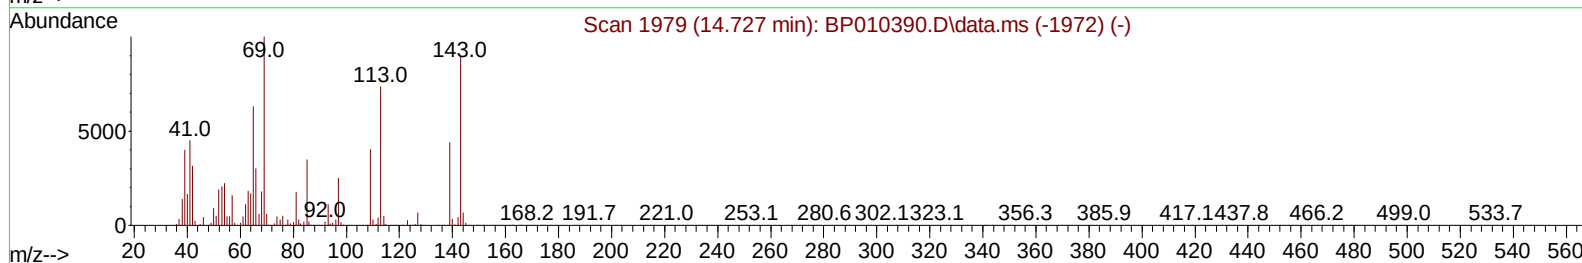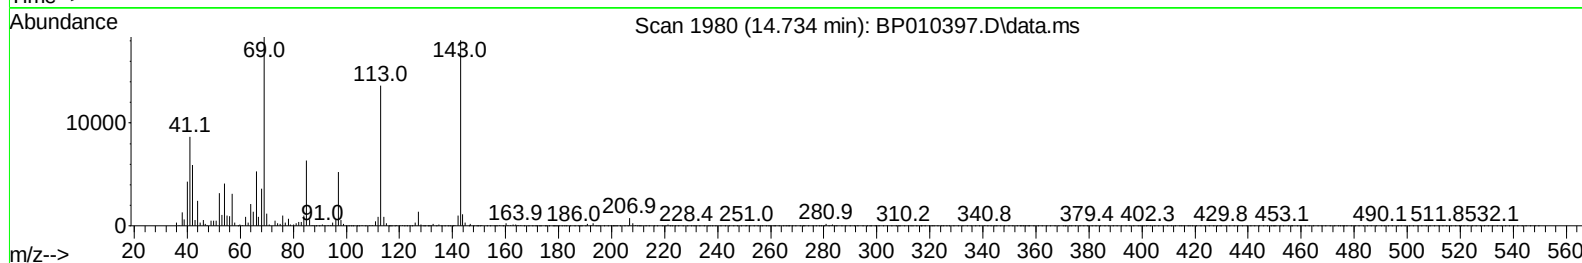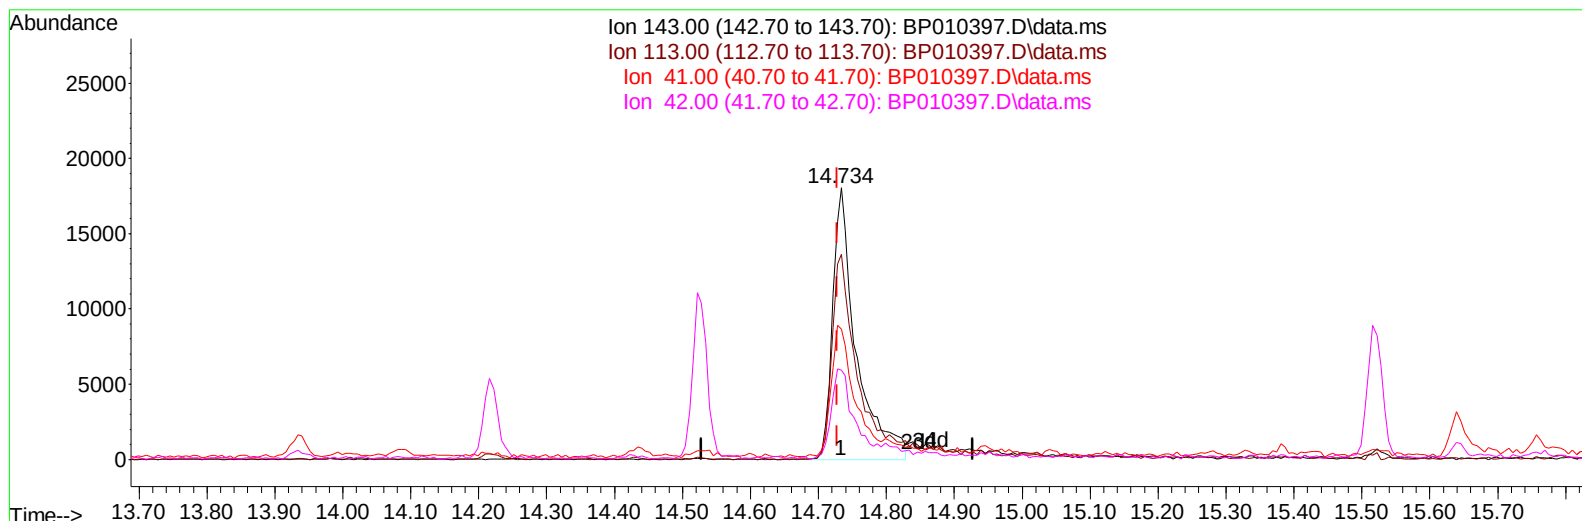

TIC: BP010397.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.006) 7.51 ng/ul m

response 43400

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.54#
41.00	23.20	48.03#
42.00	18.00	32.95#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:58:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	148609	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	645181	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	440603	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	973536	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.363	240	920083	20.000	ng/ul	# 0.00
88) Perylene-d12	23.792	264	769297	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	6150m	1.764	ng/uL	0.00
4) Pyridine-d5	3.787	84	16493m	1.666	ng/ul	0.02
7) Phenol-d5	7.064	99	149105	11.954	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	102047	12.177	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	115242	12.074	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	110425	10.417	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	60945	12.205	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	64451	12.180	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	127549	12.747	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	133773	8.992	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	528966	16.295	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	547081	14.611	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	43400m	7.511	ng/ul	0.00
60) Fluorene-d10	15.522	176	435769	15.430	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	40450	7.104	ng/ul	0.00
73) Anthracene-d10	17.381	188	715627	16.234	ng/ul	0.00
81) Pyrene-d10	19.610	212	900681	18.433	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	663880	17.186	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:58:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

