




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

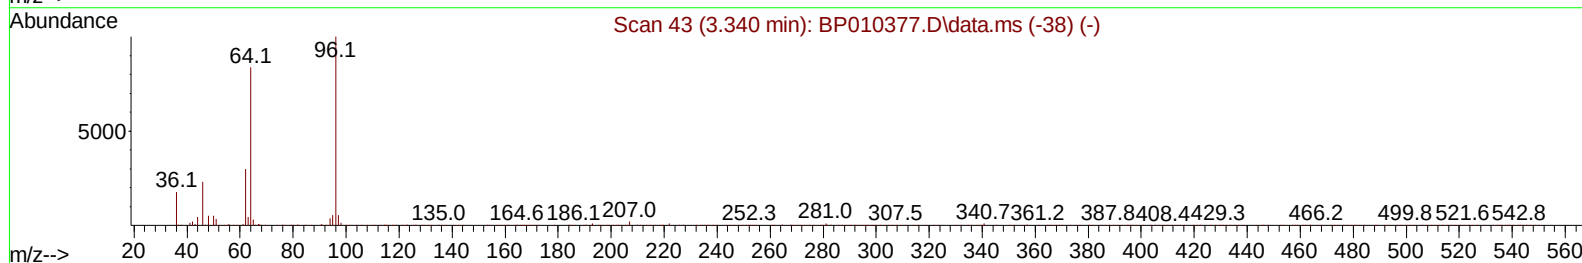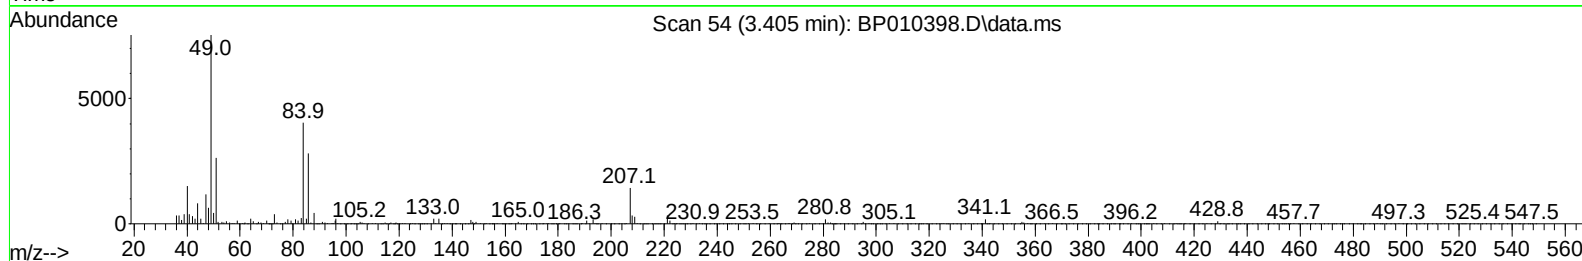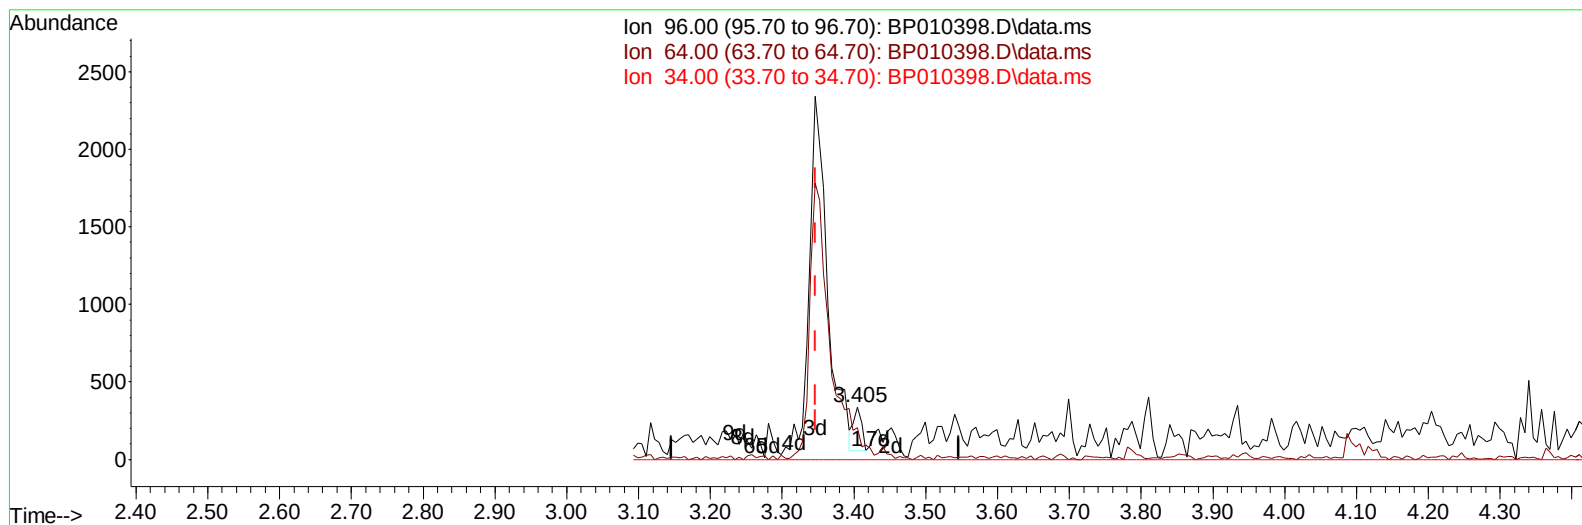

TIC: BP010398.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.405min (+ 0.059) 0.07 ng/uL

response 224

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	60.65
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

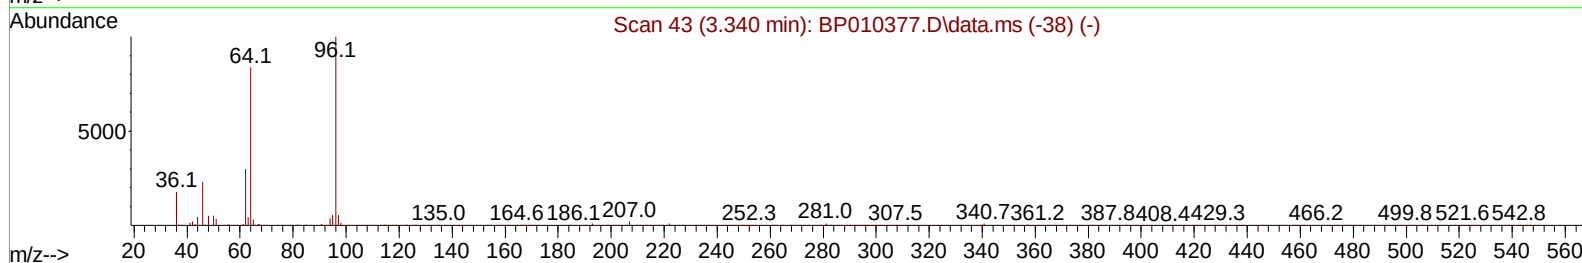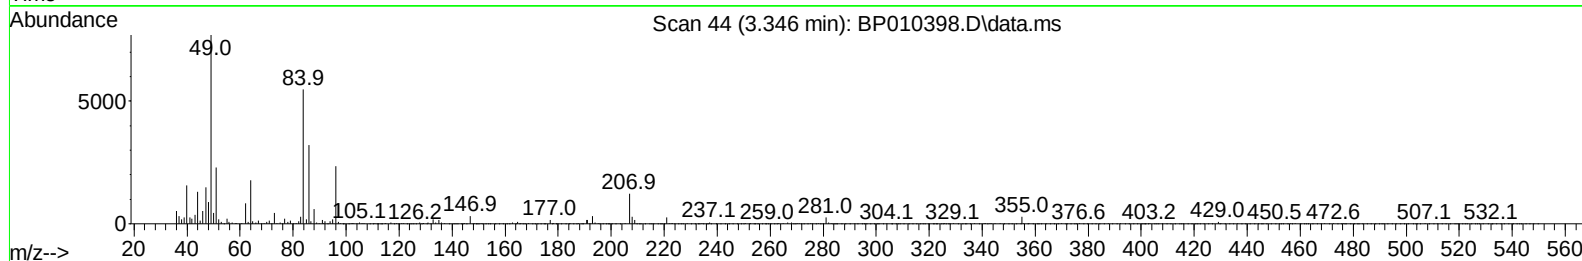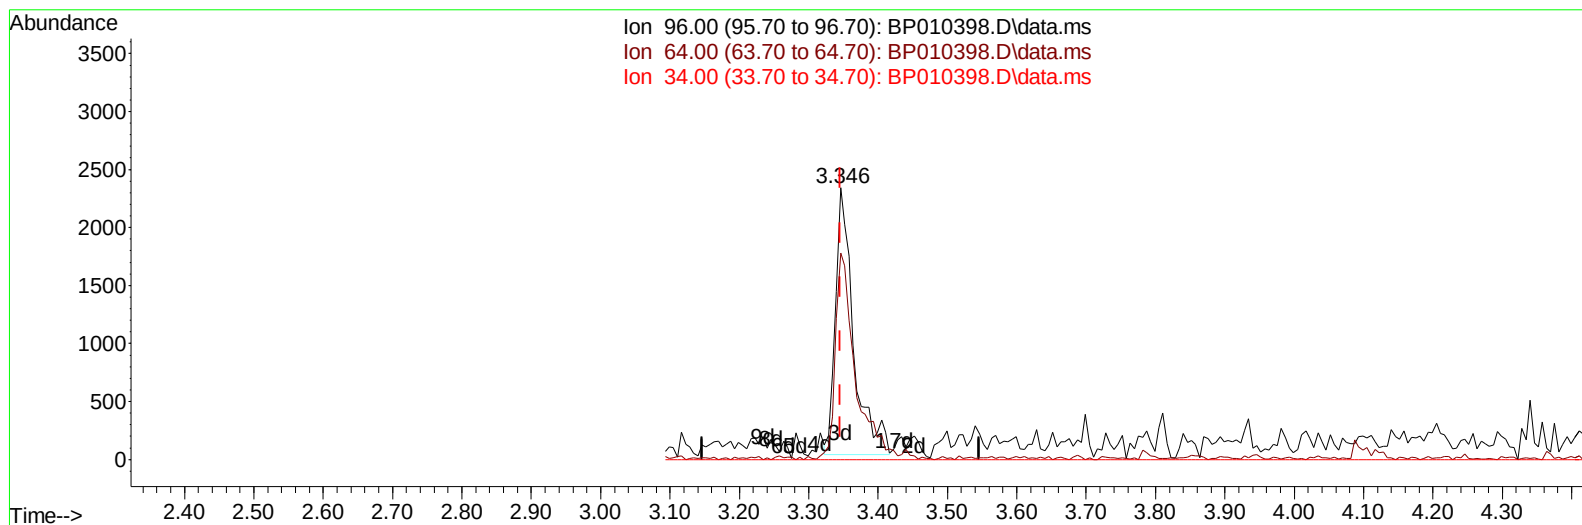

TIC: BP010398.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (0.000) 1.27 ng/uL m

response 4177

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.12#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

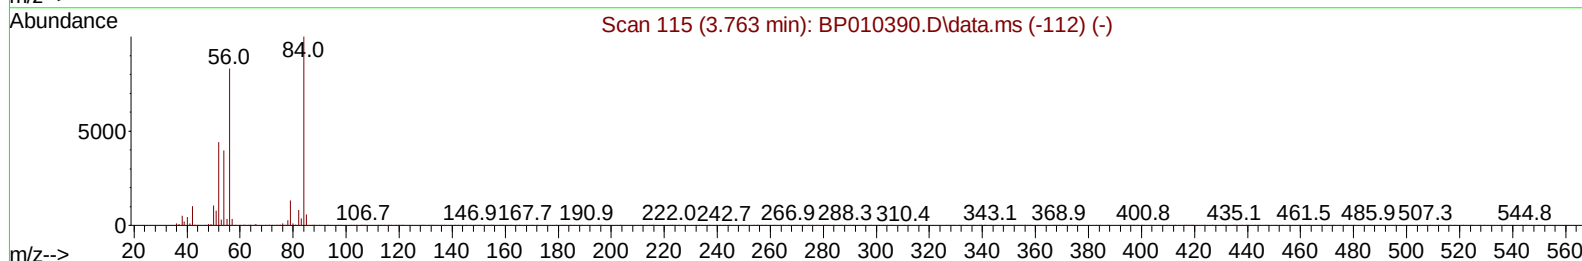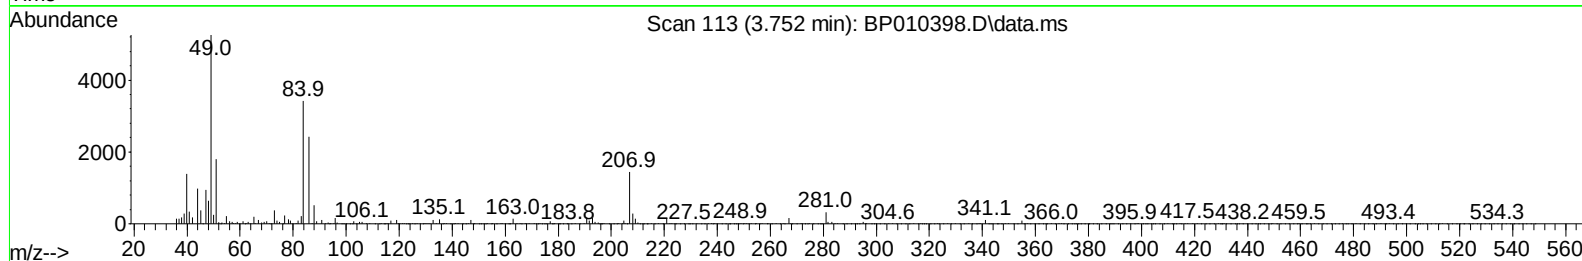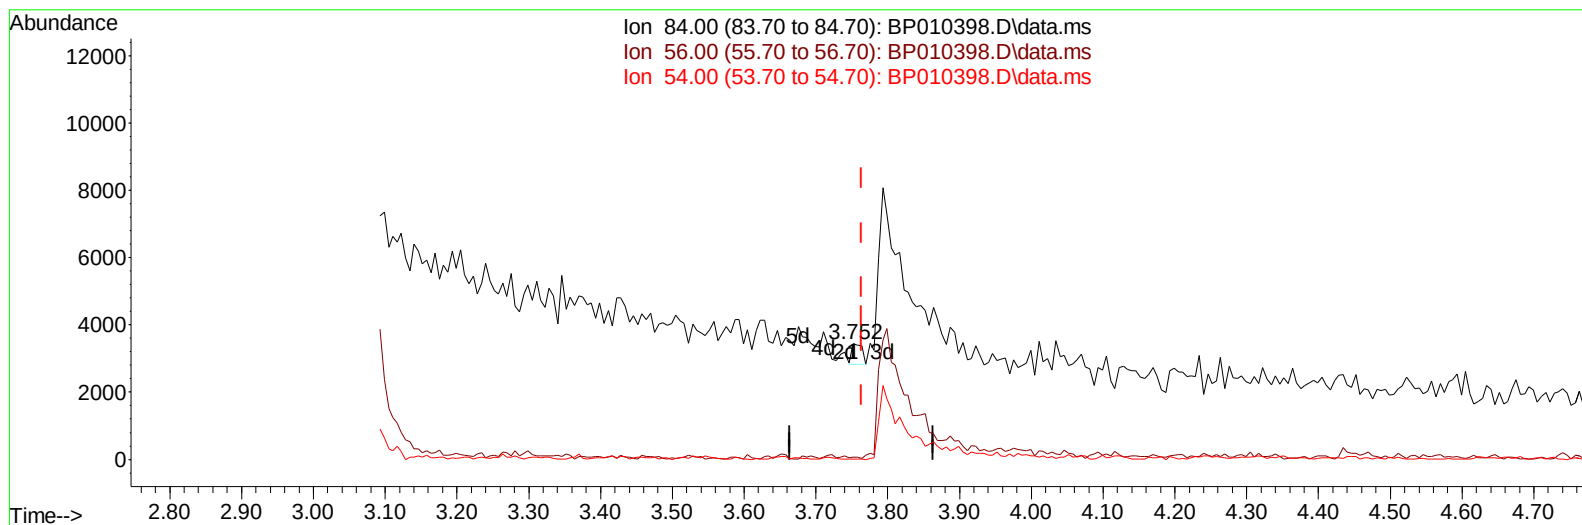

TIC: BP010398.D\data.ms

(4) Pyridine-d5 (S)

3.752min (-0.012) 0.06 ng/ul

response 601

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	1.87#
54.00	24.80	0.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

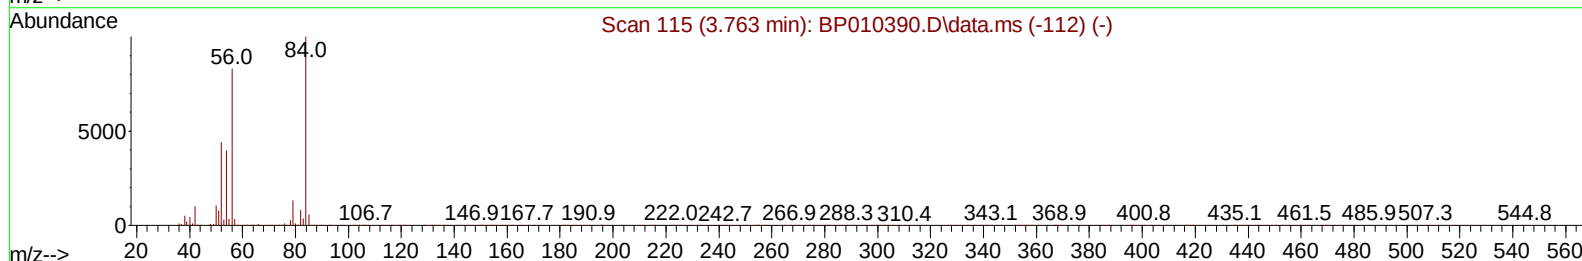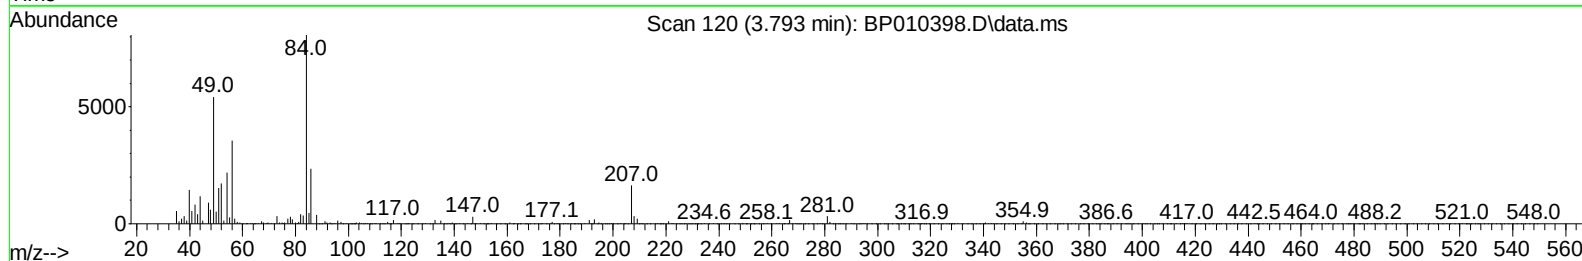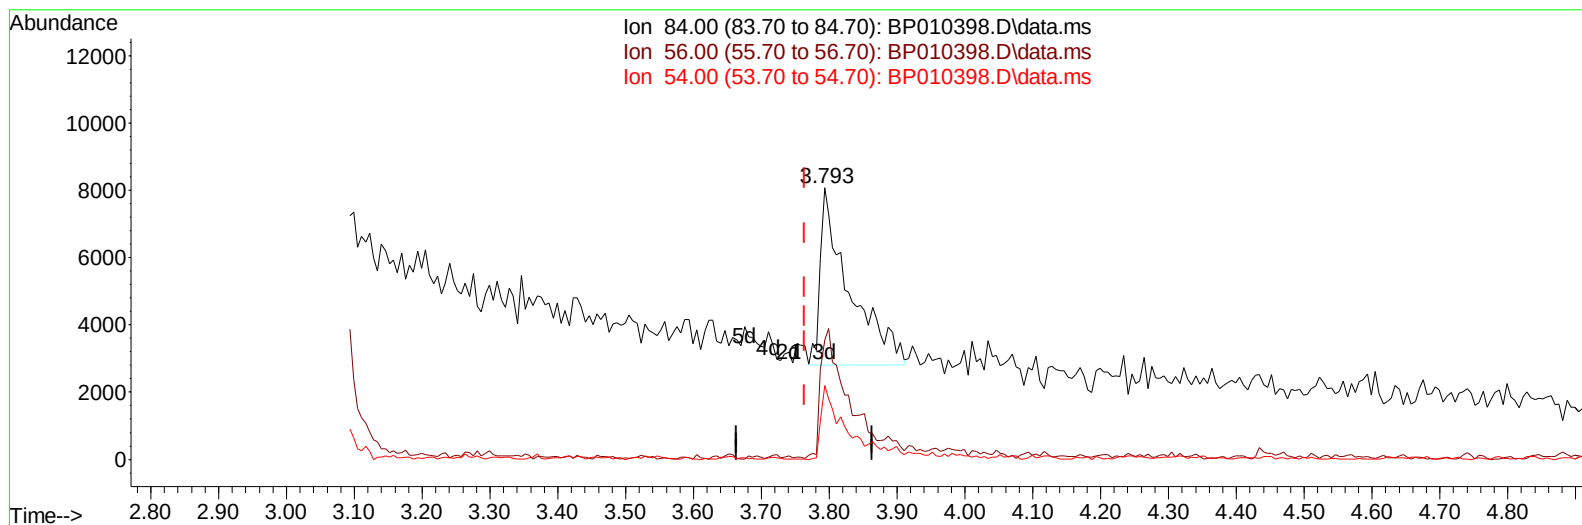

TIC: BP010398.D\data.ms

(4) Pyridine-d5 (S)

3.793min (+ 0.030) 1.68 ng/ul m

response 15681

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	44.00#
54.00	24.80	27.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

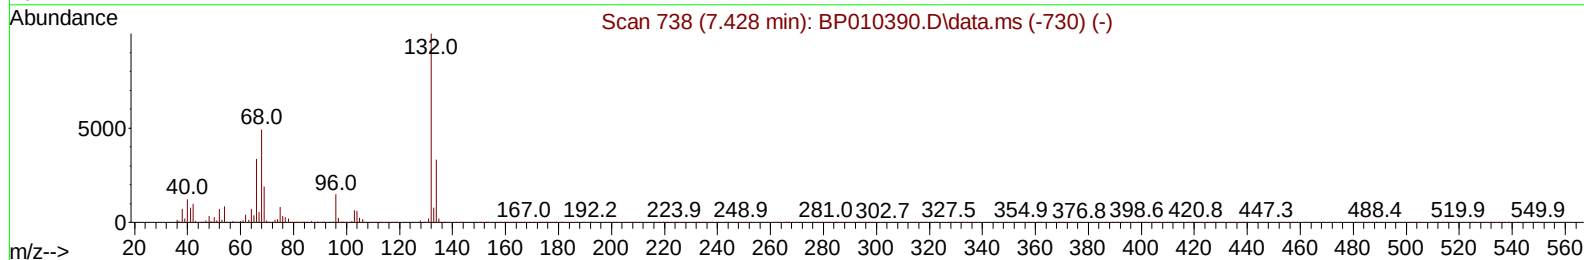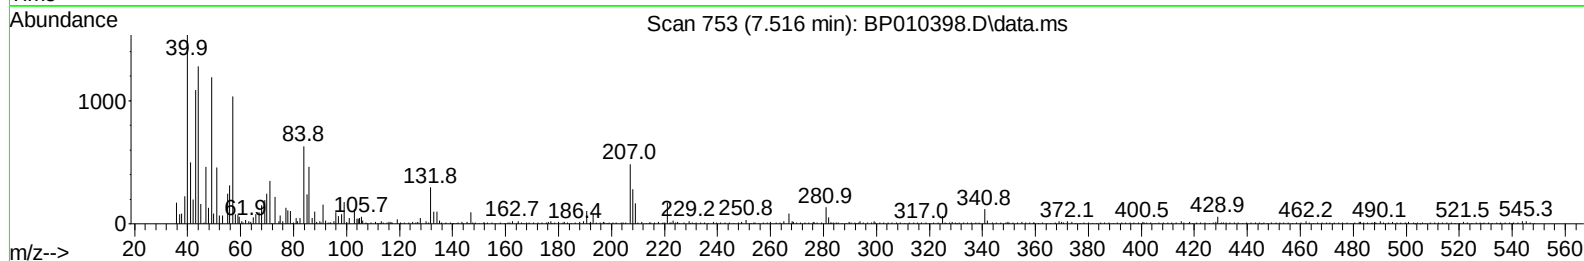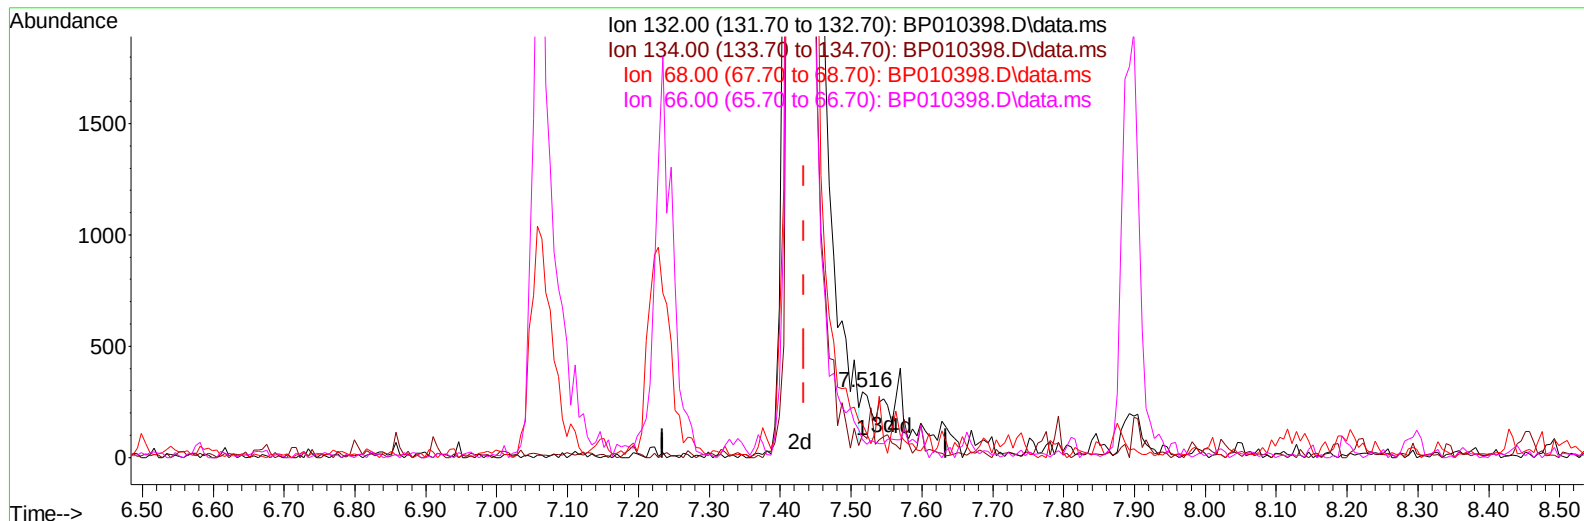

TIC: BP010398.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.516min (+ 0.082) 0.02 ng/u1

response 218

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	34.12
68.00	51.40	50.34
66.00	26.30	26.35




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

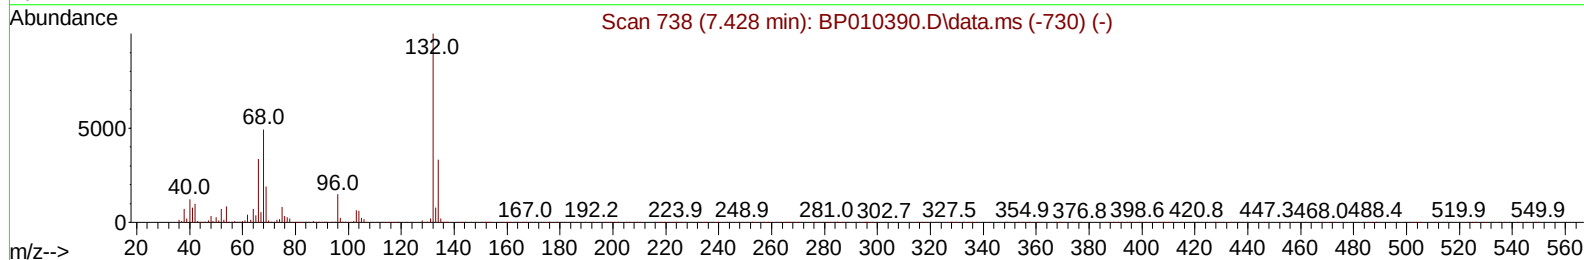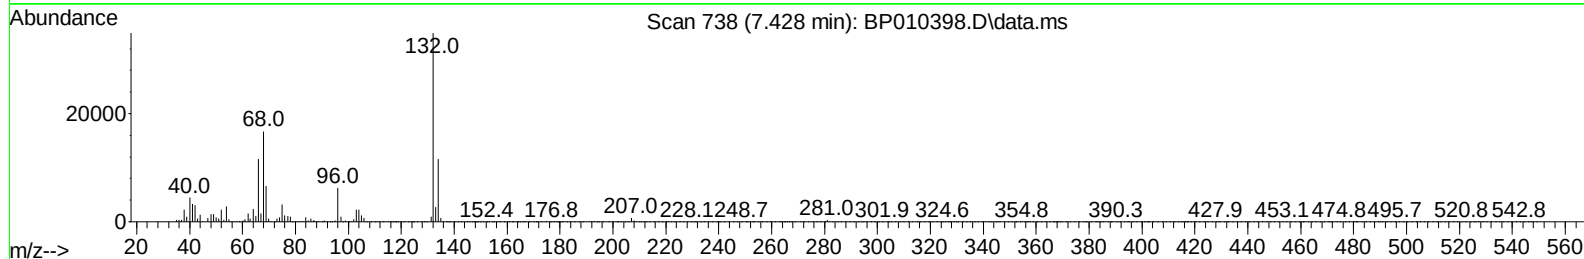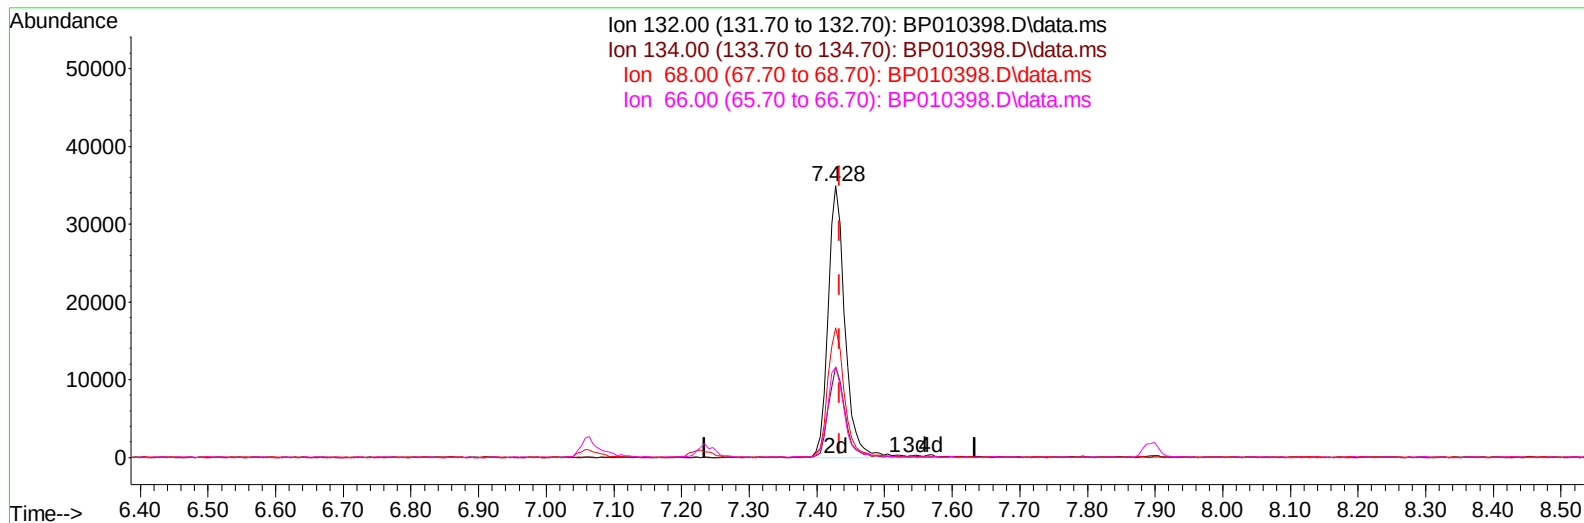

TIC: BP010398.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.428min (-0.006) 6.72 ng/ul m

response 60365

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	33.28
68.00	51.40	47.80
66.00	26.30	33.19#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

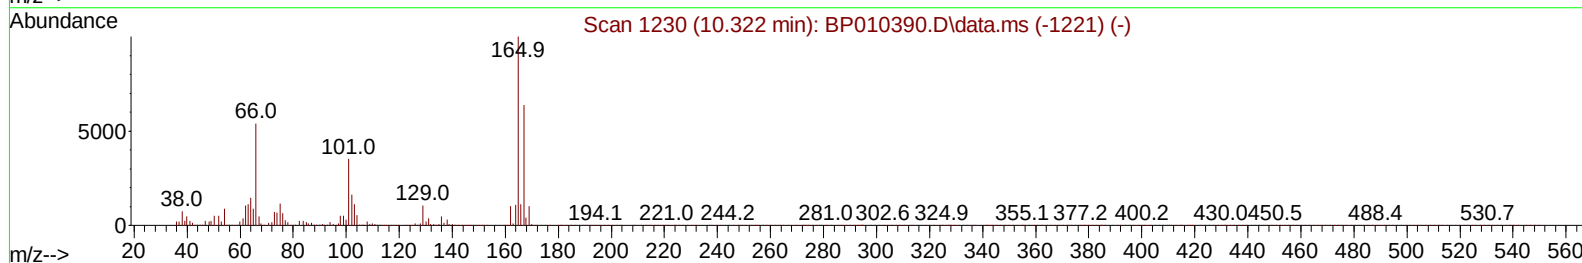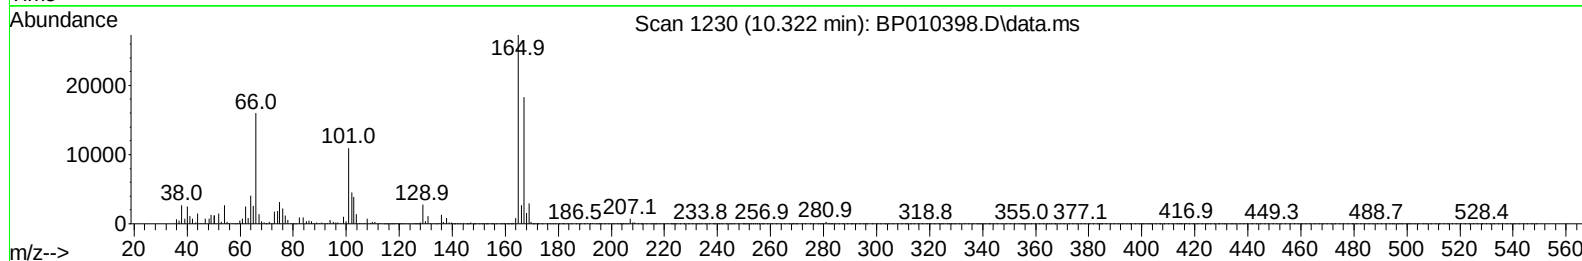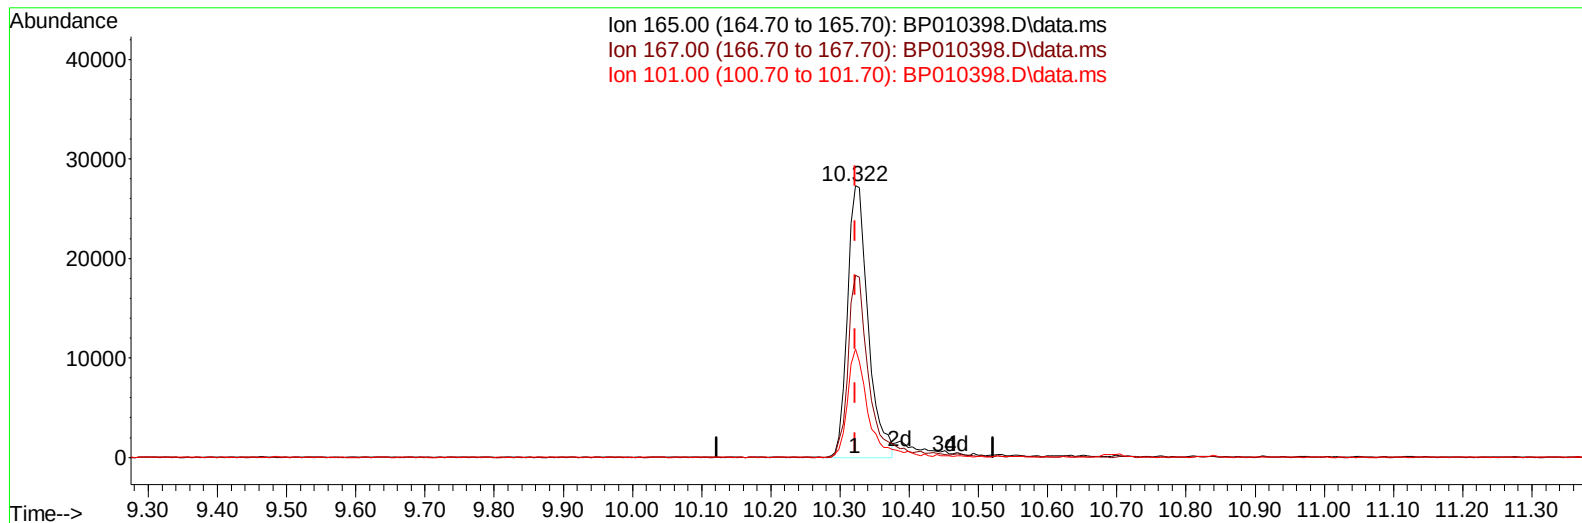

TIC: BP010398.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.322min (+ 0.000) 5.95 ng/ul

response 56201

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	67.19
101.00	49.80	40.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

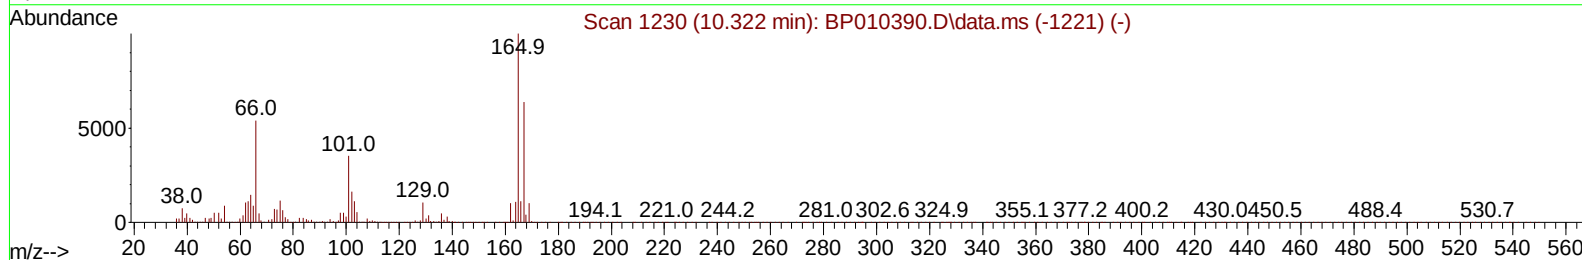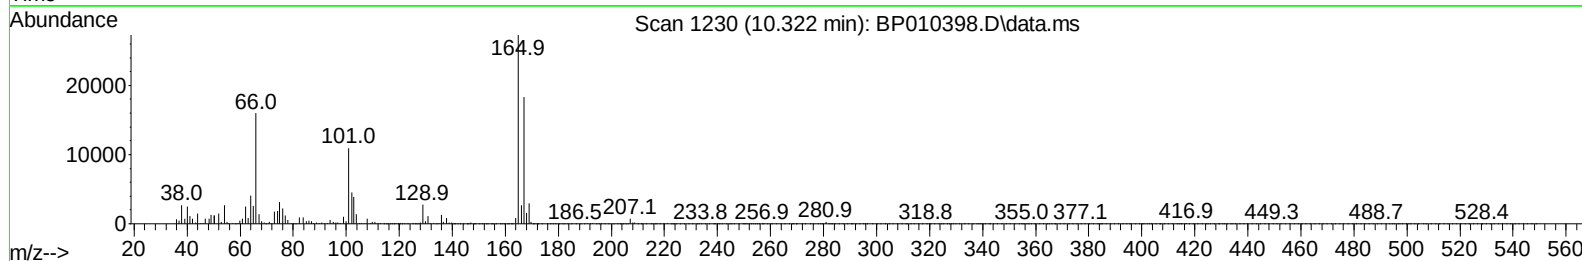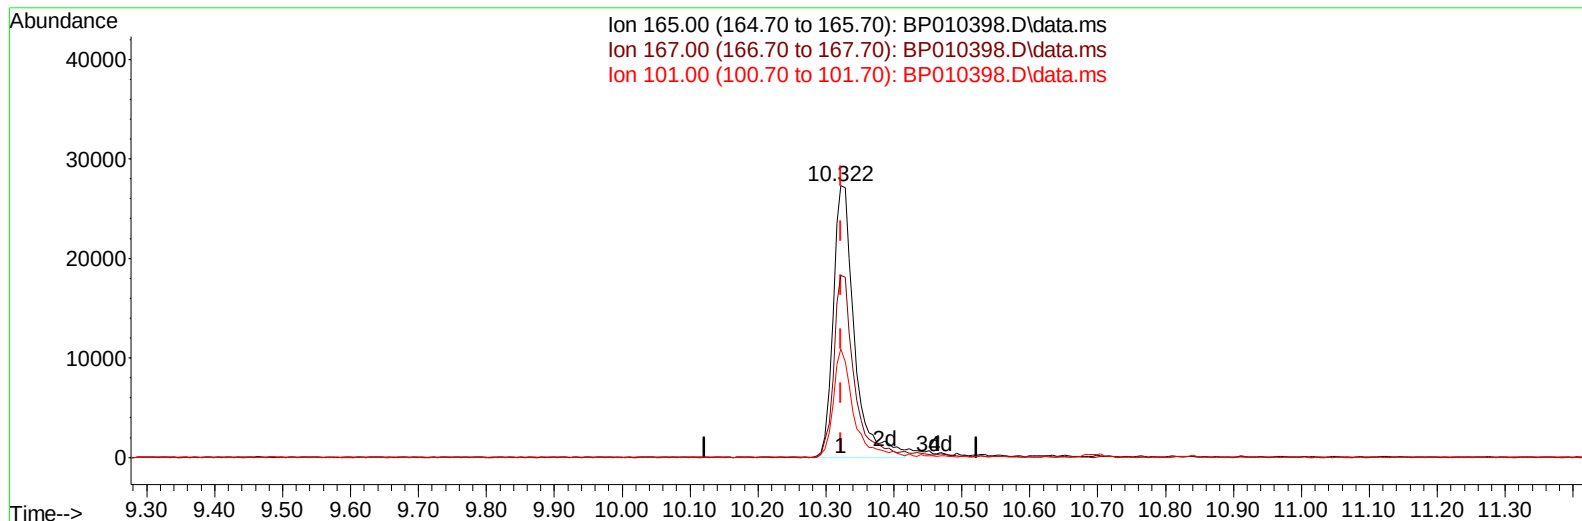

TIC: BP010398.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.322min (+ 0.000) 6.26 ng/ul m

response 59077

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	67.19
101.00	49.80	40.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

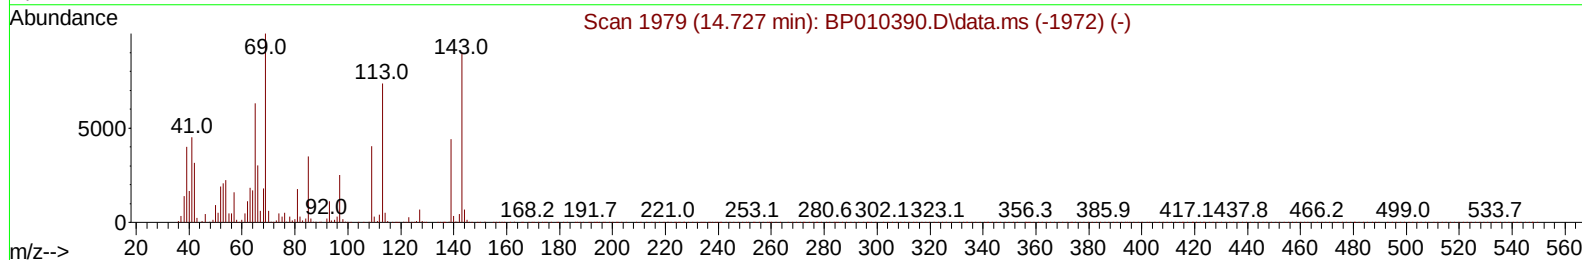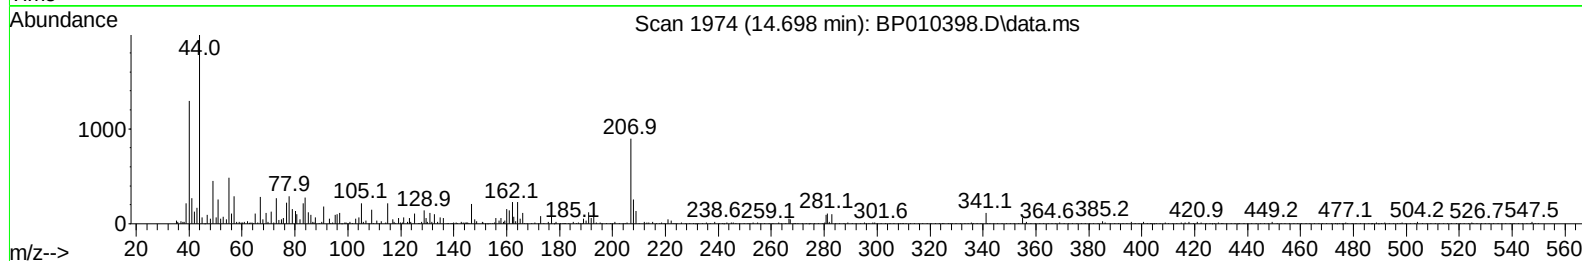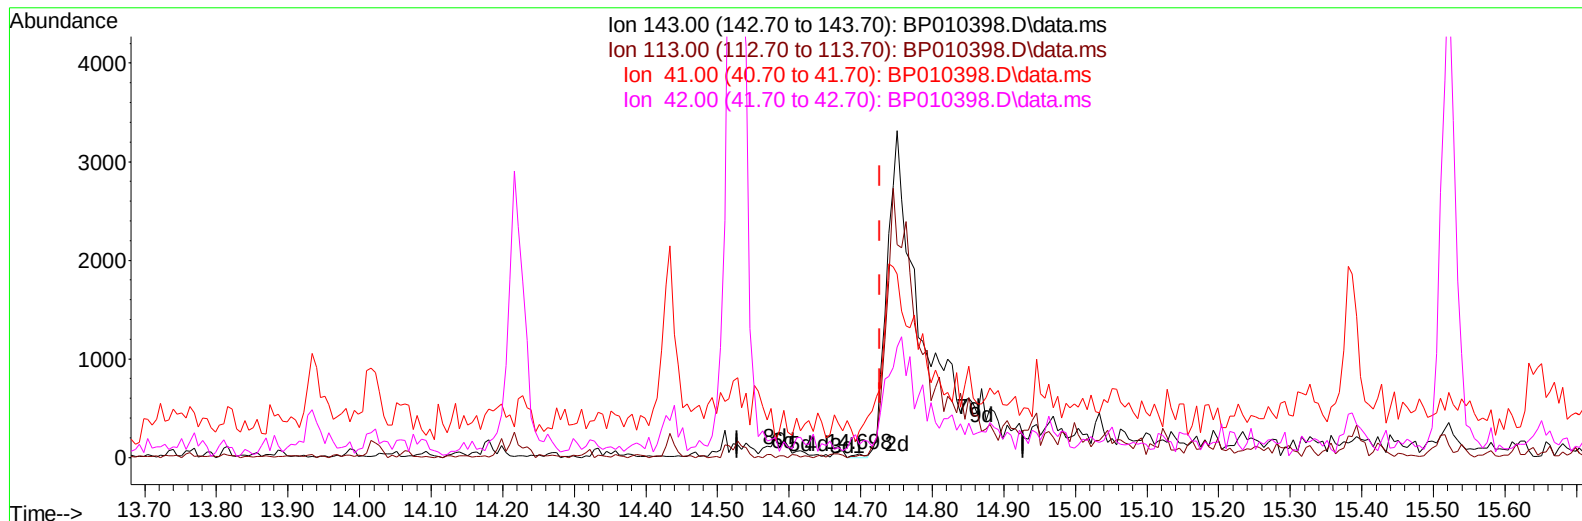

TIC: BP010398.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (-0.029) 0.01 ng/uL

response 41

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	65.79#
41.00	23.20	707.89#
42.00	18.00	344.74#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 01:58:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

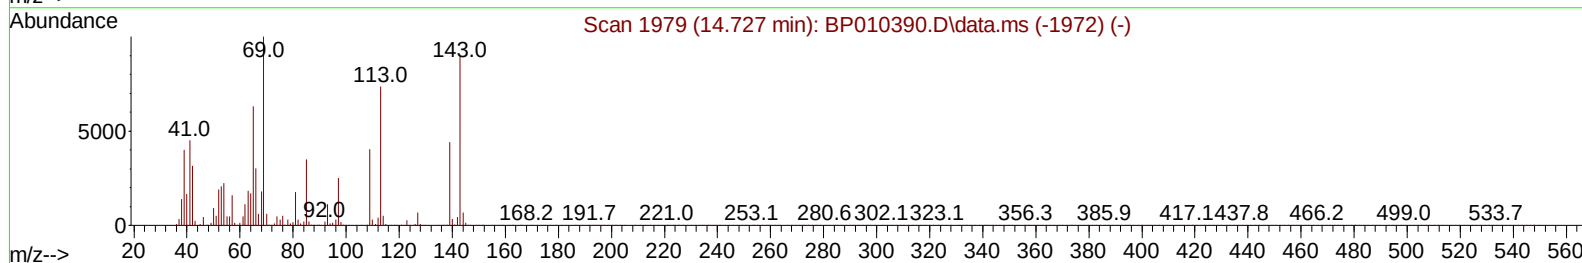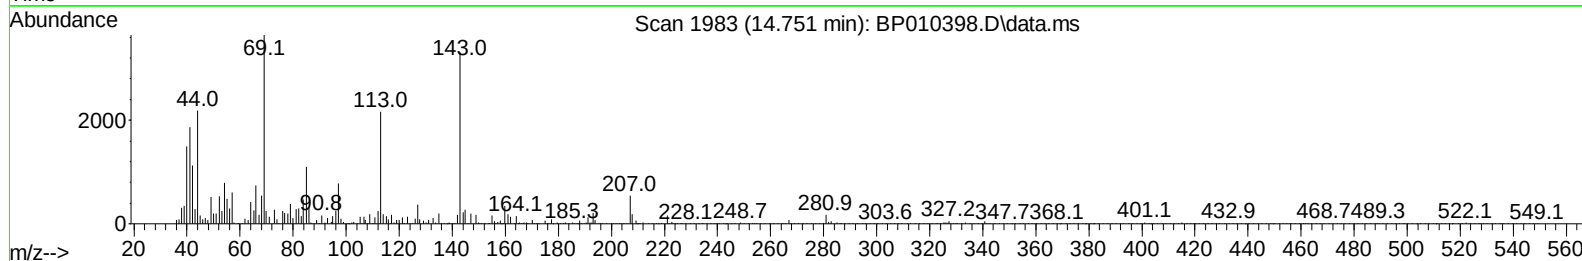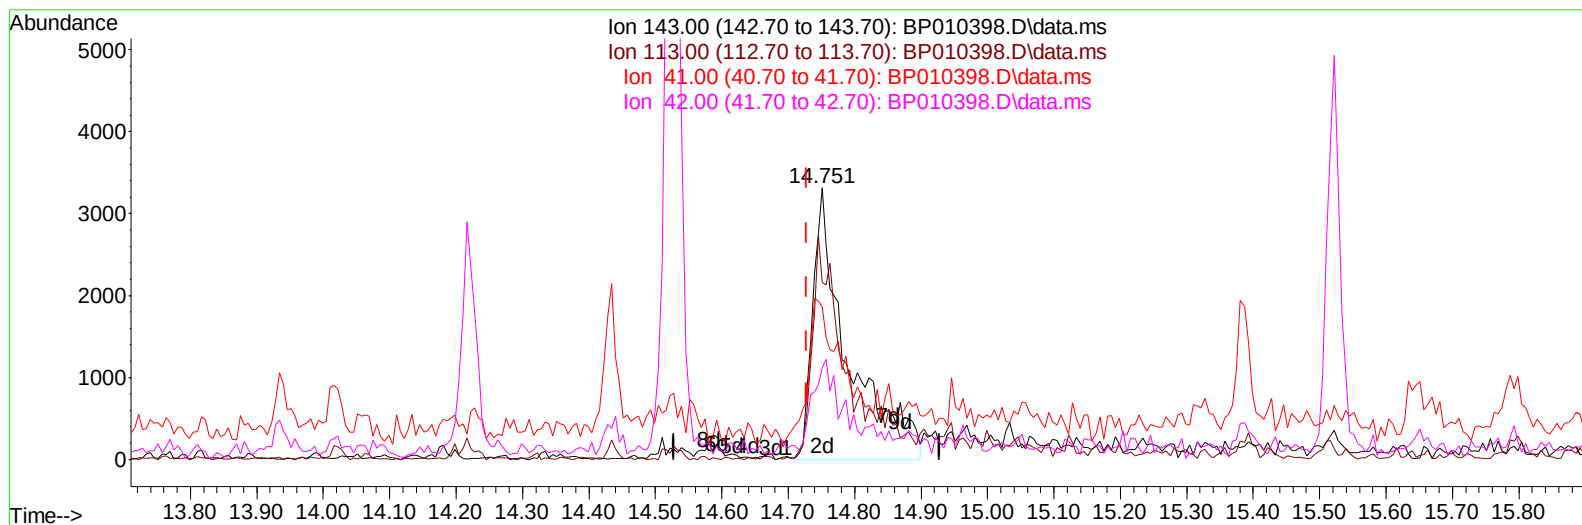

TIC: BP010398.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.024) 2.20 ng/ul m

response 12163

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	65.23#
41.00	23.20	56.23#
42.00	18.00	33.84#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:58:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	139822	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	608770	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	422399	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	925343	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.363	240	890804	20.000	ng/ul	0.00
88) Perylene-d12	23.786	264	769495	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	4177m	1.273	ng/uL	0.00
4) Pyridine-d5	3.793	84	15681m	1.684	ng/ul	0.03
7) Phenol-d5	7.063	99	68484	5.836	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	55889	7.088	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	60365m	6.722	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	62717	6.288	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	31336	6.651	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	31627	6.334	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	59077m	6.257	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	78867	5.618	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	230478	7.406	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	247471	6.894	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	12163m	2.196	ng/ul	0.02
60) Fluorene-d10	15.522	176	203114	7.502	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	10996	2.032	ng/ul	0.00
73) Anthracene-d10	17.381	188	310928	7.421	ng/ul	0.00
81) Pyrene-d10	19.610	212	397514	8.403	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	291985	7.557	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 01:58:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

