

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010391.D
 Acq On : 18 May 2022 09:43
 Operator : CG/JU
 Sample : PB144853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	56	rVB	32623	60232	1.35%	0.140%
2	3.764	112	115	138	rBV	340112	718281	16.10%	1.671%
3	4.087	166	170	174	rVB5	8575	12322	0.28%	0.029%
4	7.057	668	675	690	rBV	608201	1057375	23.70%	2.459%
5	7.222	697	703	715	rBV	490680	823209	18.45%	1.915%
6	7.428	731	738	748	rBV	642744	1052419	23.59%	2.448%
7	7.893	810	817	830	rBV	516893	874524	19.60%	2.034%
8	8.604	931	938	954	rBV	809112	1380534	30.95%	3.211%
9	9.051	1007	1014	1029	rBV	651613	1160723	26.02%	2.700%
10	9.781	1128	1138	1154	rBV	534286	954536	21.40%	2.220%
11	10.316	1222	1229	1247	rBV	743088	1382324	30.99%	3.215%
12	10.698	1286	1294	1305	rBV	778118	1339378	30.03%	3.115%
13	10.834	1310	1317	1338	rBV	516453	1035467	23.21%	2.408%
14	12.298	1559	1566	1572	rBV3	11068	24389	0.55%	0.057%
15	13.939	1835	1845	1857	rBV	1575979	2261216	50.69%	5.259%
16	14.222	1885	1893	1911	rBV	1694629	2525955	56.62%	5.875%
17	14.528	1937	1945	1955	rBV	1290874	1896842	42.52%	4.412%
18	14.722	1972	1978	2000	rBV	499712	1019492	22.85%	2.371%
19	15.522	2107	2114	2128	rBV	2214070	3246606	72.78%	7.551%
20	15.639	2128	2134	2151	rVV	628895	989069	22.17%	2.300%
21	15.763	2151	2155	2163	rVB	28930	45503	1.02%	0.106%
22	16.304	2243	2247	2253	rBV6	7988	12119	0.27%	0.028%
23	16.492	2273	2279	2281	rBV6	2294	4645	0.10%	0.011%
24	16.957	2353	2358	2363	rBV9	5115	11742	0.26%	0.027%
25	17.280	2406	2413	2423	rBV	1636831	2357217	52.84%	5.483%
26	17.380	2423	2430	2453	rVB	2486729	3719035	83.37%	8.650%
27	18.239	2573	2576	2580	rBV6	2864	4670	0.10%	0.011%
28	18.751	2660	2663	2666	rBV5	3587	6208	0.14%	0.014%
29	19.192	2733	2738	2743	rBV2	31403	44498	1.00%	0.103%
30	19.263	2745	2750	2756	rBV2	27700	41565	0.93%	0.097%
31	19.545	2796	2798	2799	rBV2	6912	5767	0.13%	0.013%
32	19.610	2803	2809	2823	rVV	3352541	4460871	100.00%	10.376%
33	21.363	3102	3107	3120	rBV	1859055	2583110	57.91%	6.008%
34	23.633	3485	3493	3499	rBV2	1842130	3679615	82.49%	8.558%
35	23.792	3513	3520	3532	rVB2	1035313	2202450	49.37%	5.123%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010391.D
Acq On : 18 May 2022 09:43
Operator : CG/JU
Sample : PB144853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42993908

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010391.D
Acq On : 18 May 2022 09:43
Operator : CG/JU
Sample : PB144853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

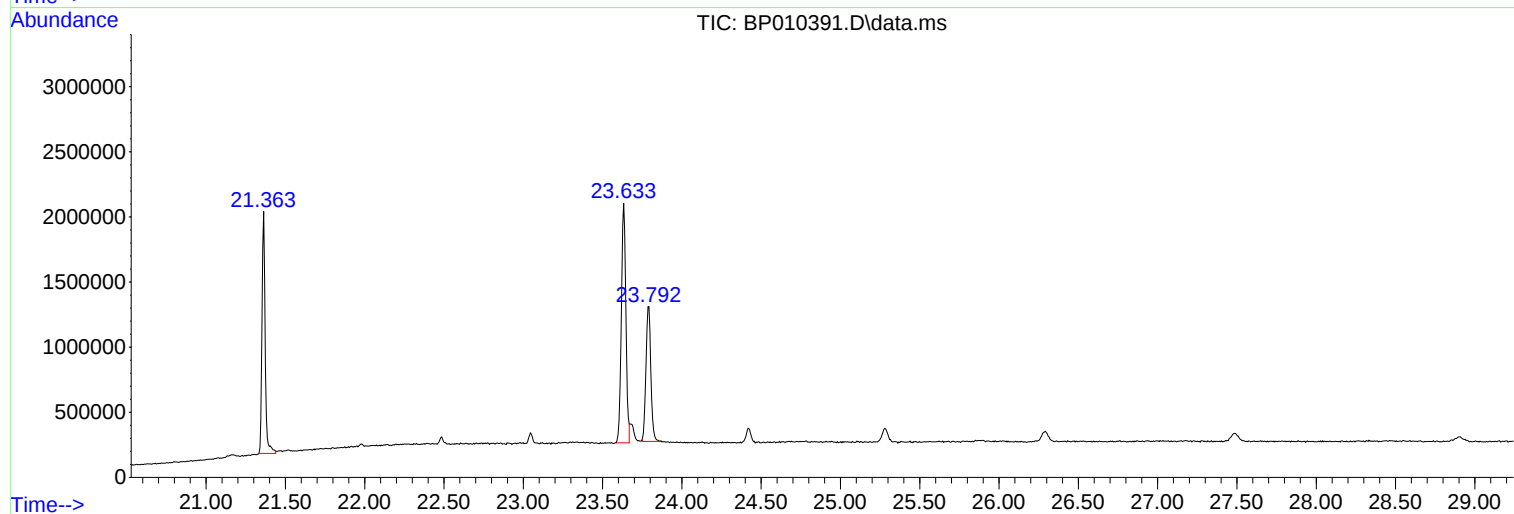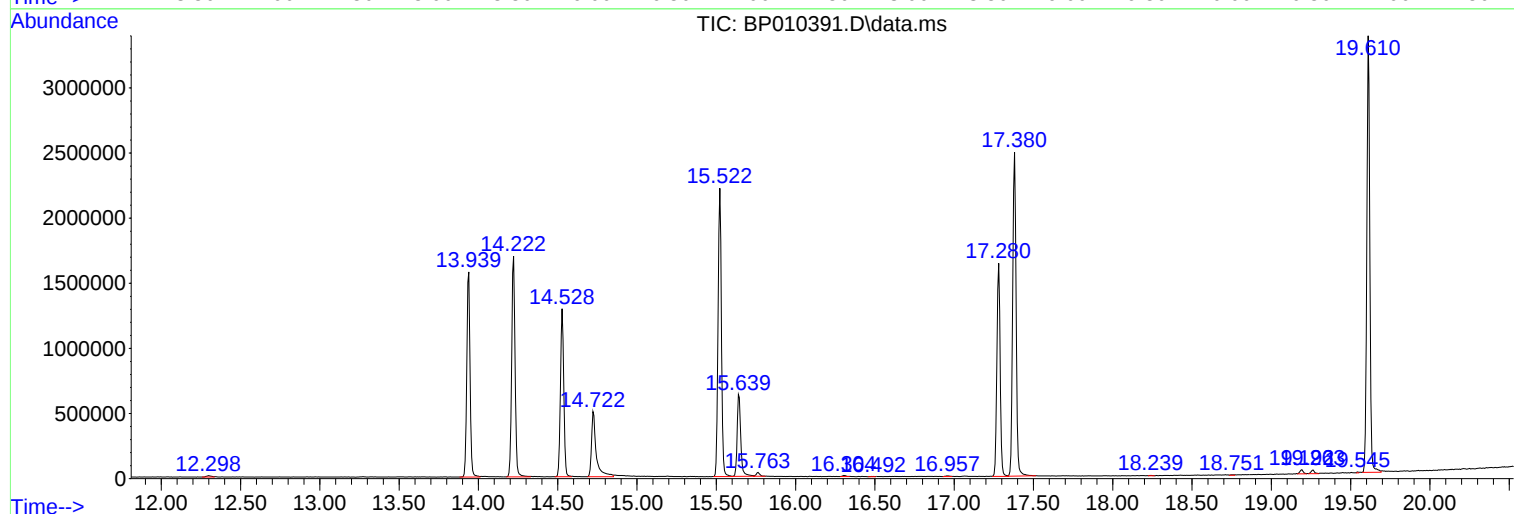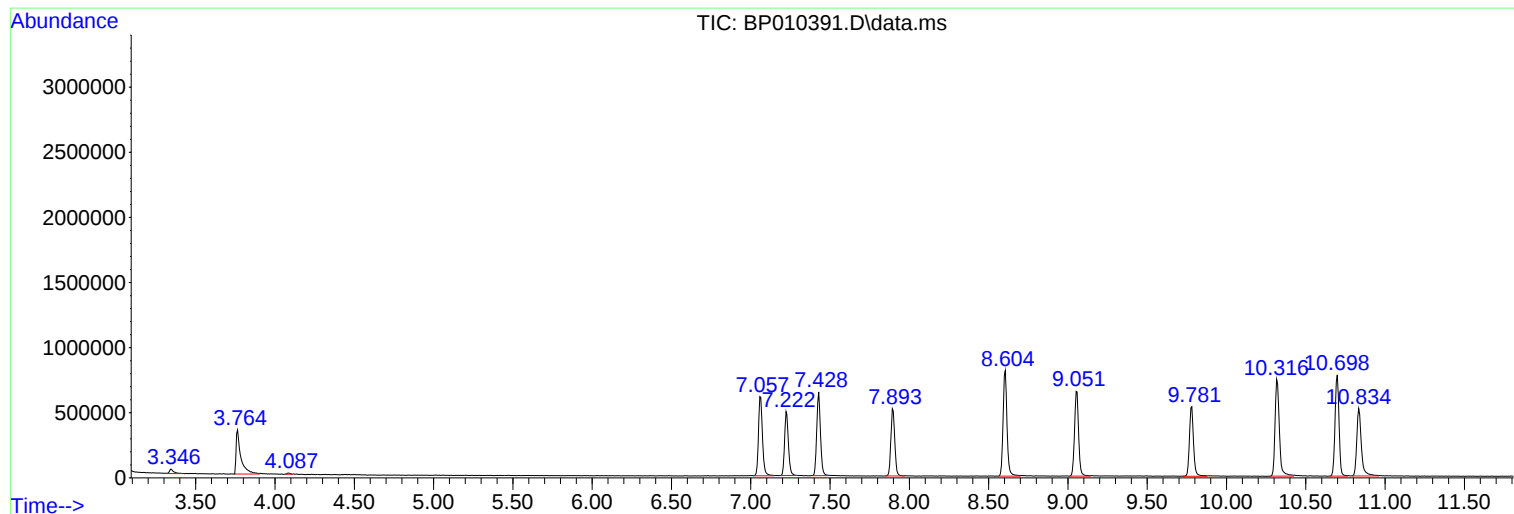

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010391.D
Acq On : 18 May 2022 09:43
Operator : CG/JU
Sample : PB144853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010391.D
Acq On : 18 May 2022 09:43
Operator : CG/JU
Sample : PB144853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------