

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	49	rBV5	11190	16087	0.64%	0.059%
2	3.793	116	120	127	rBV2	17677	39118	1.56%	0.144%
3	3.999	150	155	157	rBV5	9016	13721	0.55%	0.051%
4	4.081	166	169	175	rVB2	10782	16758	0.67%	0.062%
5	4.587	252	255	256	rBV3	3328	3314	0.13%	0.012%
6	4.999	321	325	337	rVB	34257	64585	2.57%	0.238%
7	5.446	398	401	404	rVB5	2646	2931	0.12%	0.011%
8	7.064	668	676	686	rBV	260219	473114	18.81%	1.743%
9	7.222	697	703	716	rBV	209330	353389	14.05%	1.302%
10	7.322	718	720	724	rVB4	2272	2714	0.11%	0.010%
11	7.428	731	738	749	rBV	258702	441222	17.54%	1.626%
12	7.522	749	754	758	rVB5	5344	8943	0.36%	0.033%
13	7.893	810	817	829	rBV	551926	929225	36.95%	3.424%
14	7.999	833	835	844	rVB10	3713	8830	0.35%	0.033%
15	8.328	888	891	893	rBV4	1858	2587	0.10%	0.010%
16	8.605	931	938	952	rBV	289444	517846	20.59%	1.908%
17	8.722	953	958	966	rVB	24121	43237	1.72%	0.159%
18	9.052	1007	1014	1025	rBV	269735	484909	19.28%	1.787%
19	9.369	1067	1068	1074	rVB6	2158	2920	0.12%	0.011%
20	9.781	1129	1138	1152	rBV	209412	396332	15.76%	1.460%
21	10.058	1183	1185	1188	rBV4	2331	2525	0.10%	0.009%
22	10.116	1188	1195	1207	rVV4	11007	35339	1.41%	0.130%
23	10.322	1223	1230	1244	rBV	324136	604399	24.03%	2.227%
24	10.505	1258	1261	1267	rVB8	1403	3029	0.12%	0.011%
25	10.699	1284	1294	1306	rBV	795433	1404548	55.85%	5.175%
26	10.834	1306	1317	1337	rVB	221155	491962	19.56%	1.813%
27	11.128	1365	1367	1372	rVB6	2372	3184	0.13%	0.012%
28	11.528	1431	1435	1437	rBV5	2457	3721	0.15%	0.014%
29	11.728	1464	1469	1471	rBV6	1953	3186	0.13%	0.012%
30	11.993	1510	1514	1520	rVB9	1816	3781	0.15%	0.014%
31	12.128	1533	1537	1544	rVB8	3783	7550	0.30%	0.028%
32	12.234	1548	1555	1559	rBV6	9008	19341	0.77%	0.071%
33	12.293	1561	1565	1568	rVB4	5292	6688	0.27%	0.025%
34	12.699	1628	1634	1638	rBV7	3472	5842	0.23%	0.022%
35	12.899	1663	1668	1674	rBV10	3188	7907	0.31%	0.029%
36	13.081	1694	1699	1702	rVB7	2600	3987	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.140	1705	1709	1717	rVB7	4327	8436	0.34%	0.031%
38	13.363	1743	1747	1754	rVB7	6678	12911	0.51%	0.048%
39	13.857	1826	1831	1837	rVB9	2001	4139	0.16%	0.015%
40	13.934	1837	1844	1856	rBV	815143	1199599	47.70%	4.420%
41	14.022	1856	1859	1862	rVV5	5467	8715	0.35%	0.032%
42	14.081	1865	1869	1875	rVB8	5366	10527	0.42%	0.039%
43	14.216	1882	1892	1906	rBV	787553	1232567	49.01%	4.541%
44	14.316	1908	1909	1913	rVB5	4078	3074	0.12%	0.011%
45	14.434	1923	1929	1934	rVB4	9290	13593	0.54%	0.050%
46	14.528	1938	1945	1957	rVV	1283810	1949641	77.52%	7.183%
47	14.616	1957	1960	1965	rVB7	2575	3771	0.15%	0.014%
48	14.734	1973	1980	2000	rBV	124562	333814	13.27%	1.230%
49	14.951	2013	2017	2021	rBV6	8966	14798	0.59%	0.055%
50	15.275	2067	2072	2076	rBV8	7320	11568	0.46%	0.043%
51	15.340	2076	2083	2086	rBV6	6396	9612	0.38%	0.035%
52	15.381	2087	2090	2094	rBV4	5168	6743	0.27%	0.025%
53	15.422	2094	2097	2105	rVB10	6034	11056	0.44%	0.041%
54	15.522	2107	2114	2127	rBV	1108209	1655149	65.81%	6.098%
55	15.640	2129	2134	2142	rBV	202036	319380	12.70%	1.177%
56	15.763	2150	2155	2164	rVB7	25214	53948	2.15%	0.199%
57	15.887	2173	2176	2180	rBV6	3306	4408	0.18%	0.016%
58	16.087	2207	2210	2215	rBV7	2957	5033	0.20%	0.019%
59	16.192	2225	2228	2229	rBV3	2680	2997	0.12%	0.011%
60	16.245	2231	2237	2239	rVV7	11862	18752	0.75%	0.069%
61	16.269	2239	2241	2245	rVV3	10558	14520	0.58%	0.053%
62	16.310	2245	2248	2253	rVB6	6052	9963	0.40%	0.037%
63	16.434	2261	2269	2272	rBV10	4373	9721	0.39%	0.036%
64	16.604	2294	2298	2301	rBV6	2073	2657	0.11%	0.010%
65	16.828	2331	2336	2340	rVB8	5391	9540	0.38%	0.035%
66	16.945	2351	2356	2357	rBV5	3077	4381	0.17%	0.016%
67	17.045	2367	2373	2376	rBV2	10358	17141	0.68%	0.063%
68	17.081	2376	2379	2386	rVB7	8334	18648	0.74%	0.069%
69	17.181	2394	2396	2398	rBV3	5640	5262	0.21%	0.019%
70	17.281	2403	2413	2423	rBV	1658256	2407360	95.73%	8.870%
71	17.375	2423	2429	2442	rVV	1223045	1857604	73.87%	6.844%
72	17.475	2443	2446	2451	rVB5	18956	28360	1.13%	0.104%
73	17.569	2460	2462	2468	rVB7	6571	8734	0.35%	0.032%
74	17.645	2471	2475	2476	rBV4	4806	5925	0.24%	0.022%
75	17.787	2495	2499	2503	rVB3	10272	12139	0.48%	0.045%
76	17.951	2523	2527	2531	rVB5	14111	19018	0.76%	0.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010397.D
 Acq On : 18 May 2022 13:05
 Operator : CG/JU
 Sample : N2766-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	17.998	2531	2535	2536	rBV4	2295	3076	0.12%	0.011%
78	18.110	2550	2554	2559	rVB6	11710	15025	0.60%	0.055%
79	18.163	2559	2563	2571	rBV2	57208	96483	3.84%	0.355%
80	18.234	2572	2575	2580	rVB	11934	17112	0.68%	0.063%
81	18.451	2609	2612	2616	rBV5	10350	15345	0.61%	0.057%
82	19.063	2713	2716	2720	rVB4	10399	12237	0.49%	0.045%
83	19.192	2734	2738	2744	rVB6	23619	34417	1.37%	0.127%
84	19.257	2746	2749	2752	rBV3	14931	21225	0.84%	0.078%
85	19.398	2769	2773	2777	rBV6	21089	32132	1.28%	0.118%
86	19.610	2803	2809	2816	rBV	1723853	2326210	92.50%	8.571%
87	20.504	2957	2961	2968	rBV	133829	177567	7.06%	0.654%
88	21.075	3054	3058	3063	rBV	142620	222325	8.84%	0.819%
89	21.363	3102	3107	3119	rBV	1864672	2514859	100.00%	9.266%
90	23.051	3390	3394	3398	rVB3	87433	134742	5.36%	0.496%
91	23.633	3487	3493	3499	rBV	836280	1631359	64.87%	6.011%
92	23.792	3513	3520	3537	rVB	1001364	2132469	84.79%	7.857%




Sum of corrected areas: 27140558

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

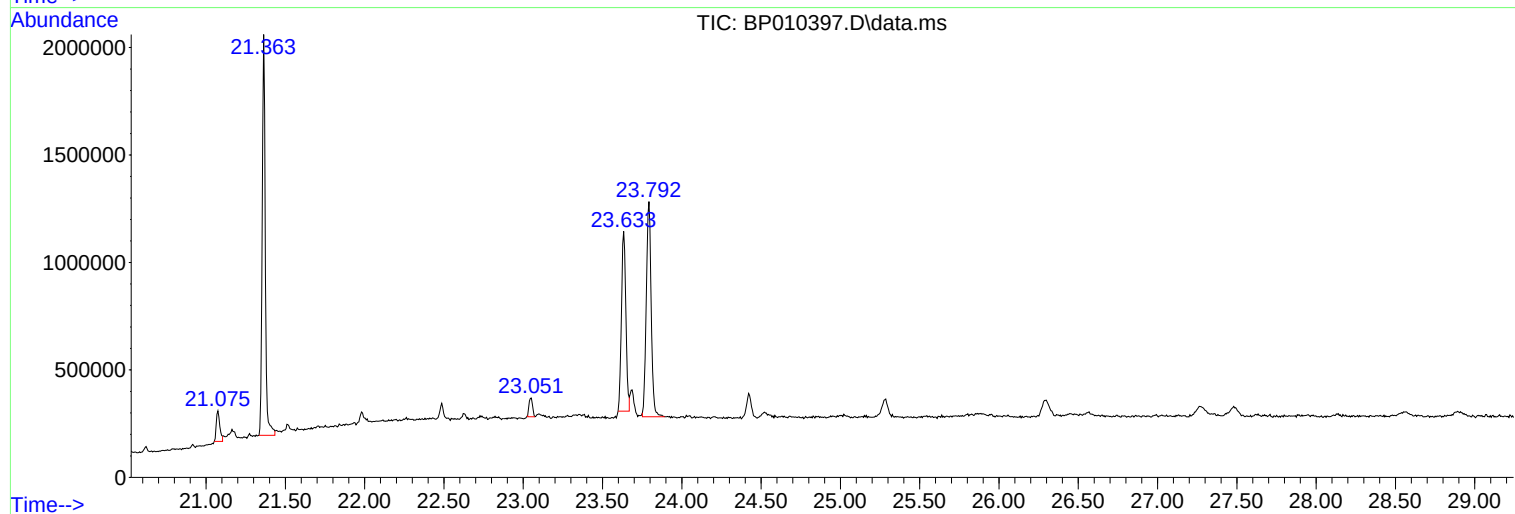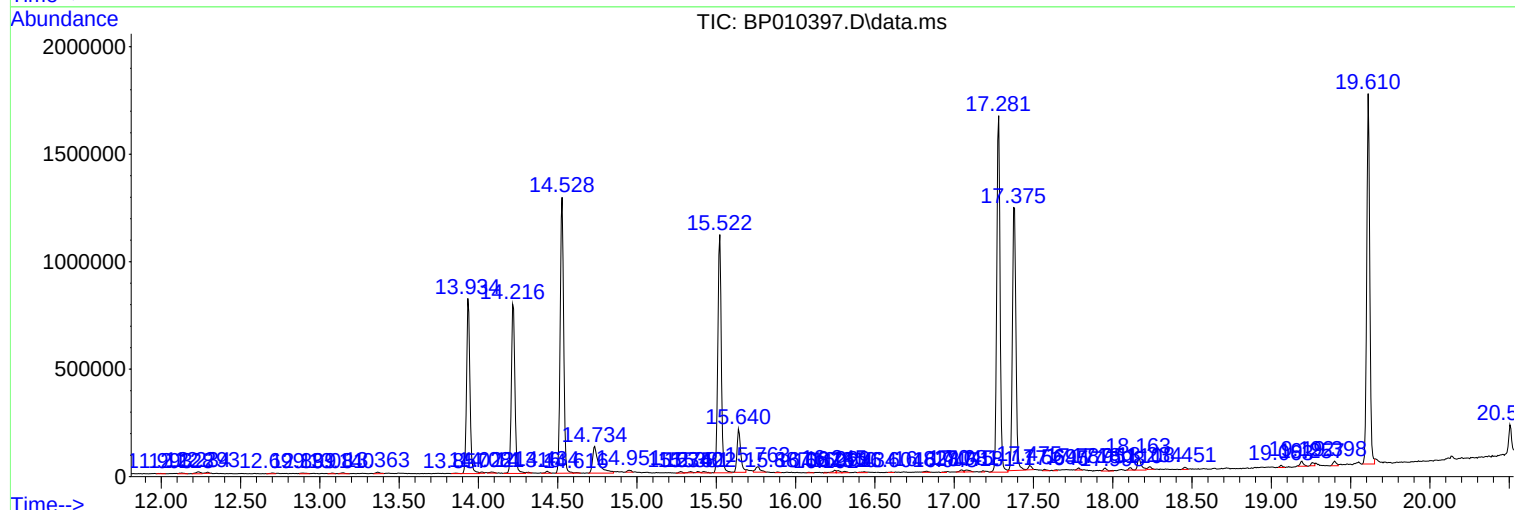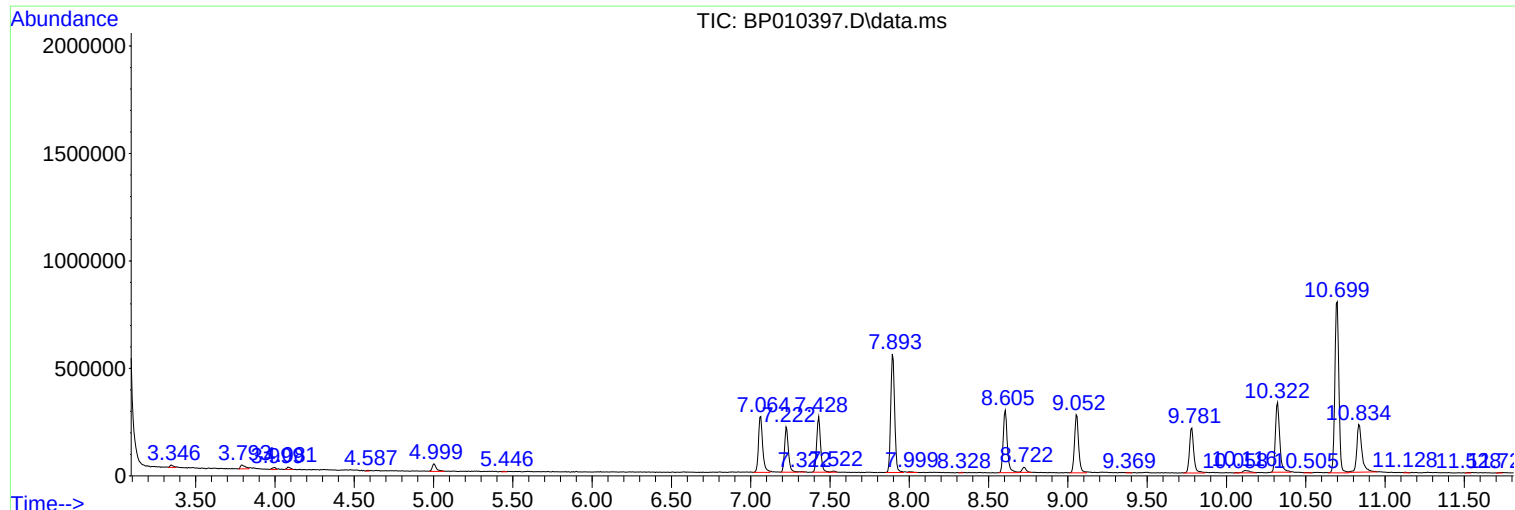

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010397.D
Acq On : 18 May 2022 13:05
Operator : CG/JU
Sample : N2766-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc