

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	42	44	52	rVB5	8801	11820	0.49%	0.063%
2	3.793	118	120	130	rBV	14717	30444	1.26%	0.161%
3	4.087	166	170	175	rVB2	12230	19186	0.79%	0.102%
4	4.922	311	312	316	rVB4	3266	3368	0.14%	0.018%
5	4.964	316	319	322	rBV5	2632	4056	0.17%	0.021%
6	5.005	322	326	335	rVB	19693	31718	1.31%	0.168%
7	5.269	366	371	376	rBV9	2202	5600	0.23%	0.030%
8	5.405	393	394	400	rVB6	2725	3549	0.15%	0.019%
9	5.599	422	427	433	rBV10	2194	4862	0.20%	0.026%
10	5.916	476	481	484	rVV6	3777	7658	0.32%	0.041%
11	6.175	523	525	529	rVB4	2789	3679	0.15%	0.019%
12	6.781	621	628	630	rBV8	2043	4407	0.18%	0.023%
13	6.893	644	647	654	rVB8	1860	3636	0.15%	0.019%
14	6.952	654	657	660	rBV4	2121	3120	0.13%	0.017%
15	7.063	668	676	688	rBV	116755	225486	9.30%	1.194%
16	7.228	698	704	716	rVV	109999	194757	8.03%	1.031%
17	7.316	716	719	725	rVB3	3676	7487	0.31%	0.040%
18	7.428	730	738	750	rVV	138507	237646	9.80%	1.259%
19	7.528	750	755	764	rVB9	7779	14250	0.59%	0.075%
20	7.893	810	817	827	rBV	526035	882749	36.40%	4.675%
21	7.975	827	831	834	rVB6	3890	5730	0.24%	0.030%
22	8.457	910	913	919	rVB7	1821	3097	0.13%	0.016%
23	8.605	932	938	946	rBV2	154840	279422	11.52%	1.480%
24	8.728	954	959	964	rVB2	14109	22837	0.94%	0.121%
25	9.052	1007	1014	1024	rBV	135872	253595	10.46%	1.343%
26	9.128	1025	1027	1032	rVB4	6355	9276	0.38%	0.049%
27	9.222	1041	1043	1045	rBV3	2876	3136	0.13%	0.017%
28	9.499	1087	1090	1093	rVB5	2758	4053	0.17%	0.021%
29	9.546	1093	1098	1105	rVB5	2077	4605	0.19%	0.024%
30	9.781	1129	1138	1148	rBV2	110444	198409	8.18%	1.051%
31	10.052	1178	1184	1187	rVB8	1975	3422	0.14%	0.018%
32	10.152	1199	1201	1205	rVB4	3162	3232	0.13%	0.017%
33	10.234	1212	1215	1220	rBV7	1882	3323	0.14%	0.018%
34	10.322	1220	1230	1247	rBV	143508	304516	12.56%	1.613%
35	10.699	1286	1294	1308	rBV	753811	1344947	55.46%	7.123%
36	10.840	1311	1318	1338	rVV	131076	307537	12.68%	1.629%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	11.075	1355	1358	1363	rVB6	2063	3456	0.14%	0.018%
38	11.187	1370	1377	1378	rBV6	4977	8410	0.35%	0.045%
39	11.381	1407	1410	1412	rVV4	1990	3092	0.13%	0.016%
40	11.404	1412	1414	1420	rVB6	2680	3590	0.15%	0.019%
41	11.734	1465	1470	1474	rVV5	5673	9779	0.40%	0.052%
42	11.887	1494	1496	1503	rVB7	3121	5475	0.23%	0.029%
43	11.993	1509	1514	1516	rBV6	2609	4842	0.20%	0.026%
44	12.128	1532	1537	1542	rBV4	11919	19310	0.80%	0.102%
45	12.304	1562	1567	1571	rVB8	3243	5748	0.24%	0.030%
46	12.504	1597	1601	1604	rBV6	2678	3538	0.15%	0.019%
47	12.810	1648	1653	1656	rBV7	2396	3966	0.16%	0.021%
48	12.969	1677	1680	1686	rVB8	2009	3380	0.14%	0.018%
49	13.075	1695	1698	1703	rVB7	7235	11342	0.47%	0.060%
50	13.134	1703	1708	1713	rBV9	3854	7376	0.30%	0.039%
51	13.363	1742	1747	1754	rBV2	16969	27434	1.13%	0.145%
52	13.428	1754	1758	1766	rVV9	7434	15739	0.65%	0.083%
53	13.493	1768	1769	1772	rVV3	2878	3357	0.14%	0.018%
54	13.522	1772	1774	1778	rVV5	2737	3788	0.16%	0.020%
55	13.593	1782	1786	1791	rVB8	2706	4738	0.20%	0.025%
56	13.940	1838	1845	1855	rBV	347679	530702	21.89%	2.811%
57	14.022	1855	1859	1863	rVB4	11084	16666	0.69%	0.088%
58	14.145	1877	1880	1885	rVB6	2856	4137	0.17%	0.022%
59	14.222	1885	1893	1902	rBV	363432	565830	23.33%	2.997%
60	14.434	1925	1929	1935	rVB	18272	24079	0.99%	0.128%
61	14.528	1937	1945	1957	rVV	1238571	1873473	77.26%	9.922%
62	14.622	1959	1961	1965	rVB5	3403	3939	0.16%	0.021%
63	14.745	1976	1982	1991	rBV5	22702	70485	2.91%	0.373%
64	14.875	2001	2004	2008	rVB6	3346	5556	0.23%	0.029%
65	14.945	2012	2016	2017	rBV4	4981	5098	0.21%	0.027%
66	15.057	2032	2035	2042	rVB8	5264	9203	0.38%	0.049%
67	15.234	2062	2065	2069	rBV6	3115	3937	0.16%	0.021%
68	15.322	2077	2080	2081	rBV3	4029	3999	0.16%	0.021%
69	15.387	2087	2091	2095	rVB2	15388	20192	0.83%	0.107%
70	15.522	2107	2114	2128	rBV	498324	778436	32.10%	4.123%
71	15.645	2130	2135	2148	rVV2	47914	88016	3.63%	0.466%
72	15.763	2152	2155	2157	rVV4	6492	8635	0.36%	0.046%
73	15.792	2157	2160	2167	rVB4	10109	14895	0.61%	0.079%
74	15.957	2182	2188	2190	rBV7	3014	5803	0.24%	0.031%
75	16.010	2195	2197	2201	rVB4	5130	5062	0.21%	0.027%
76	16.251	2234	2238	2239	rBV3	15718	20037	0.83%	0.106%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010398.D
 Acq On : 18 May 2022 13:39
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.275	2239	2242	2245	rVB3	15670	20899	0.86%	0.111%
78	16.369	2255	2258	2260	rBV4	2404	3257	0.13%	0.017%
79	16.592	2293	2296	2299	rBV5	3112	3575	0.15%	0.019%
80	16.828	2330	2336	2337	rBV5	3740	6456	0.27%	0.034%
81	17.045	2369	2373	2378	rBV4	12788	18358	0.76%	0.097%
82	17.098	2379	2382	2387	rVB5	11075	15778	0.65%	0.084%
83	17.281	2406	2413	2423	rBV	1561092	2285232	94.24%	12.103%
84	17.381	2423	2430	2442	rVV2	529862	823648	33.97%	4.362%
85	17.481	2442	2447	2451	rVB8	7673	12883	0.53%	0.068%
86	17.669	2476	2479	2483	rBV6	7085	11279	0.47%	0.060%
87	17.786	2495	2499	2505	rVB4	13989	18010	0.74%	0.095%
88	17.951	2523	2527	2533	rVB	49357	60174	2.48%	0.319%
89	18.163	2559	2563	2568	rBV5	36824	61698	2.54%	0.327%
90	18.457	2609	2613	2617	rBV2	13655	18459	0.76%	0.098%
91	18.998	2701	2705	2710	rBV7	21331	39917	1.65%	0.211%
92	19.080	2713	2719	2724	rVB3	91970	120033	4.95%	0.636%
93	19.210	2732	2741	2747	rBV3	45999	92551	3.82%	0.490%
94	19.304	2754	2757	2762	rVB3	30846	37941	1.56%	0.201%
95	19.610	2803	2809	2823	rBV	738073	1072905	44.24%	5.682%
96	20.504	2959	2961	2968	rVB3	28074	26644	1.10%	0.141%
97	21.069	3053	3057	3066	rBV2	169502	323203	13.33%	1.712%
98	21.363	3102	3107	3122	rBV	1746341	2424924	100.00%	12.843%
99	23.633	3487	3493	3498	rBV2	363162	709396	29.25%	3.757%
100	23.792	3513	3520	3531	rVB2	930689	2016954	83.18%	10.682%




Sum of corrected areas: 18881329

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

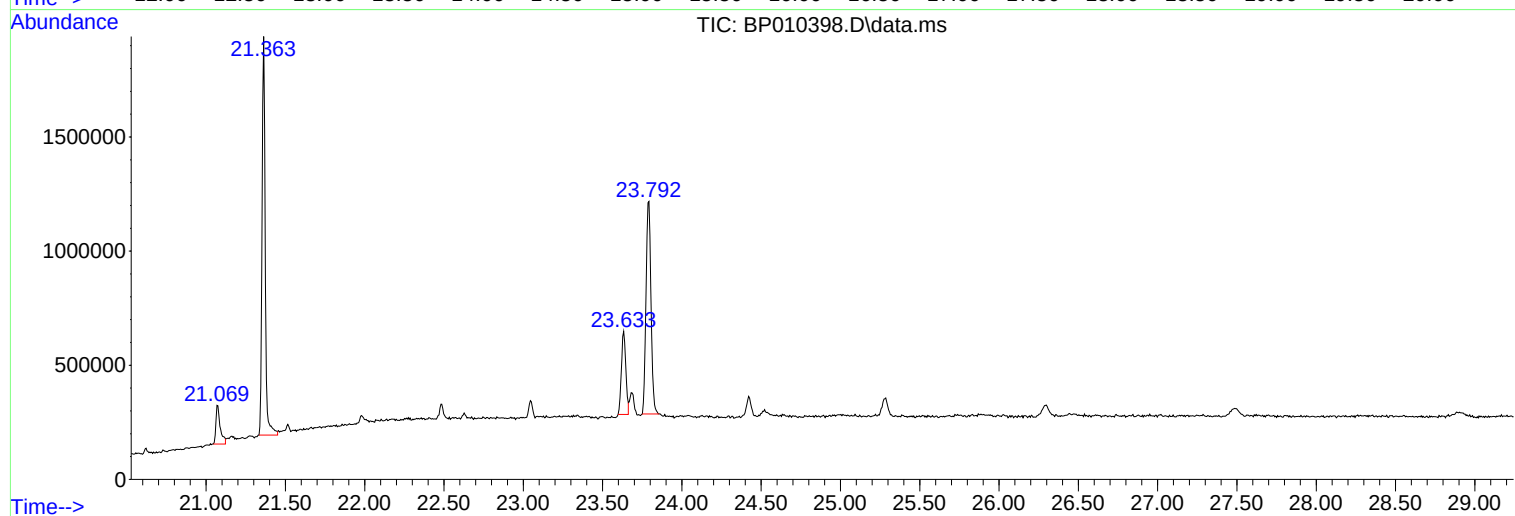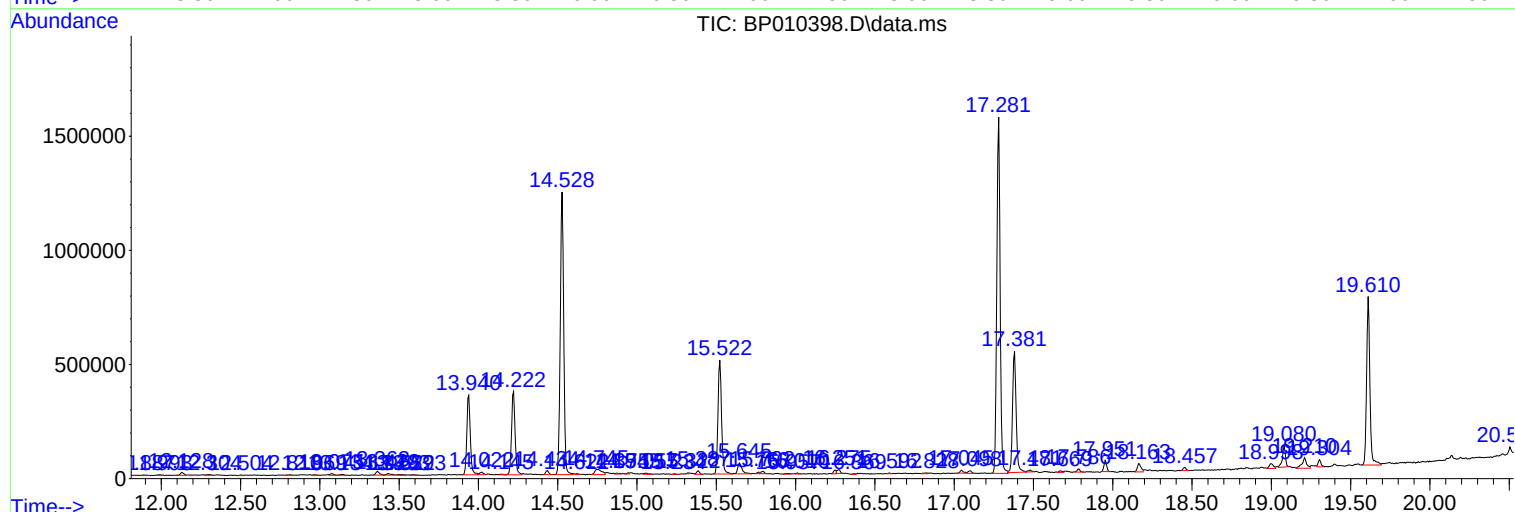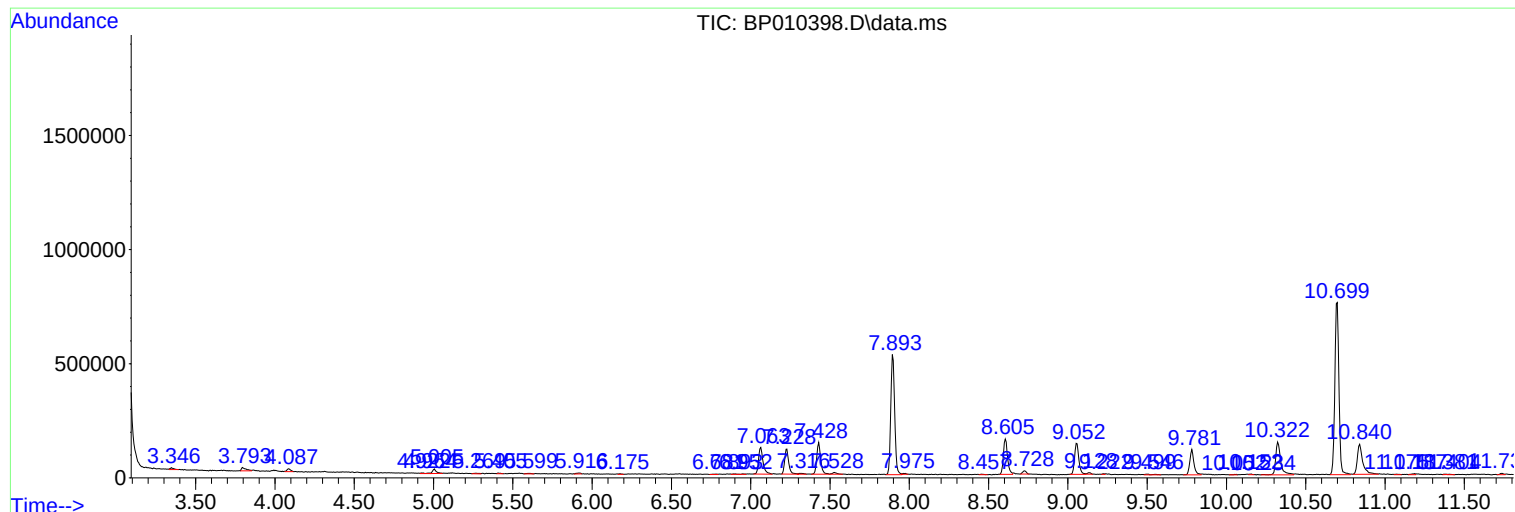

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.069 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.069	2.67 ng/ul	323203	Chrysene-d12	21.363

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	95
2			1-Docosene	308	C22H44	001599-67-3	94
3			Cyclopentadecane	210	C15H30	000295-48-7	93
4			1-Octadecene	252	C18H36	000112-88-9	92
5			n-Tetracosanol-1	354	C24H50O	000506-51-4	91

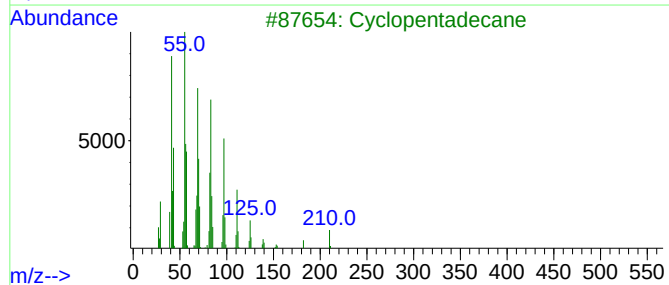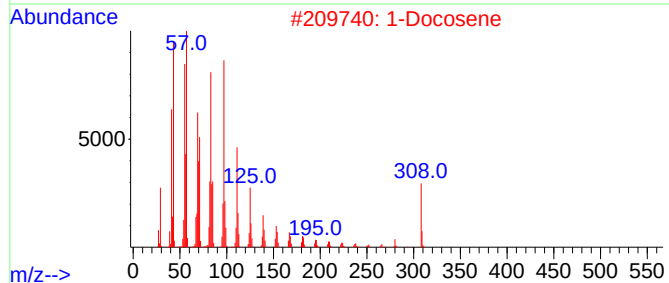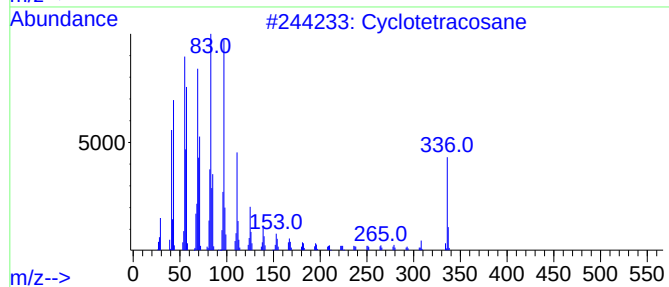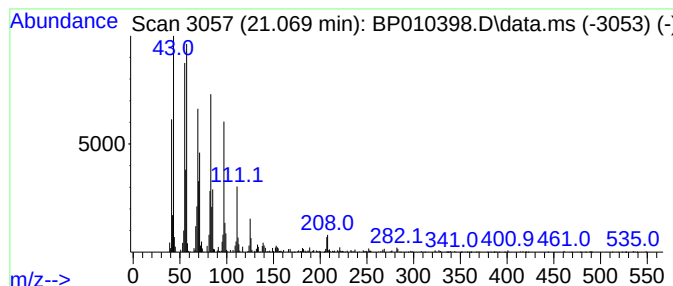

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010398.D
Acq On : 18 May 2022 13:39
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.069	2.7	ng/u1	323203	5	21.363	2424920	20.0