

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010400.D
 Acq On : 18 May 2022 14:47
 Operator : CG/JU
 Sample : N2766-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	49	rVB	17869	24299	0.91%	0.078%
2	3.693	101	103	107	rVB2	9104	9700	0.36%	0.031%
3	3.775	114	117	130	rBV	44012	104496	3.93%	0.334%
4	3.993	151	154	159	rVB4	10037	14246	0.54%	0.046%
5	4.087	166	170	174	rBV3	12196	19929	0.75%	0.064%
6	4.634	259	263	264	rBV3	2829	2841	0.11%	0.009%
7	4.811	291	293	298	rVB6	3412	5198	0.20%	0.017%
8	4.999	320	325	338	rVB	34747	62717	2.36%	0.200%
9	5.534	413	416	418	rBV3	3213	2974	0.11%	0.010%
10	5.599	425	427	433	rVB7	1805	3046	0.11%	0.010%
11	6.205	526	530	534	rBV7	1730	2844	0.11%	0.009%
12	6.887	641	646	649	rBV7	2242	3349	0.13%	0.011%
13	7.063	668	676	692	rBV2	334025	780152	29.31%	2.493%
14	7.222	694	703	715	rVV	275070	472342	17.74%	1.510%
15	7.428	730	738	751	rBV	346631	588115	22.09%	1.880%
16	7.528	751	755	760	rVV7	9311	16027	0.60%	0.051%
17	7.587	762	765	769	rVB6	1983	3325	0.12%	0.011%
18	7.893	808	817	828	rBV	533835	909044	34.15%	2.905%
19	8.604	929	938	947	rBV	441112	752533	28.27%	2.405%
20	8.722	953	958	966	rVB2	30331	52946	1.99%	0.169%
21	9.051	1007	1014	1024	rBV	350852	620833	23.32%	1.984%
22	9.493	1087	1089	1092	rVB3	2796	2714	0.10%	0.009%
23	9.781	1129	1138	1151	rBV	253096	461410	17.33%	1.475%
24	9.875	1151	1154	1155	rVV3	4818	5801	0.22%	0.019%
25	9.904	1158	1159	1166	rVB7	3559	5462	0.21%	0.017%
26	10.146	1192	1200	1205	rBV10	5897	10766	0.40%	0.034%
27	10.316	1223	1229	1248	rBV	409160	752634	28.27%	2.405%
28	10.522	1260	1264	1266	rBV5	2452	2978	0.11%	0.010%
29	10.622	1276	1281	1286	rVB2	19075	31674	1.19%	0.101%
30	10.693	1286	1293	1309	rVB	789609	1369901	51.46%	4.378%
31	10.834	1309	1317	1335	rBV	369932	750551	28.20%	2.399%
32	11.063	1351	1356	1362	rVB4	7197	14183	0.53%	0.045%
33	11.169	1371	1374	1378	rVB6	2095	2897	0.11%	0.009%
34	11.228	1380	1384	1385	rBV4	3309	3666	0.14%	0.012%
35	11.322	1395	1400	1405	rVB9	3336	6426	0.24%	0.021%
36	11.540	1432	1437	1446	rVB9	3897	9229	0.35%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010400.D
 Acq On : 18 May 2022 14:47
 Operator : CG/JU
 Sample : N2766-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	11.734	1467	1470	1476	rVB6	4504	6381	0.24%	0.020%
38	12.040	1516	1522	1531	rVB2	30163	50362	1.89%	0.161%
39	12.134	1531	1538	1543	rVV7	6242	11169	0.42%	0.036%
40	12.198	1543	1549	1557	rVV2	33969	72542	2.73%	0.232%
41	12.287	1557	1564	1572	rVV6	10093	23657	0.89%	0.076%
42	12.357	1572	1576	1583	rVB10	3935	7792	0.29%	0.025%
43	12.434	1586	1589	1594	rVB7	2451	4262	0.16%	0.014%
44	12.610	1617	1619	1623	rBV5	2751	3254	0.12%	0.010%
45	12.757	1642	1644	1648	rVB5	2335	2724	0.10%	0.009%
46	12.822	1649	1655	1660	rVB10	3083	6722	0.25%	0.021%
47	12.892	1663	1667	1671	rVV6	6997	10619	0.40%	0.034%
48	12.934	1673	1674	1682	rVV7	4035	7199	0.27%	0.023%
49	13.028	1686	1690	1693	rVV6	2919	5049	0.19%	0.016%
50	13.075	1694	1698	1704	rVV2	10338	18304	0.69%	0.058%
51	13.139	1704	1709	1715	rVB8	7687	14647	0.55%	0.047%
52	13.363	1740	1747	1753	rBV5	13648	28655	1.08%	0.092%
53	13.592	1784	1786	1790	rVB5	2003	2804	0.11%	0.009%
54	13.698	1802	1804	1806	rBV3	3013	3452	0.13%	0.011%
55	13.739	1808	1811	1813	rBV4	3352	3190	0.12%	0.010%
56	13.804	1819	1822	1824	rBV4	3048	4191	0.16%	0.013%
57	13.851	1826	1830	1831	rBV4	3998	3731	0.14%	0.012%
58	13.934	1838	1844	1853	rBV	909036	1291591	48.52%	4.128%
59	14.016	1855	1858	1863	rVV2	20886	31675	1.19%	0.101%
60	14.057	1863	1865	1872	rVB8	9092	12431	0.47%	0.040%
61	14.222	1883	1893	1904	rBV	930379	1436390	53.96%	4.590%
62	14.363	1913	1917	1924	rVB7	7993	15446	0.58%	0.049%
63	14.434	1924	1929	1935	rVB	28628	41115	1.54%	0.131%
64	14.528	1935	1945	1955	rBV	1292664	1939964	72.88%	6.200%
65	14.734	1974	1980	1992	rBV	72618	191308	7.19%	0.611%
66	14.939	2011	2015	2020	rBV7	15413	32332	1.21%	0.103%
67	15.057	2031	2035	2039	rVB5	20327	30338	1.14%	0.097%
68	15.116	2043	2045	2048	rBV4	4517	5299	0.20%	0.017%
69	15.328	2076	2081	2087	rBV5	15798	29057	1.09%	0.093%
70	15.381	2087	2090	2095	rVB2	38255	48164	1.81%	0.154%
71	15.522	2108	2114	2121	rBV	1292718	1877130	70.52%	5.999%
72	15.639	2130	2134	2150	rVB	86836	167724	6.30%	0.536%
73	15.792	2151	2160	2166	rVV2	57858	114497	4.30%	0.366%
74	15.886	2172	2176	2182	rVB8	13357	19825	0.74%	0.063%
75	15.945	2182	2186	2191	rBV6	14712	27570	1.04%	0.088%
76	16.004	2192	2196	2203	rVB7	17265	24365	0.92%	0.078%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
 Data File : BP010400.D
 Acq On : 18 May 2022 14:47
 Operator : CG/JU
 Sample : N2766-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.092	2207	2211	2215	rBV7	6892	13991	0.53%	0.045%
78	16.181	2222	2226	2230	rBV7	11009	20372	0.77%	0.065%
79	16.245	2233	2237	2239	rBV2	76428	103849	3.90%	0.332%
80	16.269	2239	2241	2246	rVB	85226	113015	4.25%	0.361%
81	16.622	2299	2301	2304	rBV4	7057	9078	0.34%	0.029%
82	16.651	2304	2306	2310	rVB2	14326	15842	0.60%	0.051%
83	17.045	2369	2373	2376	rBV	47354	55425	2.08%	0.177%
84	17.098	2377	2382	2387	rVB	149494	210413	7.90%	0.672%
85	17.280	2407	2413	2422	rBV	1531723	2317737	87.07%	7.407%
86	17.380	2423	2430	2440	rVV2	1364862	2122979	79.75%	6.785%
87	17.475	2443	2446	2452	rVV8	24152	36238	1.36%	0.116%
88	17.704	2482	2485	2490	rBV	26307	40765	1.53%	0.130%
89	17.780	2495	2498	2504	rVB	51499	64744	2.43%	0.207%
90	17.875	2509	2514	2521	rVB6	21873	56052	2.11%	0.179%
91	18.163	2560	2563	2568	rBV4	54219	75892	2.85%	0.243%
92	18.451	2609	2612	2616	rBV	33939	45424	1.71%	0.145%
93	19.610	2803	2809	2814	rBV	2064853	2661998	100.00%	8.507%
94	20.621	2978	2981	2983	rVB2	53327	54880	2.06%	0.175%
95	21.068	3054	3057	3068	rVB	284628	416828	15.66%	1.332%
96	21.363	3102	3107	3121	rVB	1832399	2565978	96.39%	8.200%
97	21.510	3130	3132	3136	rVB3	96560	104126	3.91%	0.333%
98	23.039	3390	3392	3398	rVB	137007	195963	7.36%	0.626%
99	23.627	3486	3492	3498	rBV2	1091698	2177255	81.79%	6.958%
100	23.786	3513	3519	3530	rVB2	1128196	2303788	86.54%	7.363%




Sum of corrected areas: 31290807

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010400.D
Acq On : 18 May 2022 14:47
Operator : CG/JU
Sample : N2766-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

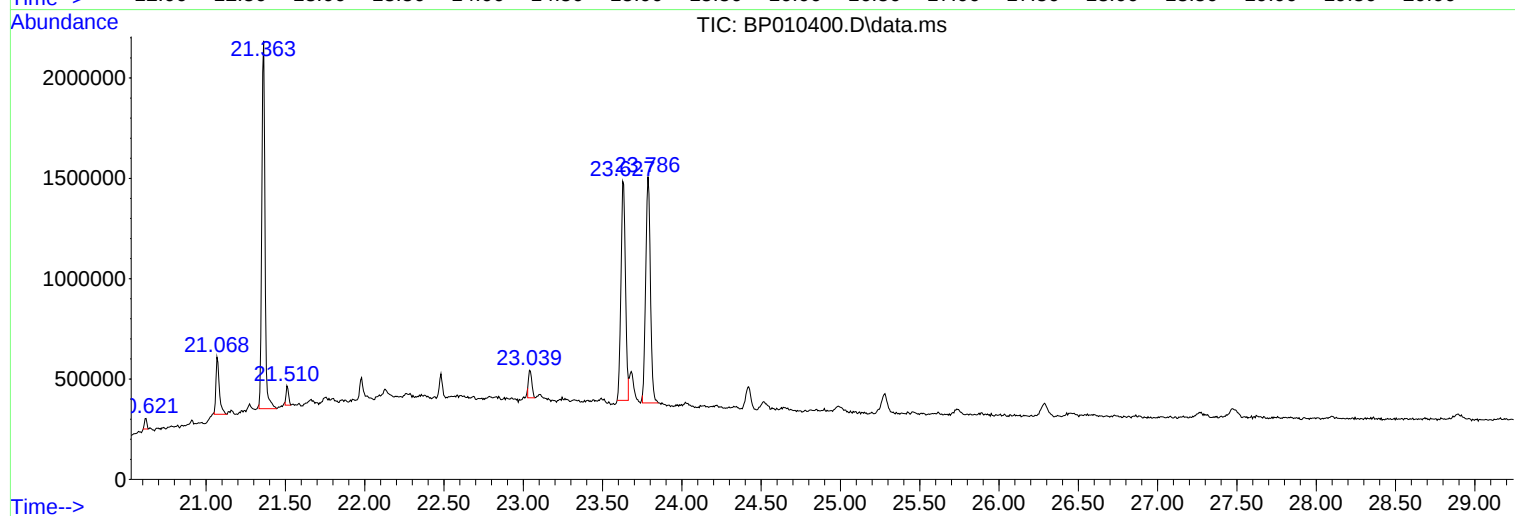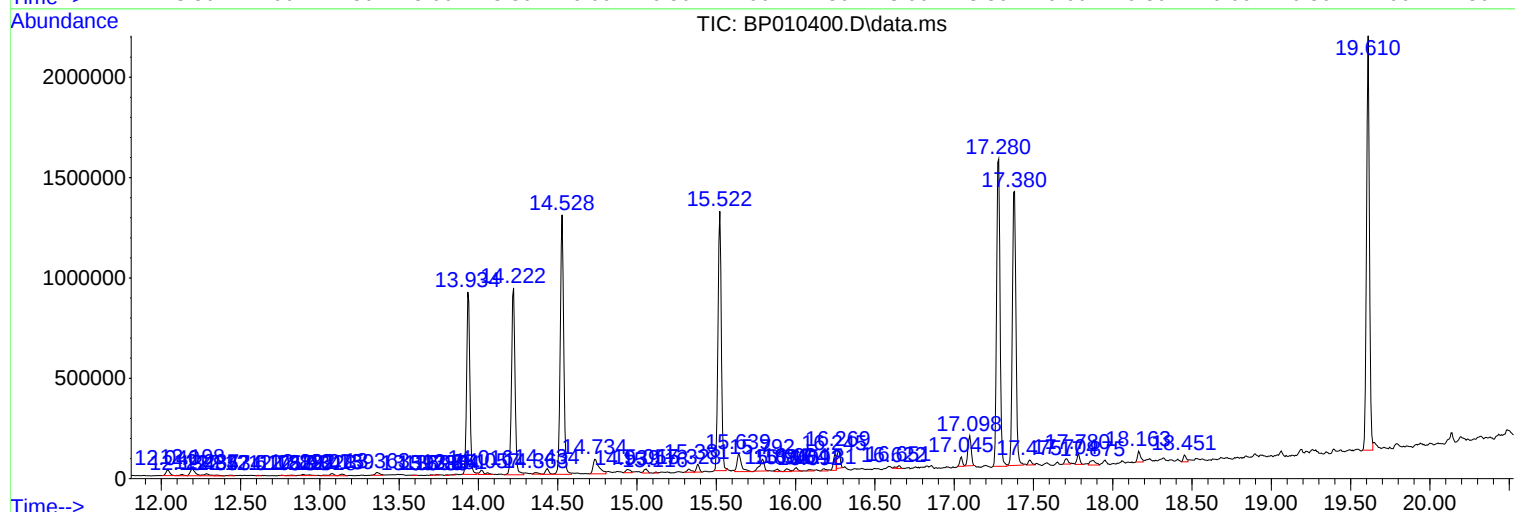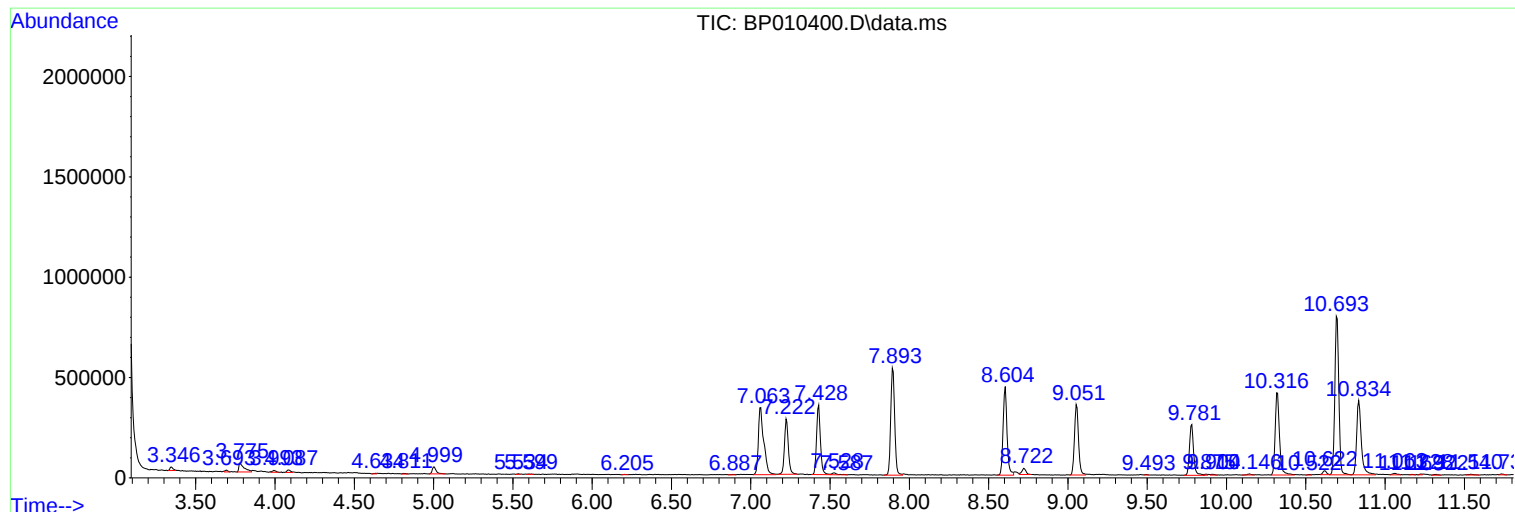

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010400.D
Acq On : 18 May 2022 14:47
Operator : CG/JU
Sample : N2766-15
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EW4G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.069	3.25 ng/ul	416828	Chrysene-d12		21.363	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Docosene		308	C22H44	001599-67-3	95
2	1-Triacontanol		438	C30H62O	000593-50-0	93
3	17-Pentatriacontene		491	C35H70	006971-40-0	91
4	Oxalic acid, octadecyl propyl ester		384	C23H44O4	1000309-27-0	91
5	Hexacosyl heptafluorobutyrate		578	C30H53F7O2	1000351-83-3	91

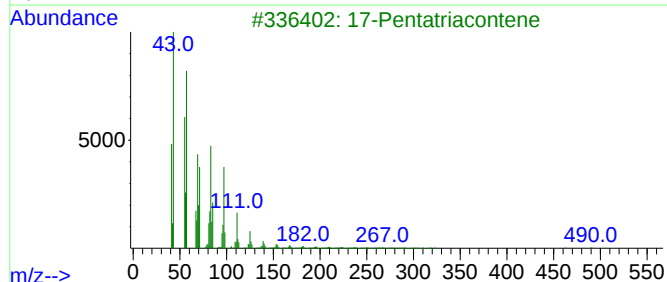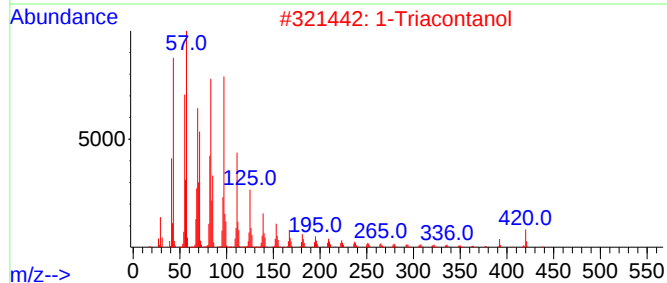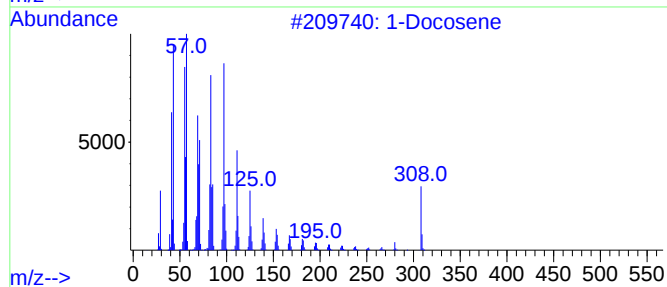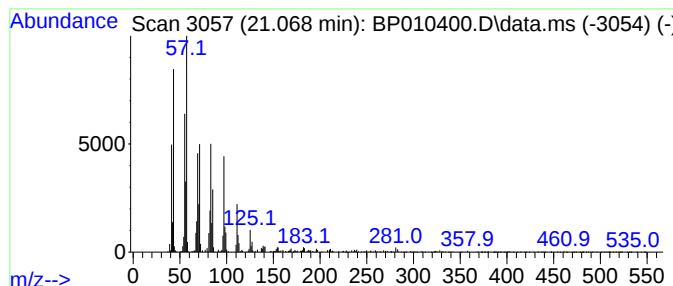

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051822\
Data File : BP010400.D
Acq On : 18 May 2022 14:47
Operator : CG/JU
Sample : N2766-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.069	3.3	ng/u1	416828	5	21.363	2565980	20.0