



2-Nitrophenol

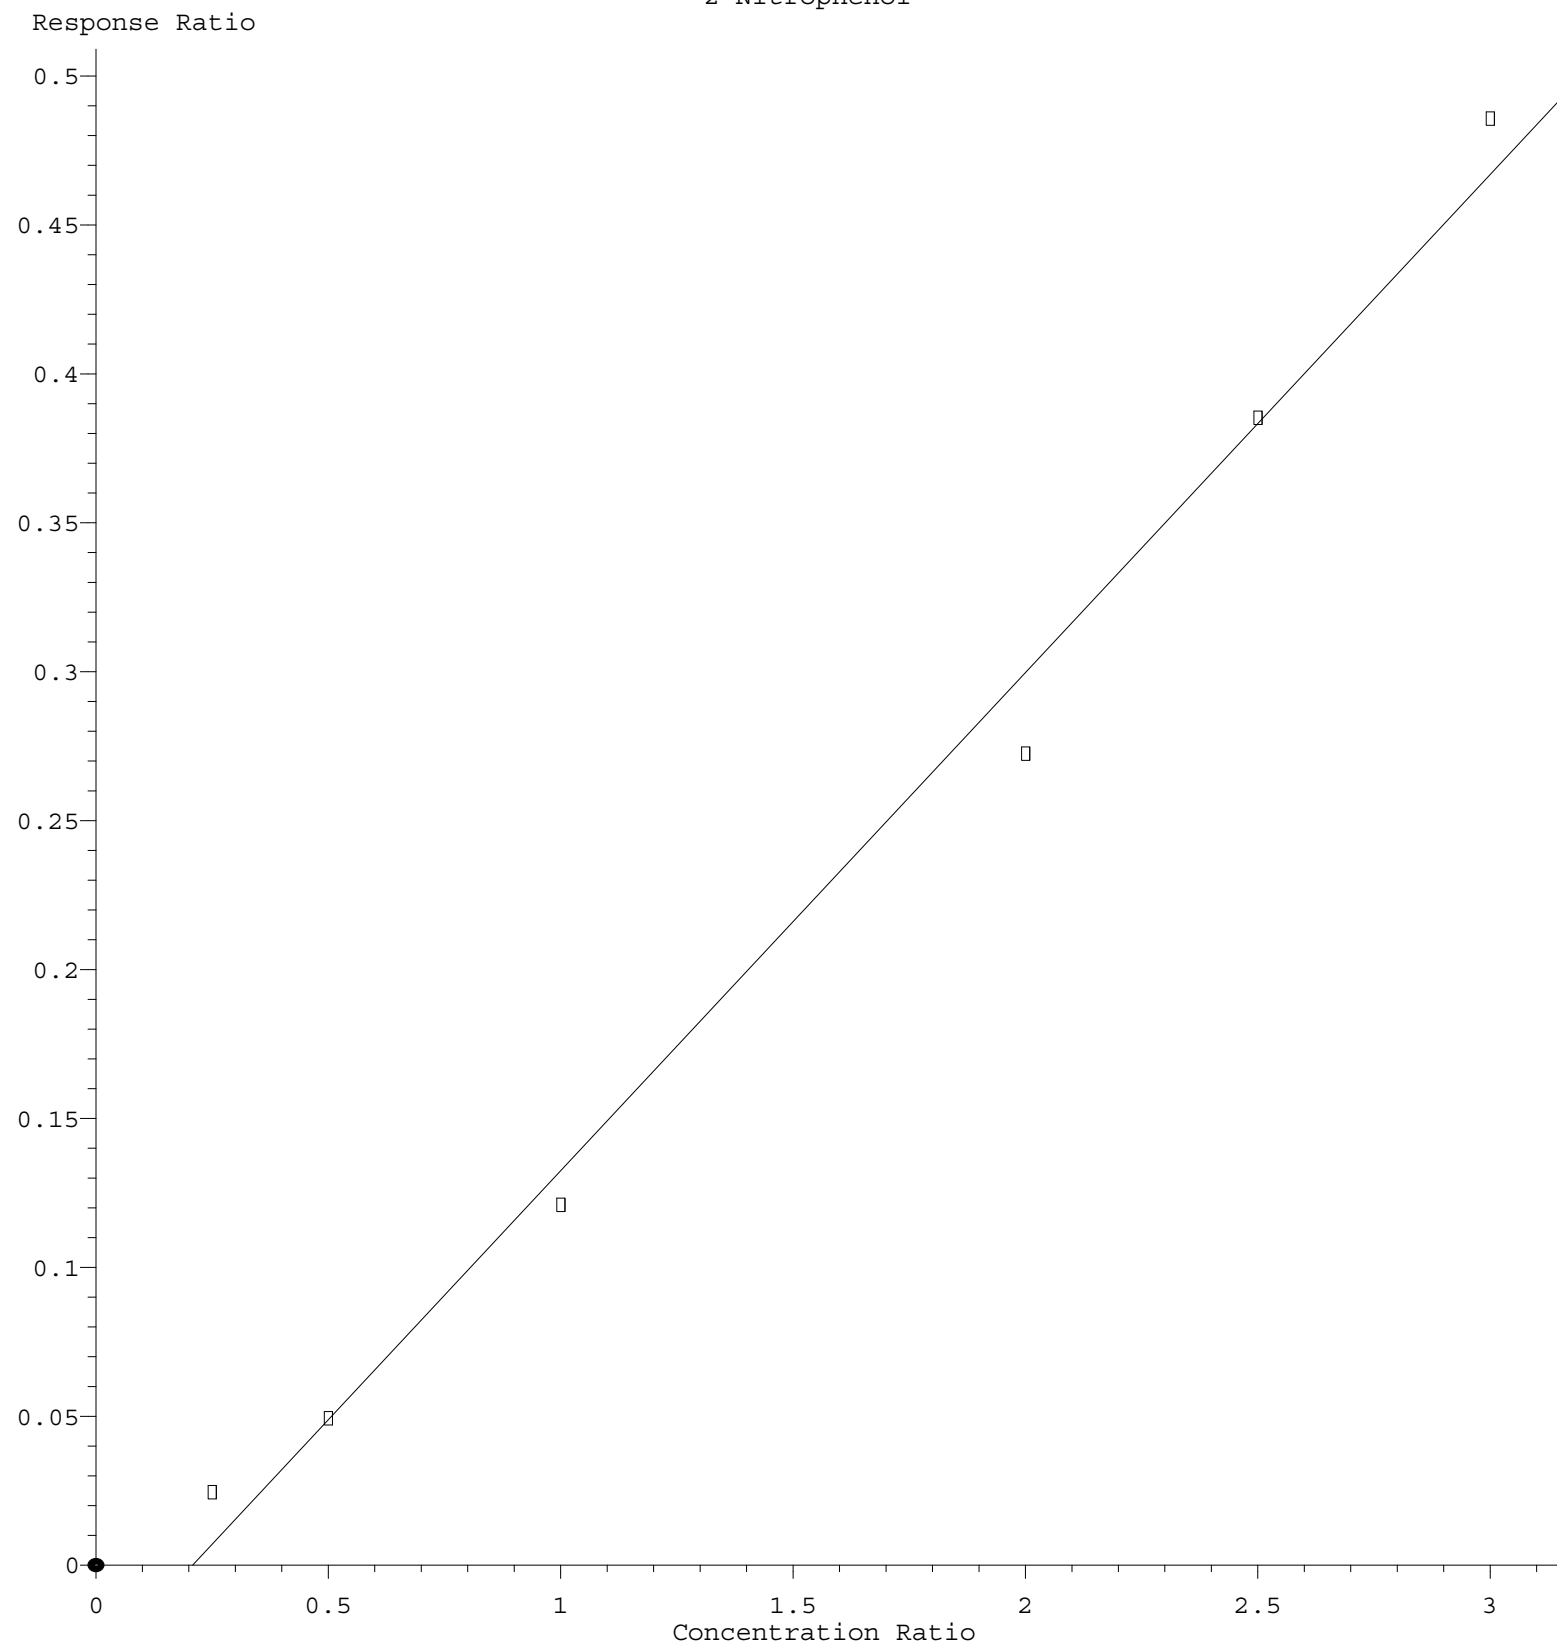

Response = 1.672e-001 * Amt - 3.474e-002
 Coef of Det (r^2) = 0.991385 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M
 Calibration Table Last Updated: Thu May 27 16:11:11 2021


Benzoic acid

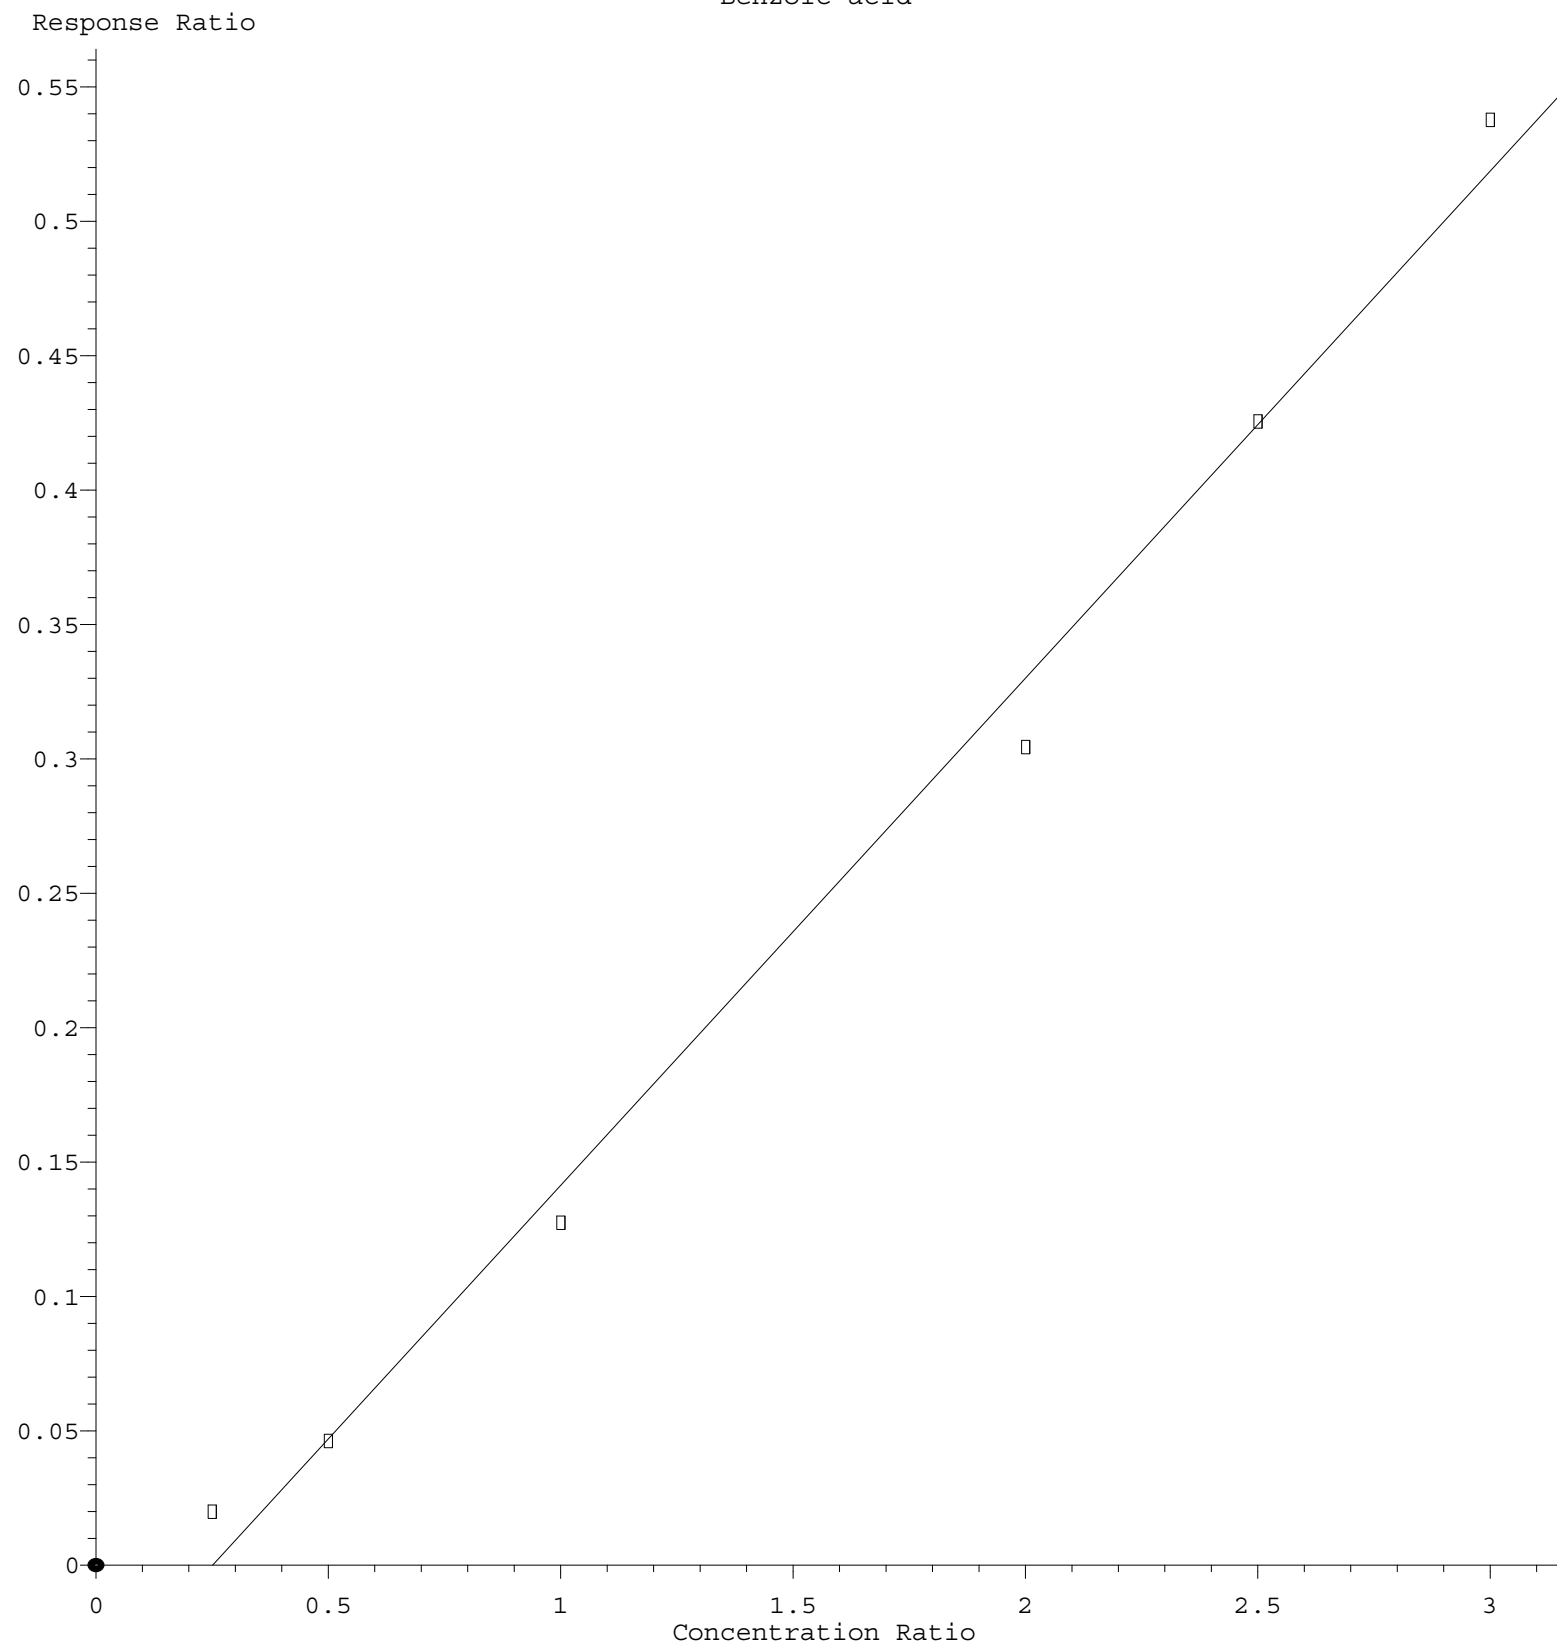

Response = 1.886e-001 * Amt - 4.728e-002
 Coef of Det (r^2) = 0.992833 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M
 Calibration Table Last Updated: Thu May 27 16:11:11 2021

2-Nitroaniline

Response Ratio

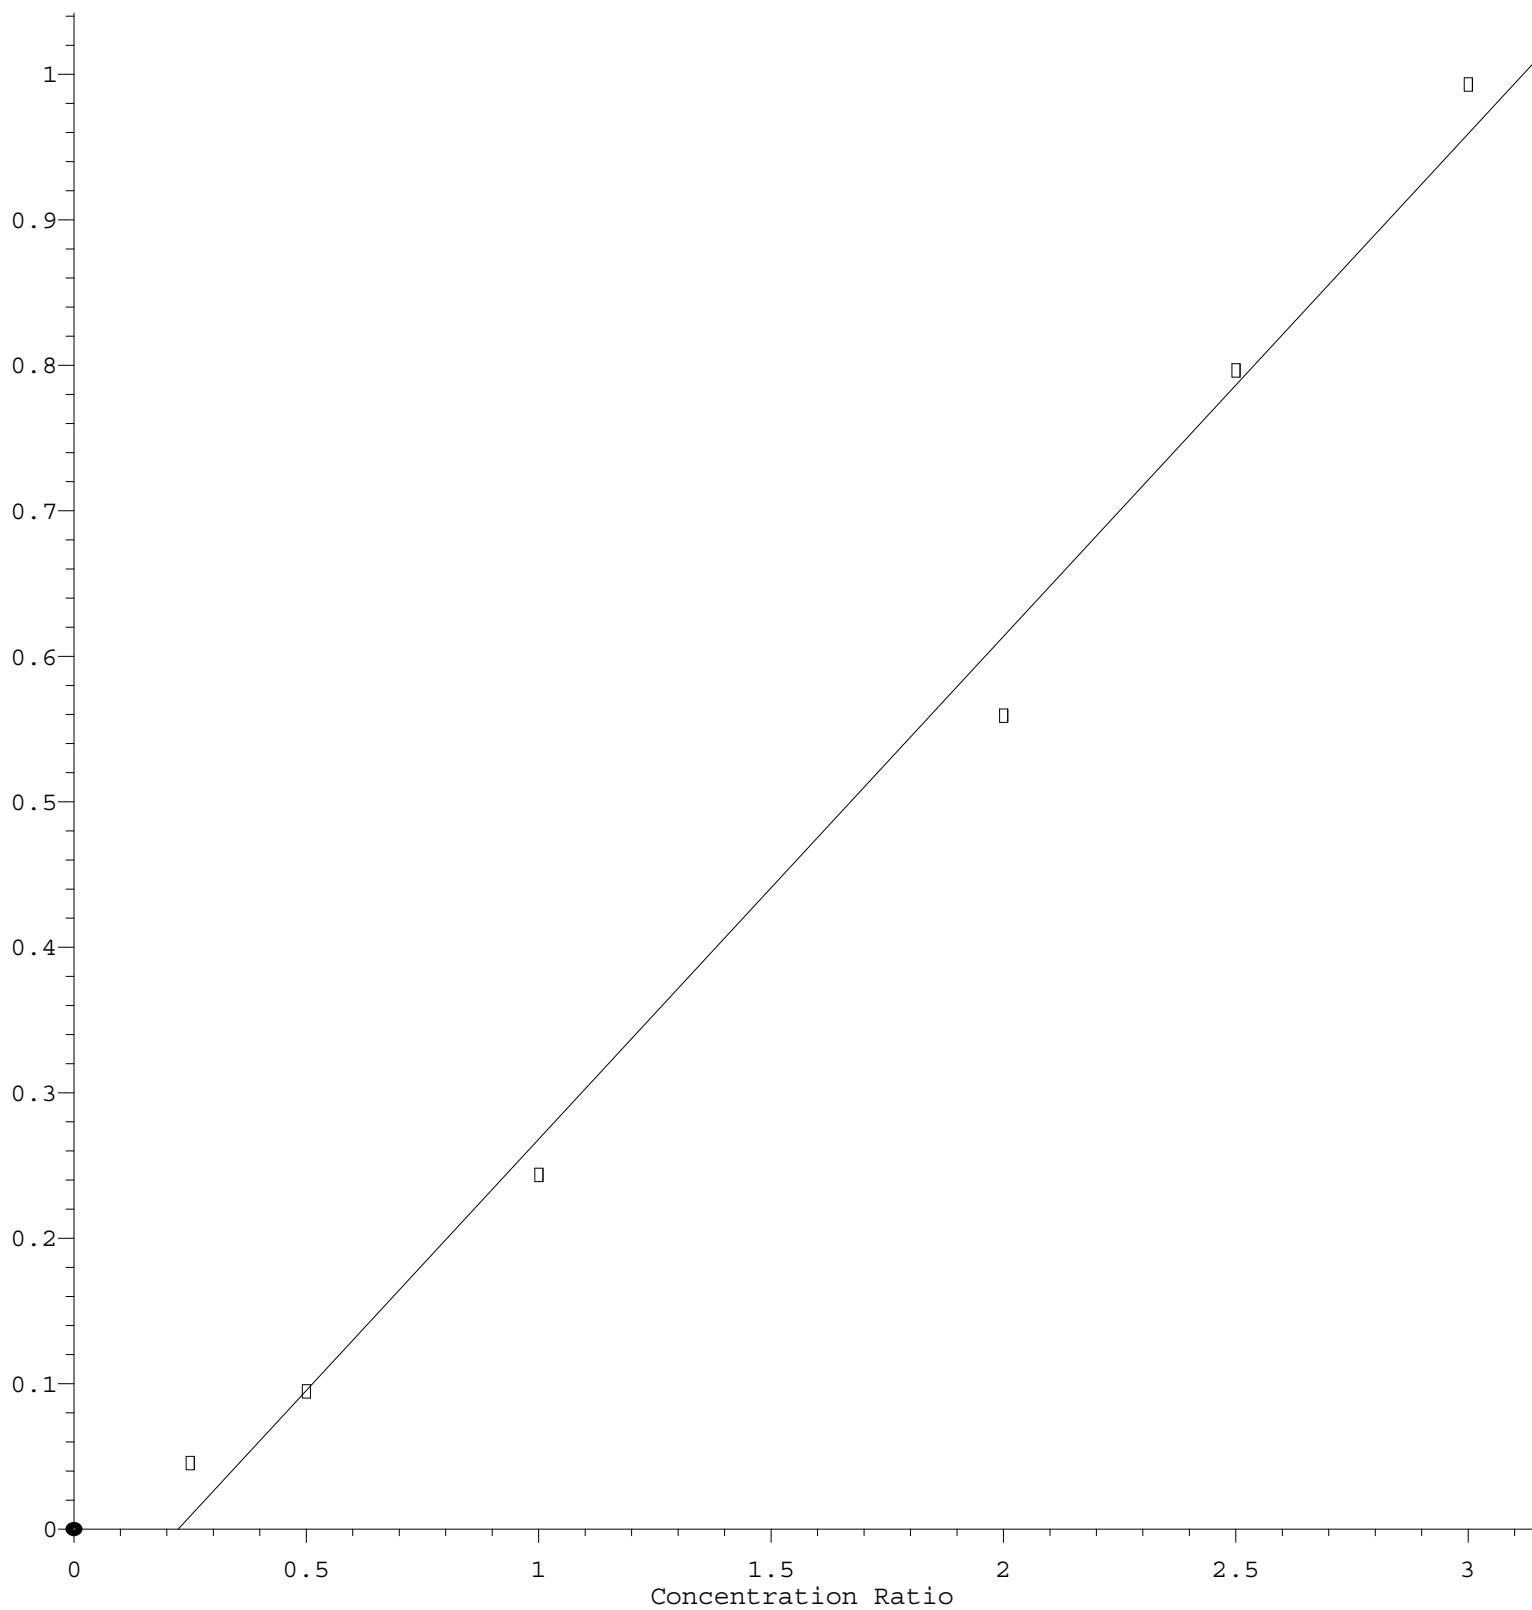

$$\text{Response} = 3.457\text{e-}001 * \text{Amt} - 7.755\text{e-}002$$


Coef of Det (r^2) = 0.991883 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021

2,6-Dinitrotoluene

Response Ratio

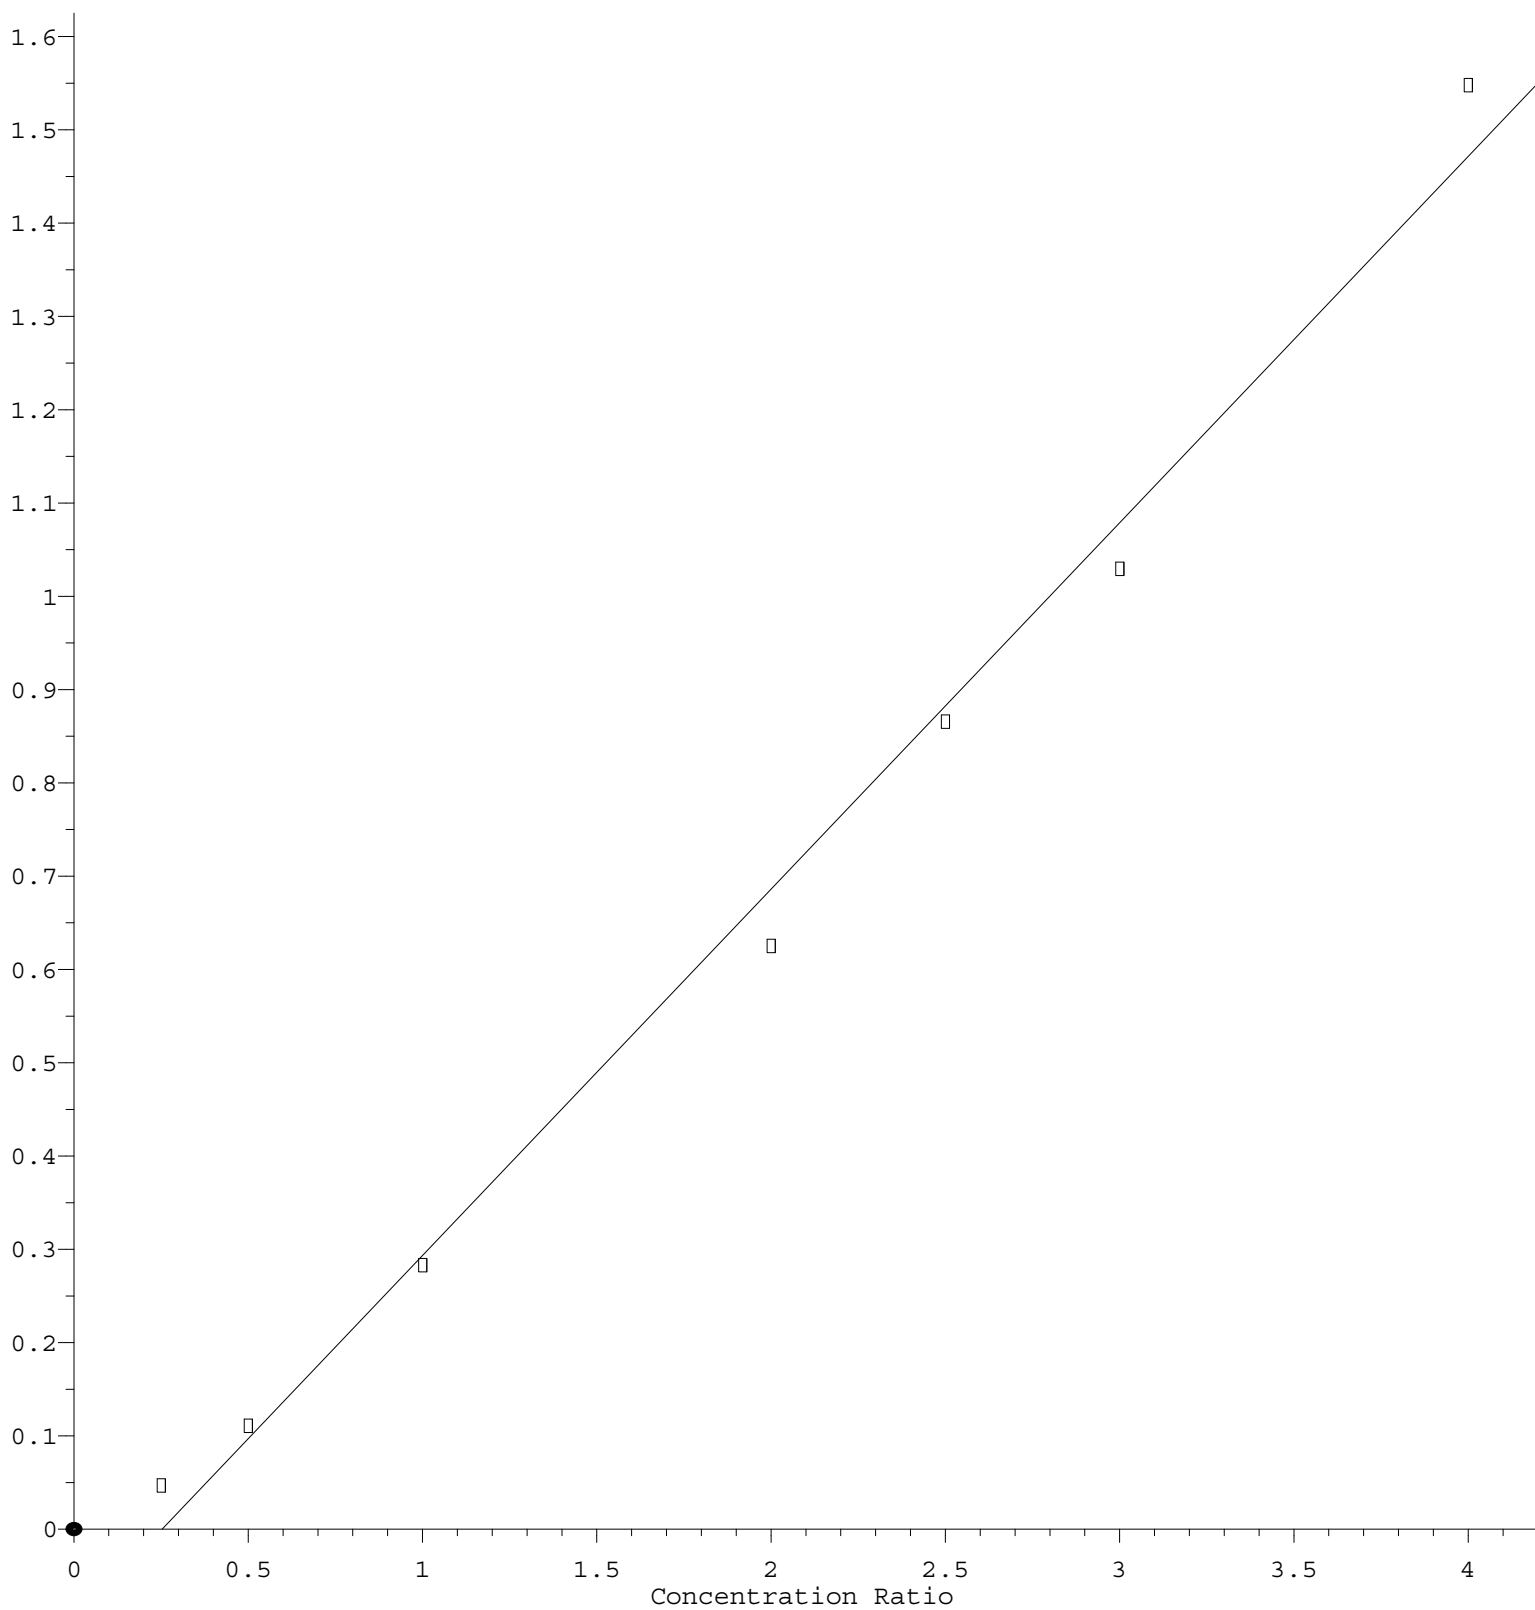

$$\text{Response} = 3.927\text{e-}001 * \text{Amt} - 9.934\text{e-}002$$


Coef of Det (r^2) = 0.991672 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021

3-Nitroaniline

Response Ratio

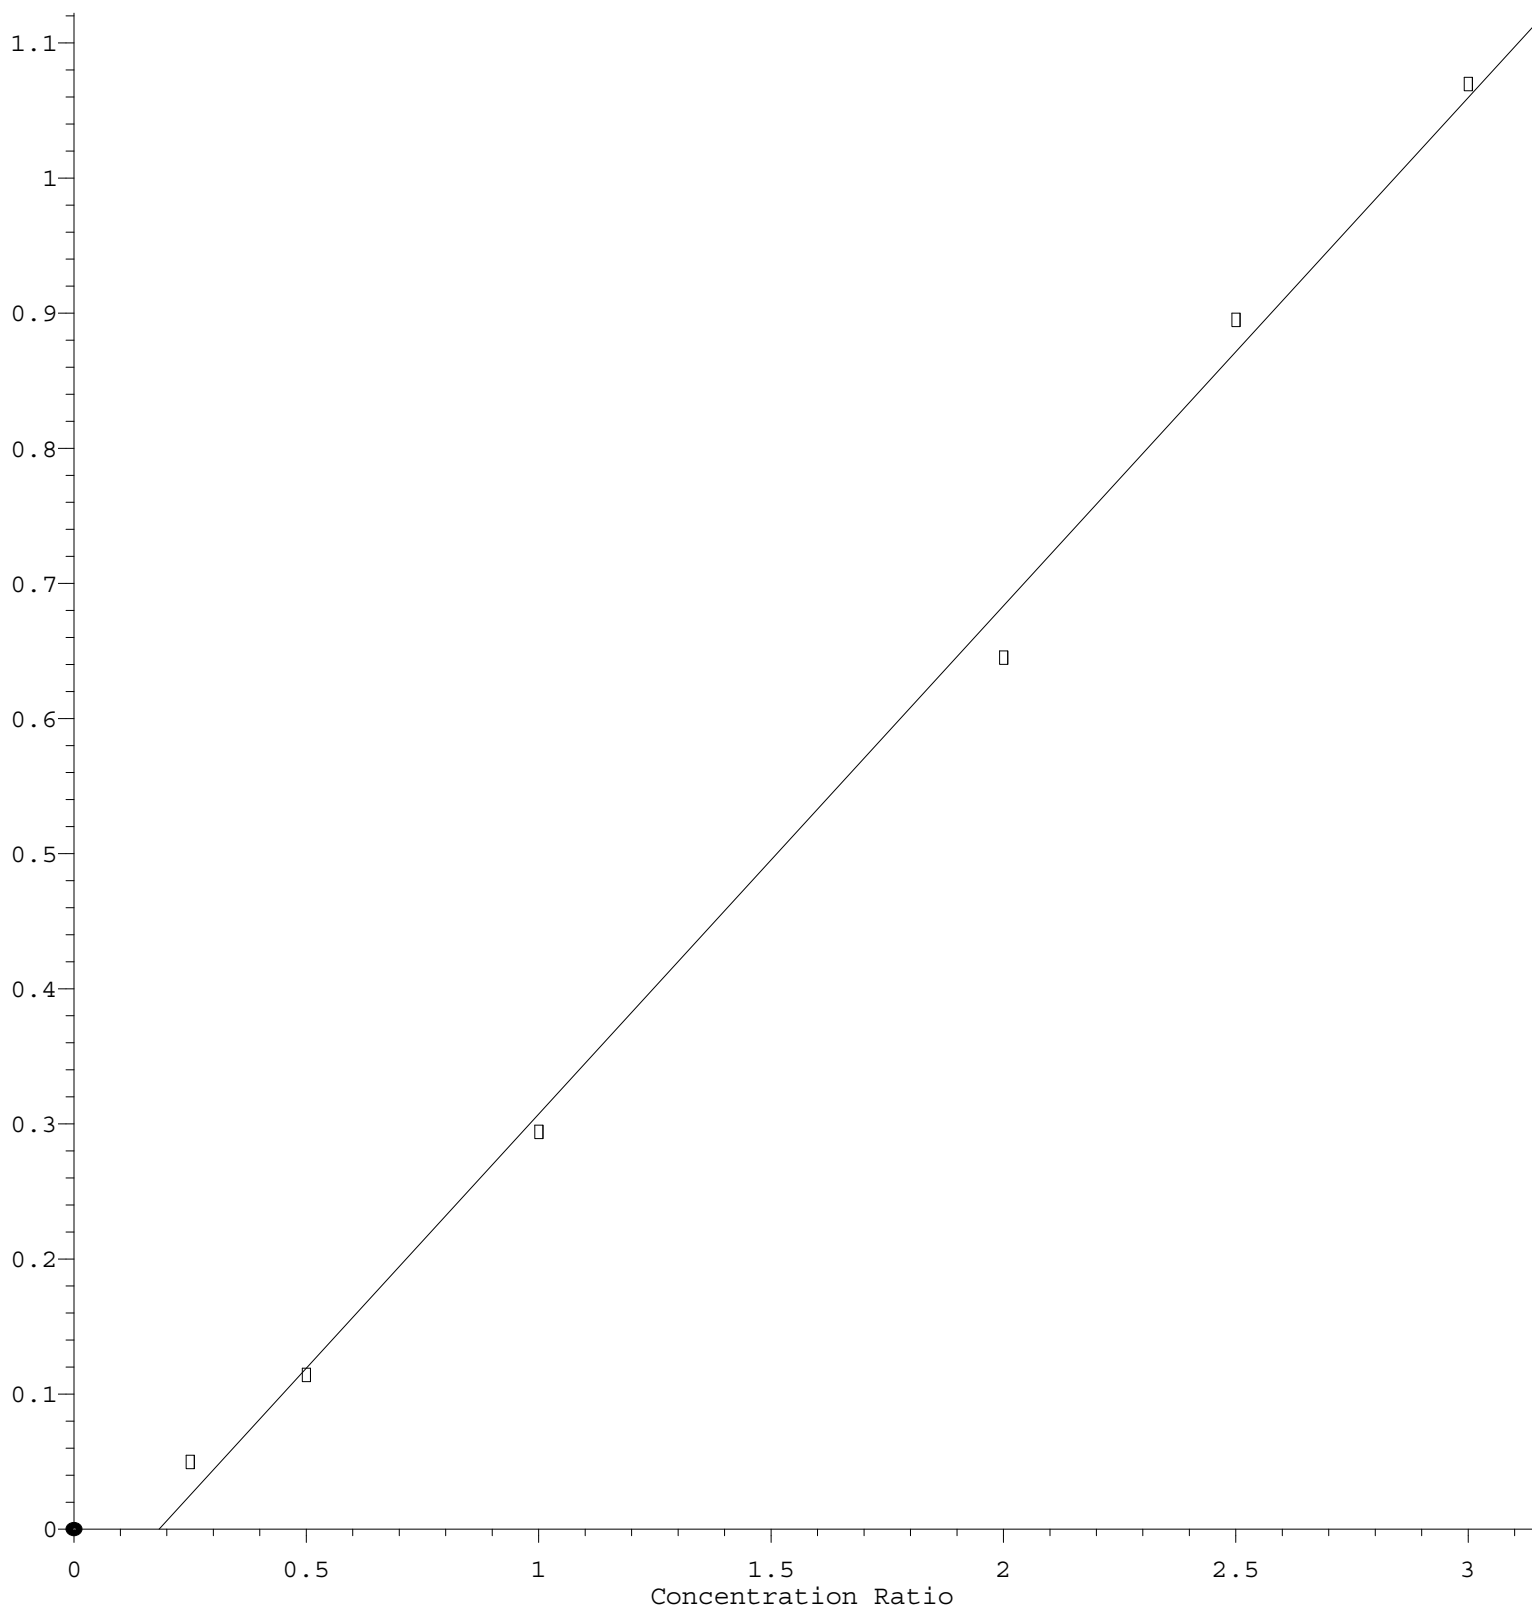


$$\text{Response} = 3.762\text{e-}001 * \text{Amt} - 6.871\text{e-}002$$

Coef of Det (r^2) = 0.996726 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021


2,4-Dinitrophenol

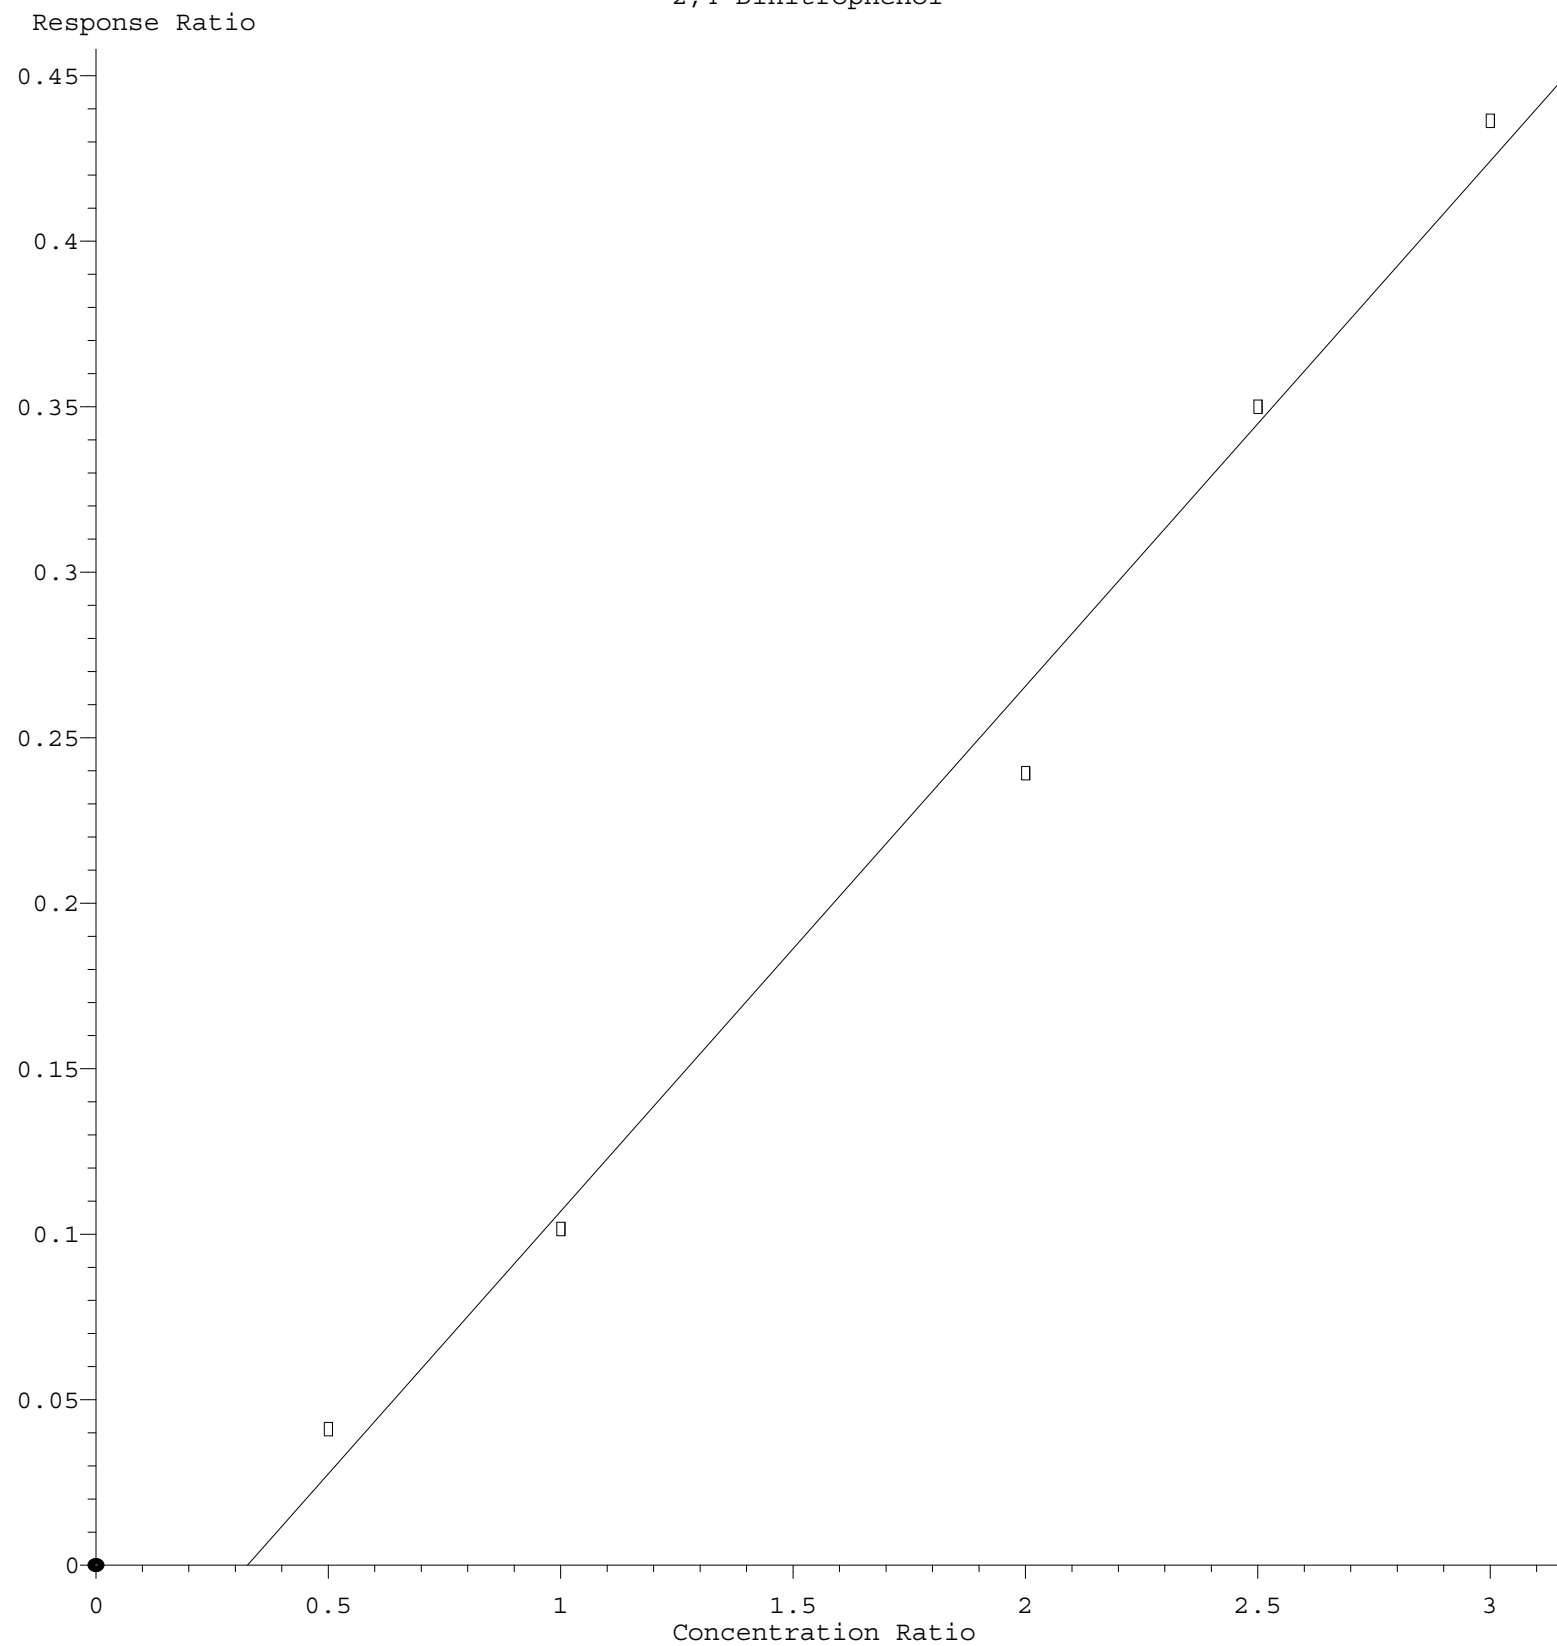

Response = $1.586 \times 10^{-1} \times \text{Amt} - 5.174 \times 10^{-2}$
 Coef of Det (r^2) = 0.990145 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M
 Calibration Table Last Updated: Thu May 27 16:11:11 2021

4-Nitrophenol

Response Ratio

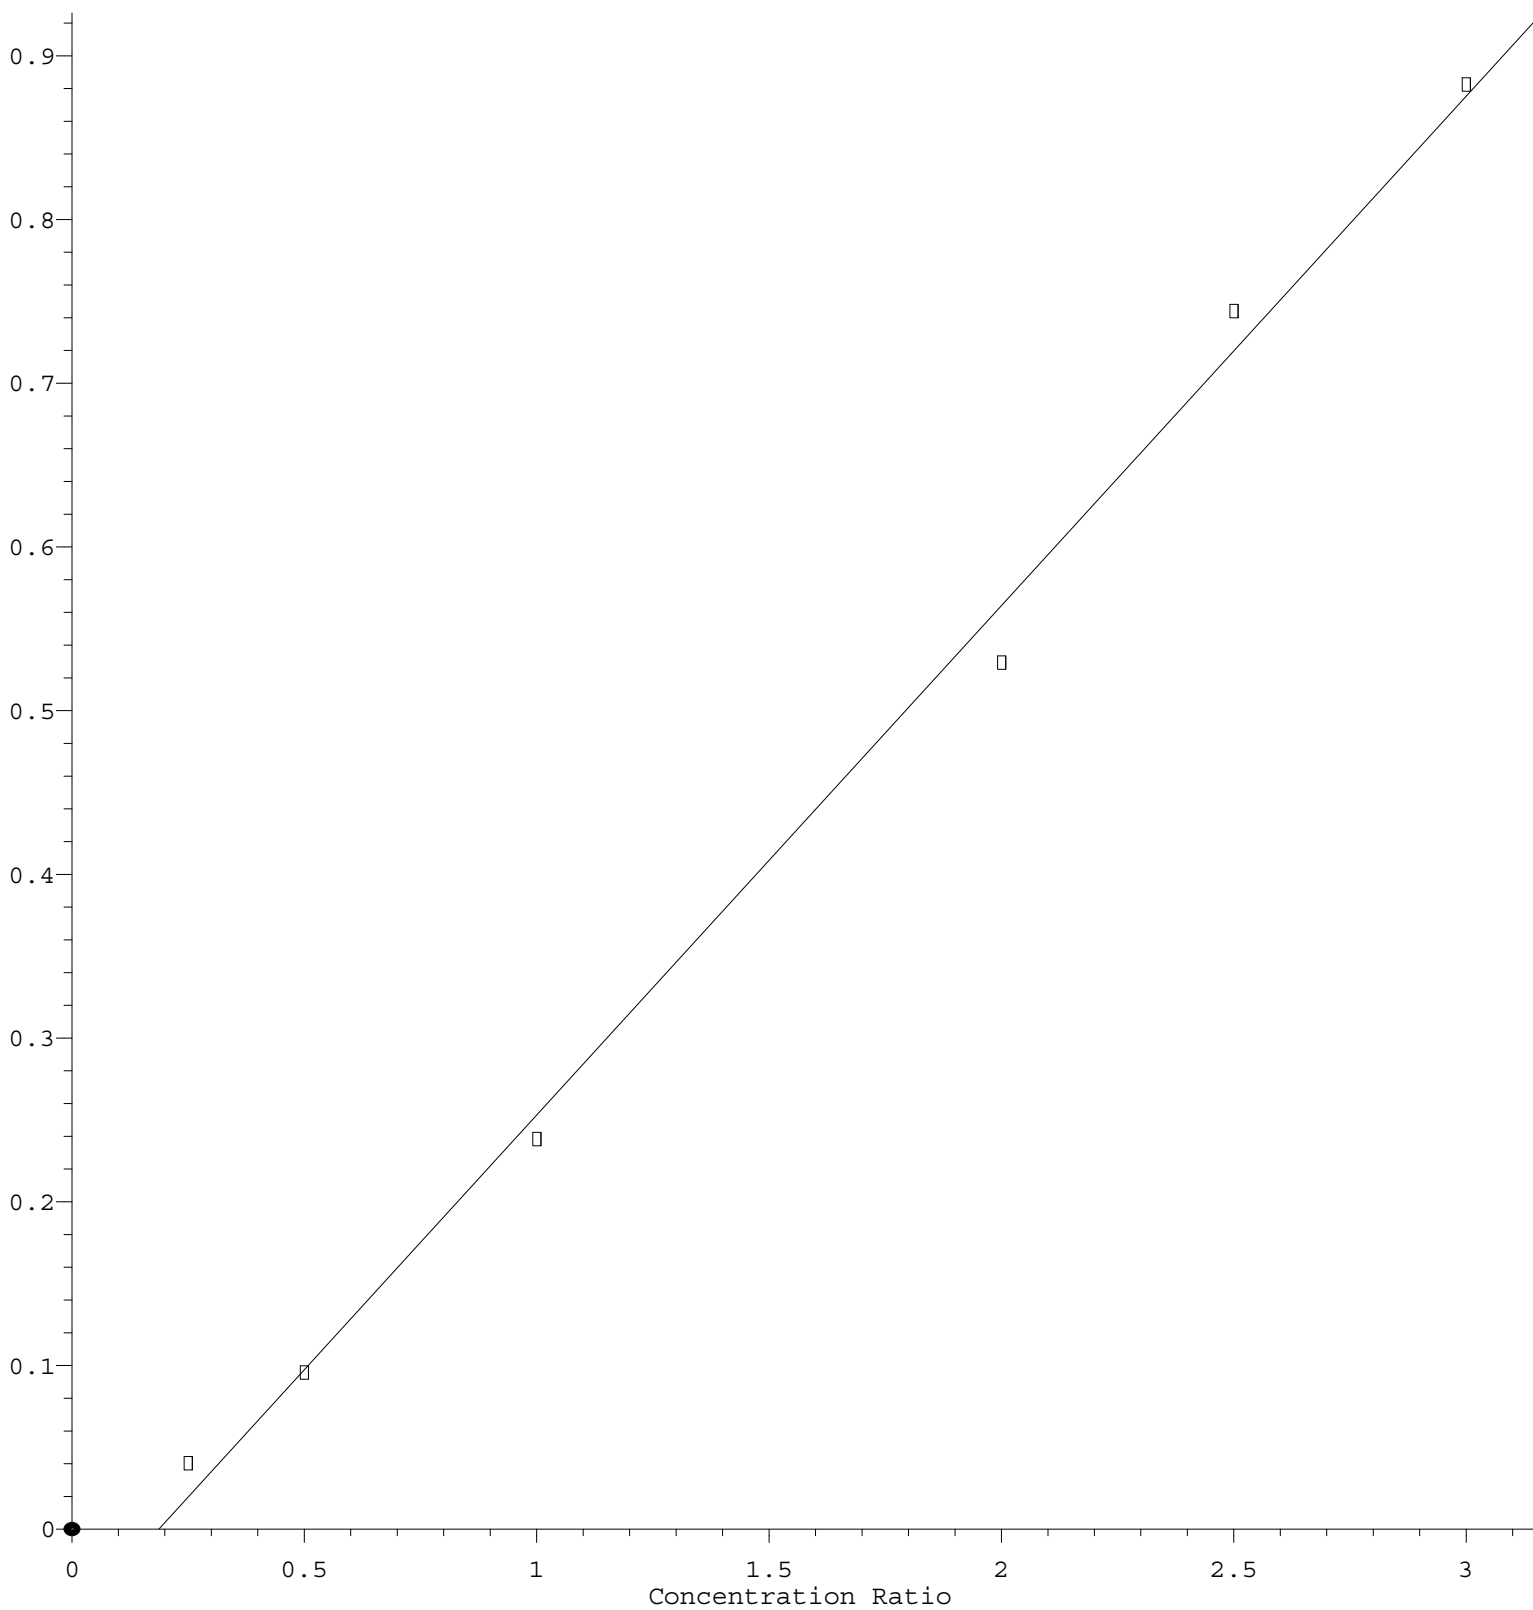

$$\text{Response} = 3.113\text{e-}001 * \text{Amt} - 5.828\text{e-}002$$


Coef of Det (r^2) = 0.995922 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021

2,4-Dinitrotoluene

Response Ratio

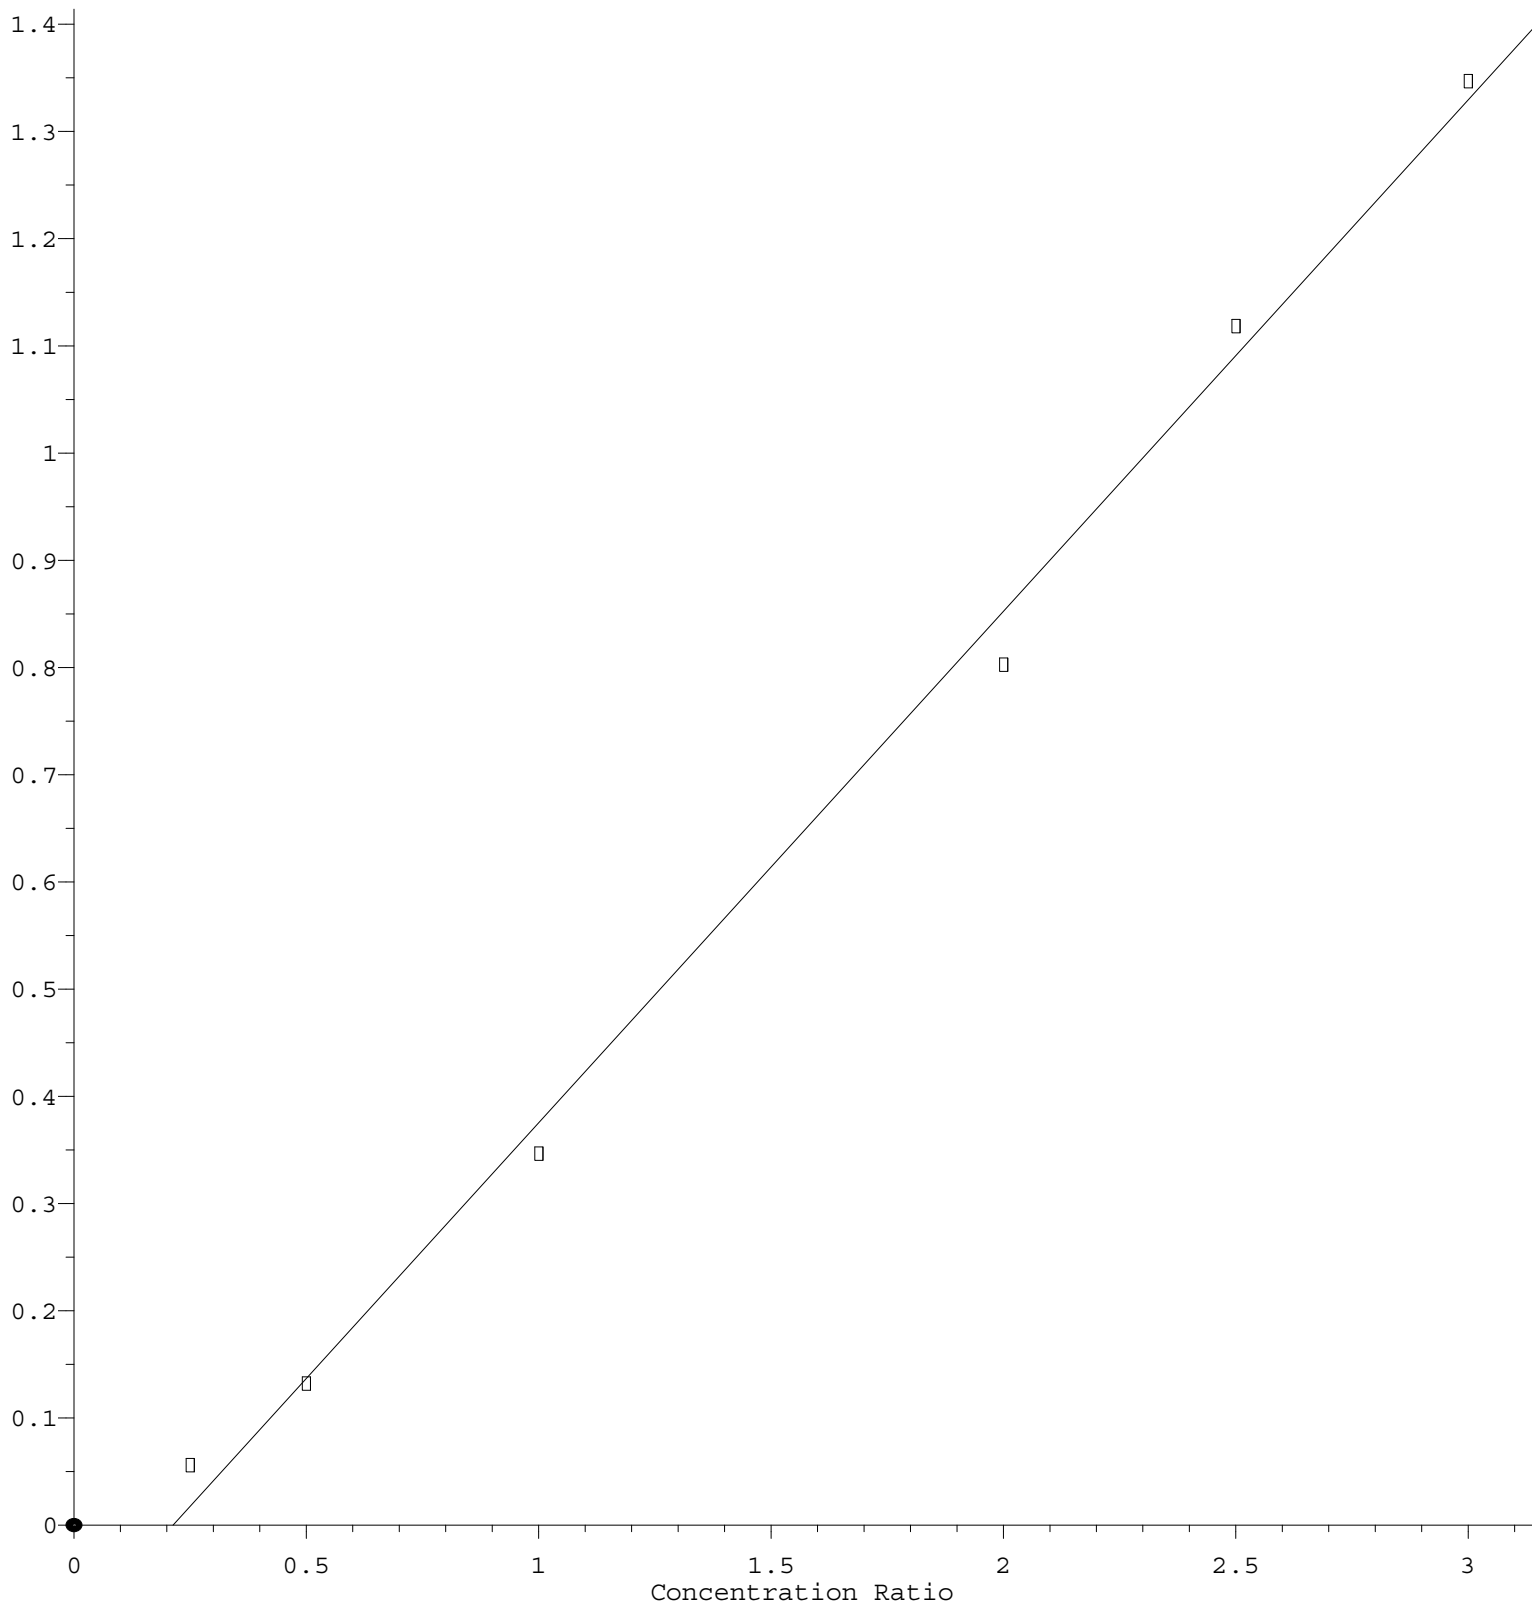

$$\text{Response} = 4.770\text{e-}001 * \text{Amt} - 1.016\text{e-}001$$


Coef of Det (r^2) = 0.995927 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021

4-Nitroaniline

Response Ratio

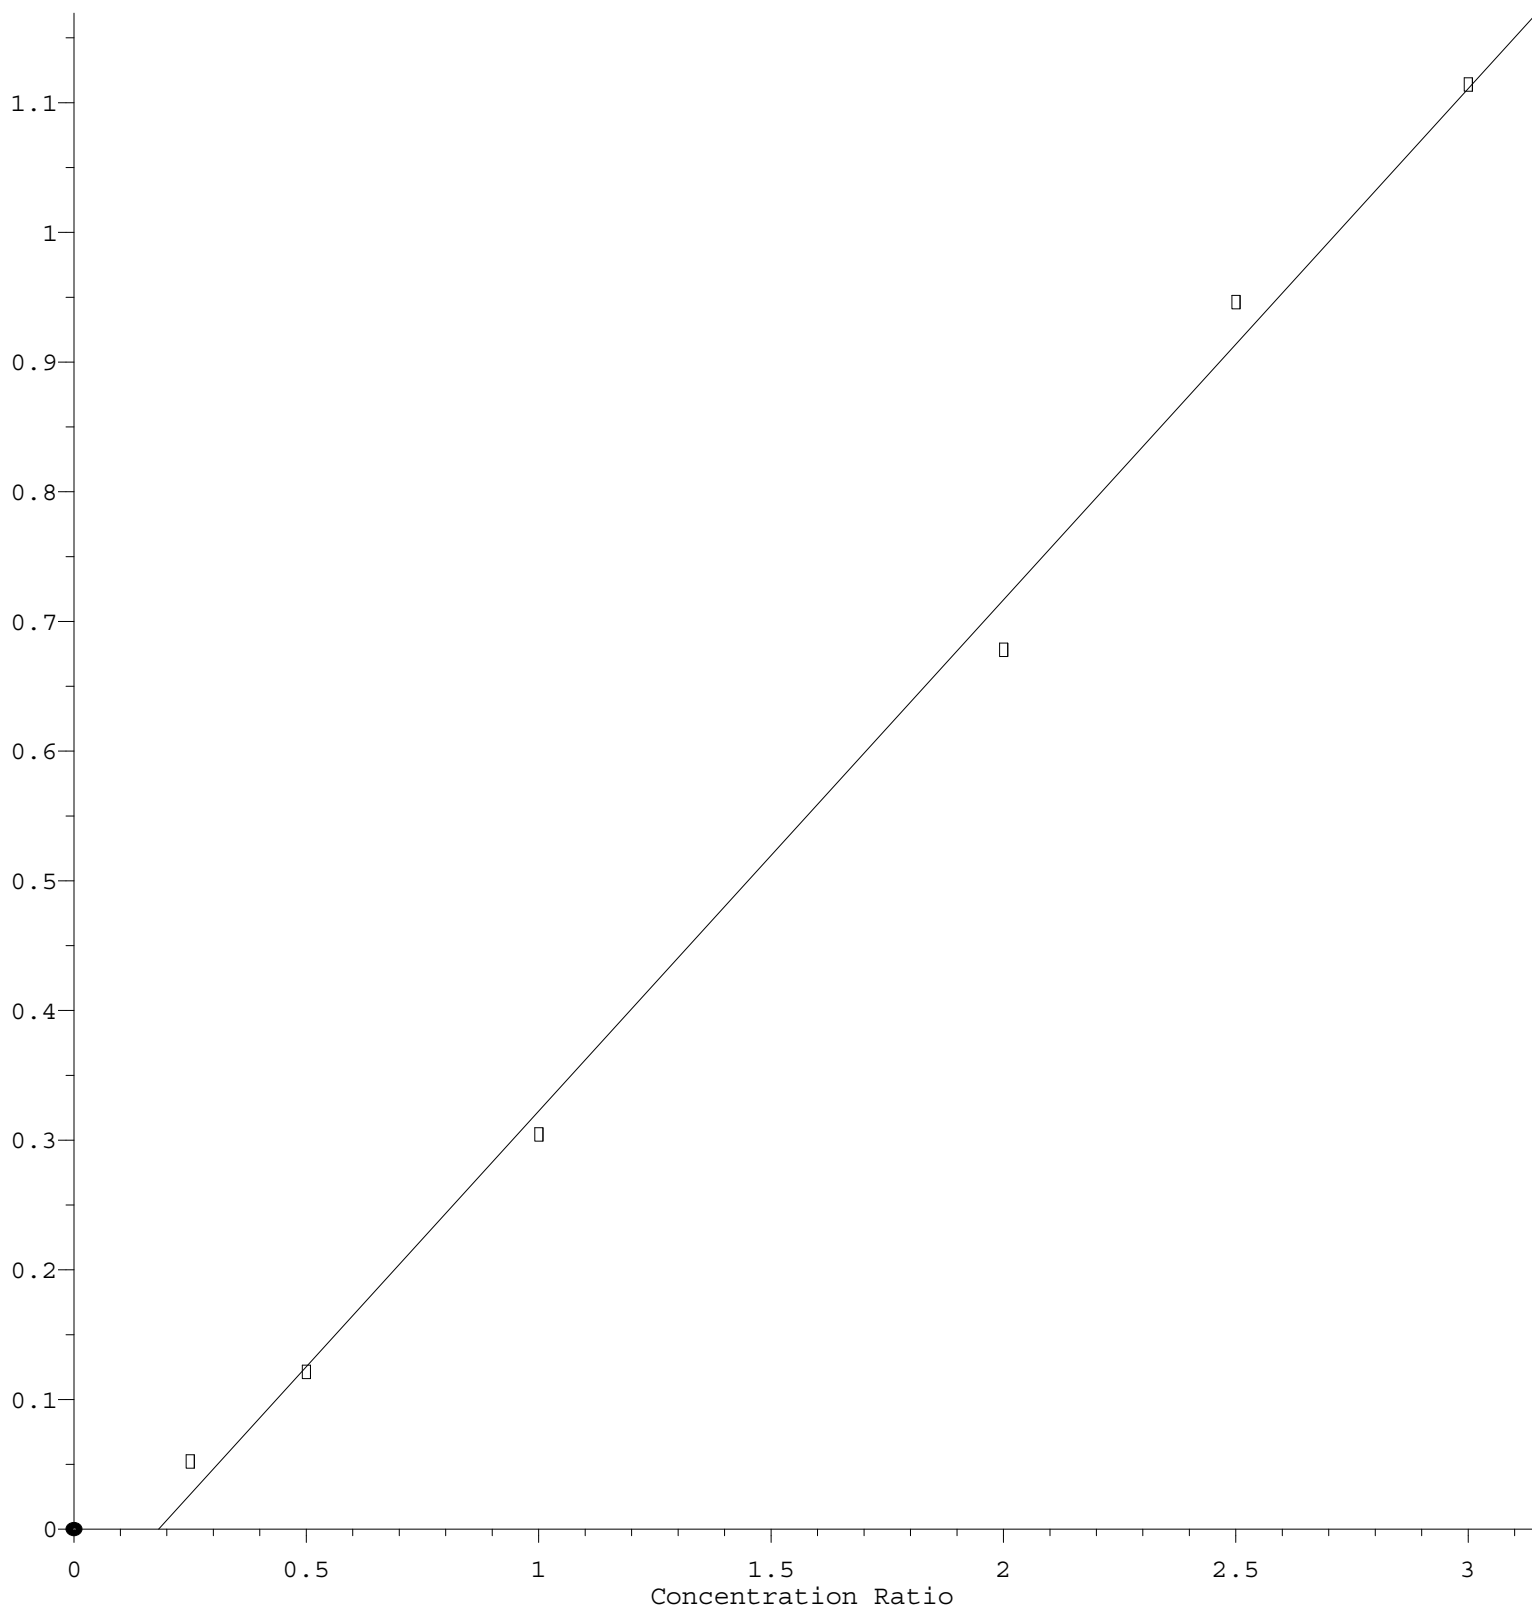


$$\text{Response} = 3.941\text{e-}001 * \text{Amt} - 7.153\text{e-}002$$

Coef of Det (r^2) = 0.996399 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021


4,6-Dinitro-2-methylphenol

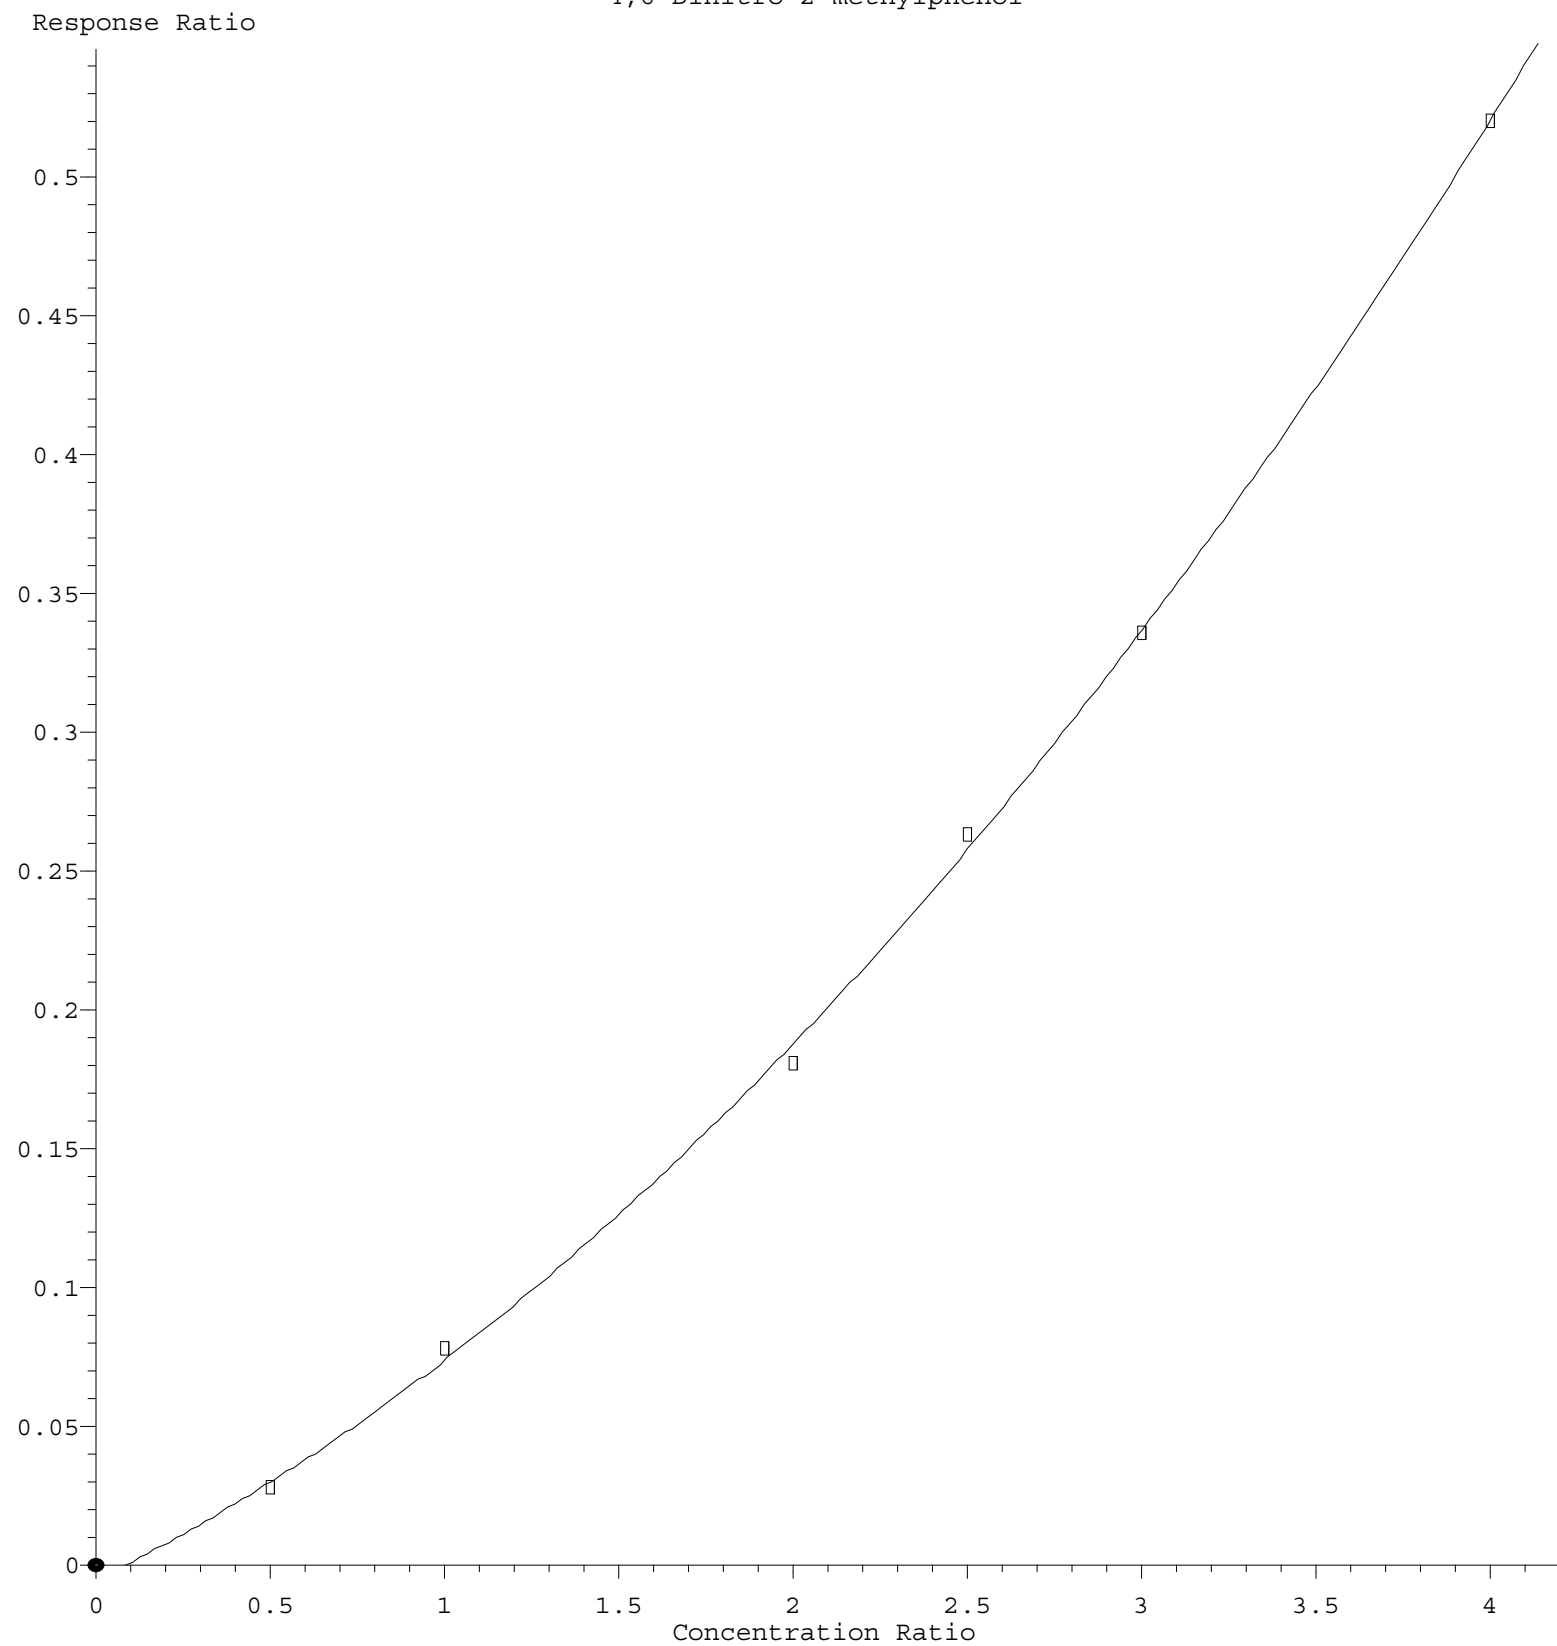

$R = 1.747e-002 A^2 + 6.151e-002 A - 5.240e-003$
Coef of Det (r^2) = 0.999387 Curve Fit: Quadratic
Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M
Calibration Table Last Updated: Thu May 27 16:11:11 2021

Butylbenzylphthalate

Response Ratio

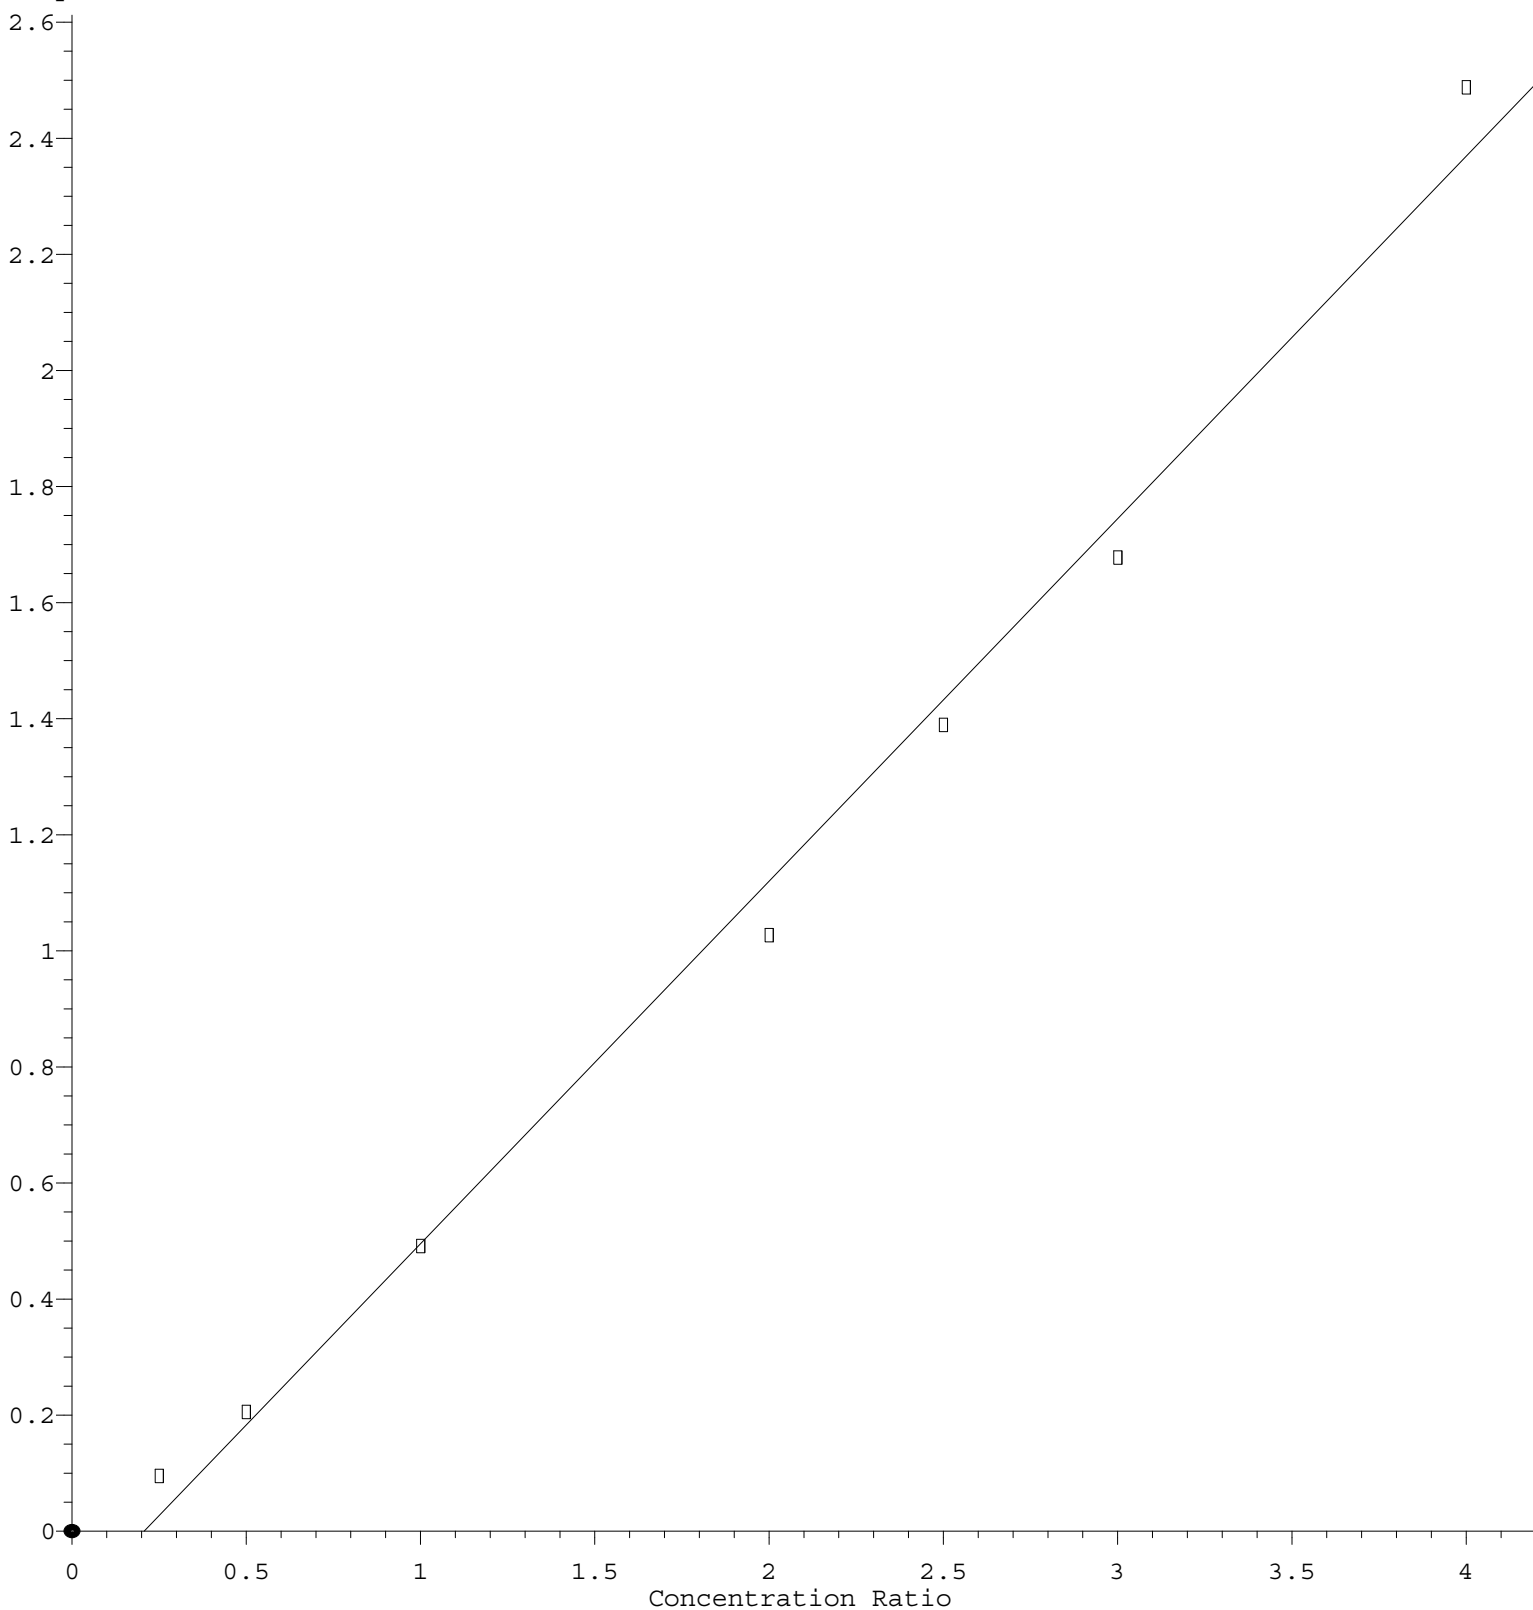

$$\text{Response} = 6.246\text{e-}001 * \text{Amt} - 1.290\text{e-}001$$

Coef of Det (r^2) = 0.992409 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP052721.M

Calibration Table Last Updated: Thu May 27 16:11:11 2021