
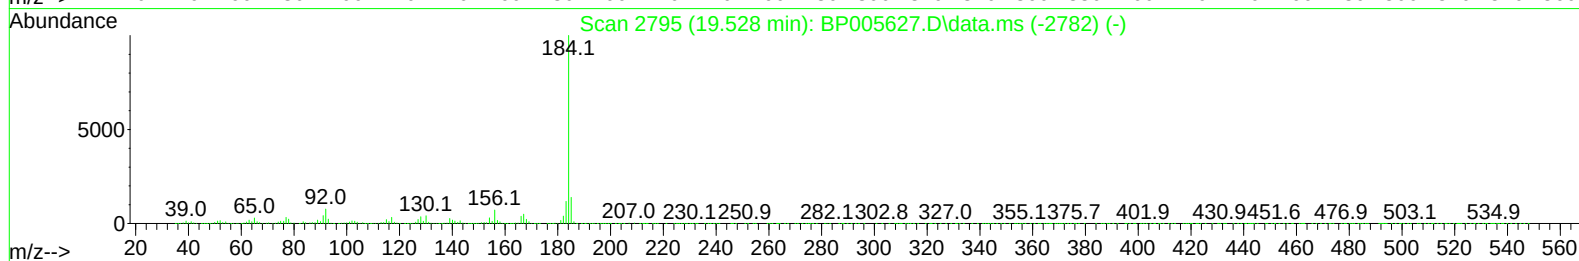
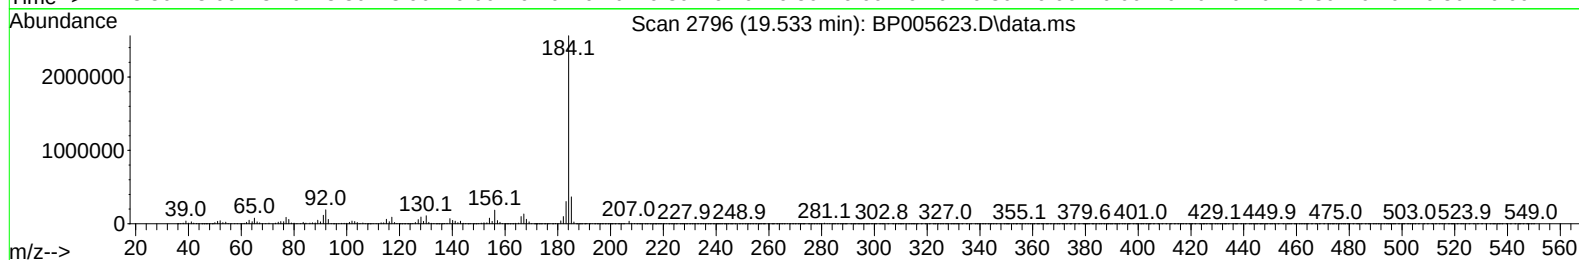


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052721\
 Data File : BP005623.D
 Acq On : 27 May 2021 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 18:31:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

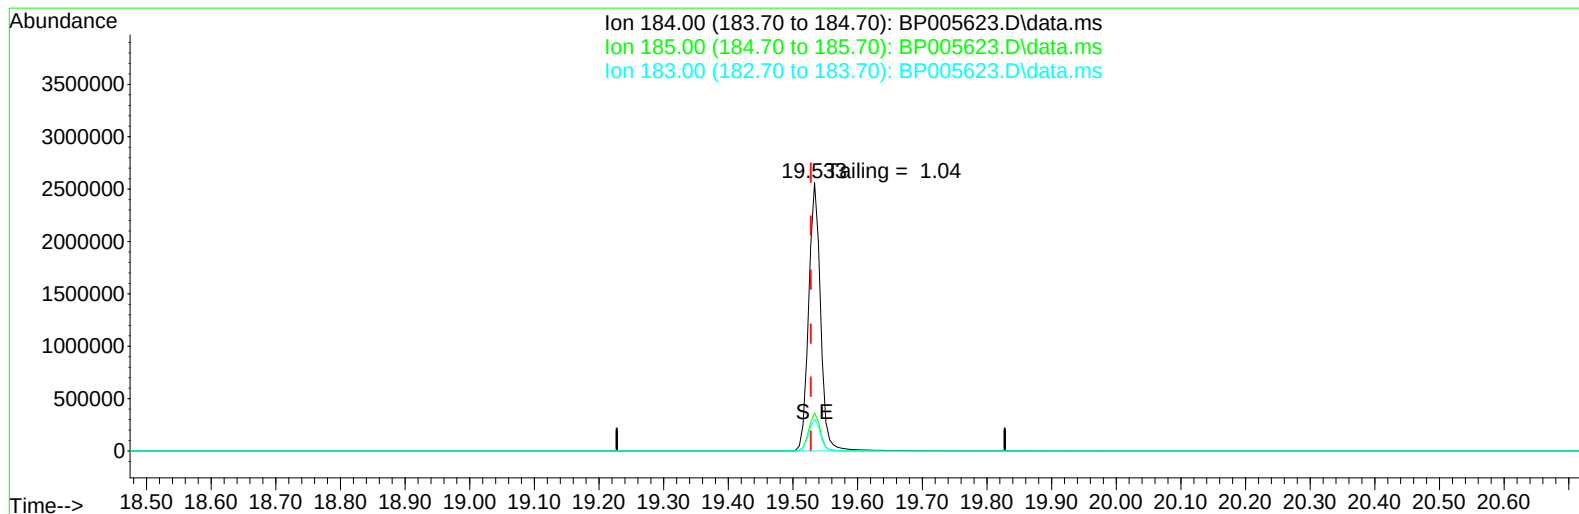




TIC: BP005623.D\data.ms

(77) Benzidine**19.533min (+ 0.006) 1191408.19 ng****response 3280827**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.27
183.00	12.30	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052721\
Data File : BP005623.D
Acq On : 27 May 2021 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 18:31:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

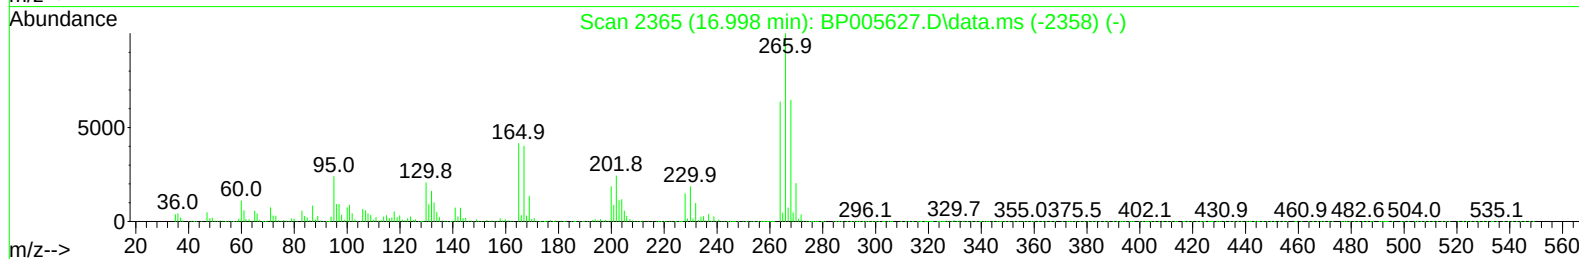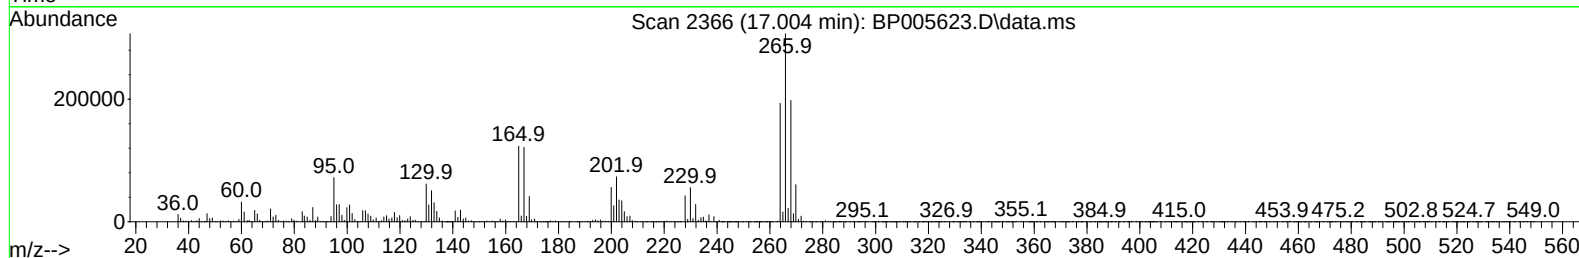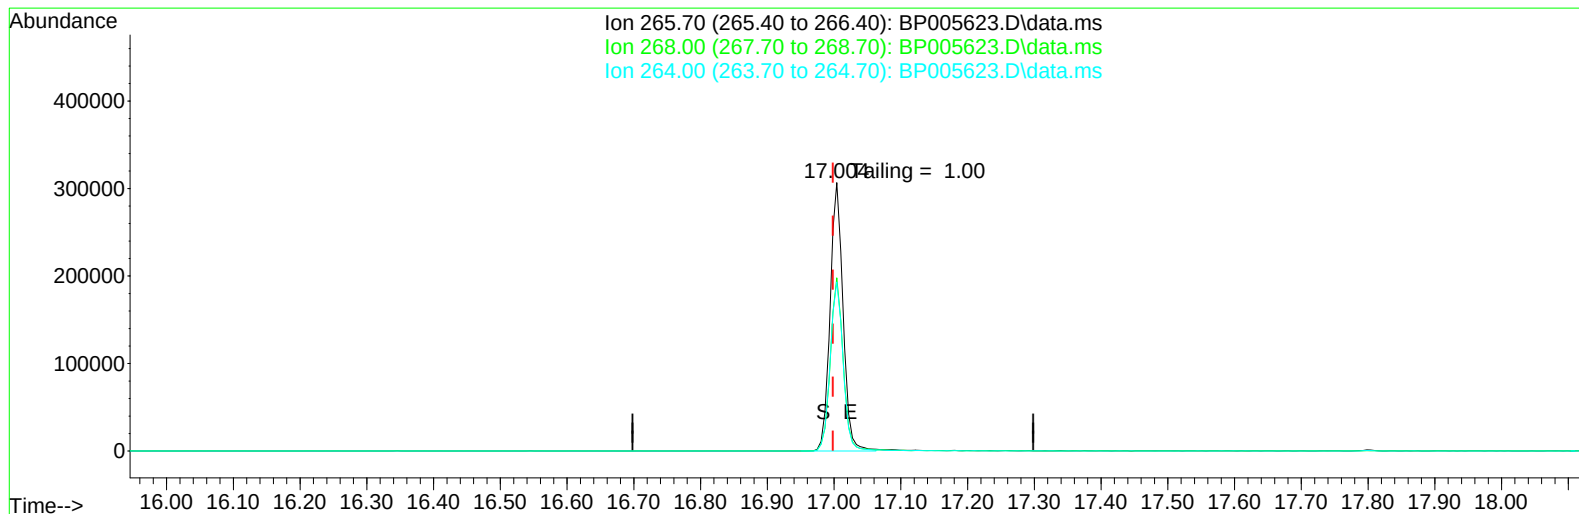

TIC: BP005623.D\data.ms

(70) Pentachlorophenol (C)

17.004min (+ 0.006) 3859008.33 ng

response 416429

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.51
264.00	67.10	62.99
0.00	0.00	0.00