
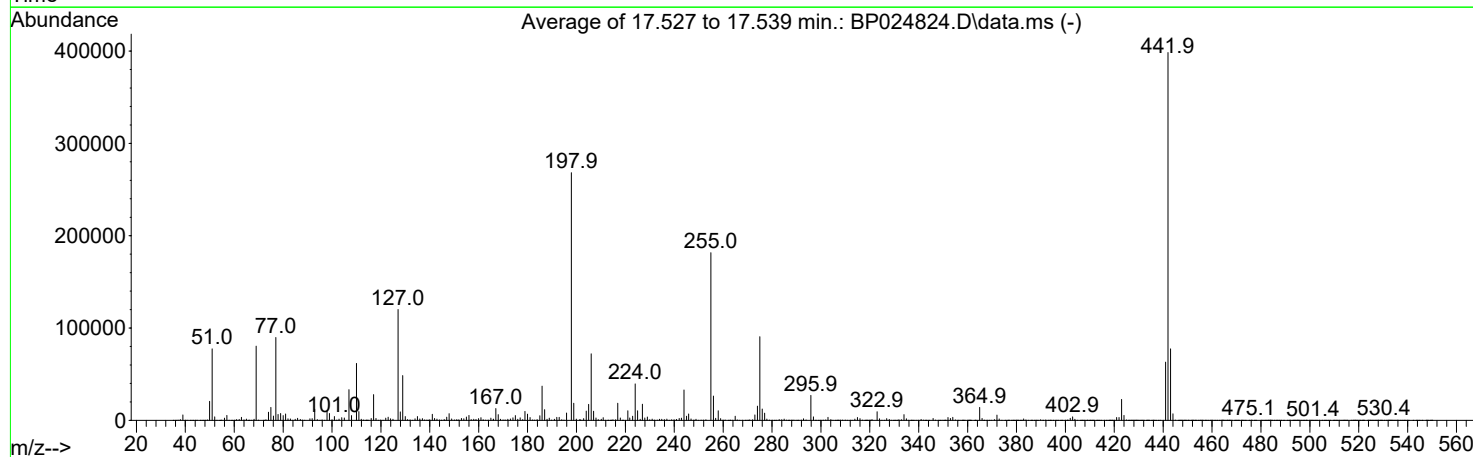


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052925\
Data File : BP024824.D
Acq On : 29 May 2025 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 28 14:16:13 2025

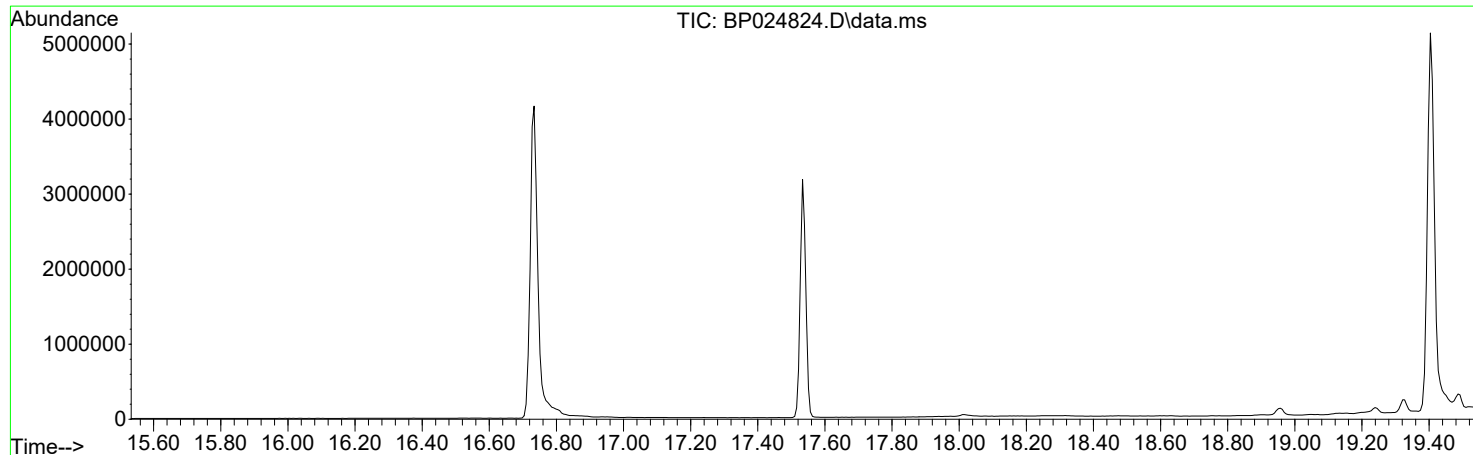

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	77392	PASS
68	69	0.00	2	1.6	1264	PASS
69	198	0.00	100	30.0	80445	PASS
70	69	0.00	2	0.5	389	PASS
127	198	10	80	44.8	120187	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	268316	PASS
199	198	5	9	6.9	18589	PASS
275	198	10	60	33.8	90684	PASS
365	198	1	100	5.2	13988	PASS
441	198	0.01	100	23.5	63160	PASS
442	442	100	100	100.0	398455	PASS
443	442	15	24	19.5	77566	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/29/2025	BNA_P	<u>BP024824.D</u>
Compound Name	Response	Retention Time
DDT	1078669	20.686
DDD	21966	20.28
DDE	2925	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24891	1103560	2.26

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052925\
Data File : BP024824.D
Acq On : 29 May 2025 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 29 12:28:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 28 14:16:13 2025
Response via : Initial Calibration

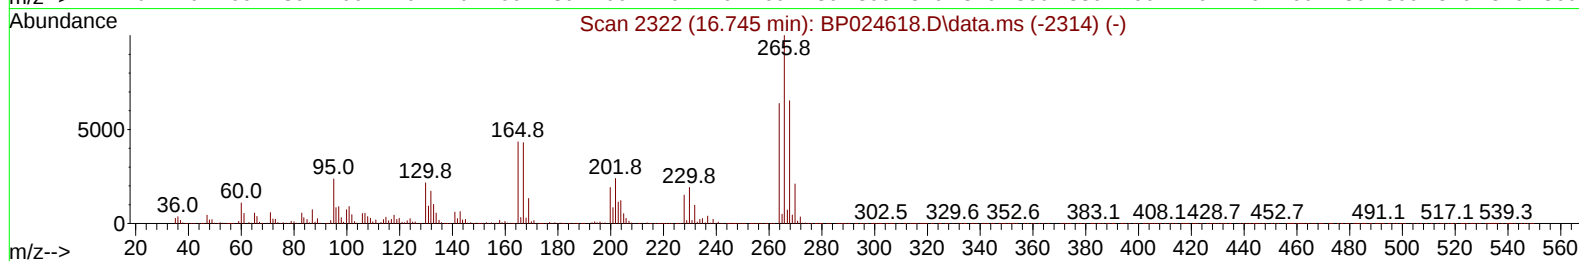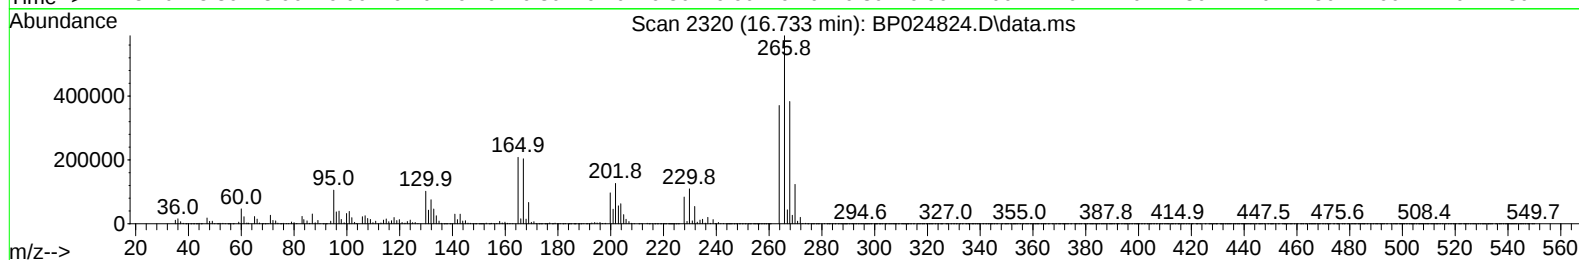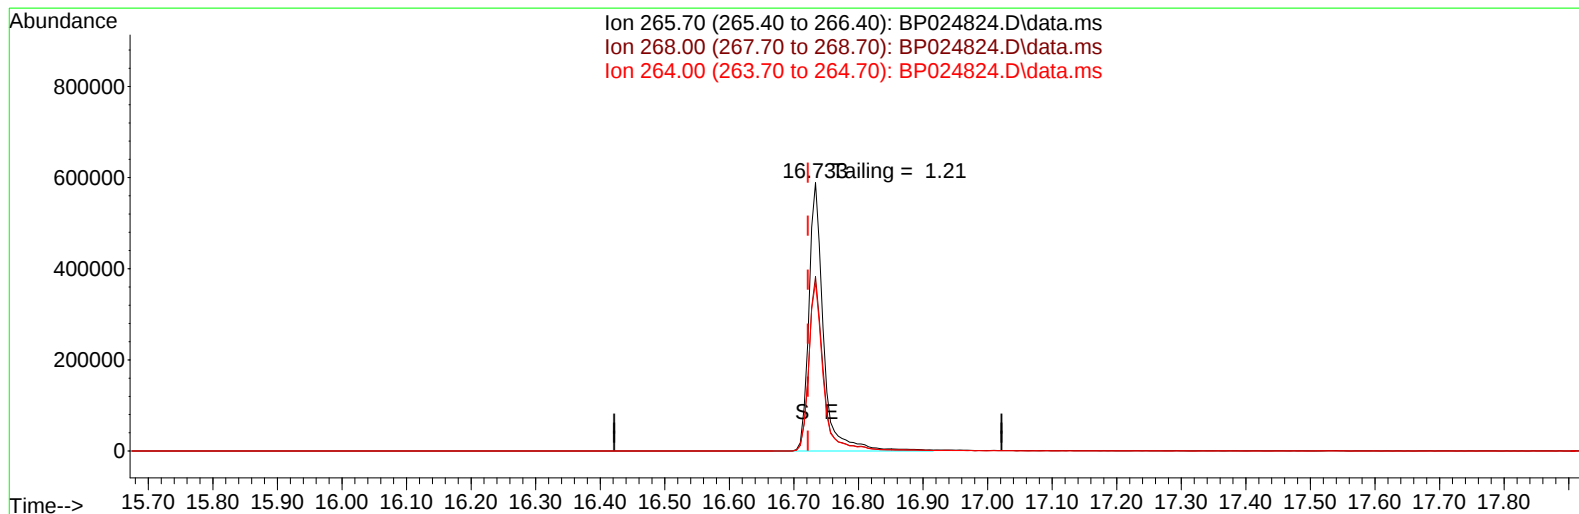

TIC: BP024824.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.012) 150796.13 ng




response 932845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.01
264.00	63.90	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052925\
Data File : BP024824.D
Acq On : 29 May 2025 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 29 12:28:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 28 14:16:13 2025
Response via : Initial Calibration

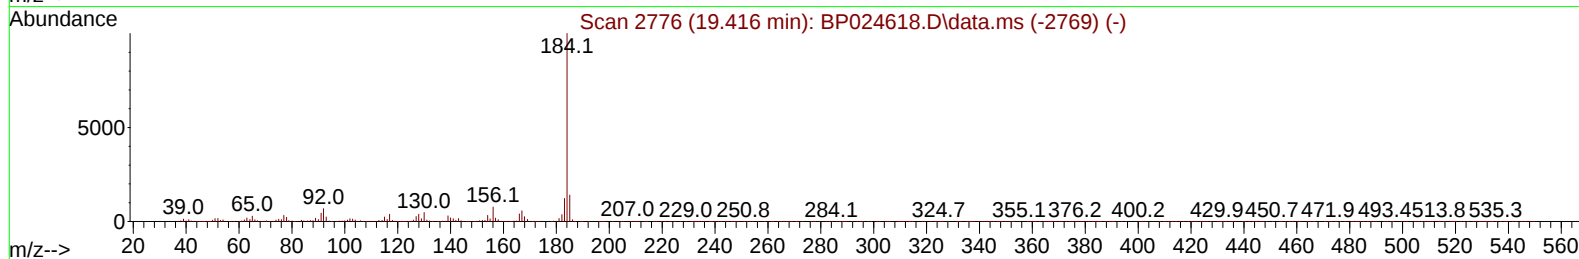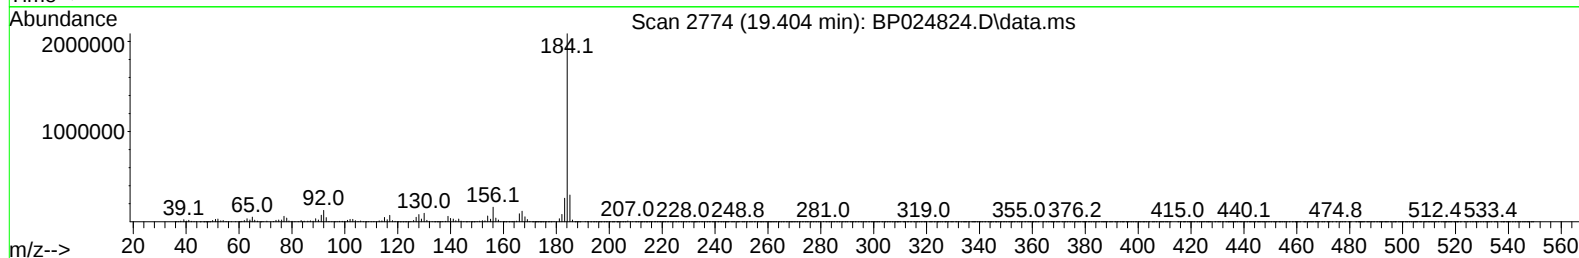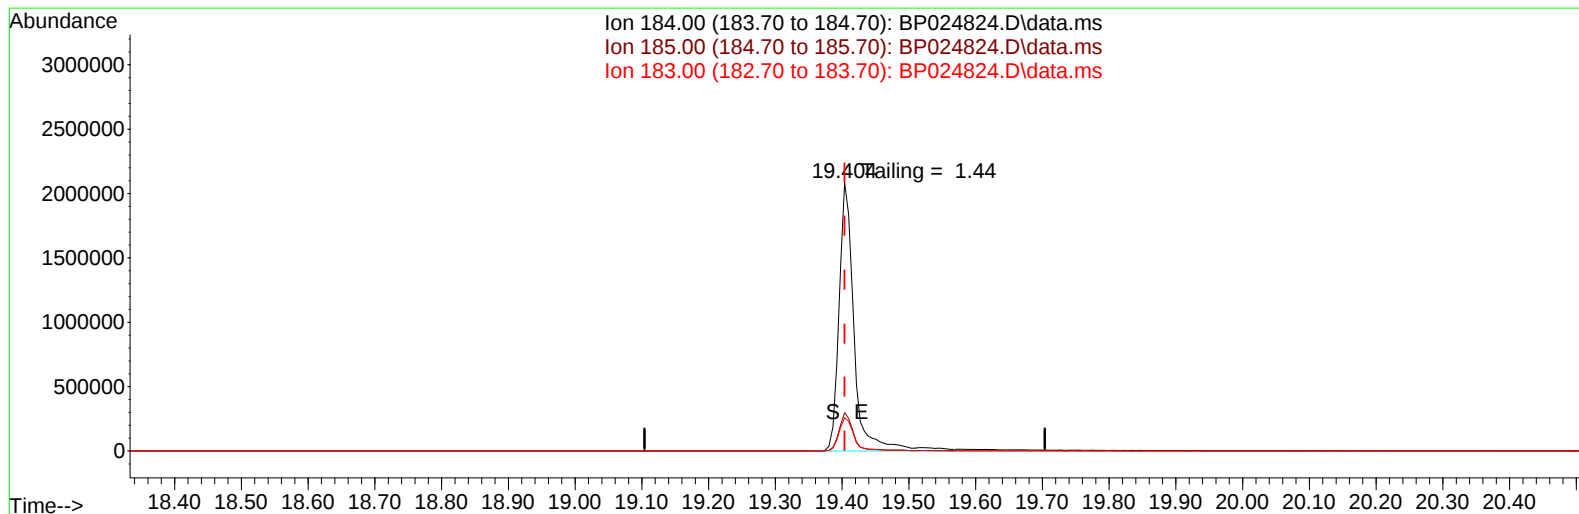

TIC: BP024824.D\data.ms

(77) Benzidine

19.404min (-0.000) 79757.81 ng

response 3219318

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.26
183.00	12.30	12.50
0.00	0.00	0.00