

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
 Data File : BP015331.D
 Acq On : 30 May 2023 13:06
 Operator : CG/JU
 Sample : PB153101BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK101

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	35	39	48	rVB	45937	74684	1.38%	0.138%
2	3.858	112	114	131	rBV	593693	946751	17.48%	1.751%
3	4.199	168	172	176	rBV	9551	13357	0.25%	0.025%
4	7.269	687	694	704	rBV	738067	1209480	22.33%	2.237%
5	7.434	715	722	730	rBV	612892	963236	17.78%	1.781%
6	7.640	748	757	767	rBV	786451	1275188	23.54%	2.358%
7	8.116	829	838	848	rBV	609130	970353	17.91%	1.794%
8	8.834	953	960	979	rBV	967881	1616481	29.84%	2.989%
9	9.293	1026	1038	1048	rBV	770737	1308422	24.15%	2.420%
10	10.022	1154	1162	1170	rBV	698446	1164253	21.49%	2.153%
11	10.569	1248	1255	1271	rBV	937219	1611743	29.75%	2.980%
12	10.951	1312	1320	1332	rBV	855198	1453388	26.83%	2.688%
13	11.087	1332	1343	1360	rBV	1037388	1788862	33.02%	3.308%
14	11.745	1449	1455	1462	rBV	4670	11918	0.22%	0.022%
15	12.528	1581	1588	1596	rBV	17088	32388	0.60%	0.060%
16	13.645	1774	1778	1782	rBV3	6254	9629	0.18%	0.018%
17	14.169	1858	1867	1879	rBV	1976780	2870871	52.99%	5.309%
18	14.463	1908	1917	1931	rBV	2142453	3237721	59.76%	5.987%
19	14.763	1960	1968	1977	rBV	1465295	2109706	38.94%	3.901%
20	14.881	1983	1988	1994	rBV10	4730	8542	0.16%	0.016%
21	14.969	1996	2003	2020	rBV	771602	1412899	26.08%	2.613%
22	15.157	2032	2035	2048	rVB7	16985	35610	0.66%	0.066%
23	15.757	2130	2137	2144	rBV	2809703	3977548	73.42%	7.355%
24	15.886	2152	2159	2171	rBV	1071633	1555954	28.72%	2.877%
25	15.998	2173	2178	2185	rVB2	14953	26584	0.49%	0.049%
26	16.539	2268	2270	2275	rVB6	3827	5834	0.11%	0.011%
27	16.839	2318	2321	2326	rVV6	4255	6806	0.13%	0.013%
28	16.898	2327	2331	2336	rVB8	4429	7630	0.14%	0.014%
29	17.186	2378	2380	2385	rVB6	3859	5745	0.11%	0.011%
30	17.310	2397	2401	2406	rBV4	4528	6929	0.13%	0.013%
31	17.522	2430	2437	2447	rBV	1951250	2735837	50.50%	5.059%
32	17.622	2447	2454	2463	rBV	3313187	4550467	84.00%	8.415%
33	18.374	2578	2582	2589	rBV2	71810	117156	2.16%	0.217%
34	19.421	2756	2760	2764	rBV	47500	58705	1.08%	0.109%
35	19.486	2768	2771	2776	rVV	44503	56970	1.05%	0.105%
36	19.604	2788	2791	2795	rBV5	27240	42837	0.79%	0.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015331.D
Acq On : 30 May 2023 13:06
Operator : CG/JU
Sample : PB153101BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	19.845	2826	2832	2839	rBV	4211918	5379488	99.30%	9.948%
38	21.604	3126	3131	3141	rVB	2194703	2889209	53.33%	5.343%
39	24.004	3532	3539	3548	rVB2	2571717	5417528	100.00%	10.018%
40	24.174	3561	3568	3581	rVB	1442019	3109768	57.40%	5.751%




Sum of corrected areas: 54076477

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015331.D
Acq On : 30 May 2023 13:06
Operator : CG/JU
Sample : PB153101BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

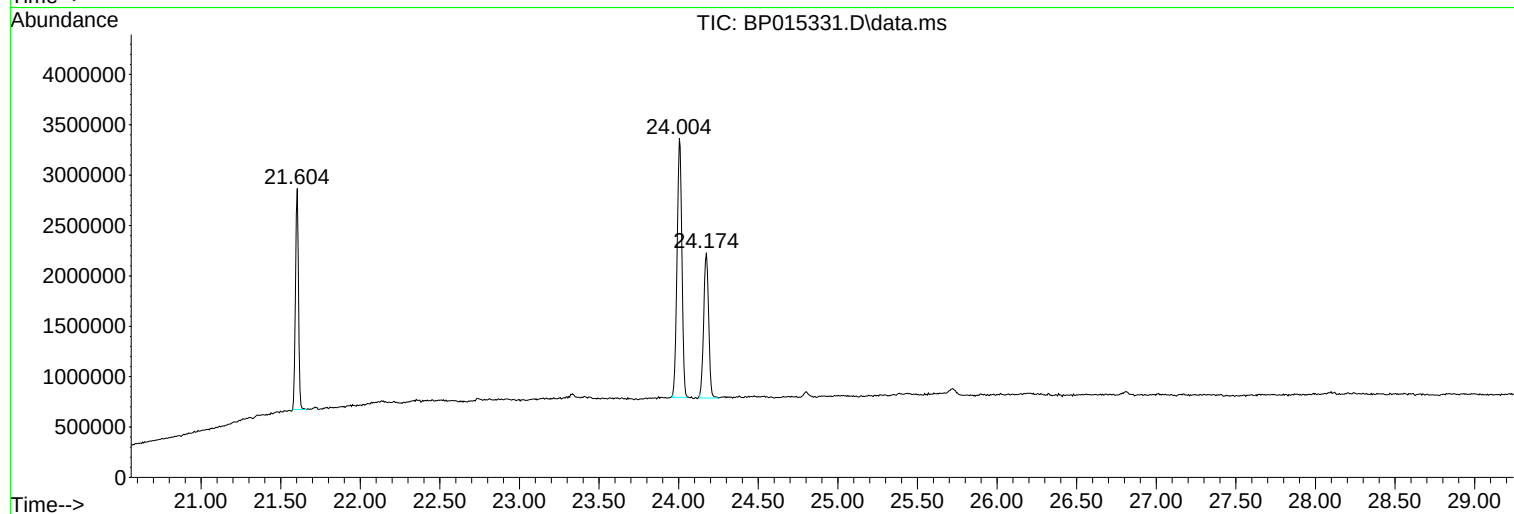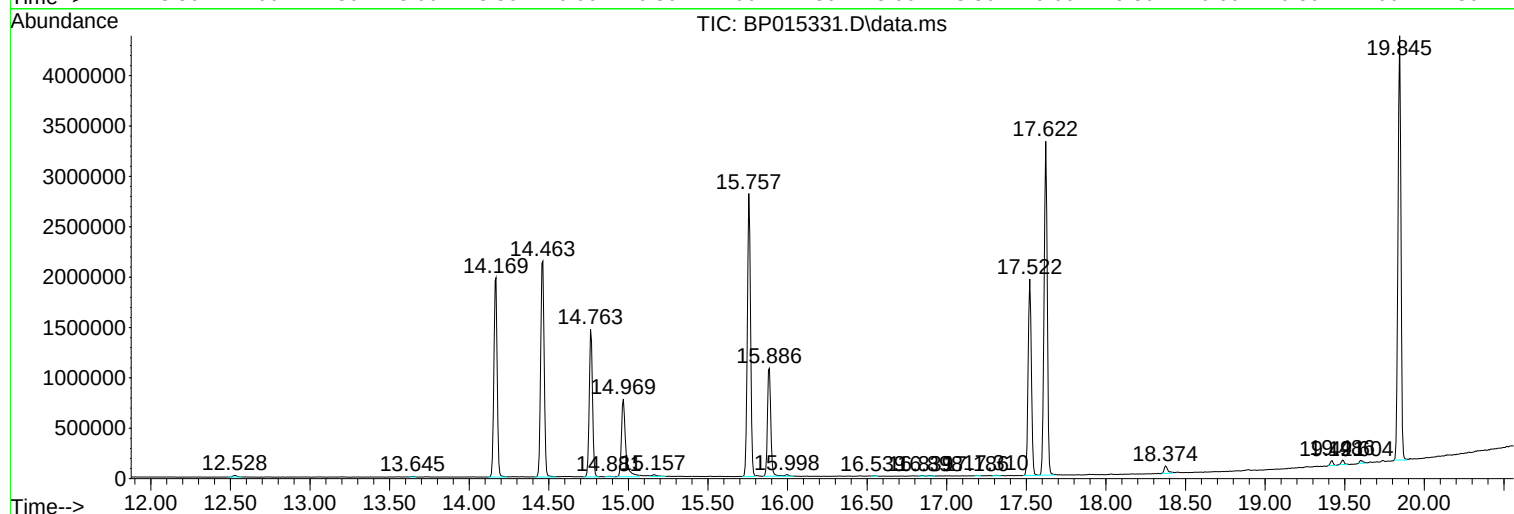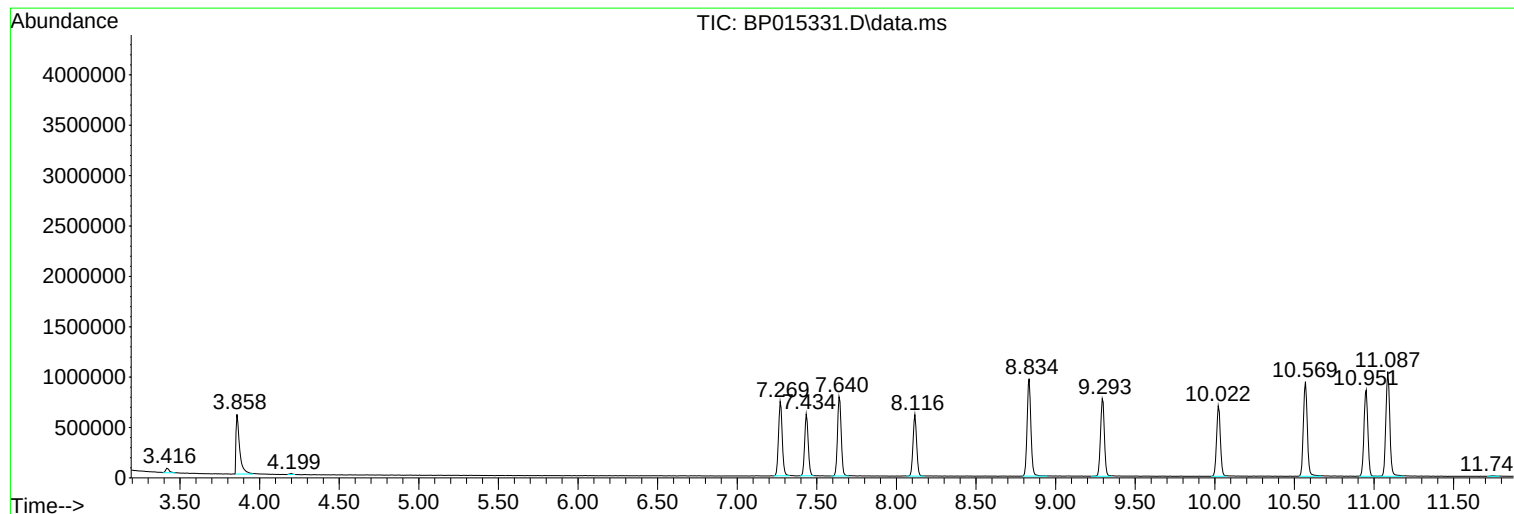

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015331.D
Acq On : 30 May 2023 13:06
Operator : CG/JU
Sample : PB153101BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015331.D
Acq On : 30 May 2023 13:06
Operator : CG/JU
Sample : PB153101BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc