

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
 Data File : BP015332.D
 Acq On : 30 May 2023 13:40
 Operator : CG/JU
 Sample : PB153103BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	36	39	50	rVB	56314	87534	1.47%	0.149%
2	3.858	111	114	135	rBV	650313	1026836	17.22%	1.746%
3	4.199	169	172	176	rVB4	8440	10760	0.18%	0.018%
4	7.269	685	694	704	rBV	789208	1305907	21.90%	2.221%
5	7.434	712	722	735	rVB	676853	1041239	17.46%	1.771%
6	7.640	749	757	767	rBV	864132	1369135	22.96%	2.328%
7	8.116	829	838	846	rBV	646776	1065278	17.87%	1.811%
8	8.828	952	959	974	rBV	1032248	1729313	29.00%	2.941%
9	9.293	1029	1038	1048	rBV	843416	1397748	23.44%	2.377%
10	10.016	1152	1161	1172	rBV	726709	1258164	21.10%	2.139%
11	10.563	1246	1254	1269	rBV	1005015	1744963	29.27%	2.967%
12	10.946	1309	1319	1329	rBV	957407	1607137	26.95%	2.733%
13	11.081	1334	1342	1358	rBV	1100200	1917787	32.16%	3.261%
14	12.528	1581	1588	1594	rBV2	16523	33161	0.56%	0.056%
15	13.645	1770	1778	1781	rBV10	5222	11243	0.19%	0.019%
16	13.728	1787	1792	1801	rVB10	3818	6018	0.10%	0.010%
17	14.163	1858	1866	1876	rBV	2151548	3082243	51.69%	5.241%
18	14.457	1908	1916	1929	rBV	2273415	3488526	58.51%	5.932%
19	14.757	1959	1967	1976	rBV	1604563	2325104	39.00%	3.954%
20	14.875	1983	1987	1992	rBV8	4872	7795	0.13%	0.013%
21	14.963	1995	2002	2026	rBV	817015	1544986	25.91%	2.627%
22	15.163	2033	2036	2043	rVB9	7789	12772	0.21%	0.022%
23	15.751	2129	2136	2149	rBV	2996226	4306192	72.22%	7.323%
24	15.875	2151	2157	2172	rVV	1177715	1712326	28.72%	2.912%
25	15.986	2172	2176	2186	rVB3	16850	31309	0.53%	0.053%
26	16.328	2229	2234	2237	rBV6	4952	8999	0.15%	0.015%
27	16.451	2251	2255	2261	rBV8	4099	7003	0.12%	0.012%
28	16.533	2266	2269	2274	rVB7	4822	6600	0.11%	0.011%
29	17.304	2396	2400	2402	rBV4	5373	7042	0.12%	0.012%
30	17.516	2429	2436	2446	rBV	2167019	3022970	50.70%	5.140%
31	17.616	2446	2453	2469	rVV2	3475326	4924383	82.59%	8.374%
32	18.369	2578	2581	2589	rBV9	15425	27763	0.47%	0.047%
33	19.410	2755	2758	2764	rBV4	47634	64941	1.09%	0.110%
34	19.480	2767	2770	2776	rVB	45531	63088	1.06%	0.107%
35	19.839	2825	2831	2838	rBV	4276099	5913366	99.18%	10.056%
36	21.592	3124	3129	3137	rBV	2414224	3261767	54.71%	5.547%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015332.D
Acq On : 30 May 2023 13:40
Operator : CG/JU
Sample : PB153103BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	23.992	3530	3537	3547	rVB2	2845109	5962381	100.00%	10.139%
38	24.157	3559	3565	3575	rVB	1597439	3413336	57.25%	5.804%




Sum of corrected areas: 58807115

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015332.D
Acq On : 30 May 2023 13:40
Operator : CG/JU
Sample : PB153103BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

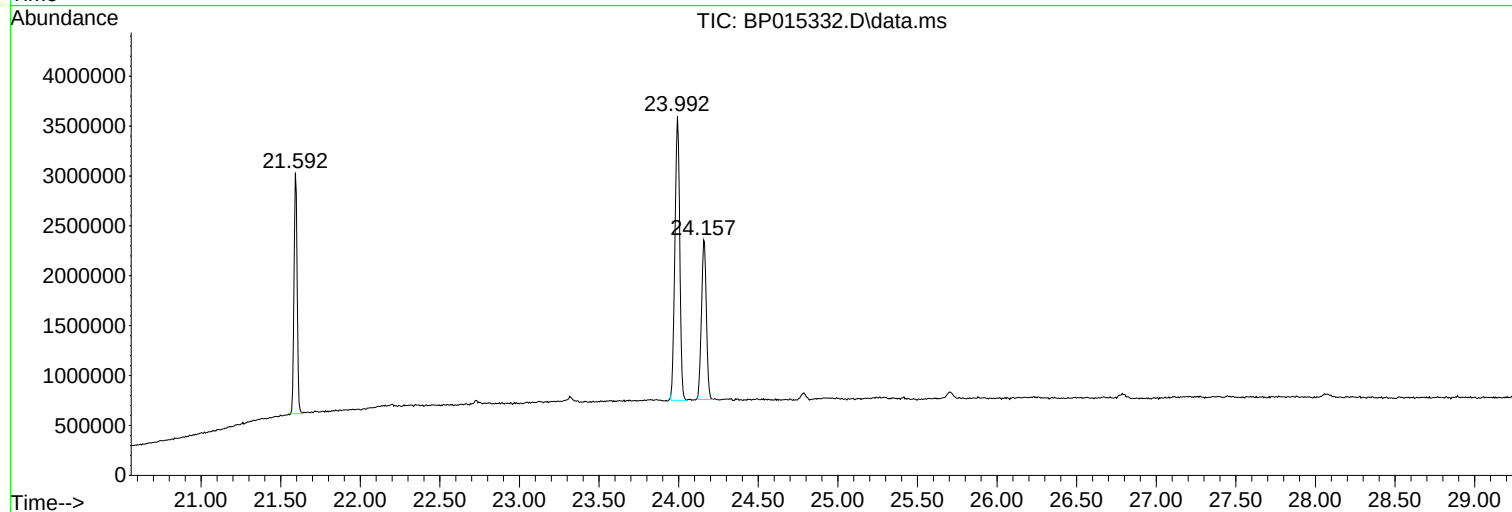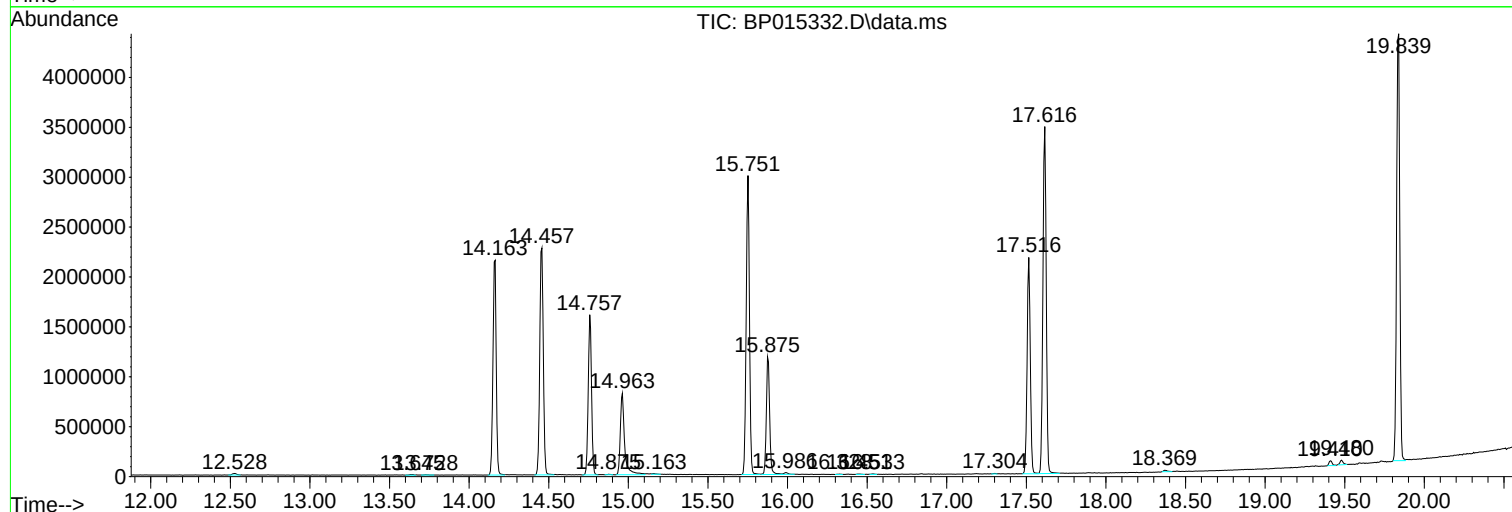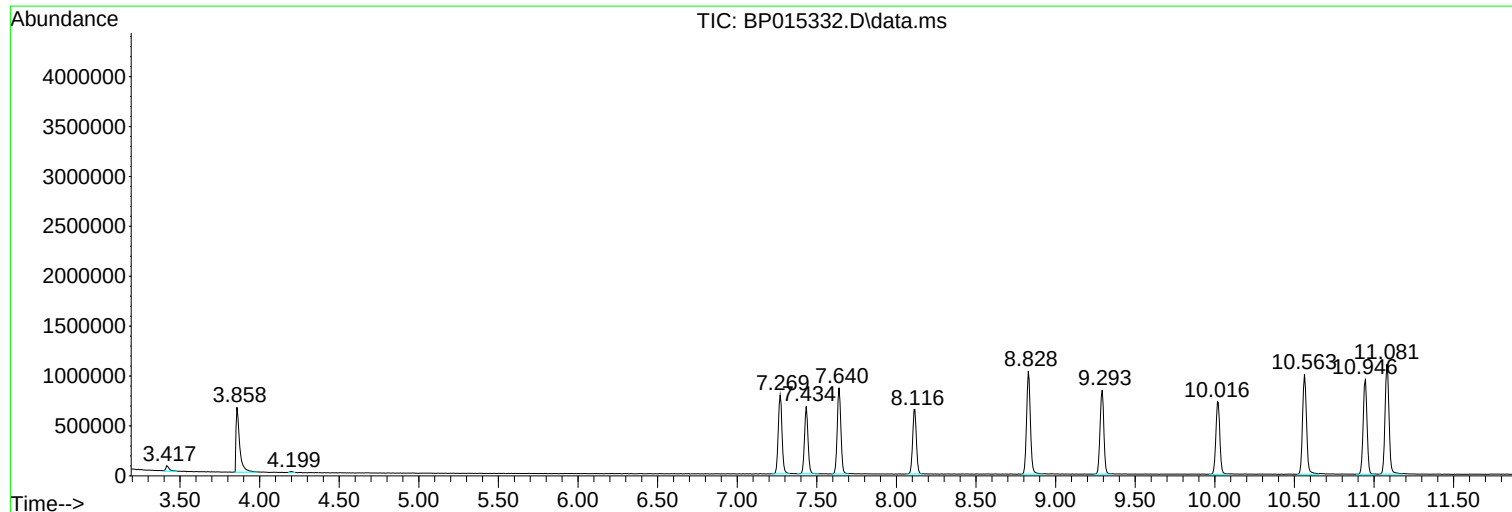

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015332.D
Acq On : 30 May 2023 13:40
Operator : CG/JU
Sample : PB153103BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053023\
Data File : BP015332.D
Acq On : 30 May 2023 13:40
Operator : CG/JU
Sample : PB153103BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc