
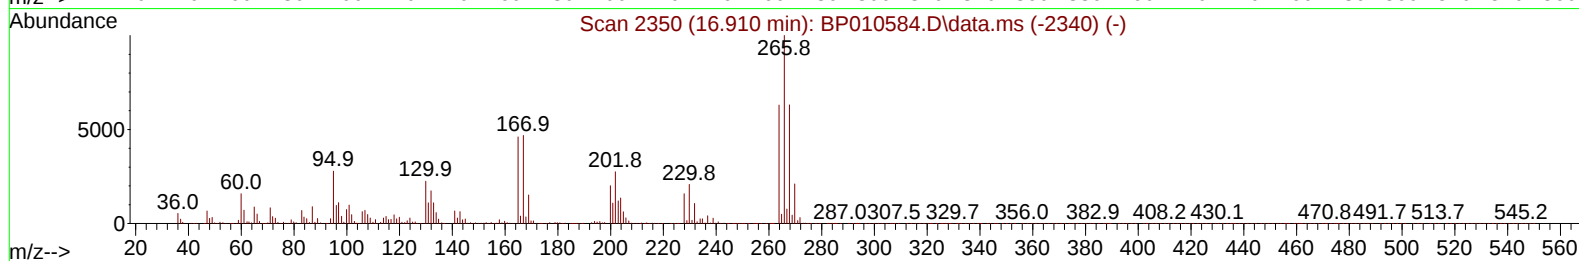
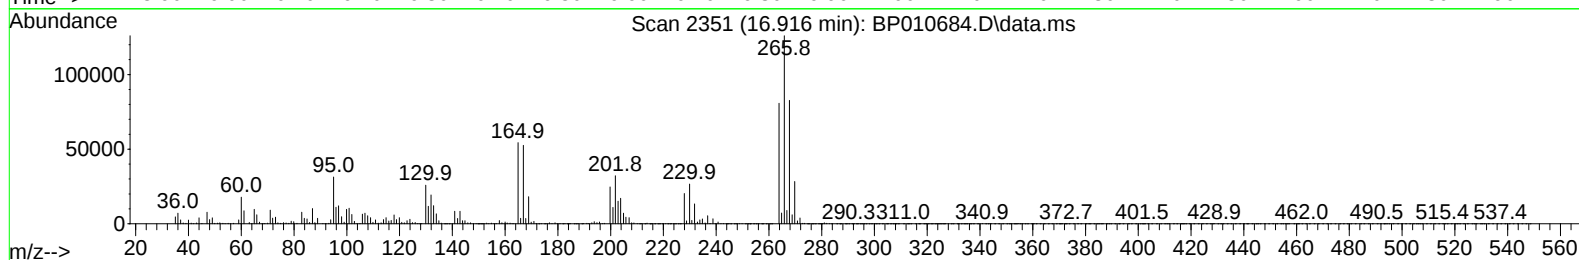


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060322\
Data File : BP010684.D
Acq On : 03 Jun 2022 10:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 04:52:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 01:56:43 2022
Response via : Initial Calibration

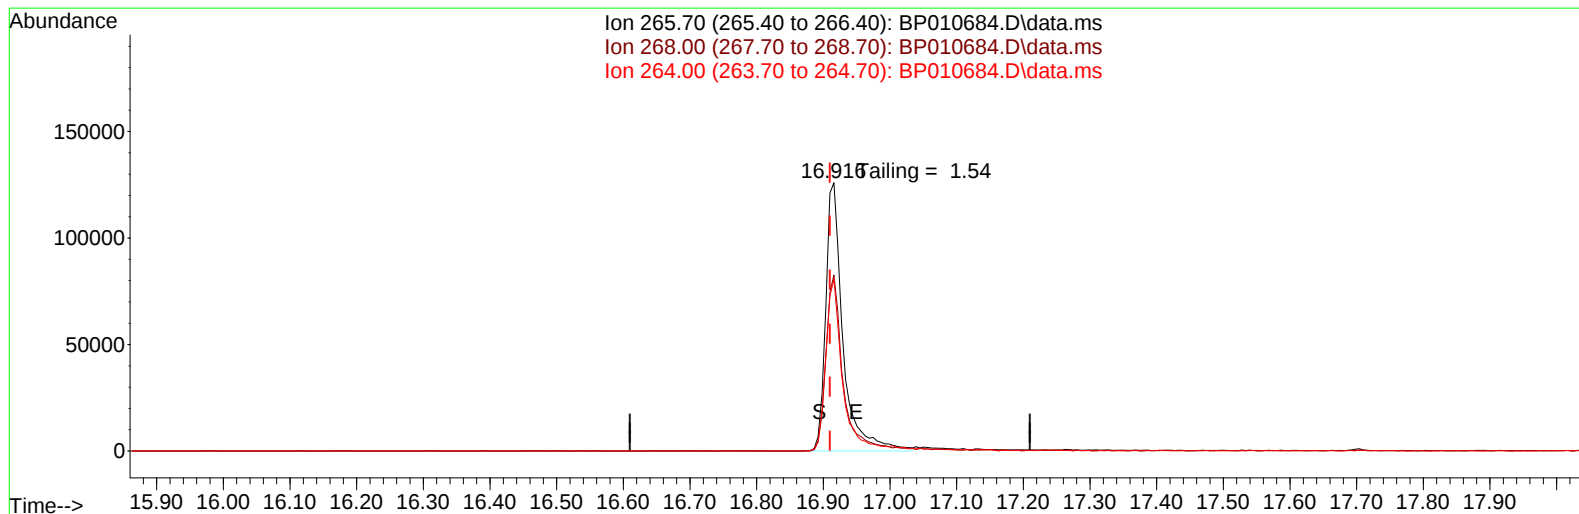

TIC: BP010684.D\data.ms

(70) Pentachlorophenol (C)




16.916min (+ 0.006) 2999317.57 ng

response 227576

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.58
264.00	63.00	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060322\
 Data File : BP010684.D
 Acq On : 03 Jun 2022 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 04:52:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 01:56:43 2022
 Response via : Initial Calibration

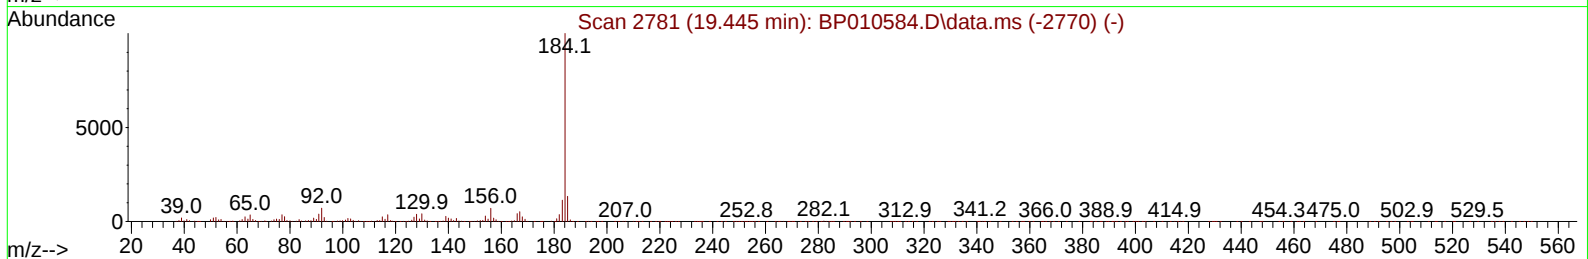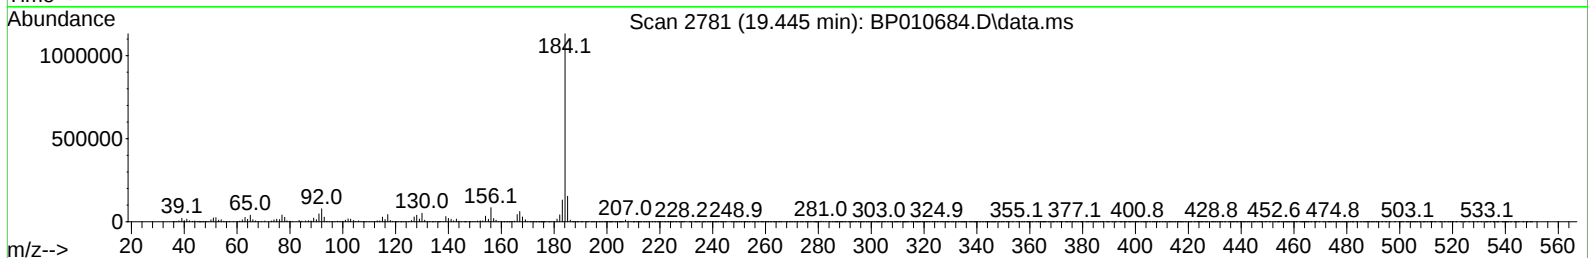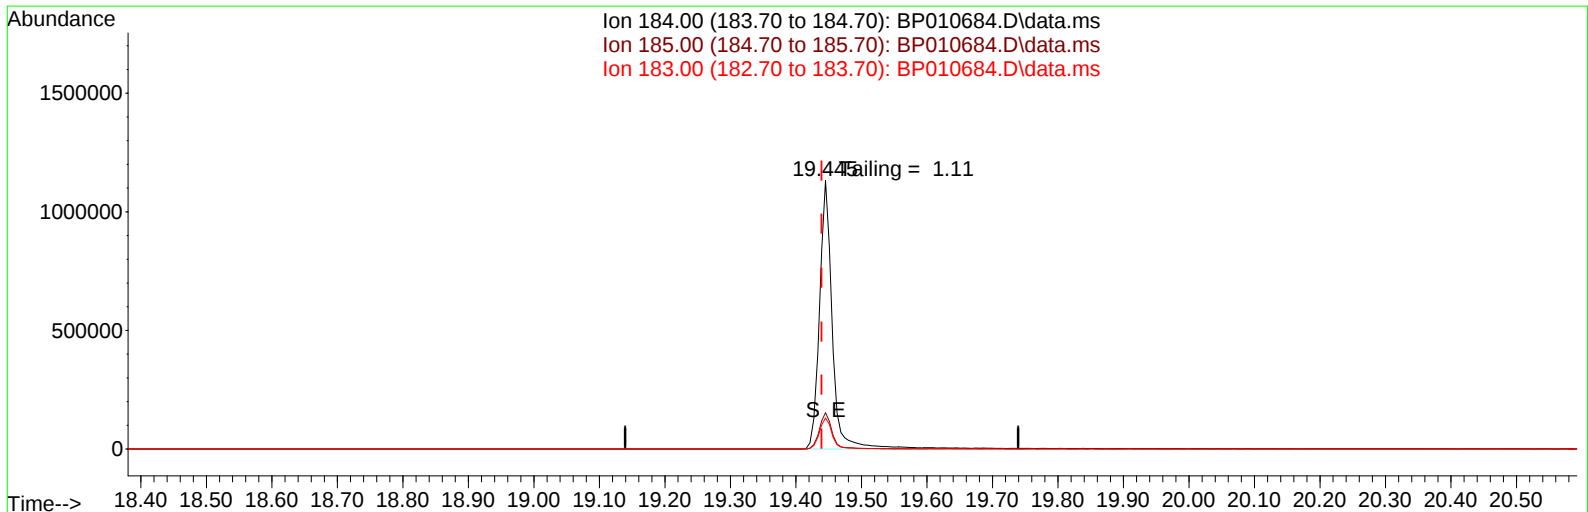

TIC: BP010684.D\data.ms

(77) Benzidine**19.445min (+ 0.006) 384518.52 ng****response 1528975**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.57
183.00	11.30	11.60
0.00	0.00	0.00