
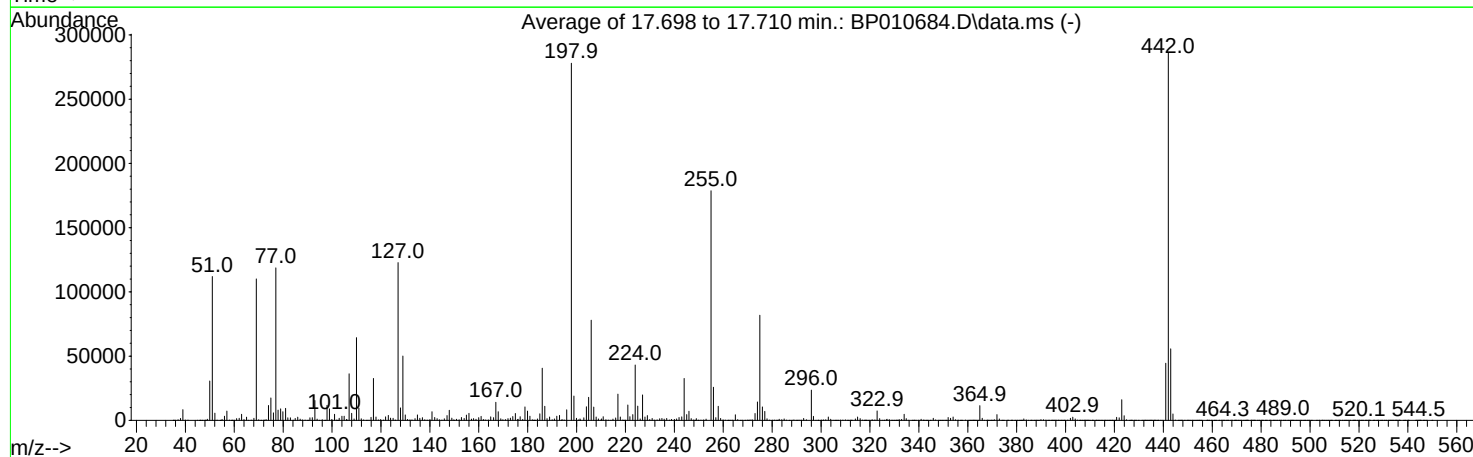


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060322\
 Data File : BP010684.D
 Acq On : 03 Jun 2022 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 04 01:56:43 2022

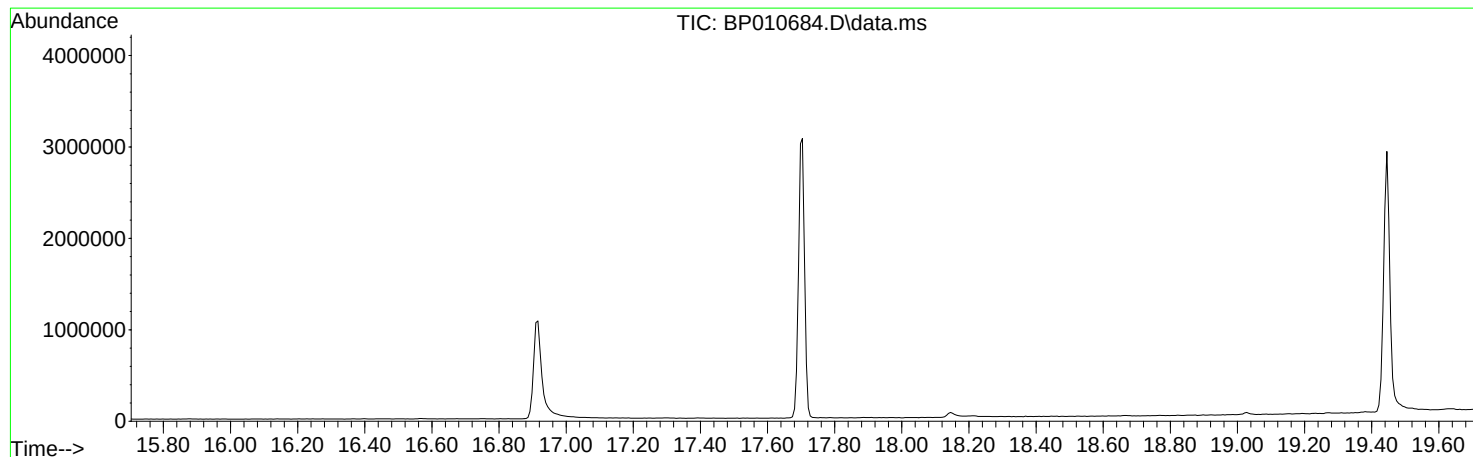

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	112022	PASS
68	69	0.00	2	1.5	1658	PASS
69	198	0.00	100	39.6	110076	PASS
70	69	0.00	2	0.4	495	PASS
127	198	10	80	44.2	122818	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	277973	PASS
199	198	5	9	6.8	18886	PASS
275	198	10	60	29.4	81792	PASS
365	198	1	100	4.1	11481	PASS
441	198	0.01	100	16.0	44456	PASS
442	442	100	100	100.0	286336	PASS
443	442	15	24	19.5	55707	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/3/2022	BNA_P	<u>BP010684.D</u>
Compound Name	Response	Retention Time
DDT	891495	20.645
DDD	18985	20.221
DDE	2409	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21394	912889	2.34

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060322\
 Data File : BP010684.D
 Acq On : 03 Jun 2022 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 04 04:52:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 01:56:43 2022
 Response via : Initial Calibration

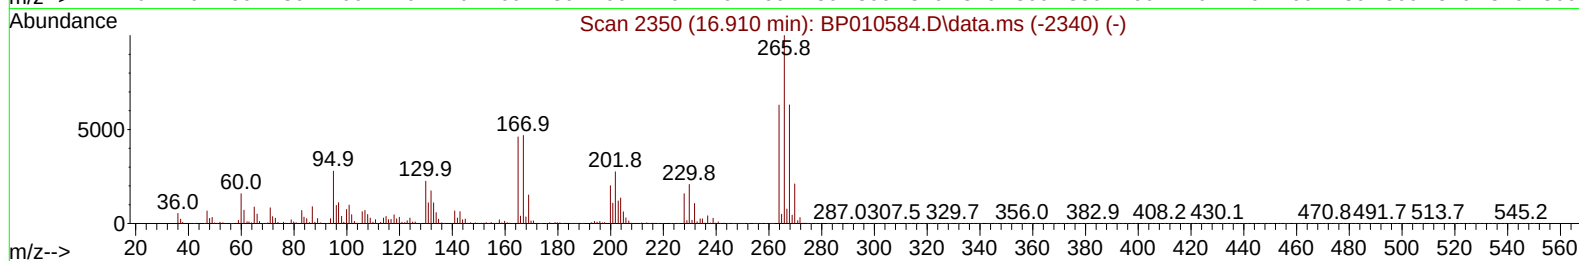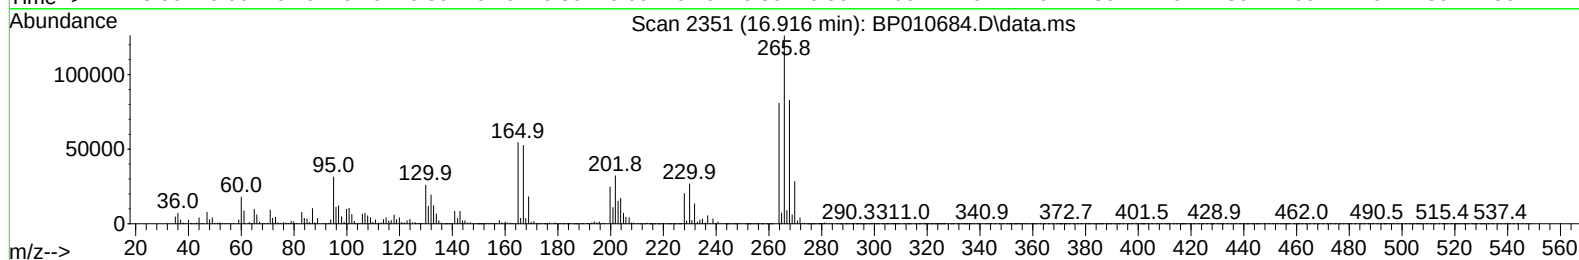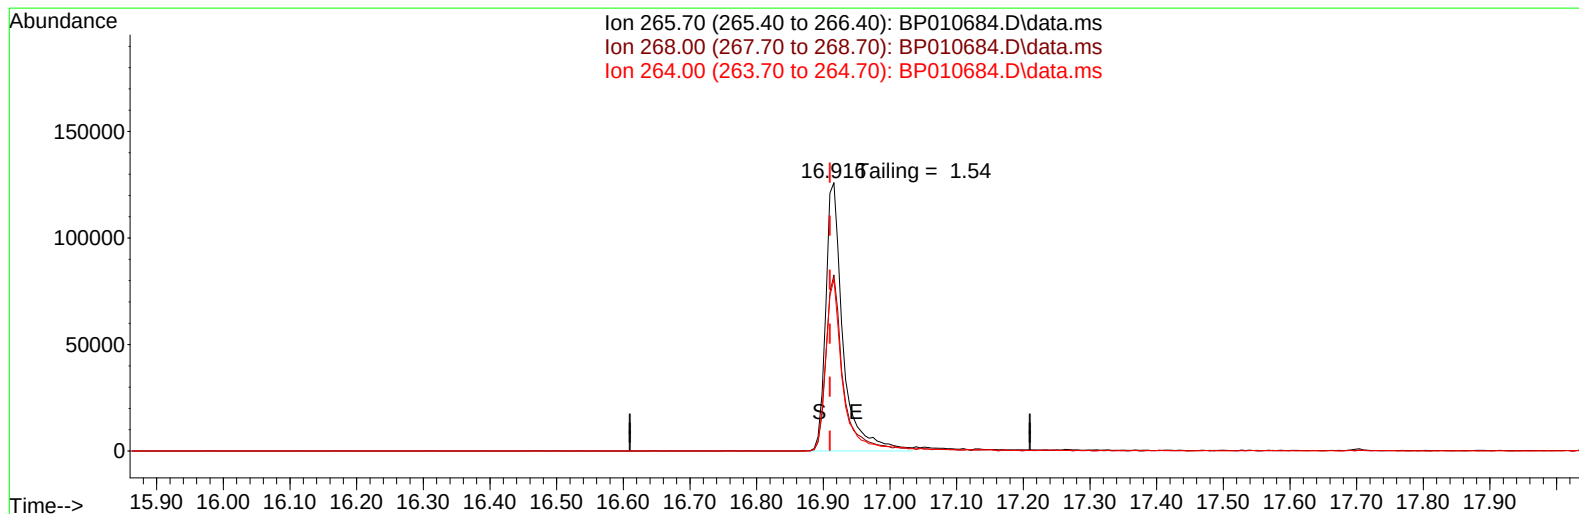

TIC: BP010684.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.006) 2999317.57 ng




response 227576

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.58
264.00	63.00	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060322\
Data File : BP010684.D
Acq On : 03 Jun 2022 10:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 04 04:52:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 01:56:43 2022
Response via : Initial Calibration

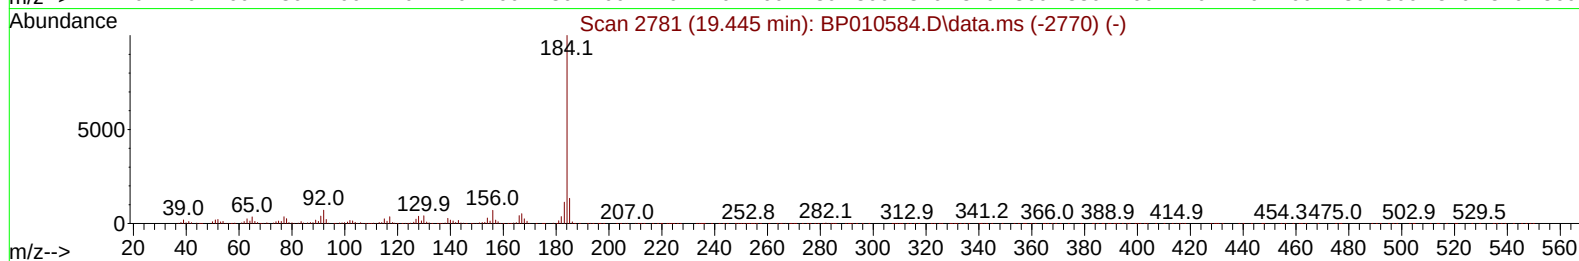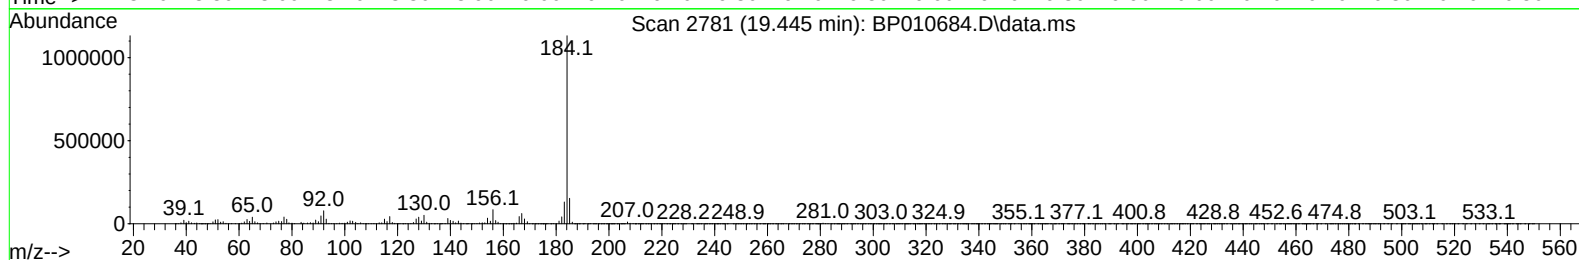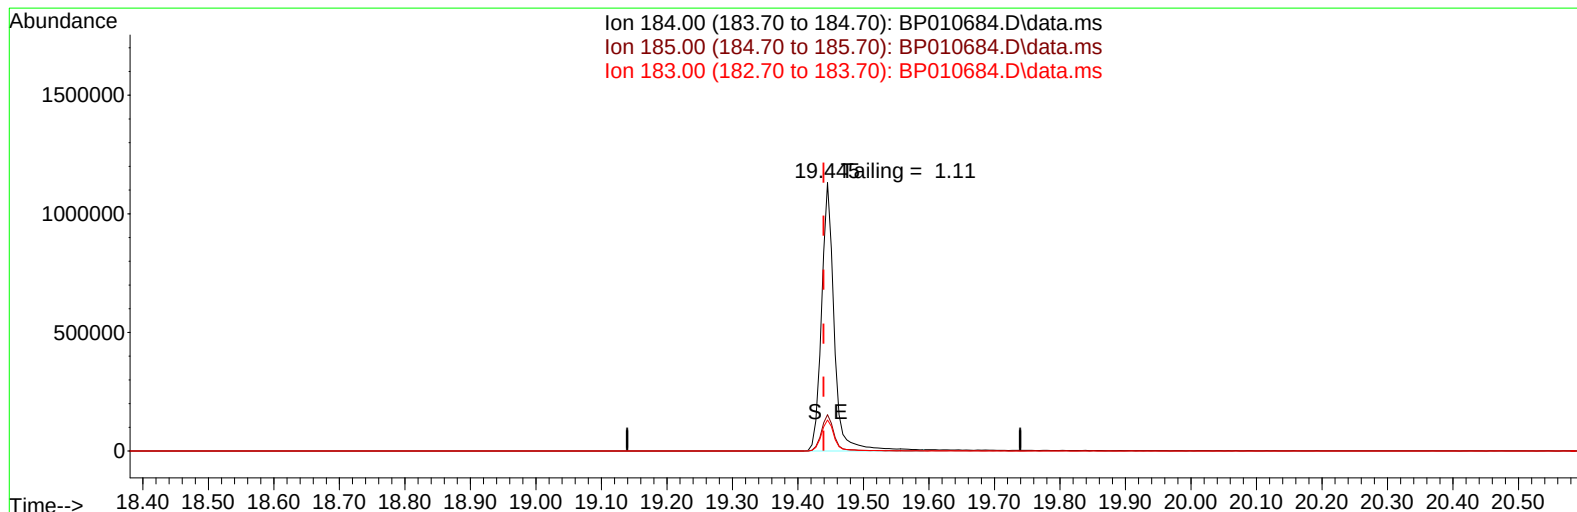

TIC: BP010684.D\data.ms

(77) Benzidine

19.445min (+ 0.006) 384518.52 ng

response 1528975

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.57
183.00	11.30	11.60
0.00	0.00	0.00