
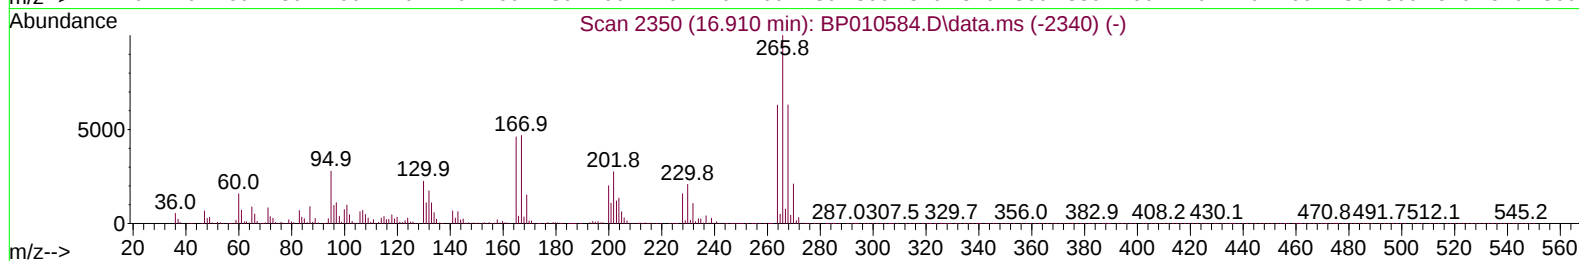
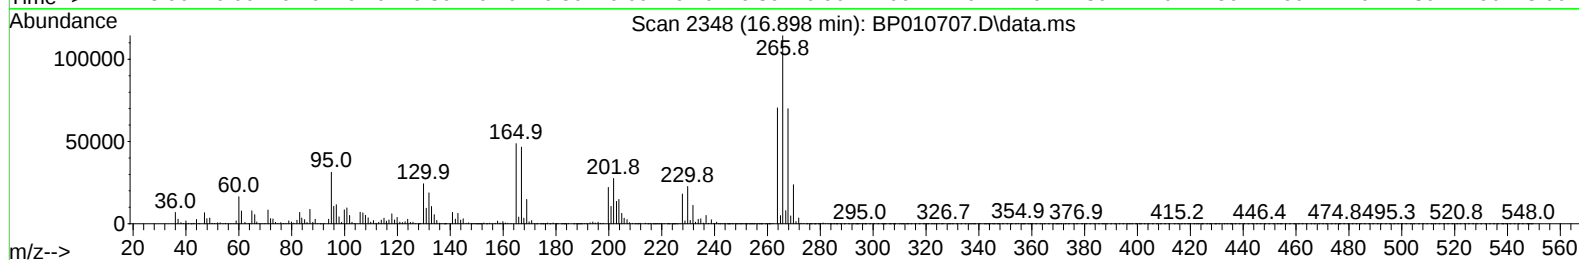


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
 Data File : BP010707.D
 Acq On : 07 Jun 2022 13:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 17:07:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 16:59:38 2022
 Response via : Initial Calibration

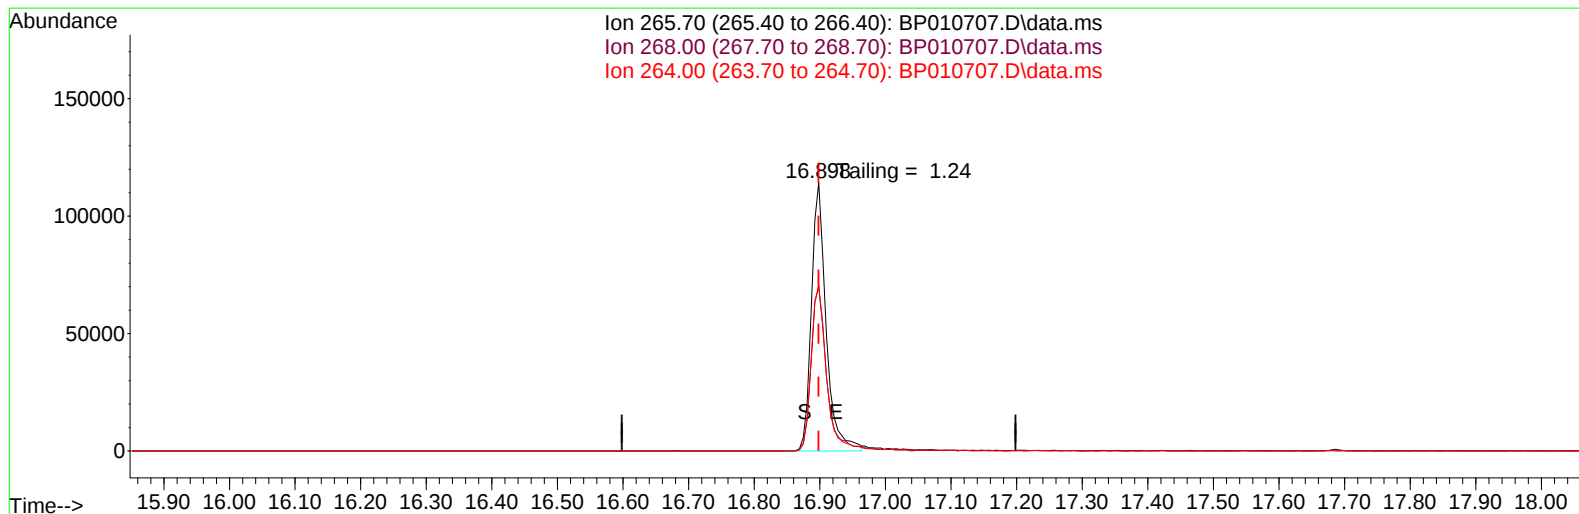

TIC: BP010707.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.000) 224536.95 ng

response 182760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.16
264.00	63.00	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
 Data File : BP010707.D
 Acq On : 07 Jun 2022 13:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 17:07:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 16:59:38 2022
 Response via : Initial Calibration

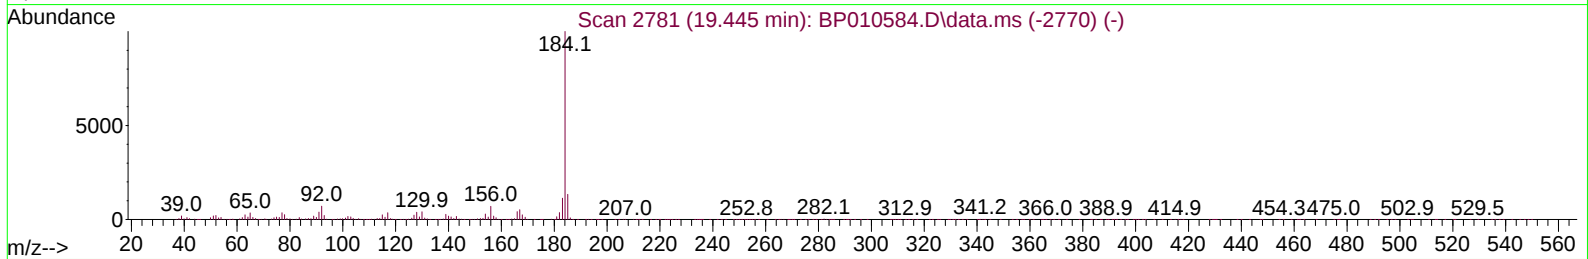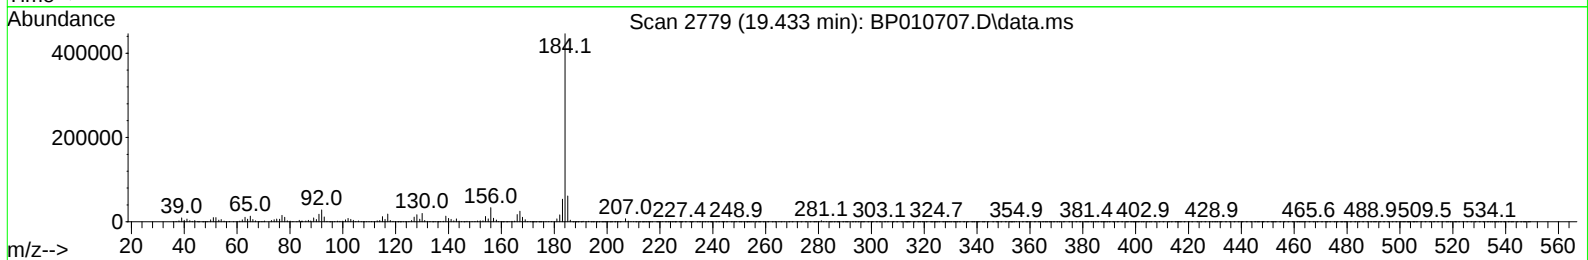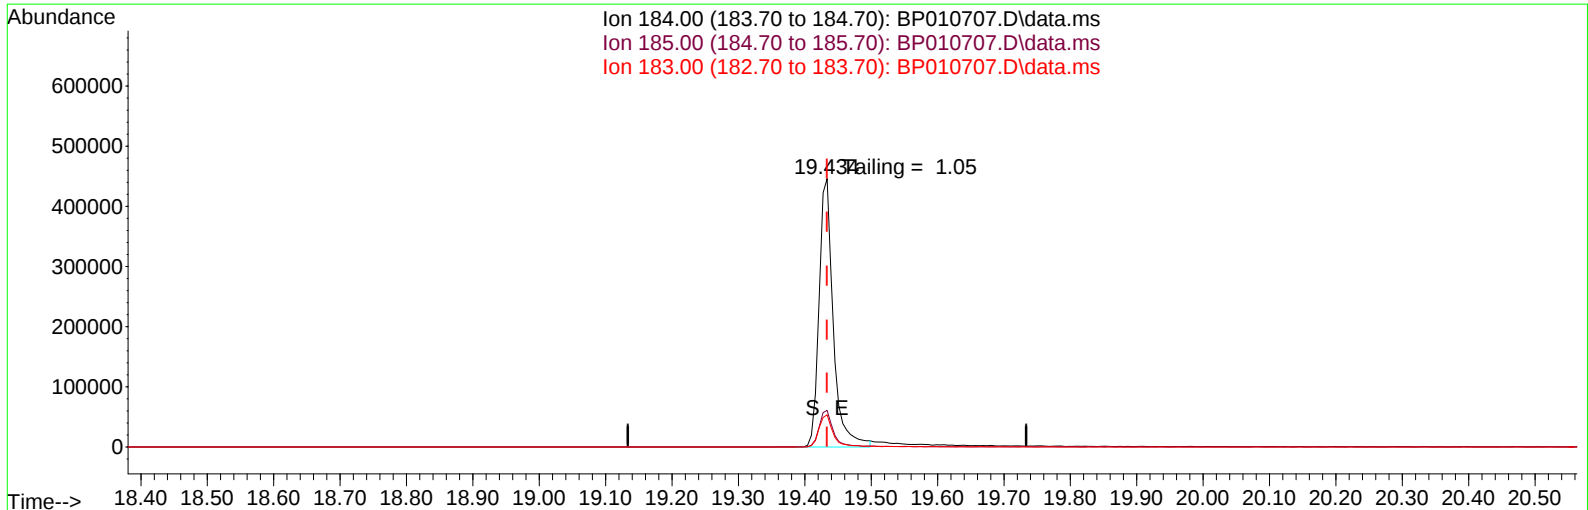

TIC: BP010707.D\data.ms

(77) Benzidine**19.433min (0.000) 35504.36 ng****response 688836**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.69
183.00	11.30	12.01
0.00	0.00	0.00