

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
 Data File : BP010716.D
 Acq On : 07 Jun 2022 19:48
 Operator : CG/JU
 Sample : PB145306BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB145306BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	417	rBV	2061381	3119810	38.13%	9.014%
2	7.017	661	668	684	rBV	1902317	3190085	38.99%	9.217%
3	7.840	800	808	816	rBV	367367	594933	7.27%	1.719%
4	8.999	998	1005	1026	rBV	1170645	2099907	25.67%	6.067%
5	10.640	1275	1284	1300	rBV	399063	778178	9.51%	2.248%
6	13.099	1691	1702	1728	rBV	2689241	4143615	50.64%	11.972%
7	14.475	1930	1936	1955	rBV	569273	941836	11.51%	2.721%
8	15.975	2183	2191	2209	rBV	1950018	3028808	37.02%	8.751%
9	17.234	2398	2405	2418	rBV	655030	1049037	12.82%	3.031%
10	19.792	2835	2840	2851	rBV	4464696	5549358	67.83%	16.033%
11	21.328	3096	3101	3106	rBV	733785	986497	12.06%	2.850%
12	21.439	3114	3120	3140	rBV	5484719	8181771	100.00%	23.638%
13	23.733	3504	3510	3519	rVB	452065	948408	11.59%	2.740%




Sum of corrected areas: 34612243

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
Data File : BP010716.D
Acq On : 07 Jun 2022 19:48
Operator : CG/JU
Sample : PB145306BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145306BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

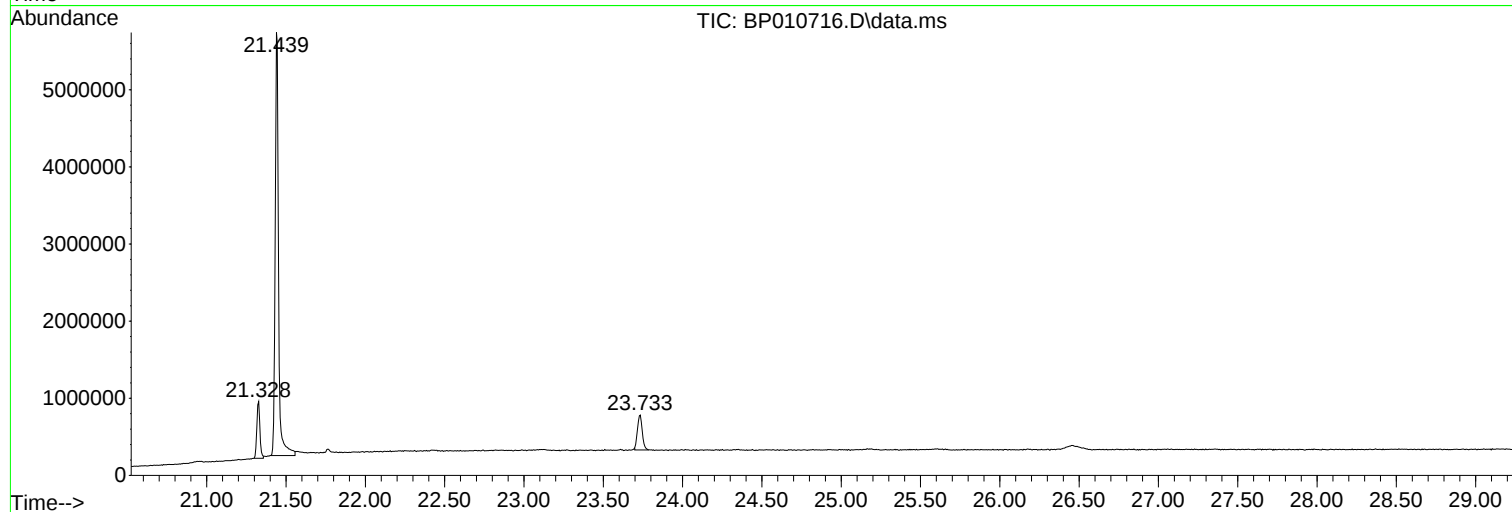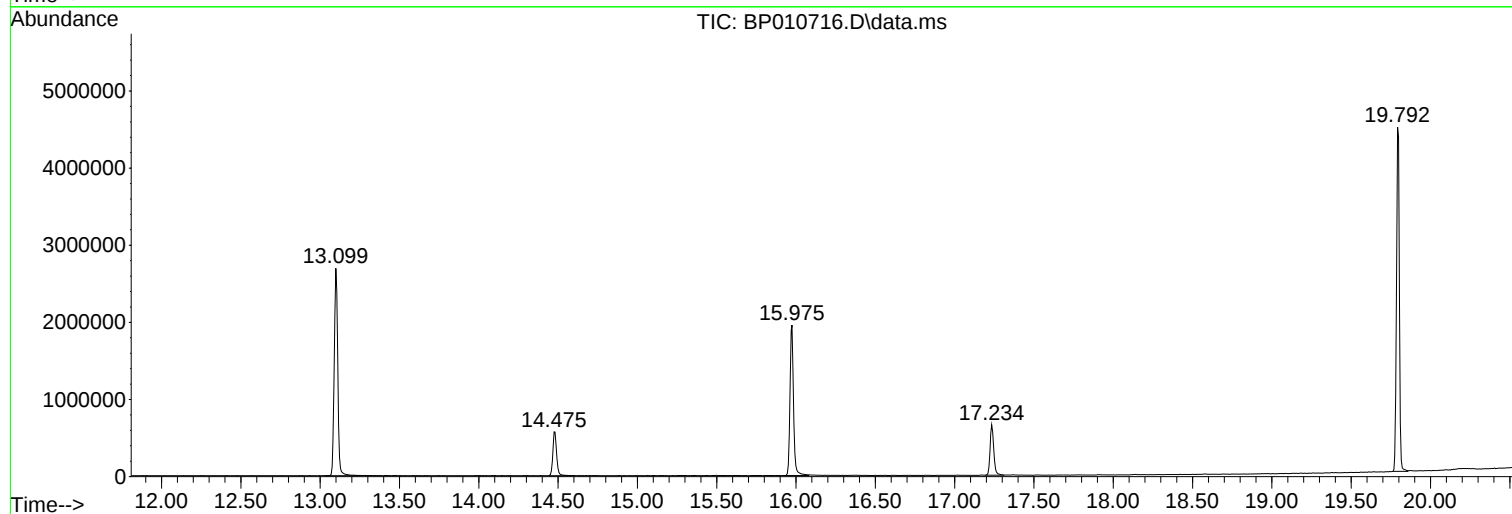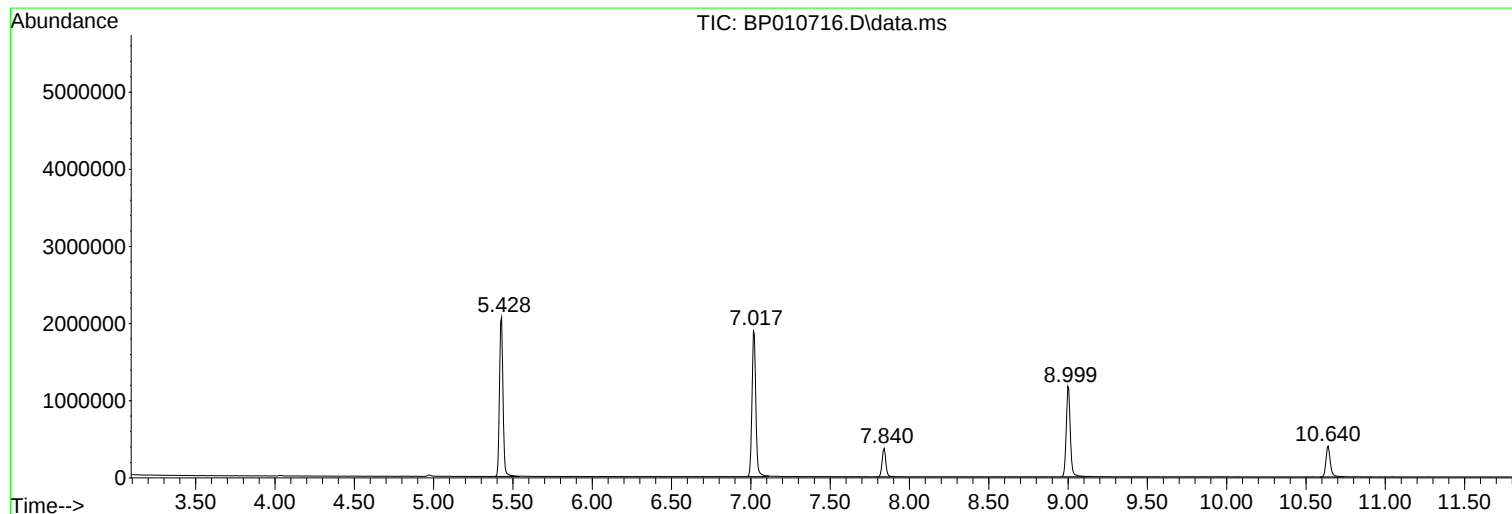

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
Data File : BP010716.D
Acq On : 07 Jun 2022 19:48
Operator : CG/JU
Sample : PB145306BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145306BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.439	165.88 ng	8181770	Chrysene-d12	21.328

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	87
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			4-Nitro-4'-methyldiphenylsulfone	277	C13H11NO4S	004094-37-5	38
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	37

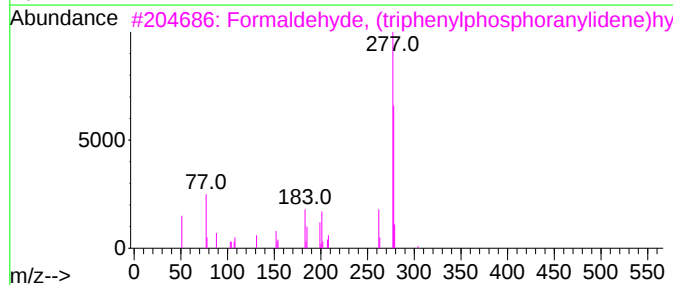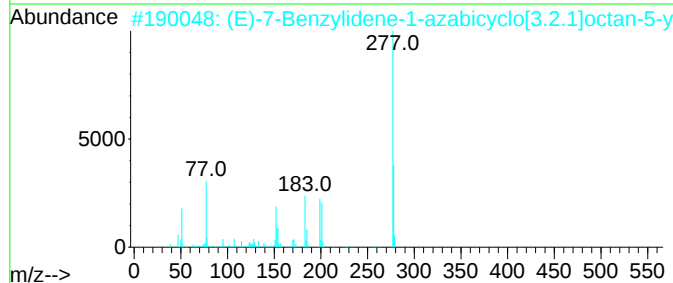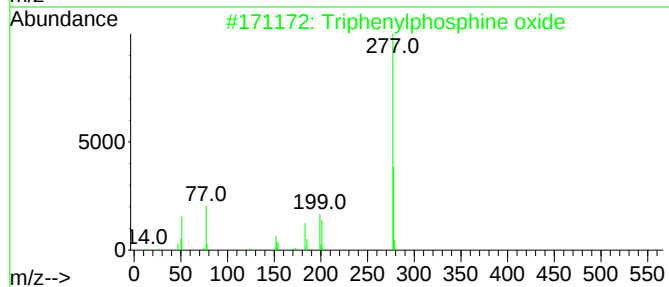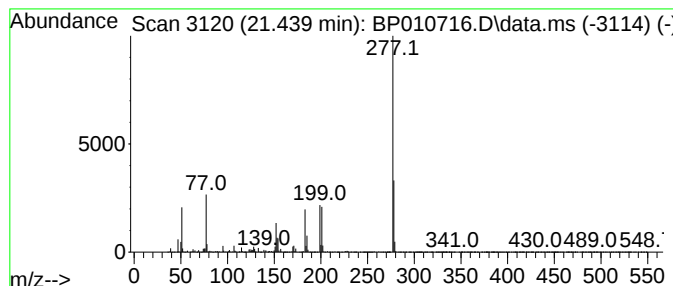

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
Data File : BP010716.D
Acq On : 07 Jun 2022 19:48
Operator : CG/JU
Sample : PB145306BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145306BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.439	165.9	ng	8181770	5	21.328	986497	20.0