


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
Data File : BP010707.D
Acq On : 07 Jun 2022 13:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 07 19:29:31 2022

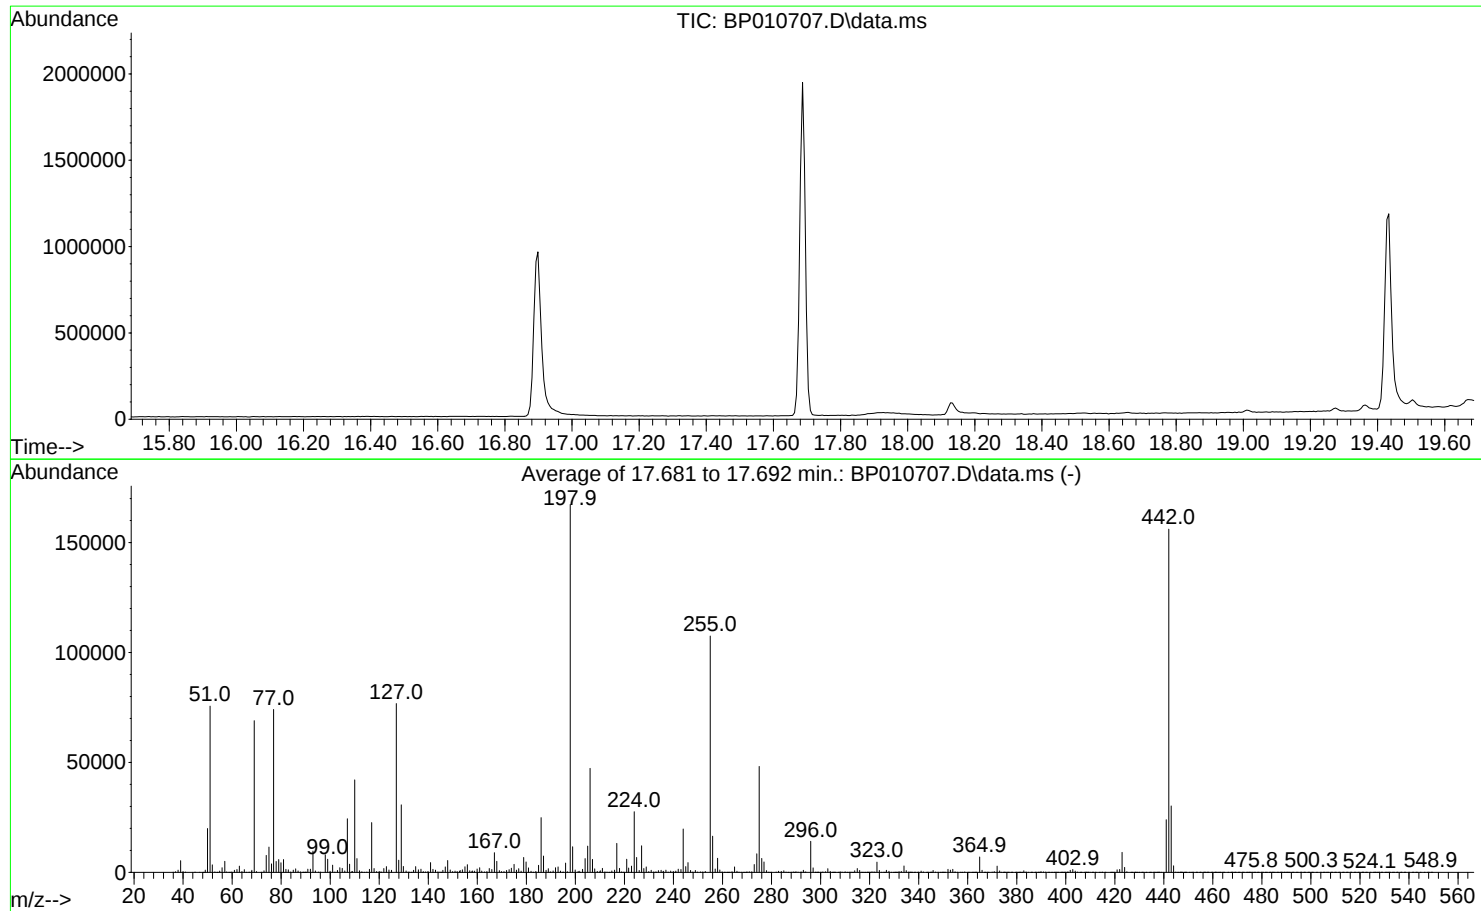




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.2	75606	PASS
68	69	0.00	2	1.4	960	PASS
69	198	0.00	100	41.2	68969	PASS
70	69	0.00	2	0.5	347	PASS
127	198	10	80	45.9	76799	PASS
197	198	0.00	2	0.2	333	PASS
198	198	100	100	100.0	167305	PASS
199	198	5	9	7.0	11663	PASS
275	198	10	60	28.8	48160	PASS
365	198	1	100	4.2	6963	PASS
441	198	0.01	100	14.3	23950	PASS
442	442	100	100	100.0	156059	PASS
443	442	15	24	19.3	30186	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
 Data File : BP010707.D
 Acq On : 07 Jun 2022 13:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 17:07:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 16:59:38 2022
 Response via : Initial Calibration

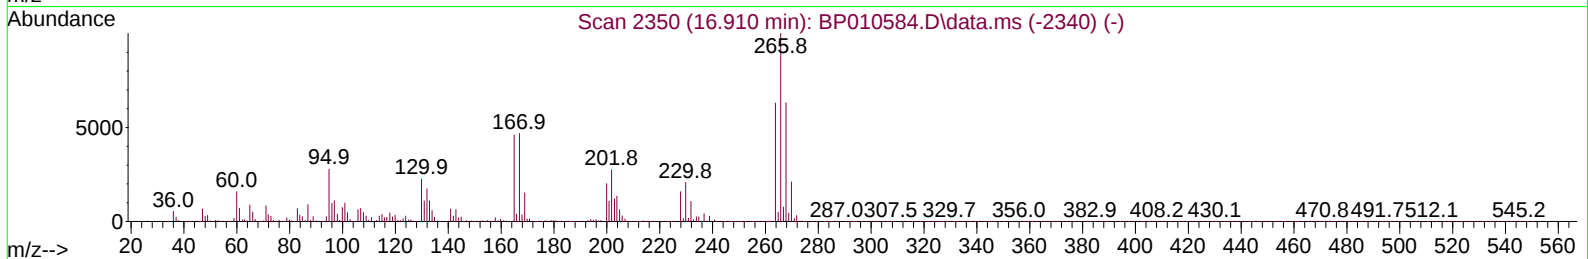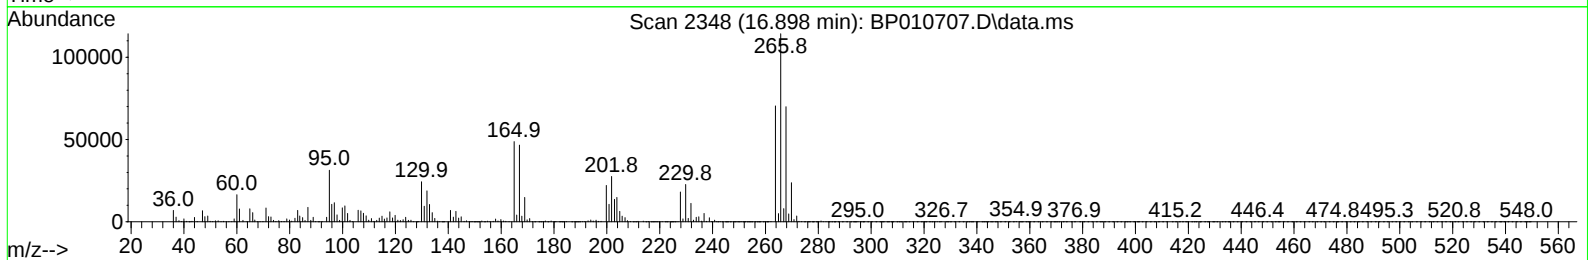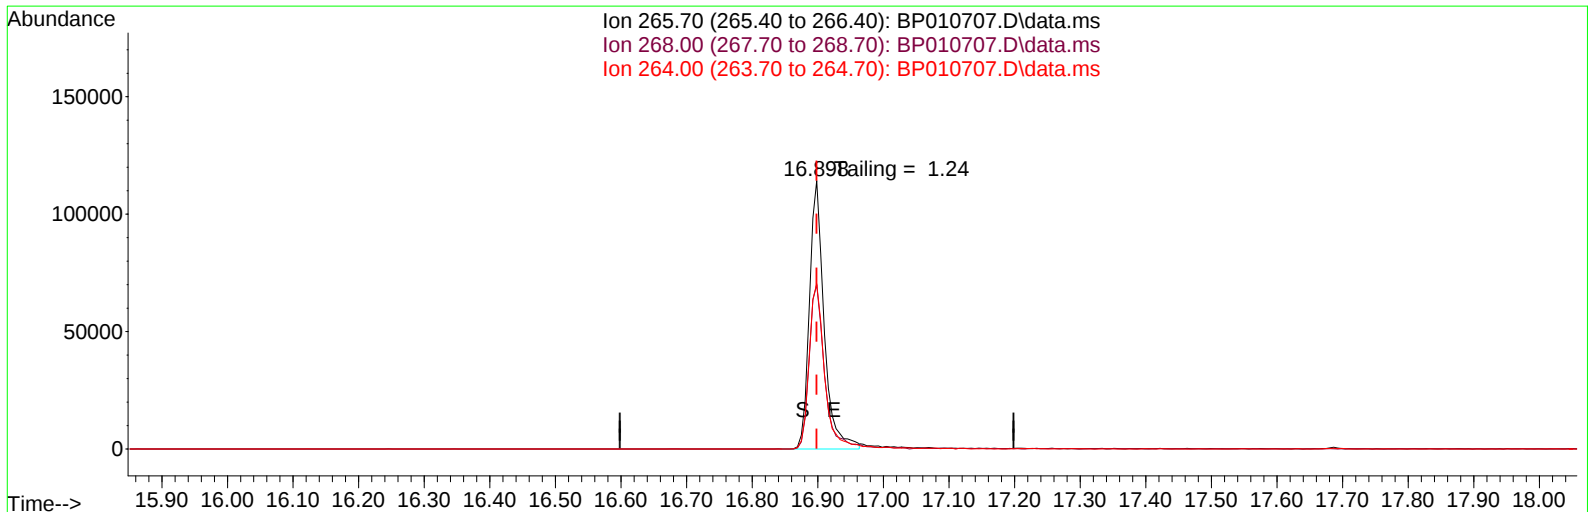

TIC: BP010707.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.000) 224536.95 ng




response 182760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.16
264.00	63.00	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060722\
Data File : BP010707.D
Acq On : 07 Jun 2022 13:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 07 17:07:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 16:59:38 2022
Response via : Initial Calibration

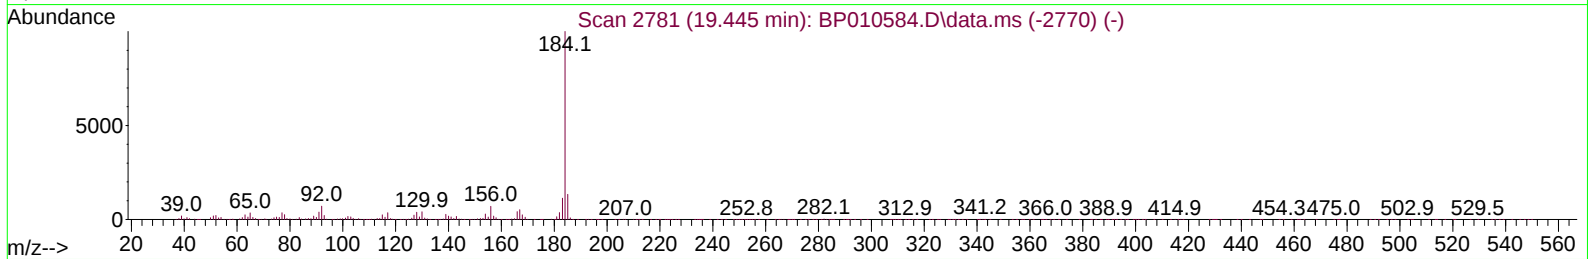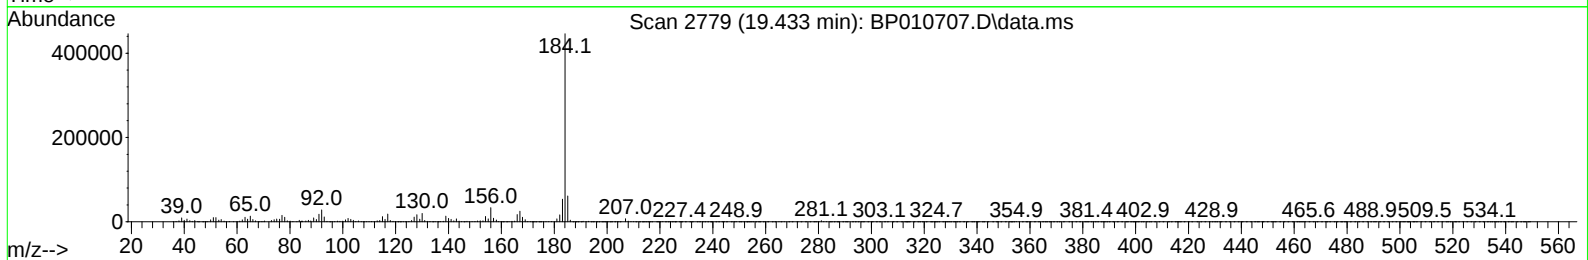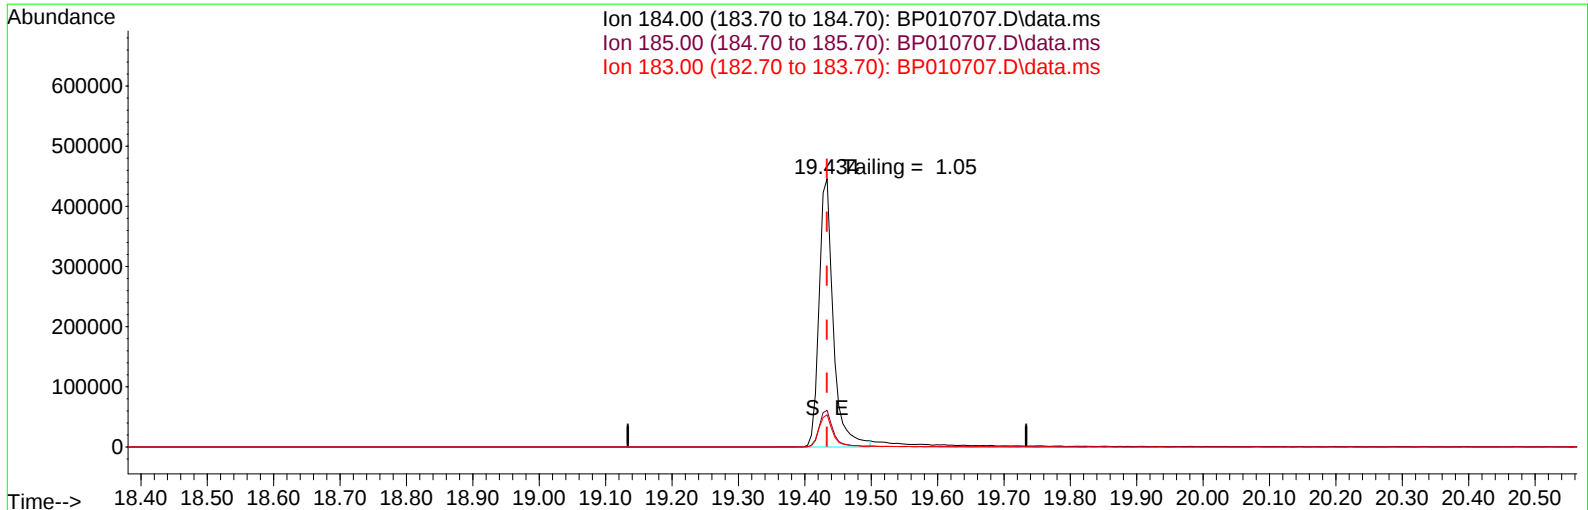

TIC: BP010707.D\data.ms

(77) Benzidine

19.433min (0.000) 35504.36 ng

response 688836

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.69
183.00	11.30	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2022	BNA_P	<u>BP010707.D</u>
Compound Name	Response	Retention Time
DDT	450243	20.63
DDD	2314	20.21
DDE	760	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3074	453317	0.68

Instrument :
BNA_P
ClientSampleId :
DFTPP