



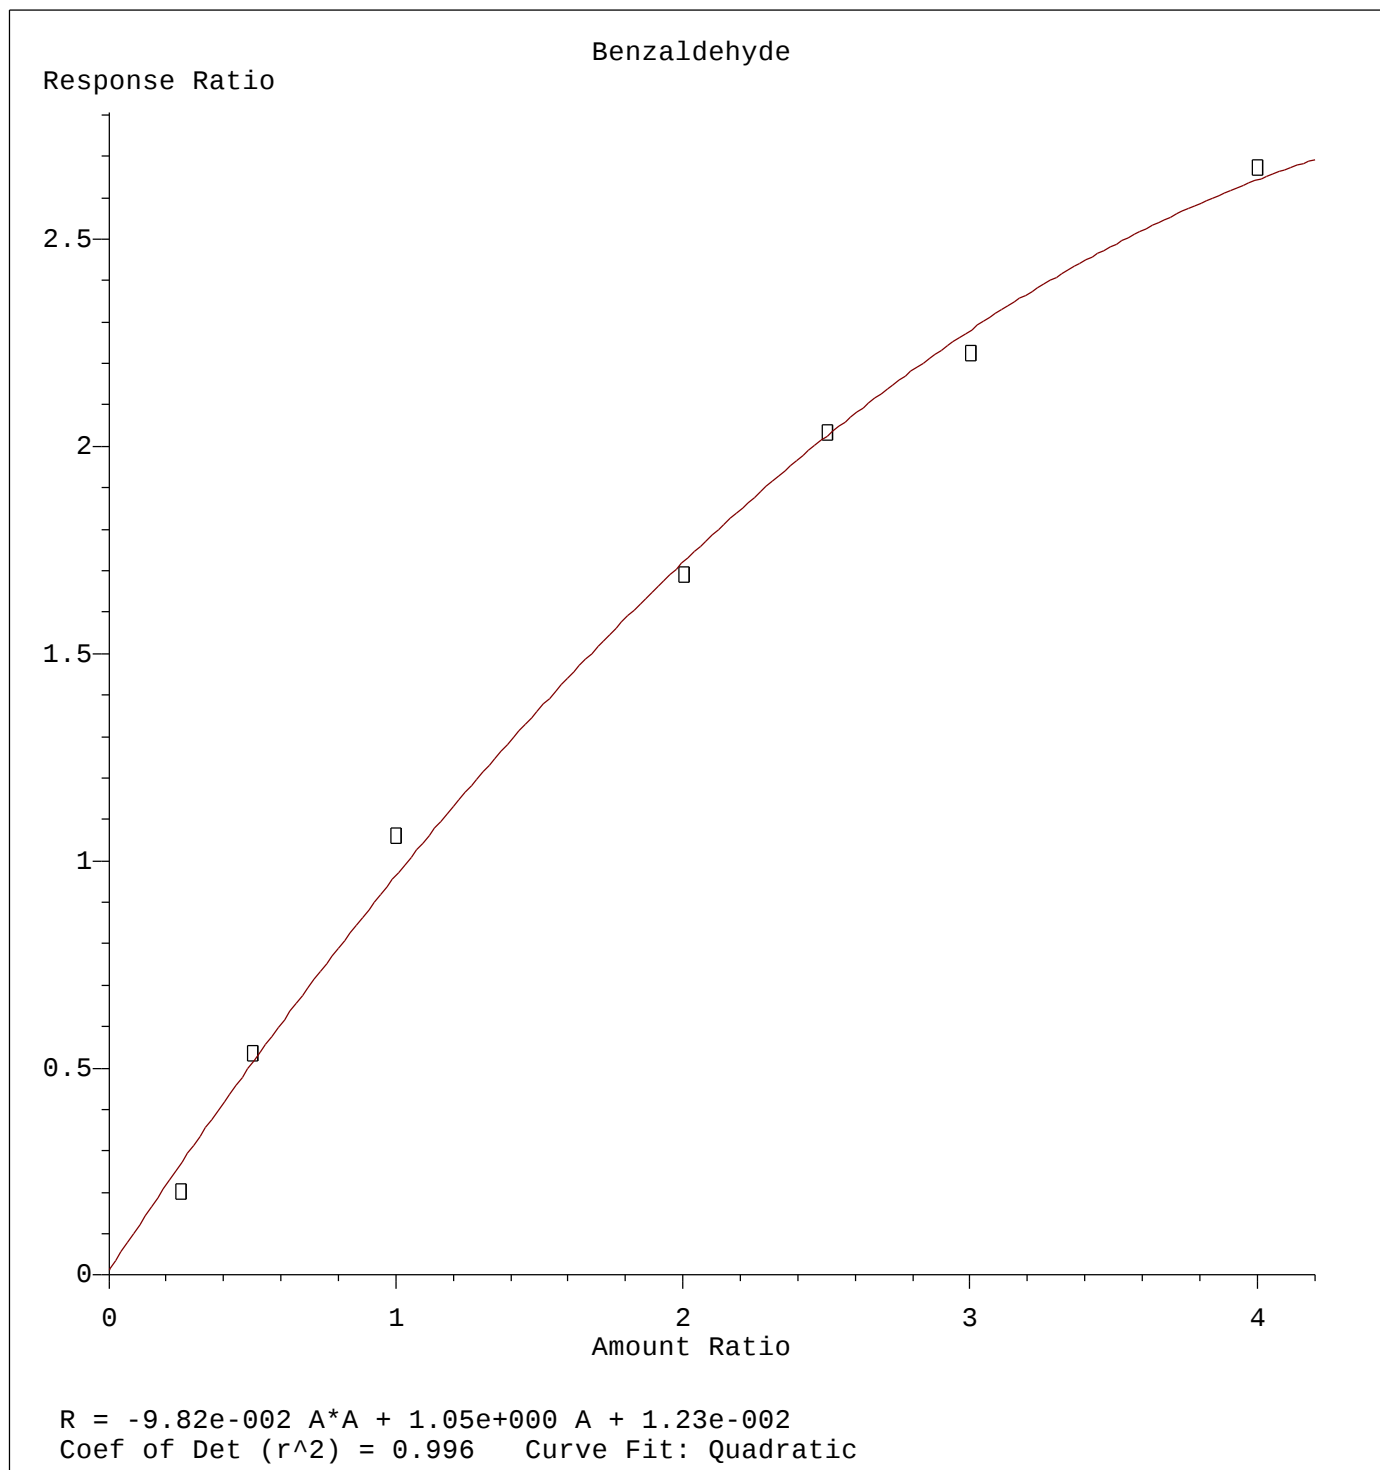


Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020

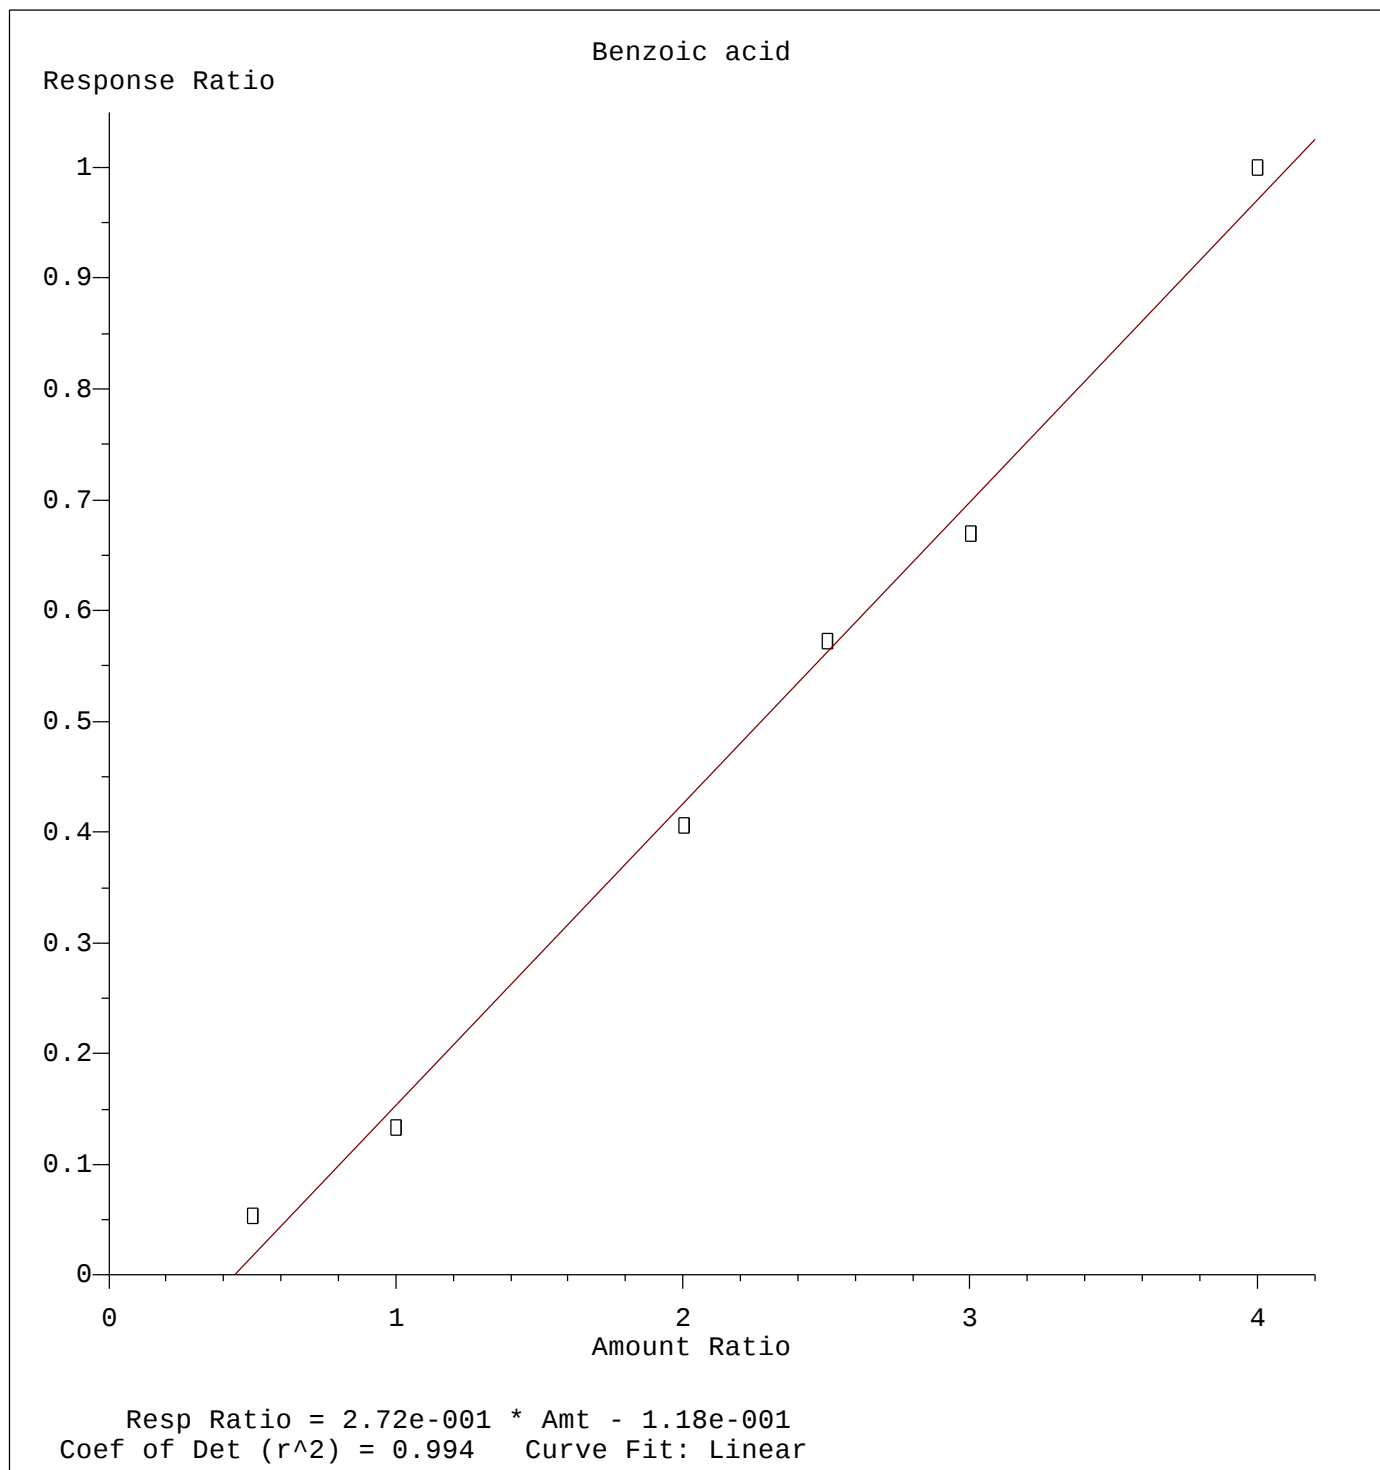

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020

Hexachlorocyclopentadiene

Response Ratio

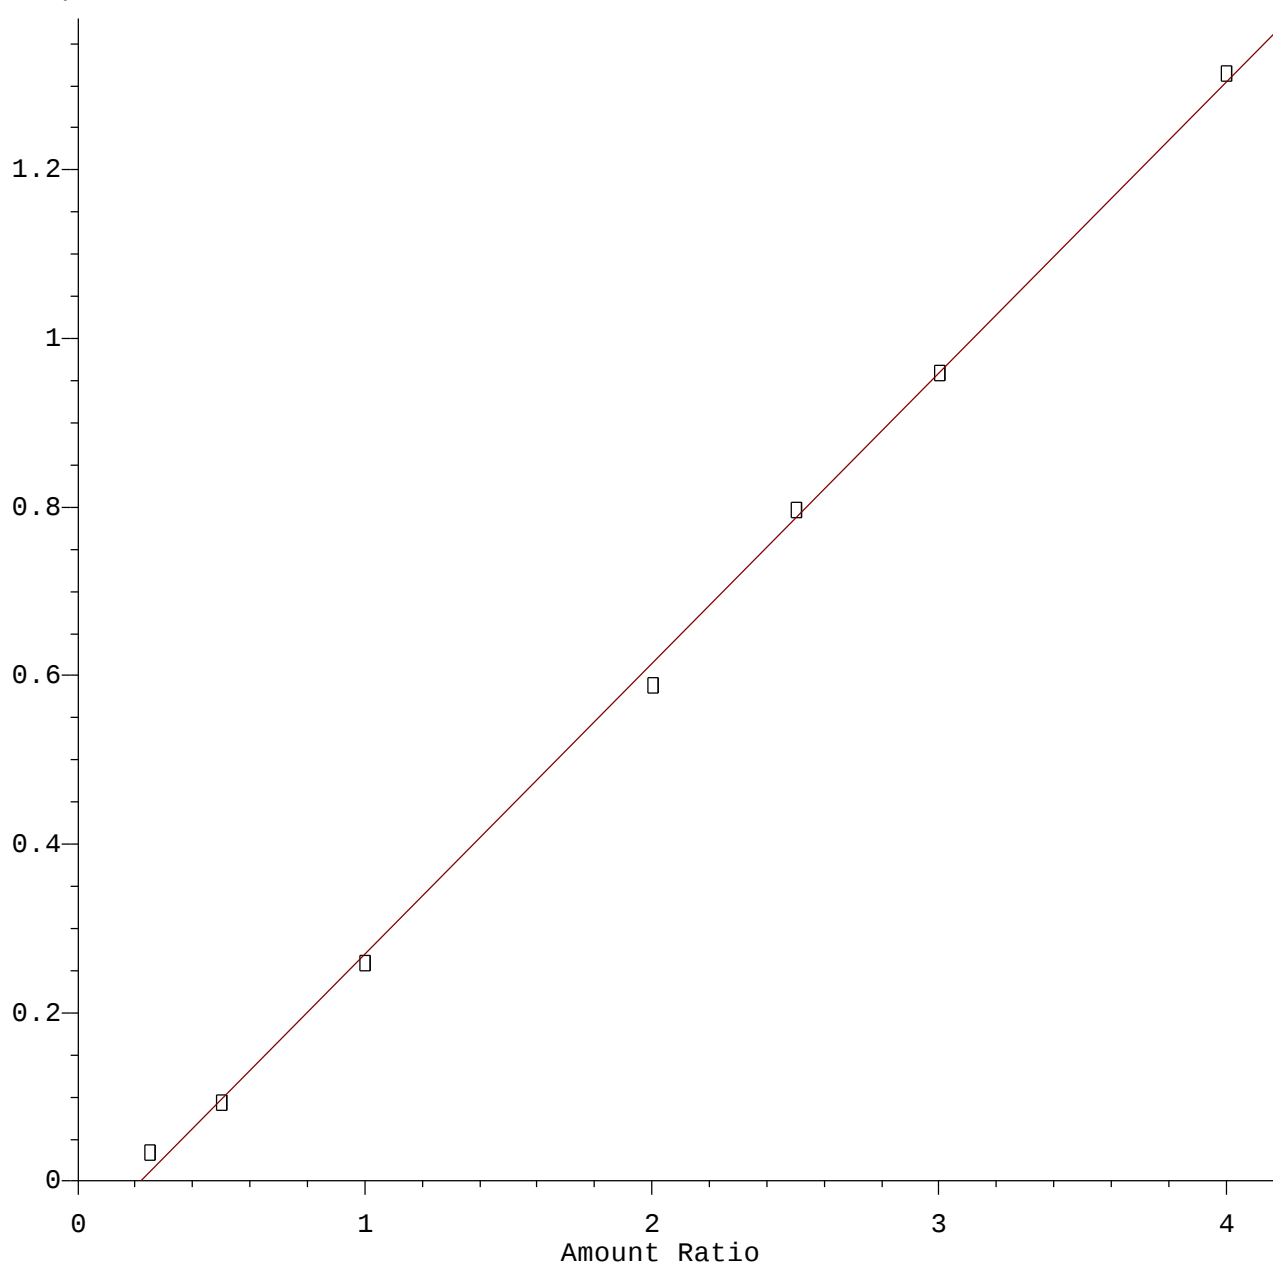


Resp Ratio = $3.45 \times 10^{-1} \times \text{Amt} - 7.56 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020


2,4-Dinitrophenol

Response Ratio

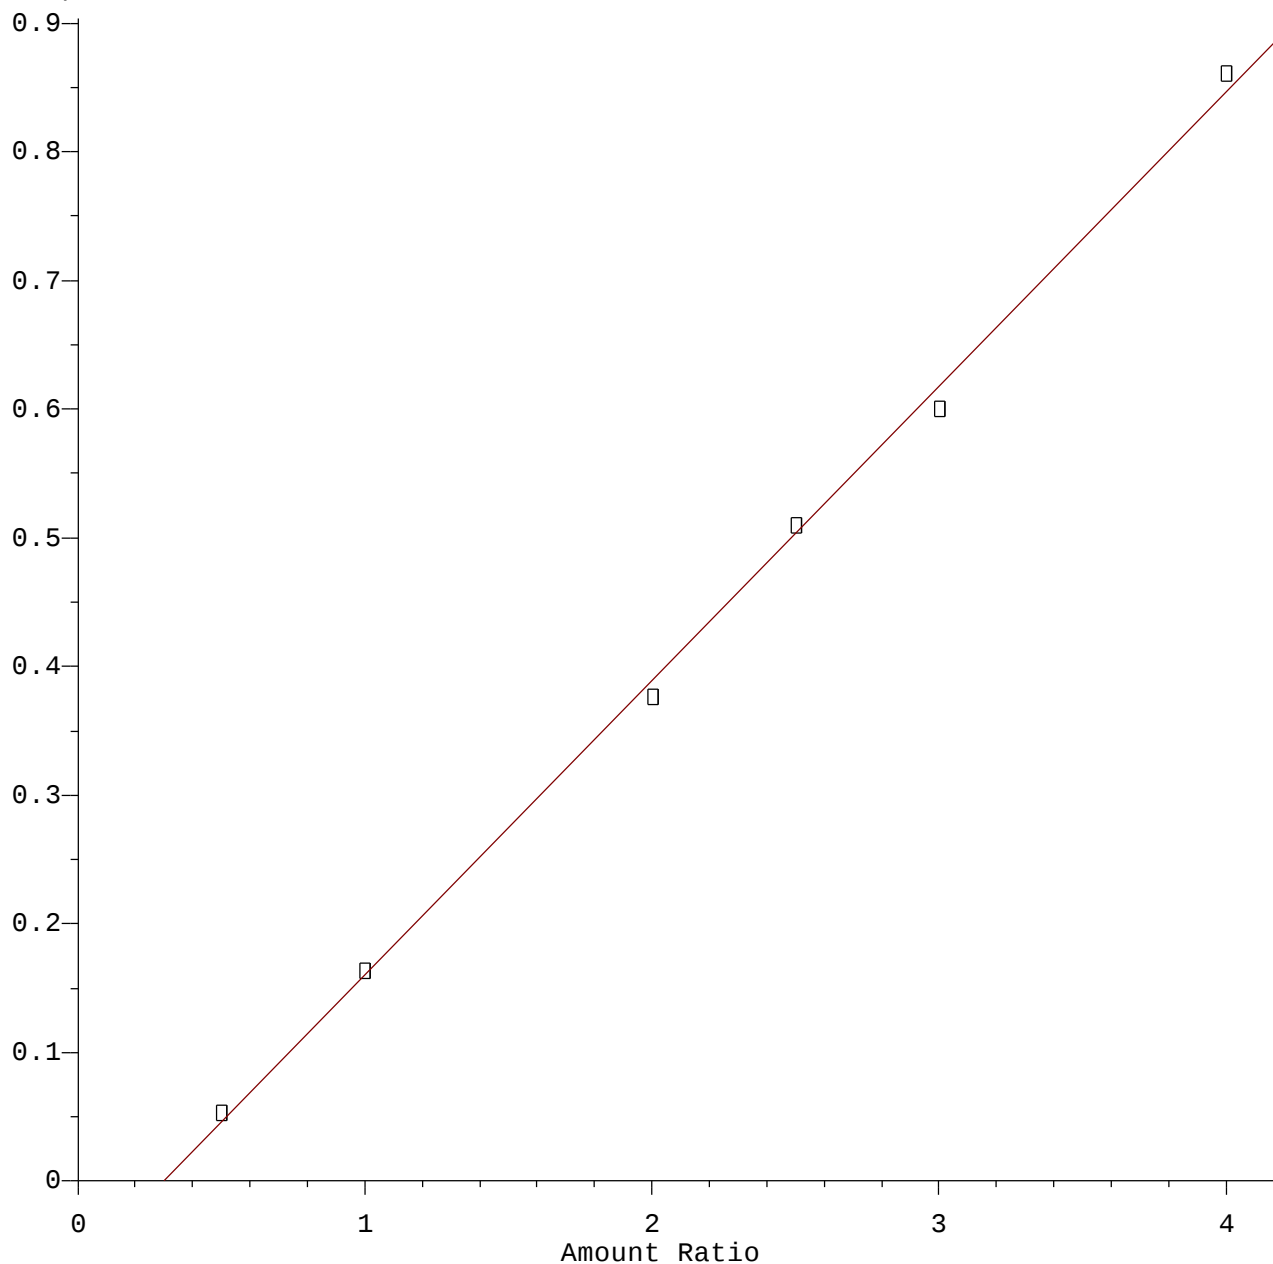


Resp Ratio = 2.29e-001 * Amt - 6.87e-002
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020

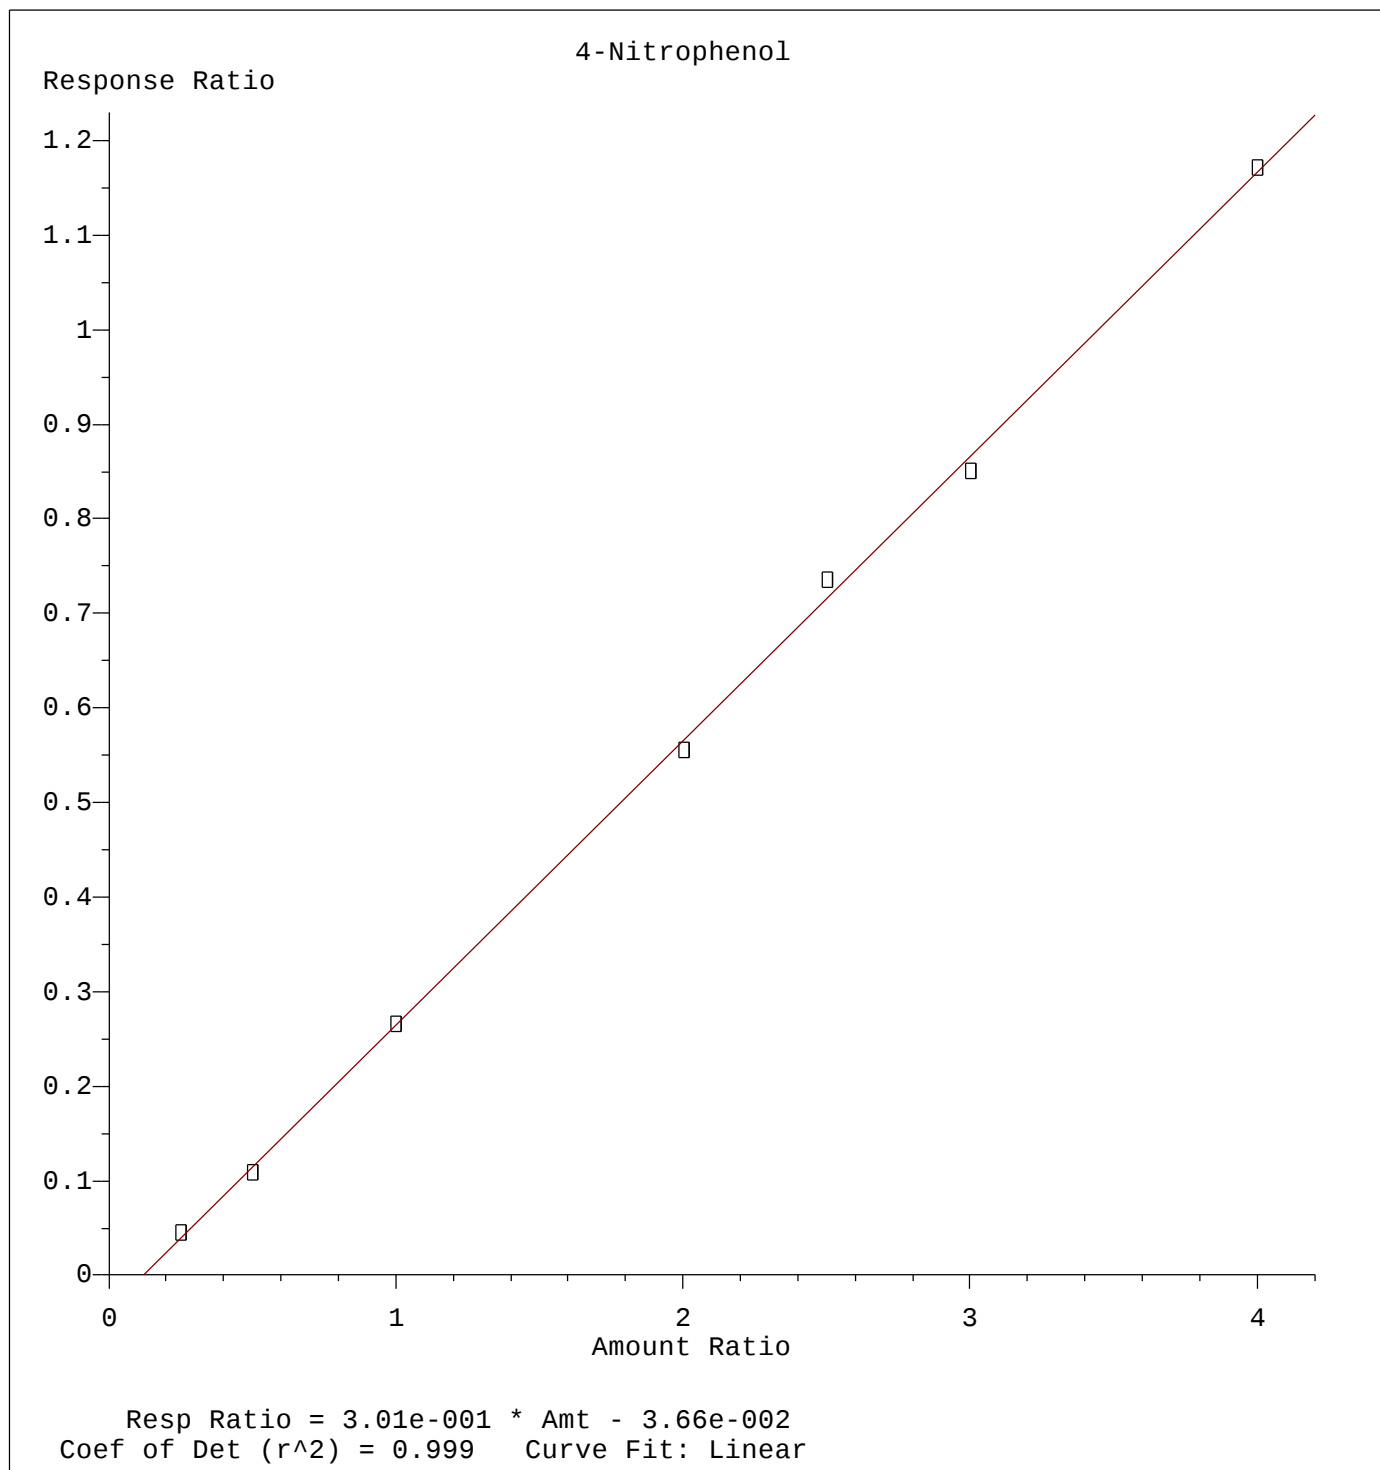


Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020

4,6-Dinitro-2-methylphenol

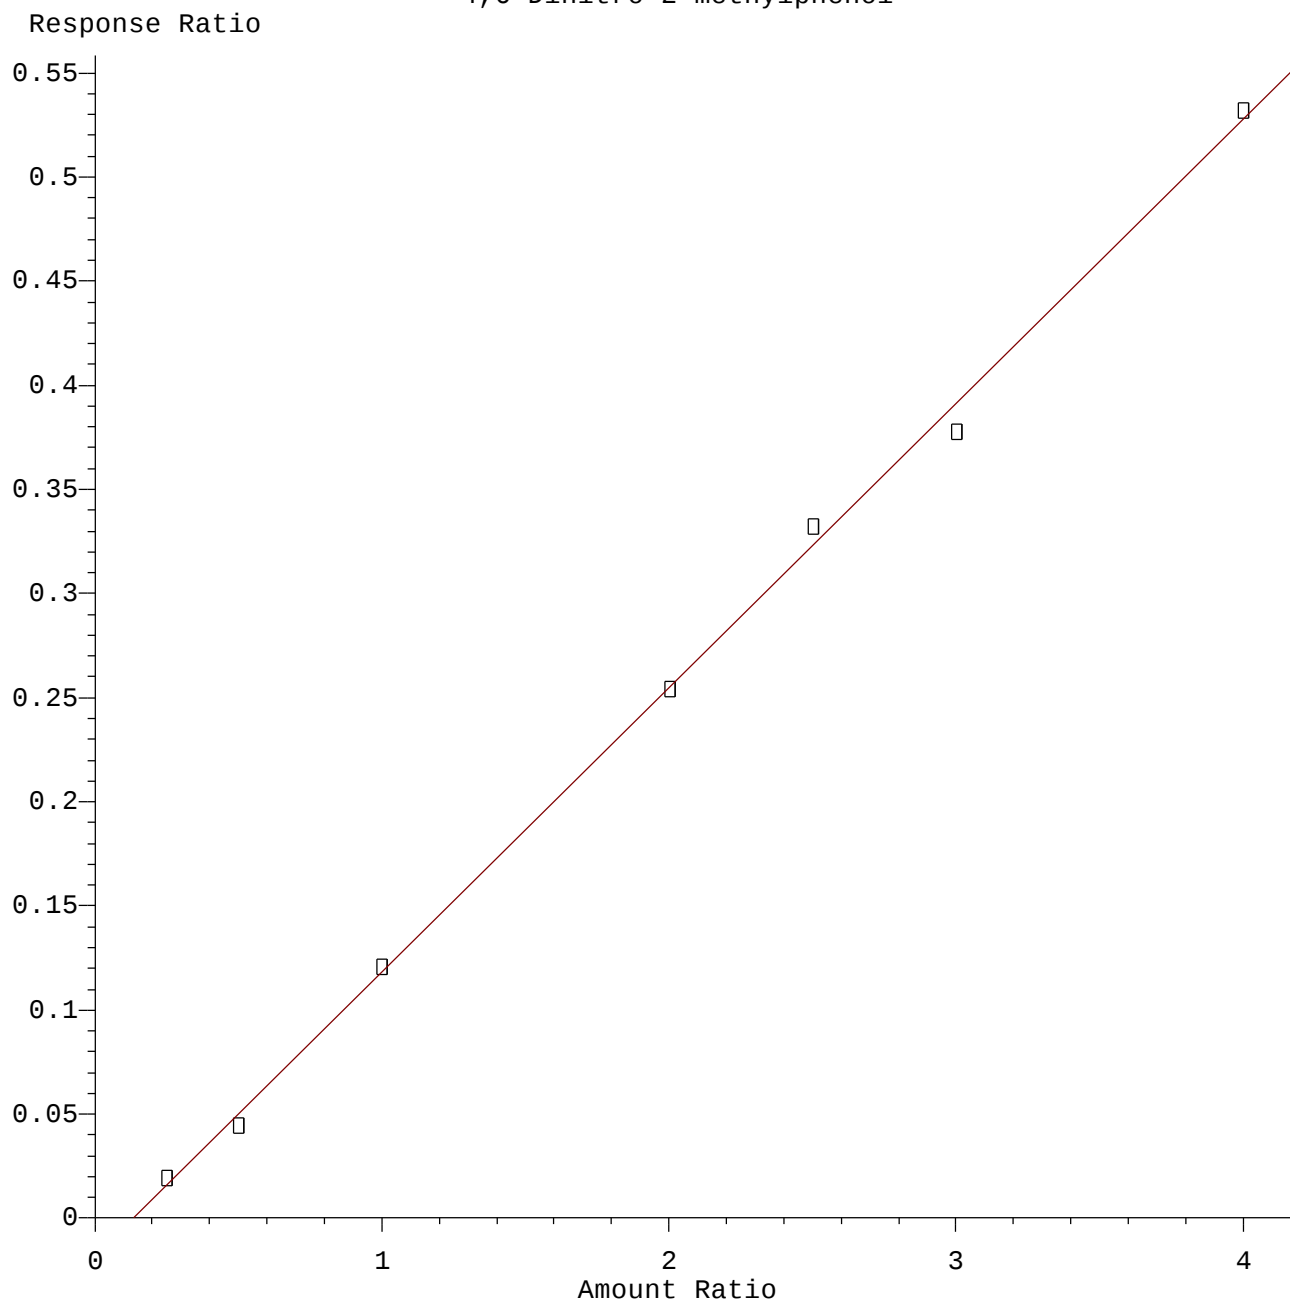


Resp Ratio = $1.36 \times 10^{-1} \times \text{Amt} - 1.85 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020

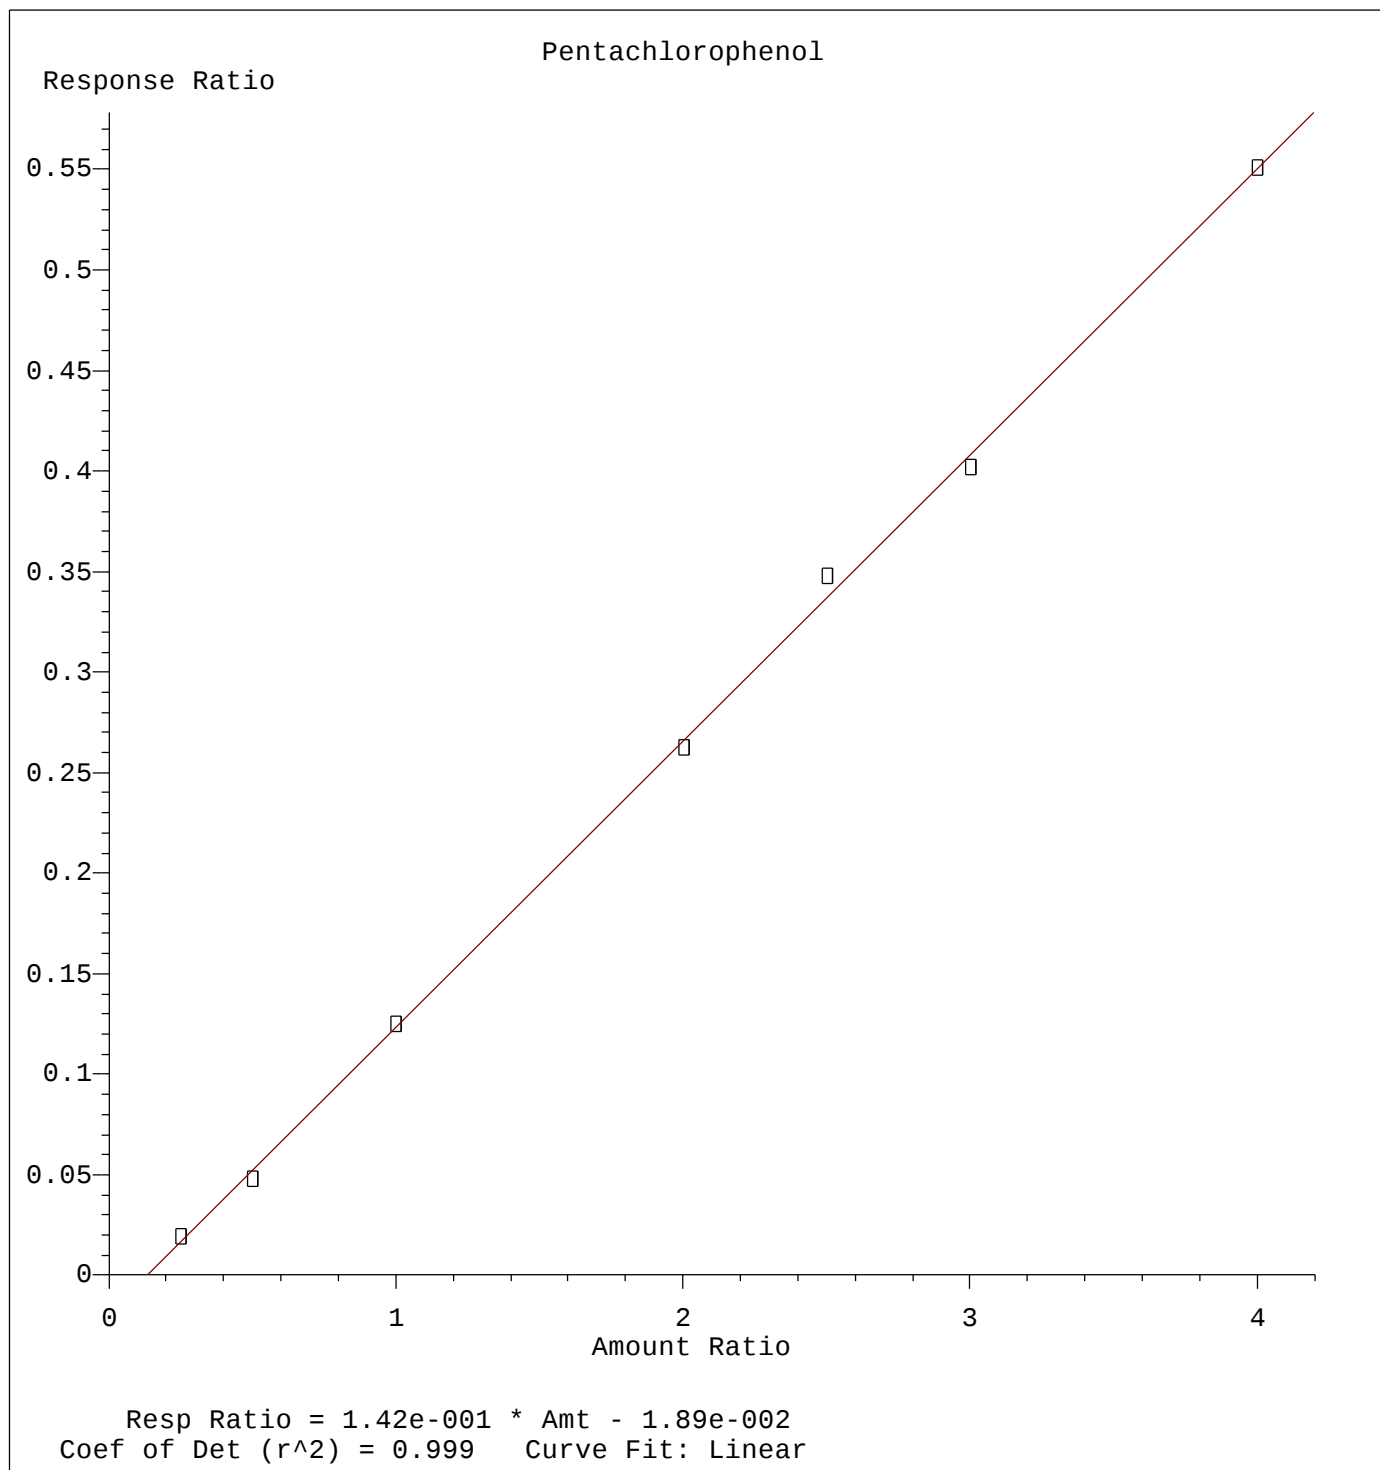

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020

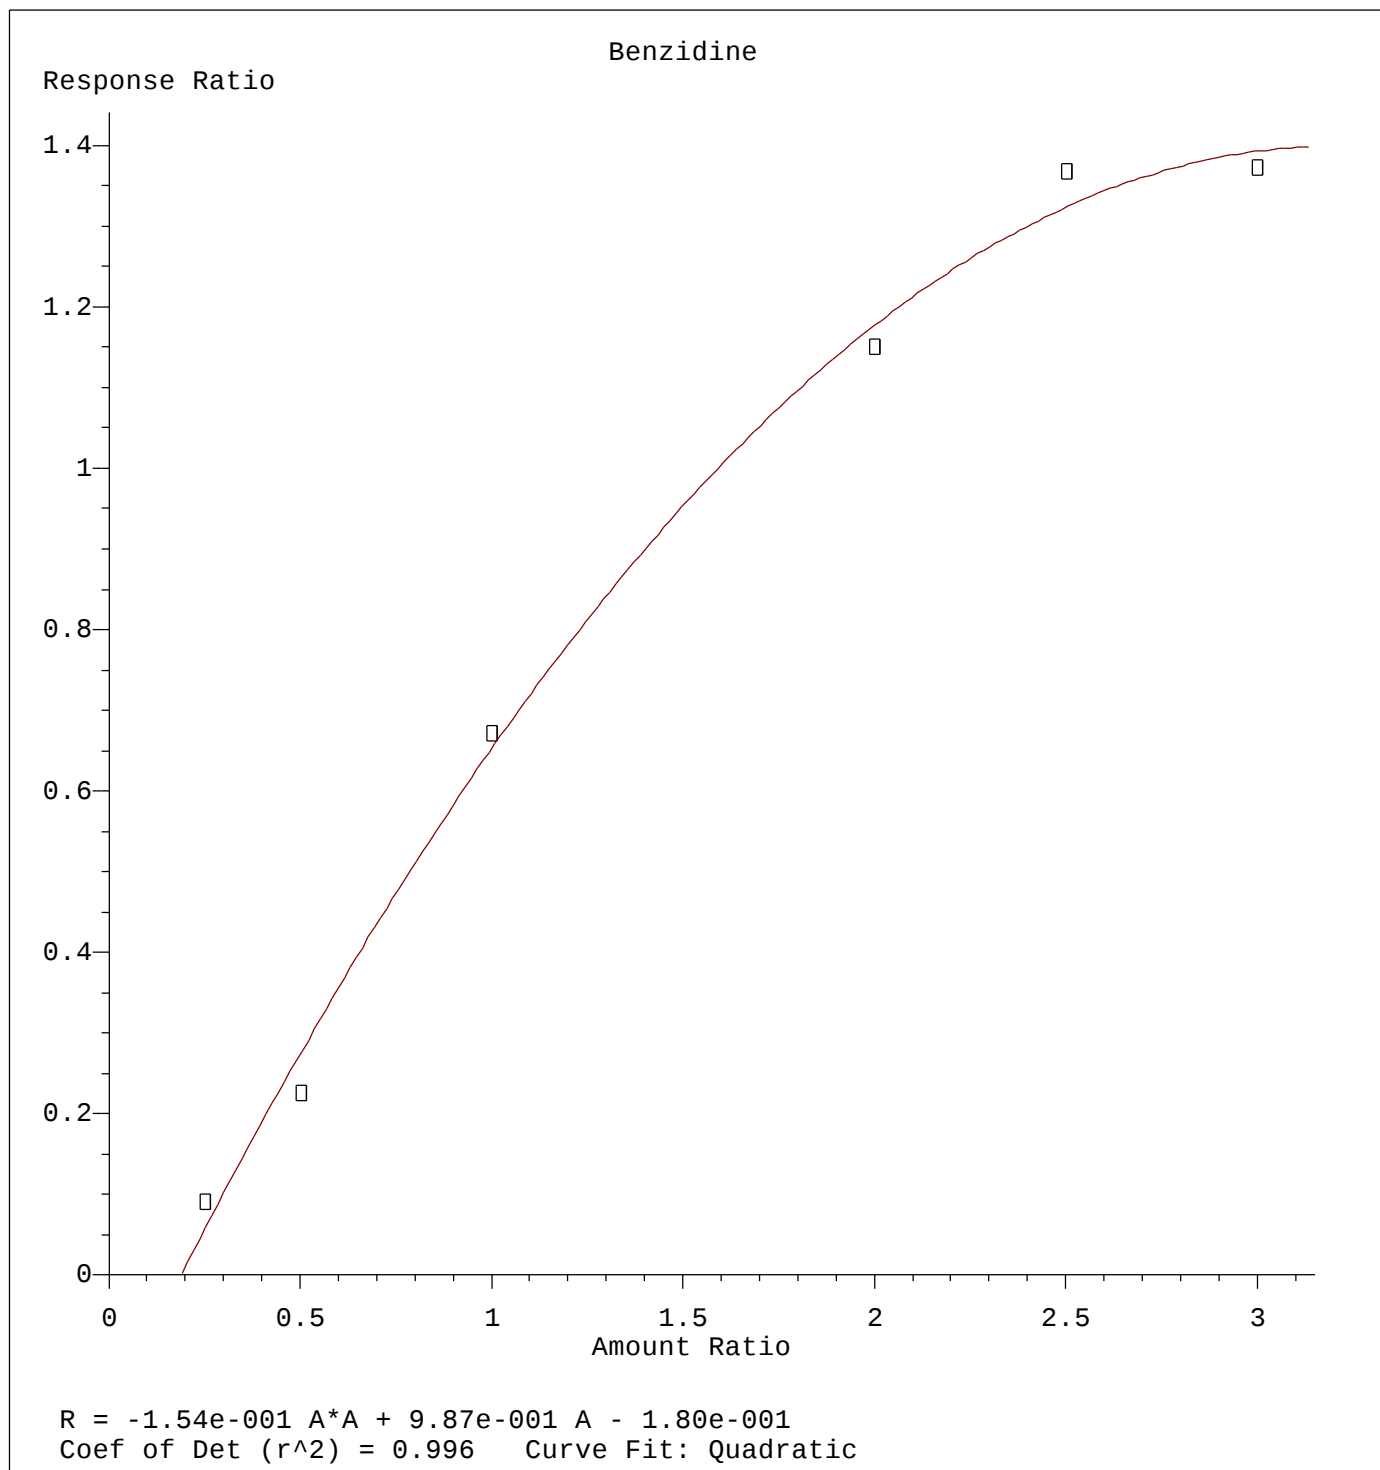

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Calibration Table Last Updated: Tue Jun 30 13:55:05 2020