
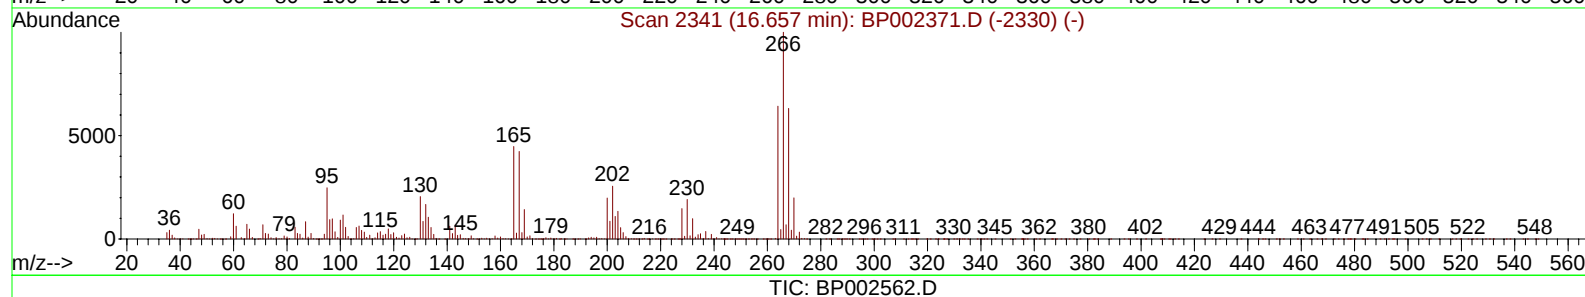
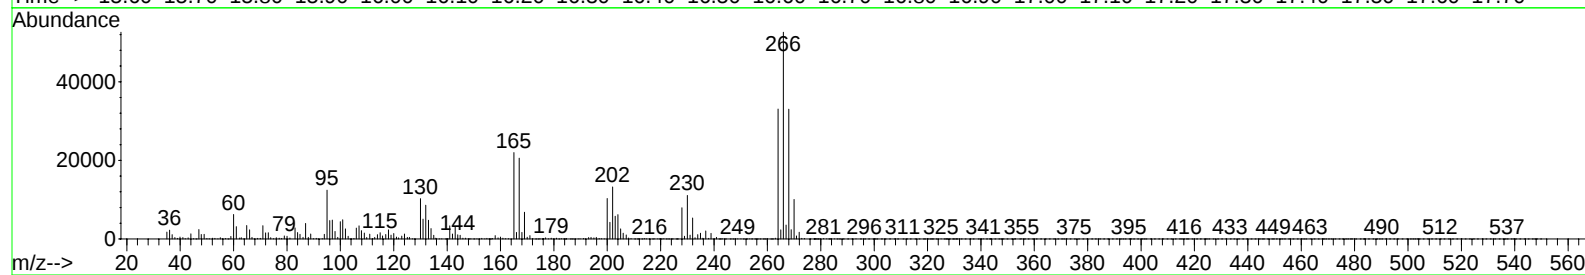


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP062920\
 Data File : BP002562.D
 Acq On : 29 Jun 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 10:53:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP0602920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 10:46:54 2020
 Response via : Initial Calibration

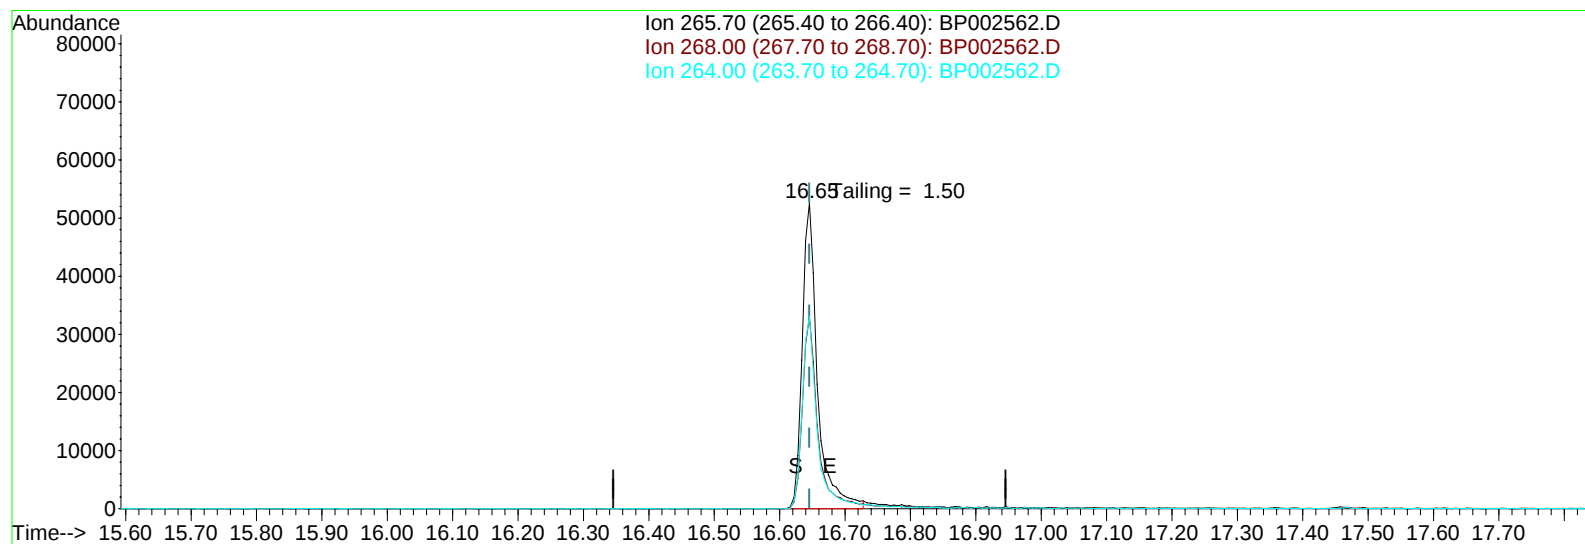

(70) Pentachlorophenol (C)




16.645min (+0.000) 496867.55ng

response 89646

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.76
264.00	64.80	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP062920\
 Data File : BP002562.D
 Acq On : 29 Jun 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 10:53:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP0602920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 10:46:54 2020
 Response via : Initial Calibration

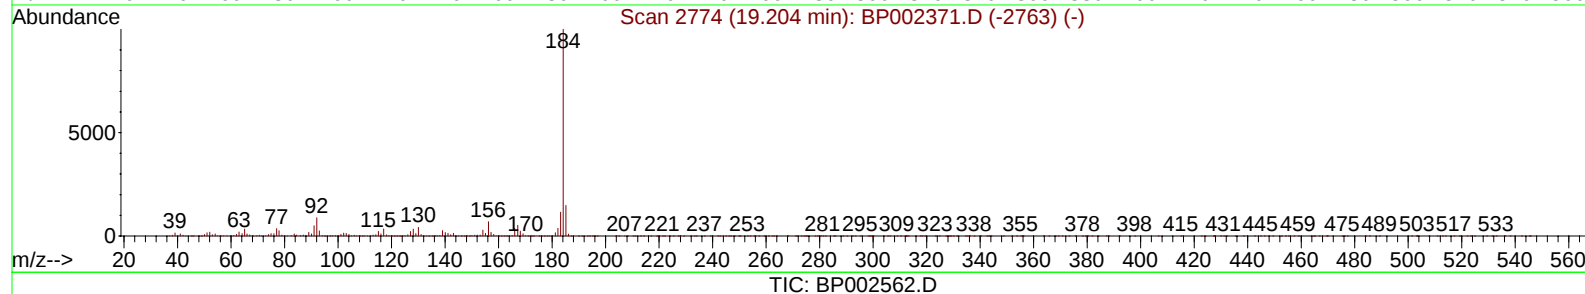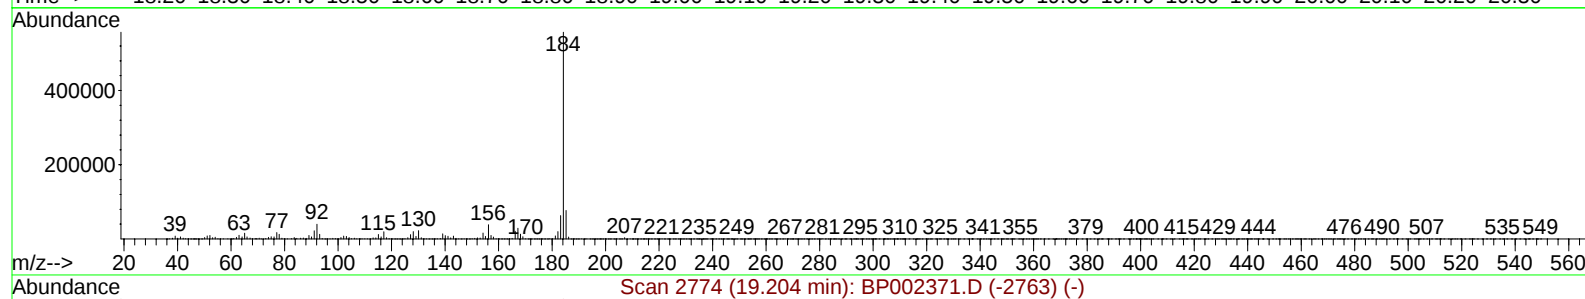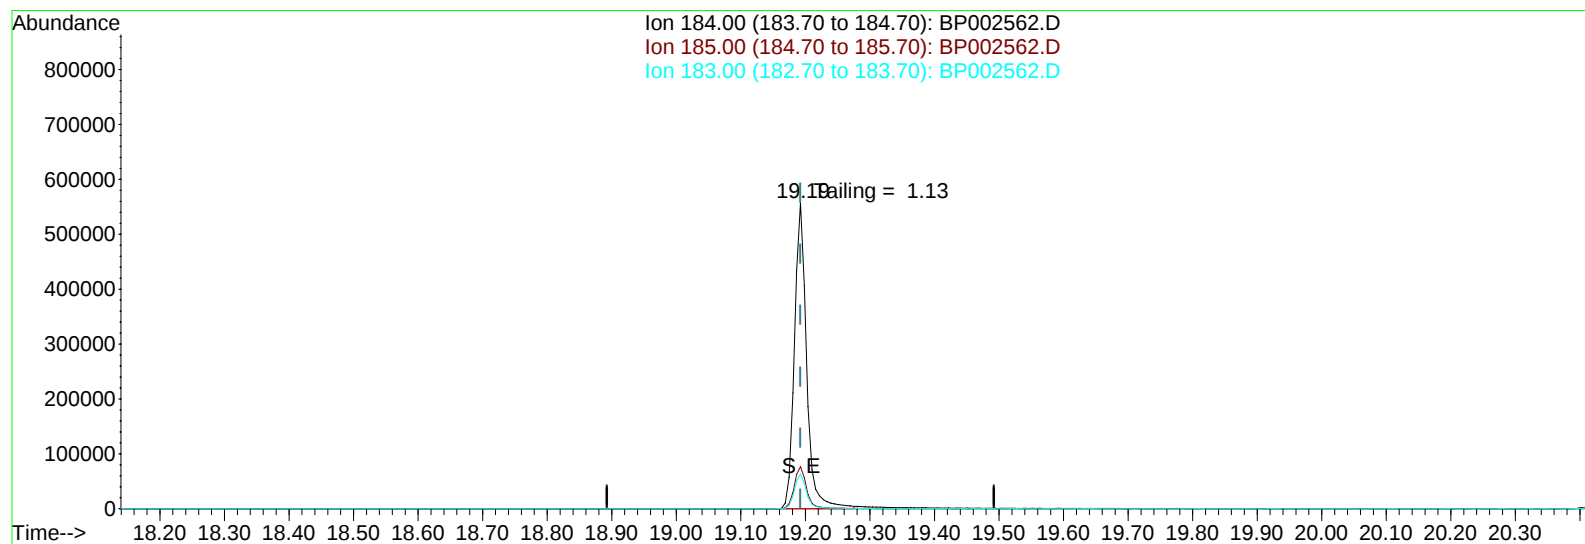

(77) Benzidine

19.192min (+0.000) 419475.90ng

response 749856

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.76
183.00	11.50	11.34
0.00	0.00	0.00