


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062920\
 Data File : BP002562.D
 Acq On : 29 Jun 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

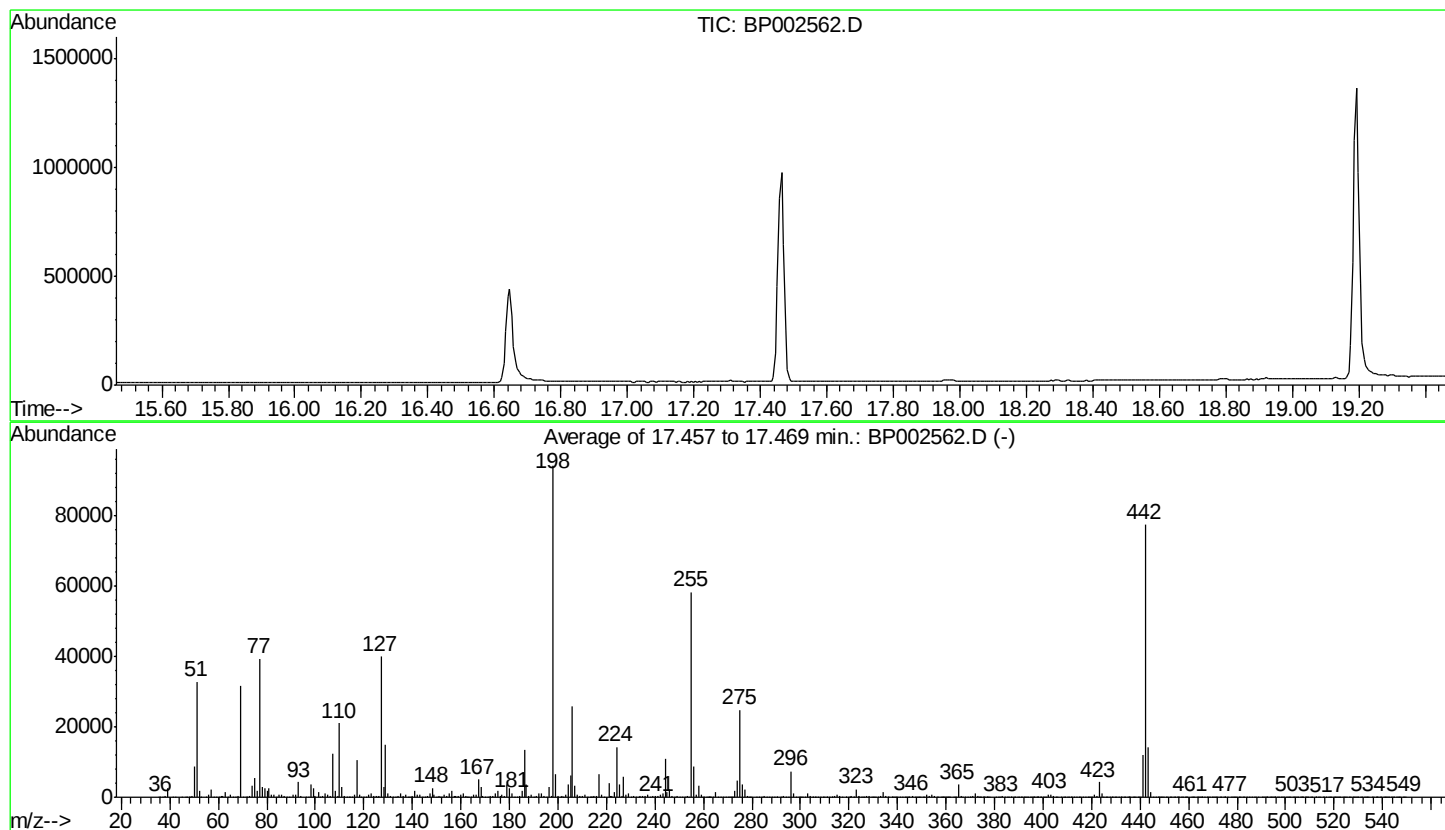

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	32768	PASS
68	69	0.00	2	1.6	494	PASS
69	198	0.00	100	33.7	31683	PASS
70	69	0.00	2	0.5	165	PASS
127	198	10	80	42.3	39801	PASS
197	198	0.00	2	0.4	344	PASS
198	198	100	100	100.0	94013	PASS
199	198	5	9	6.9	6452	PASS
275	198	10	60	26.3	24698	PASS
365	198	1	100	3.8	3573	PASS
441	198	0.01	100	12.7	11947	PASS
442	198	50	100	82.1	77170	PASS
443	442	15	24	18.6	14329	PASS