
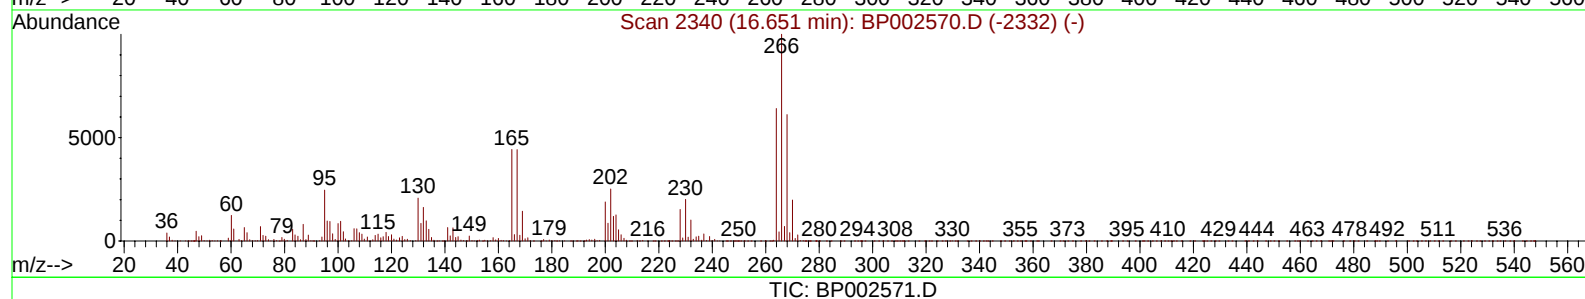
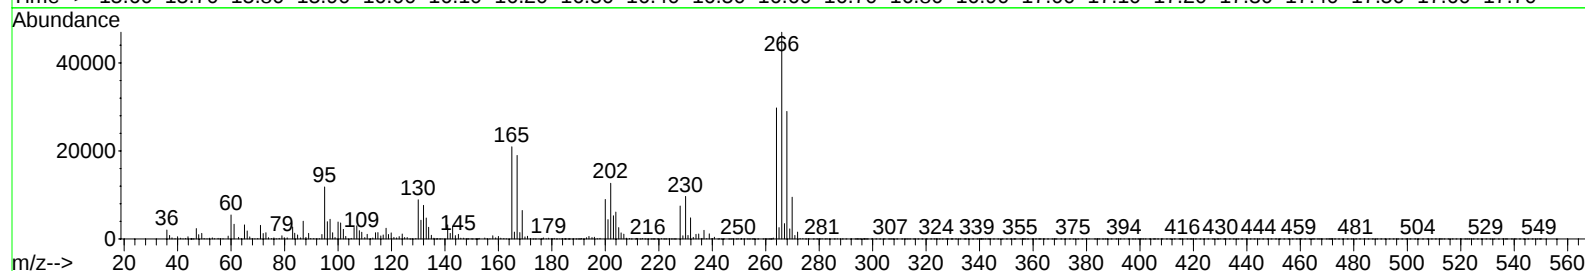


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP063020\
 Data File : BP002571.D
 Acq On : 30 Jun 2020 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 19:01:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 16:51:57 2020
 Response via : Initial Calibration

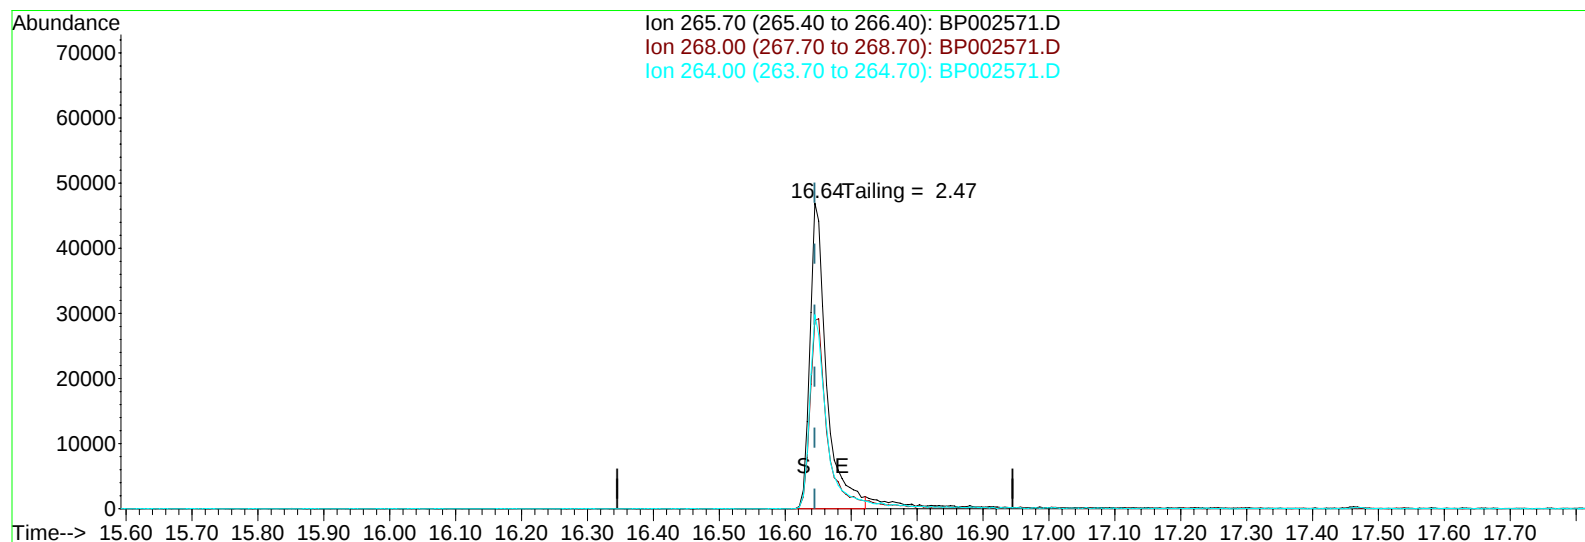

(70) Pentachlorophenol (C)




16.645min (-0.000) 723344.30ng

response 87515

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	61.69
264.00	61.60	63.41
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP063020\
 Data File : BP002571.D
 Acq On : 30 Jun 2020 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 19:01:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 16:51:57 2020
 Response via : Initial Calibration

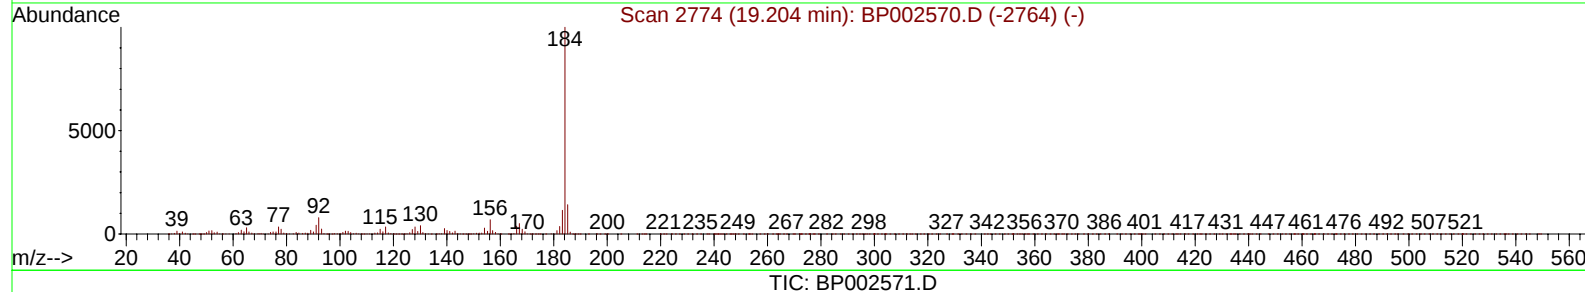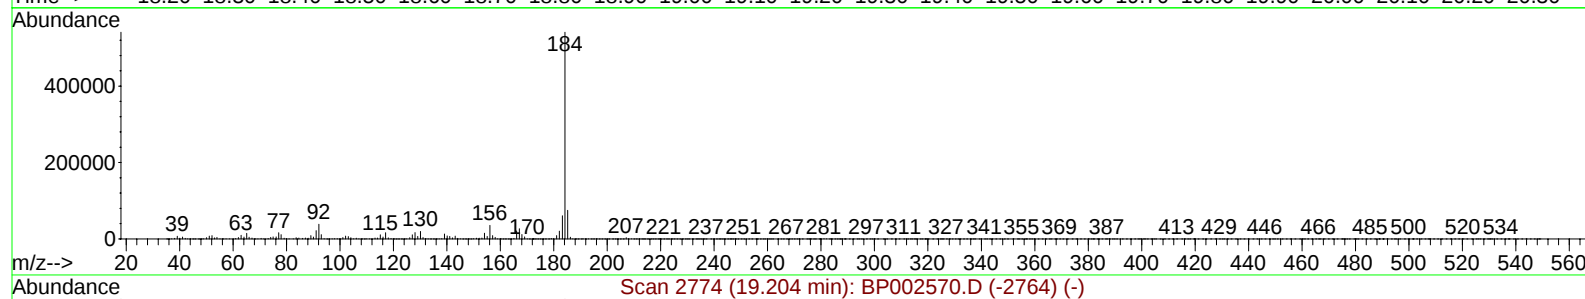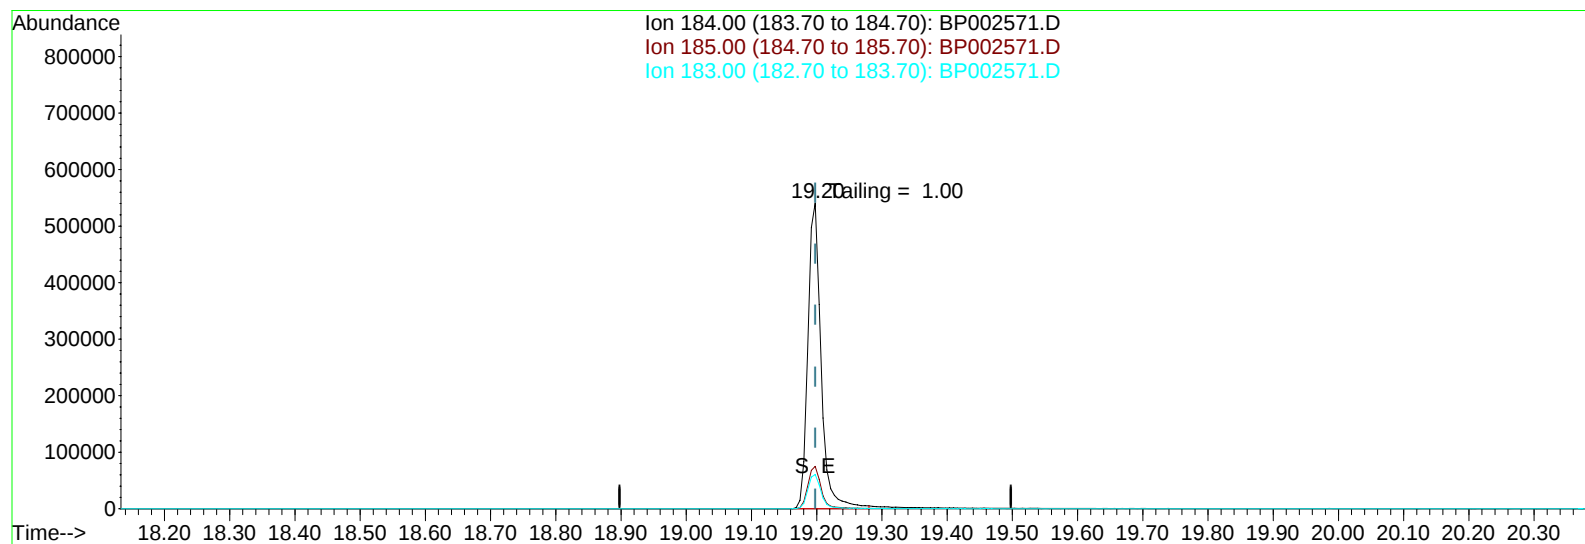

(77) Benzidine

19.198min (-0.000) -20.00ng

response 771571

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.89
183.00	11.50	11.21
0.00	0.00	0.00