

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP063020\
 Data File : BP002590.D
 Acq On : 01 Jul 2020 05:51
 Operator : CG/JU
 Sample : PB129875BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129875BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	385	392	412	rBV	2763994	4318596	43.71%	9.461%
2	6.763	652	659	678	rBV	2000085	3321006	33.61%	7.276%
3	7.569	789	796	807	rBV	555991	869970	8.81%	1.906%
4	7.887	841	850	864	rBV	1780487	2900370	29.36%	6.354%
5	8.716	983	991	1009	rBV	1864813	3143330	31.82%	6.886%
6	10.340	1260	1267	1283	rBV	686788	1234960	12.50%	2.706%
7	12.834	1684	1691	1714	rBV	3344476	5453588	55.20%	11.948%
8	14.222	1920	1927	1940	rBV2	1196158	1836907	18.59%	4.024%
9	15.722	2175	2182	2207	rBV	3019481	4621848	46.78%	10.126%
10	16.980	2388	2396	2409	rBV	1642159	2419099	24.49%	5.300%
11	19.574	2830	2837	2853	rBV	7251410	9879852	100.00%	21.645%
12	21.086	3089	3094	3105	rBV	2662103	3435784	34.78%	7.527%
13	23.280	3460	3467	3475	rBV2	1203323	2209817	22.37%	4.841%




Sum of corrected areas: 45645127

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP063020\
Data File : BP002590.D
Acq On : 01 Jul 2020 05:51
Operator : CG/JU
Sample : PB129875BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129875BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

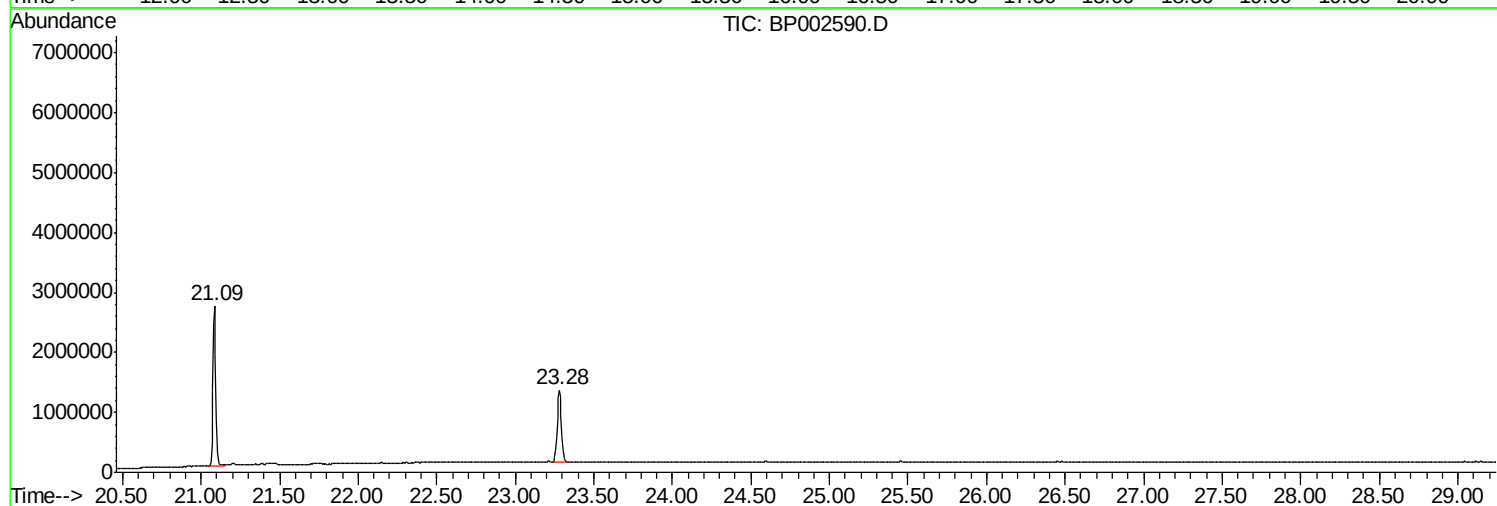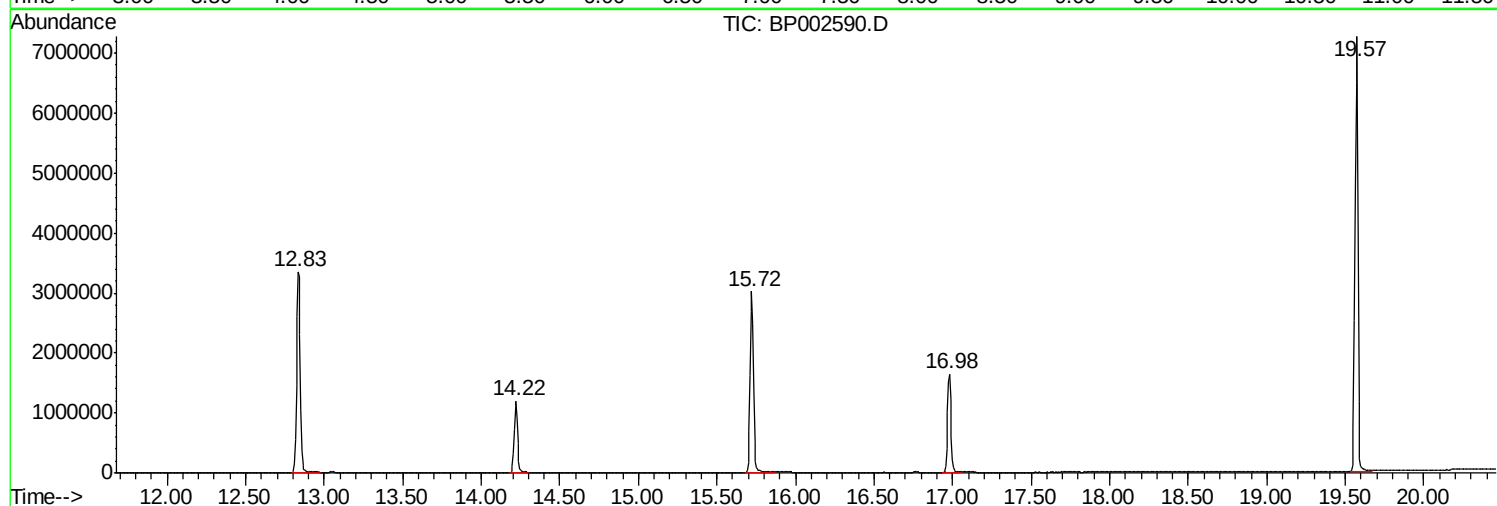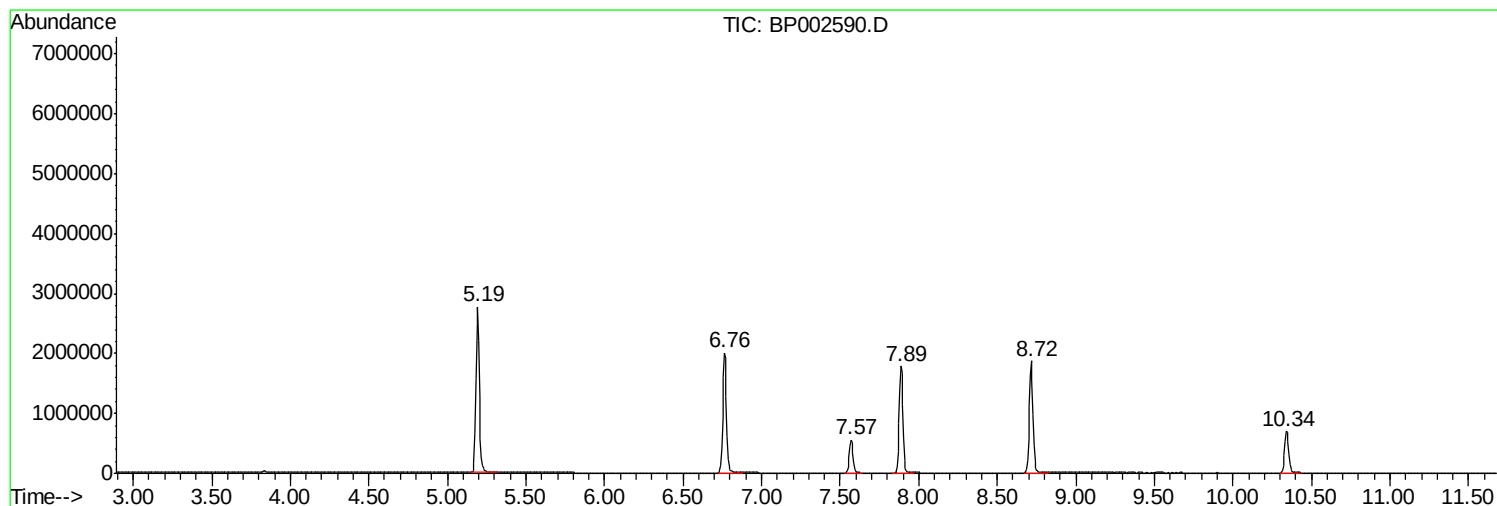

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP063020\
Data File : BP002590.D
Acq On : 01 Jul 2020 05:51
Operator : CG/JU
Sample : PB129875BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129875BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP063020\
Data File : BP002590.D
Acq On : 01 Jul 2020 05:51
Operator : CG/JU
Sample : PB129875BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129875BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc