


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP063020\
 Data File : BP002571.D
 Acq On : 30 Jun 2020 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

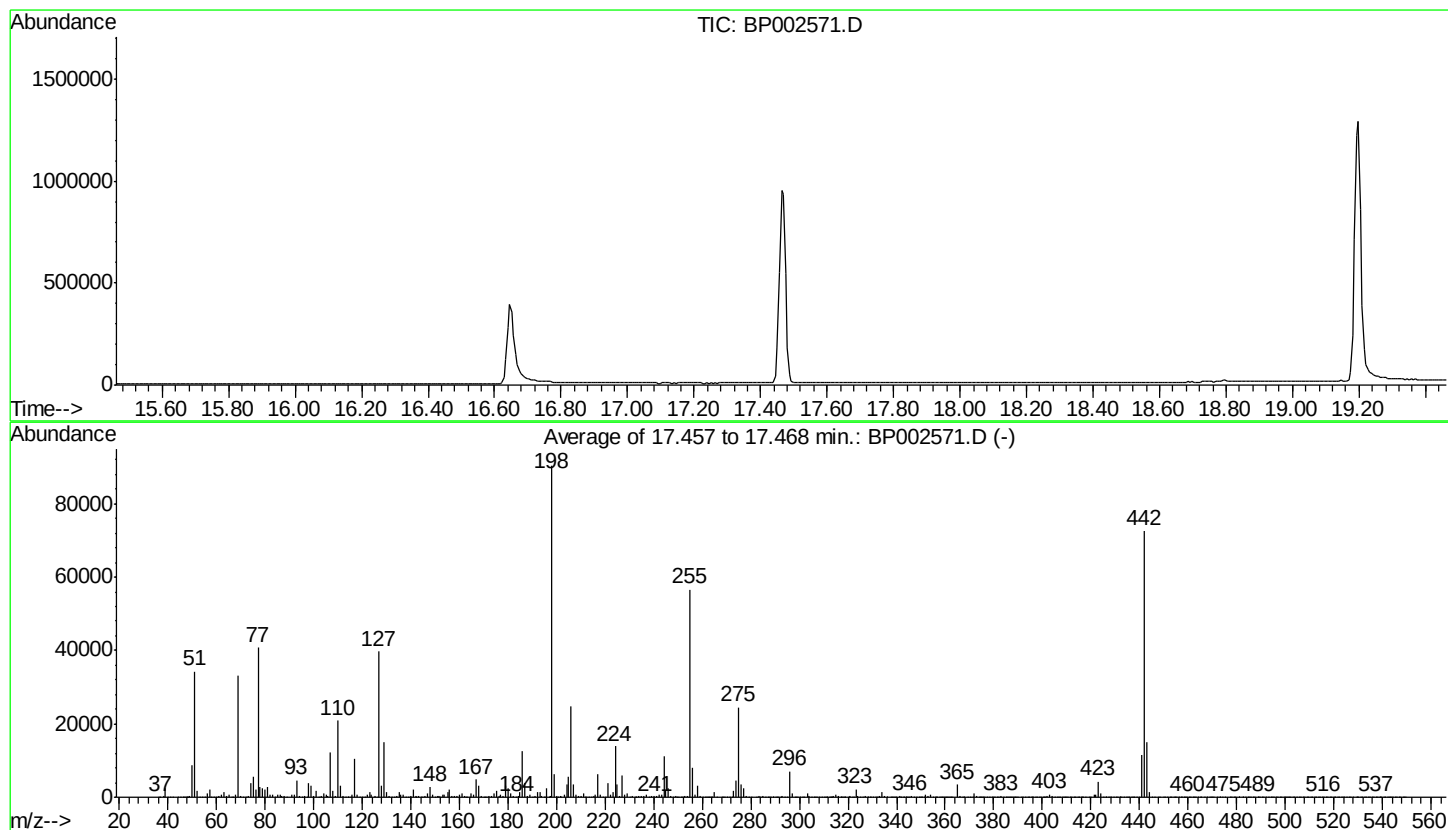

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	34314	PASS
68	69	0.00	2	1.8	597	PASS
69	198	0.00	100	36.8	33228	PASS
70	69	0.00	2	0.7	245	PASS
127	198	10	80	44.0	39749	PASS
197	198	0.00	2	0.3	234	PASS
198	198	100	100	100.0	90373	PASS
199	198	5	9	7.1	6422	PASS
275	198	10	60	27.2	24544	PASS
365	198	1	100	3.7	3351	PASS
441	198	0.01	100	12.7	11494	PASS
442	198	50	100	80.4	72700	PASS
443	442	15	24	20.8	15102	PASS