


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP063020\
 Data File : BP002583.D
 Acq On : 01 Jul 2020 01:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

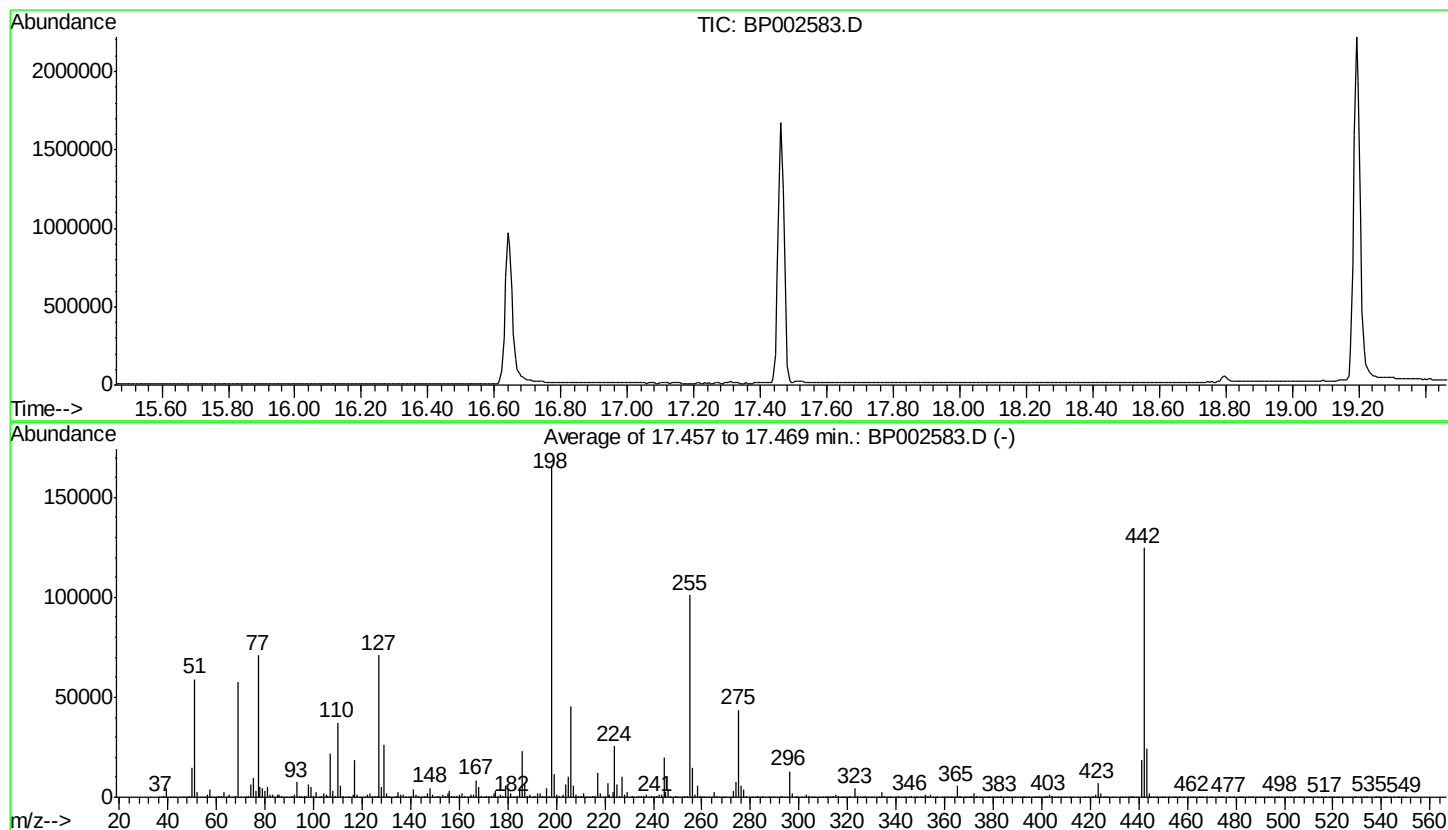

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	59201	PASS
68	69	0.00	2	1.7	976	PASS
69	198	0.00	100	34.7	57605	PASS
70	69	0.00	2	0.5	287	PASS
127	198	10	80	42.7	70914	PASS
197	198	0.00	2	0.5	784	PASS
198	198	100	100	100.0	165895	PASS
199	198	5	9	6.8	11250	PASS
275	198	10	60	26.3	43590	PASS
365	198	1	100	3.4	5711	PASS
441	198	0.01	100	11.4	18851	PASS
442	198	50	100	75.3	124851	PASS
443	442	15	24	19.4	24165	PASS