

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010935.D
 Acq On : 07 Jul 2022 12:17
 Operator : CG/JU
 Sample : PB146062BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	16	19	28	rVB	148159	191570	2.49%	0.228%
2	3.610	86	89	108	rBV	1693020	2469392	32.12%	2.937%
3	3.922	139	142	149	rVB	33901	45636	0.59%	0.054%
4	6.881	637	645	659	rBV	1759240	2681040	34.87%	3.188%
5	7.045	666	673	681	rBV	1510325	2256916	29.35%	2.684%
6	7.234	698	705	717	rBV	1814097	2801058	36.43%	3.331%
7	7.704	778	785	794	rVB	1440539	2263174	29.43%	2.692%
8	8.416	899	906	915	rBV	2103065	3195539	41.56%	3.800%
9	8.863	974	982	994	rBV	1569000	2465728	32.07%	2.932%
10	9.581	1096	1104	1119	rBV	1108715	1750656	22.77%	2.082%
11	10.116	1187	1195	1207	rBV	1776868	2925363	38.05%	3.479%
12	10.492	1251	1259	1269	rBV	1800009	2995968	38.96%	3.563%
13	10.639	1277	1284	1301	rBV	1927390	3175555	41.30%	3.777%
14	12.086	1525	1530	1537	rBV	32389	54907	0.71%	0.065%
15	12.304	1564	1567	1573	rVB7	4837	9689	0.13%	0.012%
16	13.775	1811	1817	1827	rBV	2761395	3769864	49.03%	4.483%
17	14.045	1856	1863	1883	rBV	3172729	4651292	60.49%	5.532%
18	14.357	1909	1916	1929	rBV	2413242	3392755	44.13%	4.035%
19	14.569	1943	1952	1968	rBV	1164181	1787309	23.25%	2.126%
20	14.780	1986	1988	1993	rVB6	5929	8973	0.12%	0.011%
21	15.357	2079	2086	2095	rBV	4167910	5863962	76.27%	6.974%
22	15.474	2100	2106	2122	rVV	901559	1270080	16.52%	1.510%
23	15.598	2122	2127	2135	rVB	51680	80675	1.05%	0.096%
24	16.145	2216	2220	2225	rVB5	13253	20009	0.26%	0.024%
25	16.798	2327	2331	2337	rVB9	7061	12644	0.16%	0.015%
26	17.121	2379	2386	2396	rBV	2720611	3782180	49.19%	4.498%
27	17.221	2397	2403	2418	rVV	4589834	6198309	80.61%	7.371%
28	19.045	2710	2713	2717	rBV	52511	66528	0.87%	0.079%
29	19.115	2721	2725	2731	rBV2	52947	76898	1.00%	0.091%
30	19.474	2780	2786	2795	rBV	5367414	7207521	93.74%	8.572%
31	21.233	3080	3085	3093	rBV	3505344	4395220	57.16%	5.227%
32	23.445	3454	3461	3470	rVB2	4165265	7688891	100.00%	9.144%
33	23.598	3480	3487	3498	rVB	2337923	4529578	58.91%	5.387%




Sum of corrected areas: 84084879

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010935.D
Acq On : 07 Jul 2022 12:17
Operator : CG/JU
Sample : PB146062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK062

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

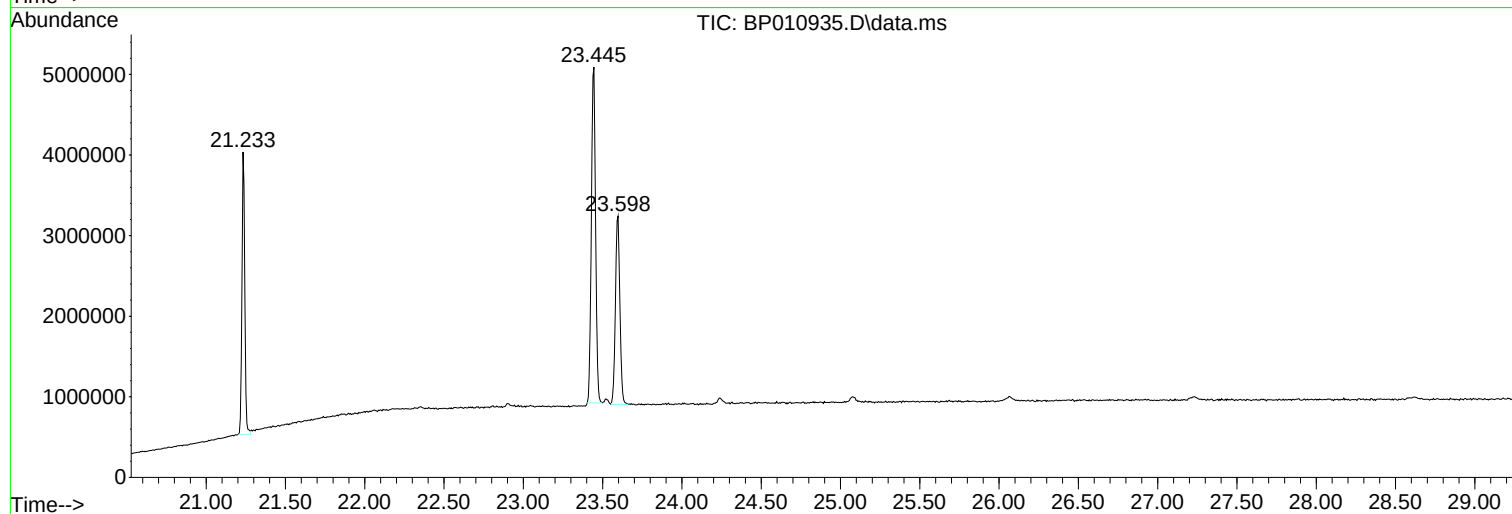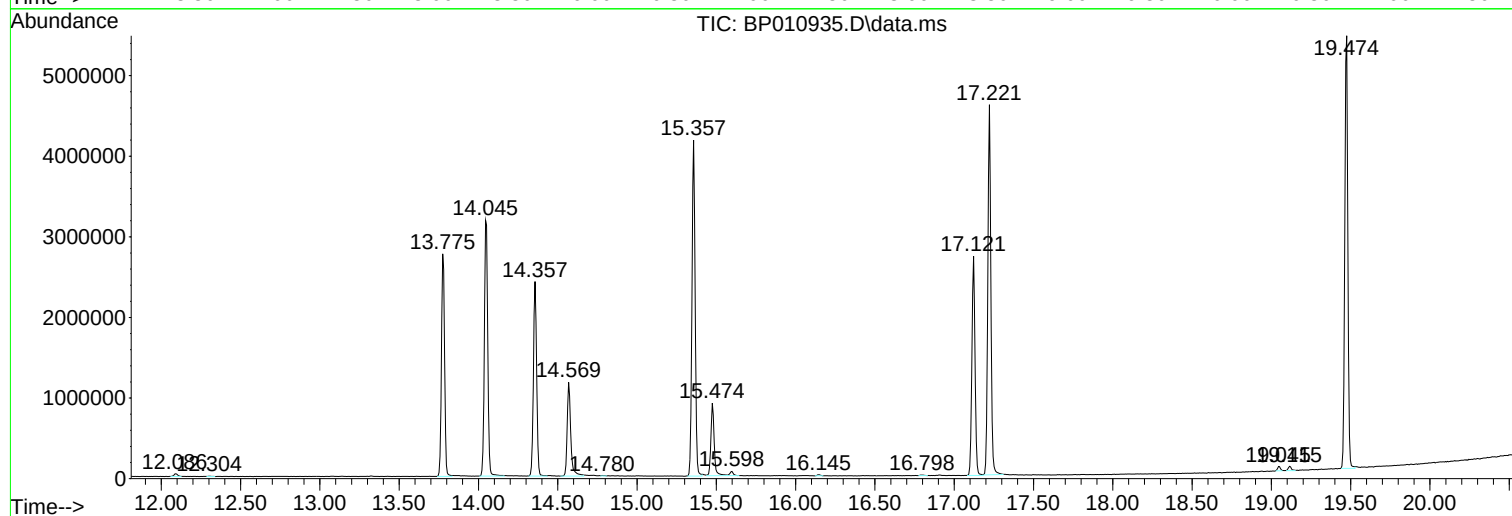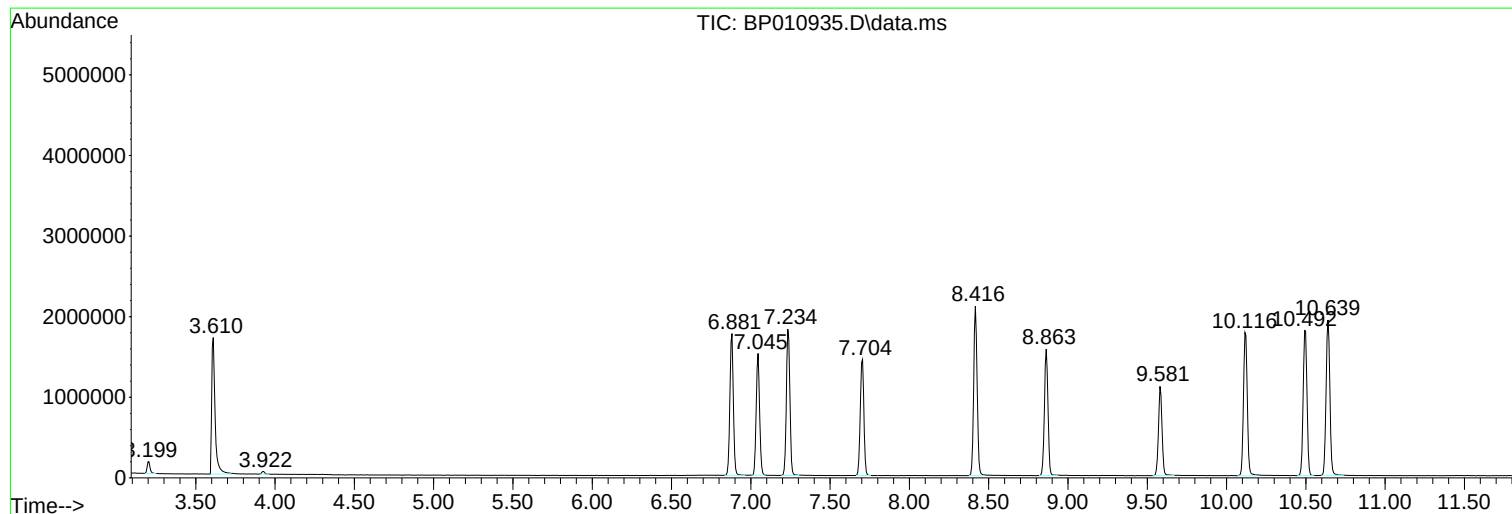

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010935.D
Acq On : 07 Jul 2022 12:17
Operator : CG/JU
Sample : PB146062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK062

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010935.D
Acq On : 07 Jul 2022 12:17
Operator : CG/JU
Sample : PB146062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK062

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------