

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010937.D
 Acq On : 07 Jul 2022 13:25
 Operator : CG/JU
 Sample : N3577-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB323

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	10	14	17	rBV2	43630	59801	0.66%	0.073%
2	3.199	17	19	27	rVB	115791	145589	1.61%	0.178%
3	3.476	63	66	76	rVB2	22483	35596	0.39%	0.044%
4	3.611	86	89	107	rBV	537435	816061	9.02%	1.000%
5	3.834	122	127	134	rVB	49725	74401	0.82%	0.091%
6	3.923	139	142	151	rVB	35951	48790	0.54%	0.060%
7	4.440	226	230	235	rBV6	7208	10366	0.11%	0.013%
8	4.746	279	282	288	rVB3	7668	11054	0.12%	0.014%
9	4.846	293	299	304	rBV2	22322	43231	0.48%	0.053%
10	5.428	394	398	404	rVB	13777	20920	0.23%	0.026%
11	6.705	612	615	620	rBV7	6362	12544	0.14%	0.015%
12	6.881	637	645	653	rVB	364970	558540	6.18%	0.685%
13	7.046	666	673	682	rBV	1576652	2359241	26.09%	2.892%
14	7.122	682	686	691	rVB	16739	24083	0.27%	0.030%
15	7.234	697	705	716	rBV	1452068	2220919	24.56%	2.723%
16	7.328	717	721	725	rVB6	8382	13737	0.15%	0.017%
17	7.705	777	785	793	rBV	1587963	2489438	27.53%	3.052%
18	7.775	793	797	802	rVB4	8912	16481	0.18%	0.020%
19	8.416	899	906	918	rBV	1042121	1611501	17.82%	1.976%
20	8.863	974	982	993	rBV	1662253	2609256	28.86%	3.199%
21	8.981	1000	1002	1007	rBV5	6248	9181	0.10%	0.011%
22	9.287	1048	1054	1059	rVB	9562	15243	0.17%	0.019%
23	9.581	1096	1104	1117	rBV	1128633	1773273	19.61%	2.174%
24	10.116	1188	1195	1212	rBV	1643863	2736569	30.26%	3.355%
25	10.499	1252	1260	1267	rBV	1969800	3291092	36.40%	4.035%
26	10.640	1275	1284	1299	rBV	1009274	1700856	18.81%	2.085%
27	11.305	1391	1397	1402	rBV10	5905	13587	0.15%	0.017%
28	12.093	1524	1531	1537	rVB	34974	58587	0.65%	0.072%
29	12.310	1562	1568	1573	rVB10	5442	11074	0.12%	0.014%
30	12.969	1676	1680	1686	rVB9	6778	11887	0.13%	0.015%
31	13.087	1695	1700	1705	rBV9	4453	9924	0.11%	0.012%
32	13.193	1714	1718	1726	rBV5	12748	28455	0.31%	0.035%
33	13.775	1811	1817	1828	rBV	2872359	3897050	43.10%	4.778%
34	14.046	1854	1863	1876	rBV	3233987	4813751	53.24%	5.901%
35	14.357	1909	1916	1929	rBV	2569347	3652142	40.39%	4.477%
36	14.569	1946	1952	1963	rBV	175161	301251	3.33%	0.369%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010937.D
 Acq On : 07 Jul 2022 13:25
 Operator : CG/JU
 Sample : N3577-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB323

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.793	1986	1990	1995	rVB8	8335	12319	0.14%	0.015%
38	15.198	2051	2059	2067	rBV2	29976	53393	0.59%	0.065%
39	15.357	2079	2086	2100	rBV	4404323	6314226	69.83%	7.741%
40	15.475	2100	2106	2122	rVV	1027971	1434675	15.87%	1.759%
41	15.598	2122	2127	2134	rVB2	54173	94993	1.05%	0.116%
42	16.145	2215	2220	2228	rVB7	16180	29035	0.32%	0.036%
43	16.604	2295	2298	2304	rBV8	4671	9307	0.10%	0.011%
44	16.798	2327	2331	2338	rVB10	7468	12761	0.14%	0.016%
45	16.904	2342	2349	2350	rBV7	9445	15273	0.17%	0.019%
46	16.928	2350	2353	2361	rVB3	16649	28257	0.31%	0.035%
47	17.122	2379	2386	2396	rBV	2839171	3984757	44.07%	4.885%
48	17.222	2396	2403	2418	rVV	5186992	7196160	79.58%	8.822%
49	17.816	2499	2504	2508	rBV2	39443	53083	0.59%	0.065%
50	18.257	2577	2579	2583	rBV5	8244	12457	0.14%	0.015%
51	18.957	2696	2698	2704	rVB7	15732	18835	0.21%	0.023%
52	19.045	2710	2713	2718	rVB3	58851	72505	0.80%	0.089%
53	19.116	2721	2725	2729	rVB	56200	75352	0.83%	0.092%
54	19.469	2780	2785	2792	rBV	6435046	8311011	91.91%	10.189%
55	21.233	3080	3085	3090	rBV	3751881	4551882	50.34%	5.580%
56	23.439	3453	3460	3469	rBV2	4879721	9042267	100.00%	11.085%
57	23.592	3480	3486	3496	rVB	2457349	4742769	52.45%	5.814%




Sum of corrected areas: 81570788

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010937.D
Acq On : 07 Jul 2022 13:25
Operator : CG/JU
Sample : N3577-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

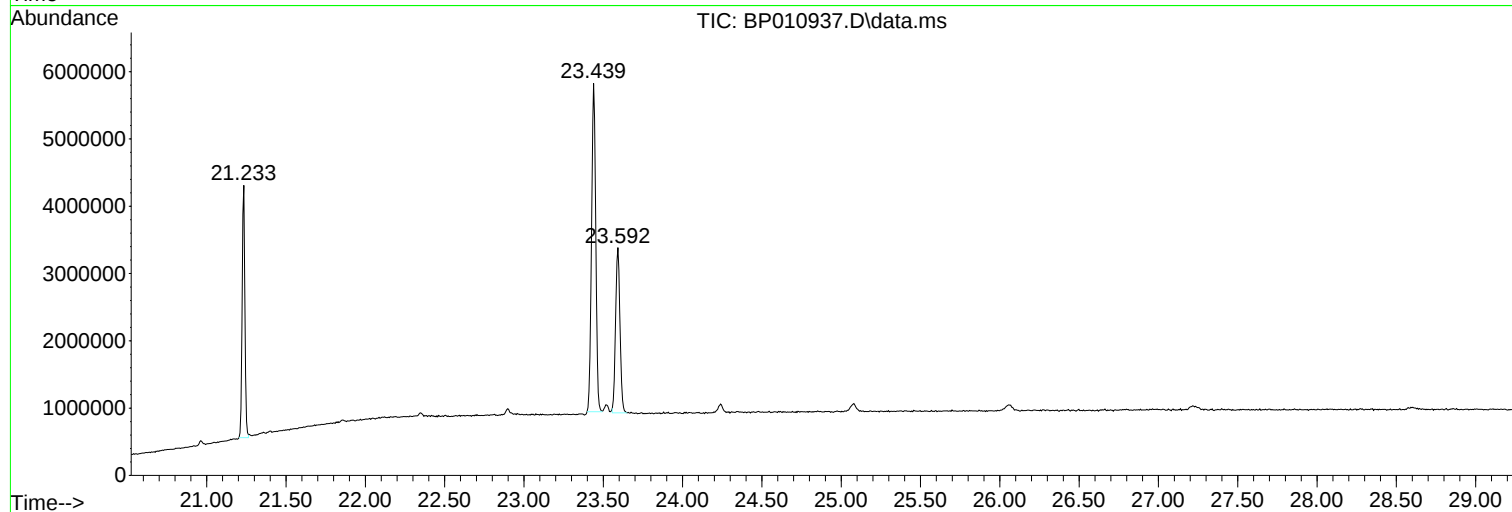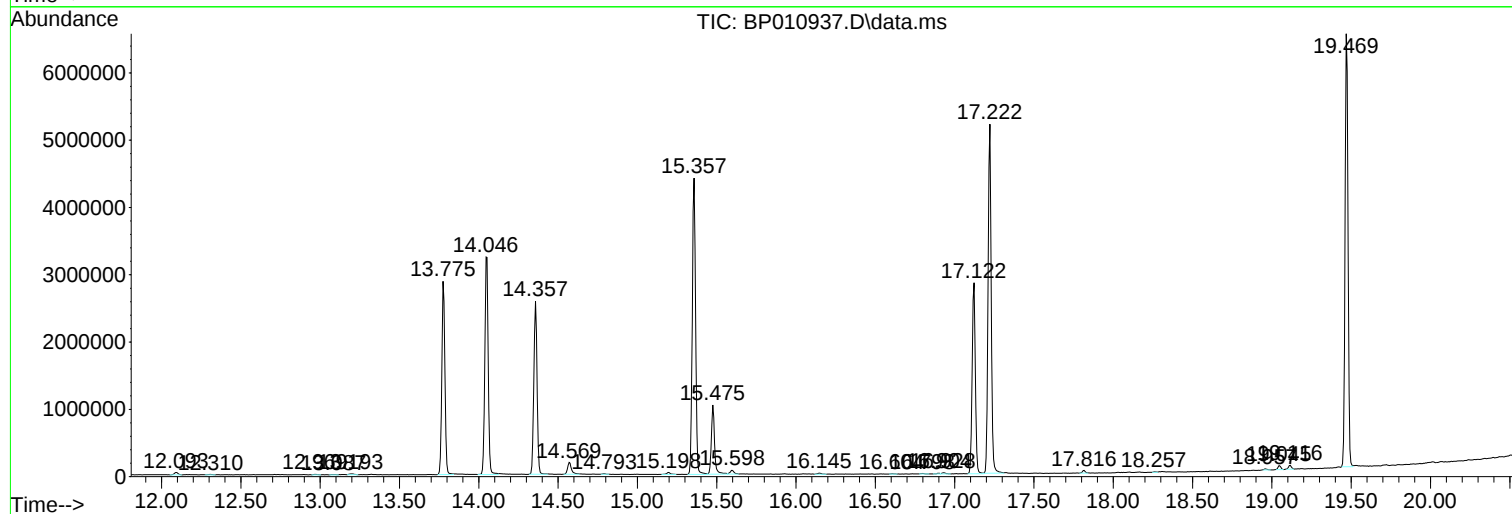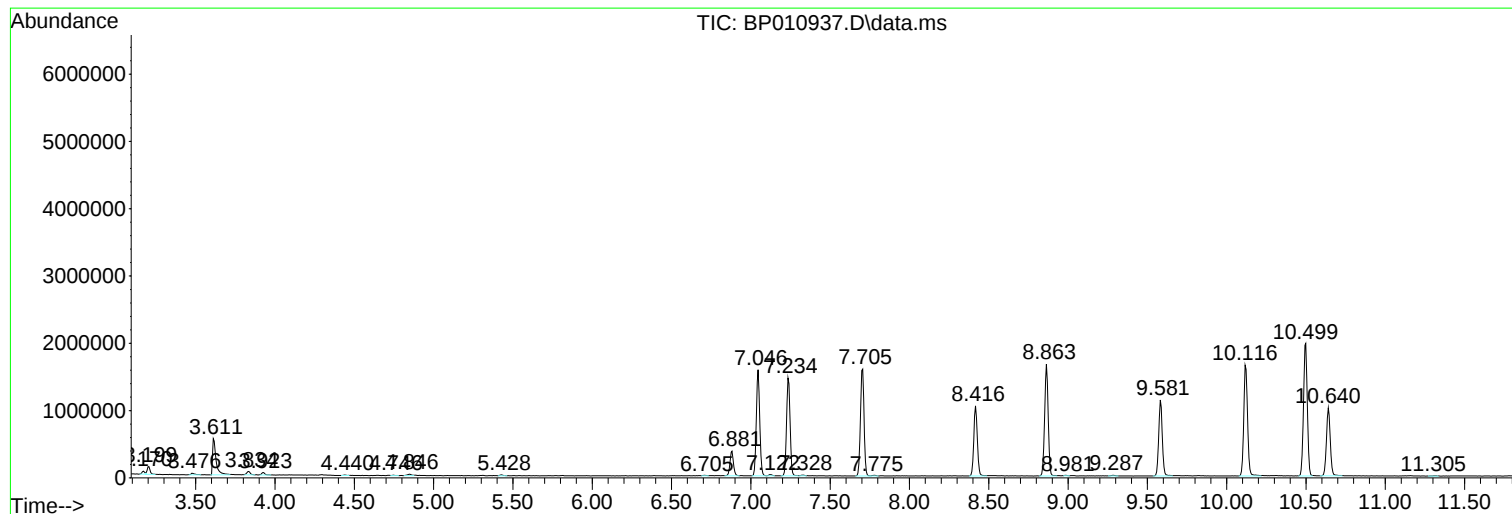

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010937.D
Acq On : 07 Jul 2022 13:25
Operator : CG/JU
Sample : N3577-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010937.D
Acq On : 07 Jul 2022 13:25
Operator : CG/JU
Sample : N3577-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc