

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010938.D
 Acq On : 07 Jul 2022 13:59
 Operator : CG/JU
 Sample : N3577-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	10	14	17	rBV	72169	93764	0.93%	0.102%
2	3.205	17	20	26	rVB	126594	158886	1.58%	0.173%
3	3.616	86	90	104	rBV	510099	795380	7.93%	0.868%
4	3.834	122	127	136	rVB	53856	82836	0.83%	0.090%
5	3.928	138	143	148	rVB	31380	42922	0.43%	0.047%
6	4.440	224	230	236	rBV2	30642	44472	0.44%	0.049%
7	4.746	279	282	287	rVB4	7650	10738	0.11%	0.012%
8	4.834	293	297	301	rVB	8399	10725	0.11%	0.012%
9	5.428	394	398	402	rVB	12201	17293	0.17%	0.019%
10	6.881	636	645	656	rBV	395245	611661	6.10%	0.668%
11	7.046	666	673	681	rBV	1697272	2539420	25.31%	2.772%
12	7.122	683	686	692	rVB2	11474	18119	0.18%	0.020%
13	7.234	698	705	718	rBV	1545713	2403626	23.95%	2.624%
14	7.328	718	721	727	rVB5	10977	17089	0.17%	0.019%
15	7.704	776	785	793	rBV	1435952	2243324	22.36%	2.449%
16	7.775	793	797	802	rVB6	7544	13784	0.14%	0.015%
17	8.416	899	906	918	rBV	1176957	1785725	17.80%	1.949%
18	8.863	974	982	996	rBV	1839919	2884365	28.74%	3.148%
19	9.287	1050	1054	1060	rVB4	9703	13785	0.14%	0.015%
20	9.581	1096	1104	1116	rBV	1241970	1977570	19.71%	2.159%
21	10.116	1186	1195	1210	rBV	1855759	3064863	30.54%	3.345%
22	10.498	1251	1260	1267	rBV	1874256	3067264	30.57%	3.348%
23	10.640	1275	1284	1295	rBV	1804099	2960228	29.50%	3.231%
24	11.304	1391	1397	1399	rBV5	7400	10969	0.11%	0.012%
25	12.092	1525	1531	1537	rVV2	39295	67970	0.68%	0.074%
26	12.969	1676	1680	1685	rBV7	8085	12343	0.12%	0.013%
27	13.204	1712	1720	1724	rBV2	26945	45196	0.45%	0.049%
28	13.322	1737	1740	1748	rVB7	7678	13624	0.14%	0.015%
29	13.775	1810	1817	1831	rBV	3484030	4827656	48.11%	5.270%
30	14.045	1855	1863	1882	rBV	3939242	5781210	57.61%	6.311%
31	14.357	1908	1916	1925	rBV	2593690	3688488	36.76%	4.026%
32	14.569	1946	1952	1965	rBV	222746	375991	3.75%	0.410%
33	14.786	1986	1989	1994	rVB7	12621	19555	0.19%	0.021%
34	15.198	2051	2059	2062	rBV2	30413	49482	0.49%	0.054%
35	15.357	2079	2086	2100	rBV	5239095	7632860	76.06%	8.332%
36	15.475	2100	2106	2120	rVV	1224825	1745948	17.40%	1.906%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010938.D
 Acq On : 07 Jul 2022 13:59
 Operator : CG/JU
 Sample : N3577-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	15.598	2122	2127	2138	rVB	66868	115783	1.15%	0.126%
38	16.092	2209	2211	2216	rVV4	11411	15548	0.15%	0.017%
39	16.145	2216	2220	2227	rVB4	20578	31496	0.31%	0.034%
40	16.792	2327	2330	2337	rVB7	10159	16349	0.16%	0.018%
41	16.898	2343	2348	2351	rBV5	19326	29987	0.30%	0.033%
42	16.933	2351	2354	2361	rVB4	12760	22079	0.22%	0.024%
43	17.122	2379	2386	2396	rBV	3038194	4207662	41.93%	4.593%
44	17.222	2396	2403	2418	rVV	6018511	8391060	83.62%	9.159%
45	17.639	2471	2474	2477	rBV5	9710	12636	0.13%	0.014%
46	17.816	2499	2504	2507	rBV3	35441	48549	0.48%	0.053%
47	18.027	2537	2540	2542	rBV4	11910	15409	0.15%	0.017%
48	18.098	2550	2552	2556	rVB	12449	15293	0.15%	0.017%
49	19.045	2709	2713	2718	rBV2	72458	99658	0.99%	0.109%
50	19.116	2721	2725	2729	rVB	62804	87825	0.88%	0.096%
51	19.468	2780	2785	2794	rBV	7037642	9601418	95.68%	10.481%
52	20.963	3036	3039	3045	rBV2	157487	218825	2.18%	0.239%
53	21.233	3080	3085	3093	rBV	3937500	4706528	46.90%	5.137%
54	23.439	3453	3460	3470	rBV2	5319715	10034727	100.00%	10.953%
55	23.592	3480	3486	3496	rVB2	2570197	4812174	47.96%	5.253%


Sum of corrected areas: 91612137

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010938.D
Acq On : 07 Jul 2022 13:59
Operator : CG/JU
Sample : N3577-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

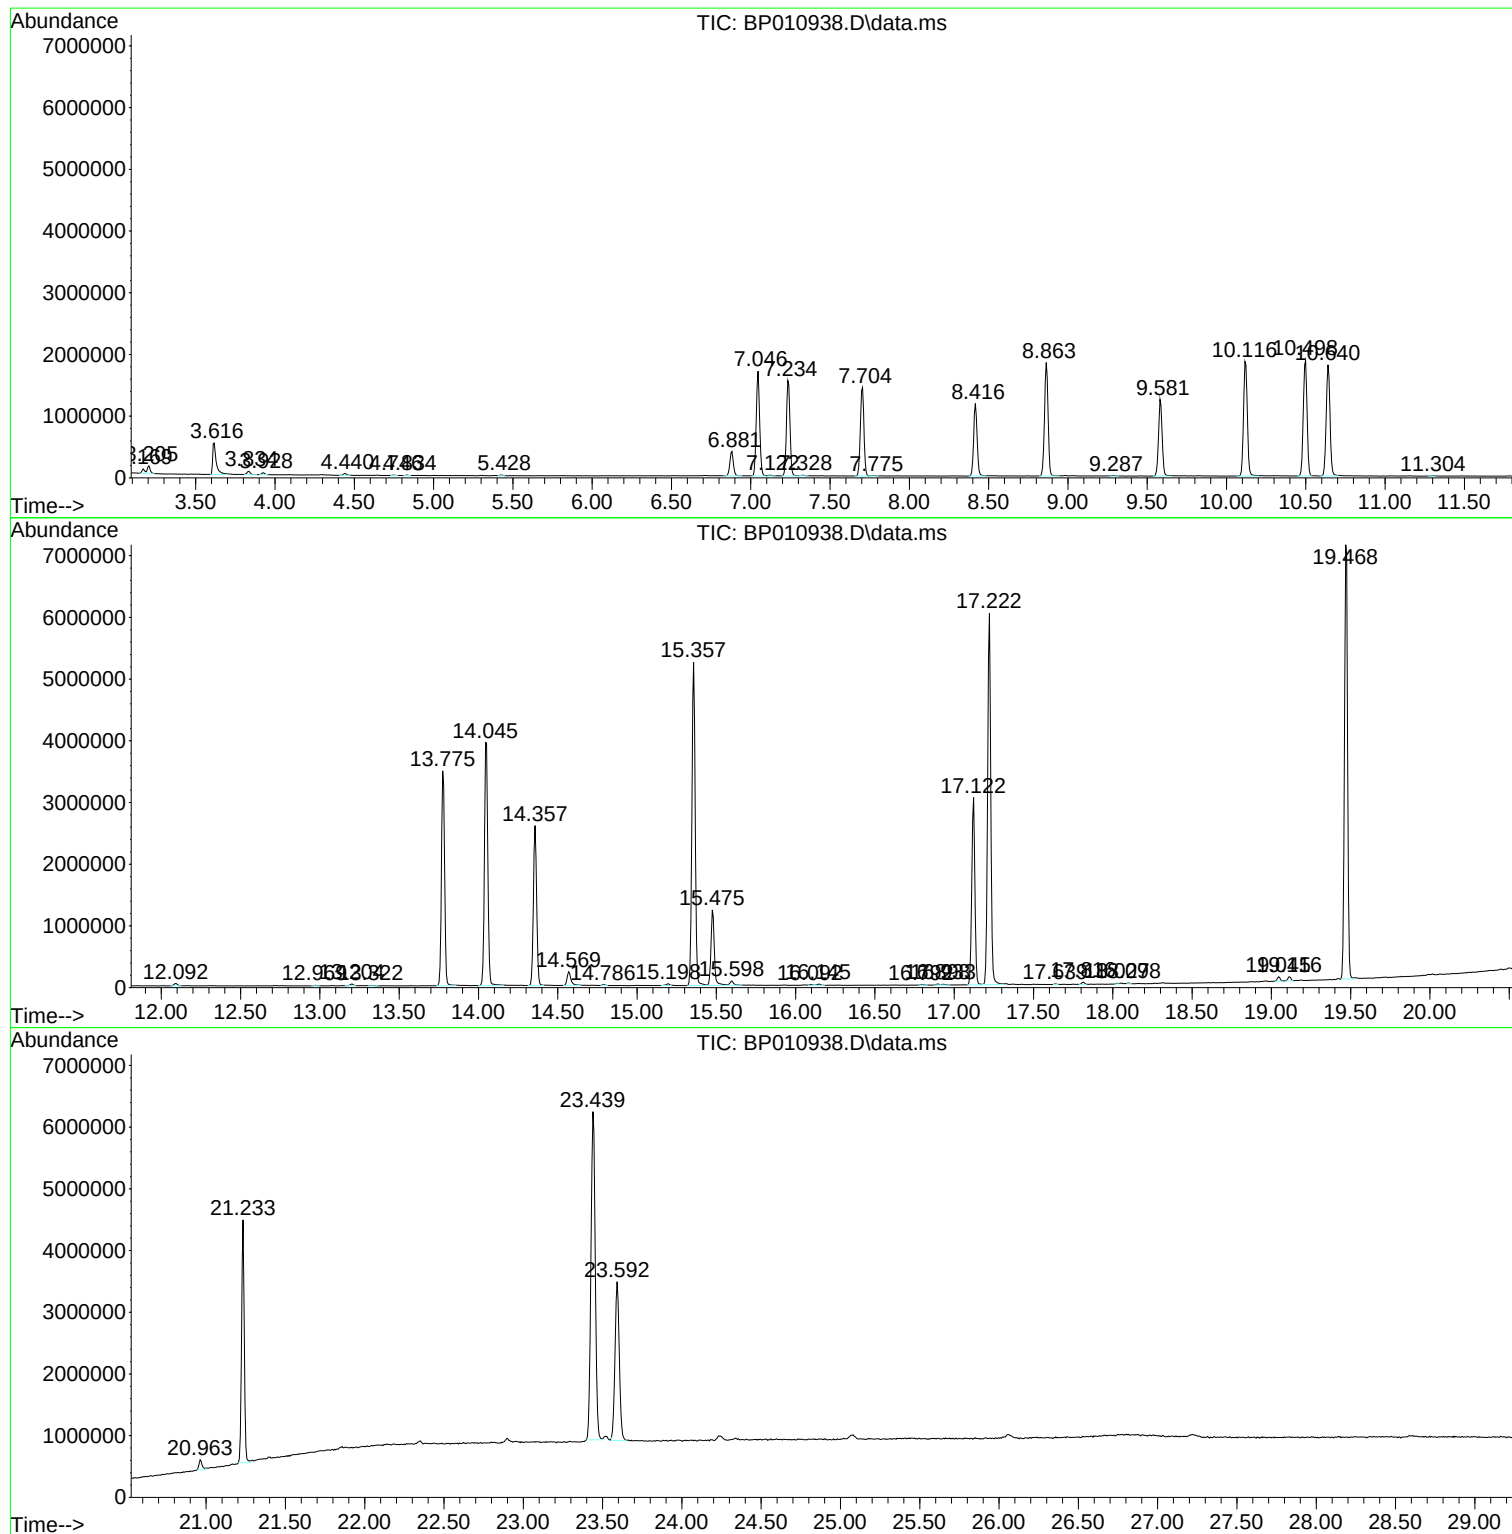

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010938.D
Acq On : 07 Jul 2022 13:59
Operator : CG/JU
Sample : N3577-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010938.D
Acq On : 07 Jul 2022 13:59
Operator : CG/JU
Sample : N3577-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------