

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010939.D
 Acq On : 07 Jul 2022 14:34
 Operator : CG/JU
 Sample : N3577-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB324

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	10	14	17	rBV	59831	74286	0.81%	0.085%
2	3.199	17	19	25	rVB	97365	116615	1.27%	0.134%
3	3.481	64	67	74	rVB2	13602	19180	0.21%	0.022%
4	3.611	87	89	113	rBV	599402	897108	9.77%	1.031%
5	3.834	122	127	131	rBV	53173	73803	0.80%	0.085%
6	3.923	139	142	147	rVB	32501	38626	0.42%	0.044%
7	4.293	202	205	210	rVB7	6883	10351	0.11%	0.012%
8	4.440	226	230	240	rVB4	23280	40205	0.44%	0.046%
9	4.828	293	296	300	rBV2	6861	10344	0.11%	0.012%
10	5.428	393	398	404	rBV	13530	21072	0.23%	0.024%
11	6.511	576	582	586	rBV9	5177	10479	0.11%	0.012%
12	6.705	609	615	619	rBV8	5768	11758	0.13%	0.014%
13	6.881	637	645	652	rBV	381252	582815	6.35%	0.670%
14	7.046	663	673	682	rBV	1576292	2358545	25.68%	2.710%
15	7.122	682	686	694	rVB	20641	34092	0.37%	0.039%
16	7.234	696	705	717	rBV	1443904	2224832	24.23%	2.556%
17	7.328	717	721	728	rVB5	10229	16076	0.18%	0.018%
18	7.705	775	785	792	rBV	1335683	2102019	22.89%	2.415%
19	7.775	792	797	803	rVB5	11505	19116	0.21%	0.022%
20	8.416	899	906	914	rBV	1087087	1671518	18.20%	1.920%
21	8.863	974	982	991	rBV	1656140	2602638	28.34%	2.990%
22	8.987	999	1003	1007	rVB6	9693	13199	0.14%	0.015%
23	9.287	1048	1054	1059	rVB3	12858	22122	0.24%	0.025%
24	9.581	1095	1104	1113	rBV	1103877	1775732	19.34%	2.040%
25	10.116	1187	1195	1210	rBV	1677600	2783378	30.31%	3.198%
26	10.493	1252	1259	1267	rBV	1680463	2818727	30.70%	3.238%
27	10.640	1275	1284	1298	rBV	3592180	5898508	64.23%	6.776%
28	11.157	1369	1372	1378	rVB7	5680	10119	0.11%	0.012%
29	11.316	1391	1399	1406	rBV7	8116	19720	0.21%	0.023%
30	12.093	1525	1531	1538	rVB	35767	55385	0.60%	0.064%
31	12.310	1561	1568	1574	rBV	4588	12087	0.13%	0.014%
32	12.969	1677	1680	1687	rVB8	5972	10888	0.12%	0.013%
33	13.204	1715	1720	1726	rVB3	28374	52491	0.57%	0.060%
34	13.775	1811	1817	1833	rBV	3176562	4365932	47.54%	5.016%
35	13.893	1835	1837	1842	rVB6	7161	10742	0.12%	0.012%
36	14.051	1853	1864	1886	rBV	3600060	5208449	56.72%	5.984%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
 Data File : BP010939.D
 Acq On : 07 Jul 2022 14:34
 Operator : CG/JU
 Sample : N3577-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB324

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.269	1898	1901	1906	rVB6	6340	9559	0.10%	0.011%
38	14.357	1909	1916	1928	rBV	2307661	3308115	36.02%	3.800%
39	14.569	1946	1952	1965	rBV	209099	362514	3.95%	0.416%
40	14.787	1986	1989	1998	rVB	13749	21325	0.23%	0.024%
41	15.198	2052	2059	2063	rBV2	28756	45943	0.50%	0.053%
42	15.357	2079	2086	2092	rBV	4862744	6858550	74.69%	7.879%
43	15.404	2092	2094	2100	rVV2	77011	106351	1.16%	0.122%
44	15.475	2100	2106	2122	rVV	1120576	1582884	17.24%	1.818%
45	15.598	2122	2127	2135	rVB	57287	91269	0.99%	0.105%
46	15.928	2179	2183	2188	rVB8	6538	11732	0.13%	0.013%
47	16.145	2215	2220	2226	rBV4	16889	29604	0.32%	0.034%
48	16.792	2328	2330	2338	rVB7	10570	17091	0.19%	0.020%
49	16.898	2345	2348	2351	rBV5	10230	14340	0.16%	0.016%
50	16.934	2351	2354	2358	rVB6	12118	17029	0.19%	0.020%
51	17.122	2379	2386	2396	rBV	2699469	3763920	40.99%	4.324%
52	17.222	2396	2403	2419	rBV	5585672	7707095	83.93%	8.854%
53	17.816	2499	2504	2510	rBV	111662	135961	1.48%	0.156%
54	18.957	2694	2698	2702	rBV2	115274	132916	1.45%	0.153%
55	19.045	2709	2713	2718	rBV4	71724	96206	1.05%	0.111%
56	19.116	2721	2725	2728	rVV2	58506	72185	0.79%	0.083%
57	19.469	2780	2785	2793	rBV	6642342	8884607	96.75%	10.207%
58	21.233	3080	3085	3092	rBV	3439045	4314212	46.98%	4.956%
59	23.439	3454	3460	3470	rVB2	4923520	9183013	100.00%	10.550%
60	23.592	3480	3486	3495	rVB2	2210804	4285517	46.67%	4.923%




Sum of corrected areas: 87044895

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010939.D
Acq On : 07 Jul 2022 14:34
Operator : CG/JU
Sample : N3577-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

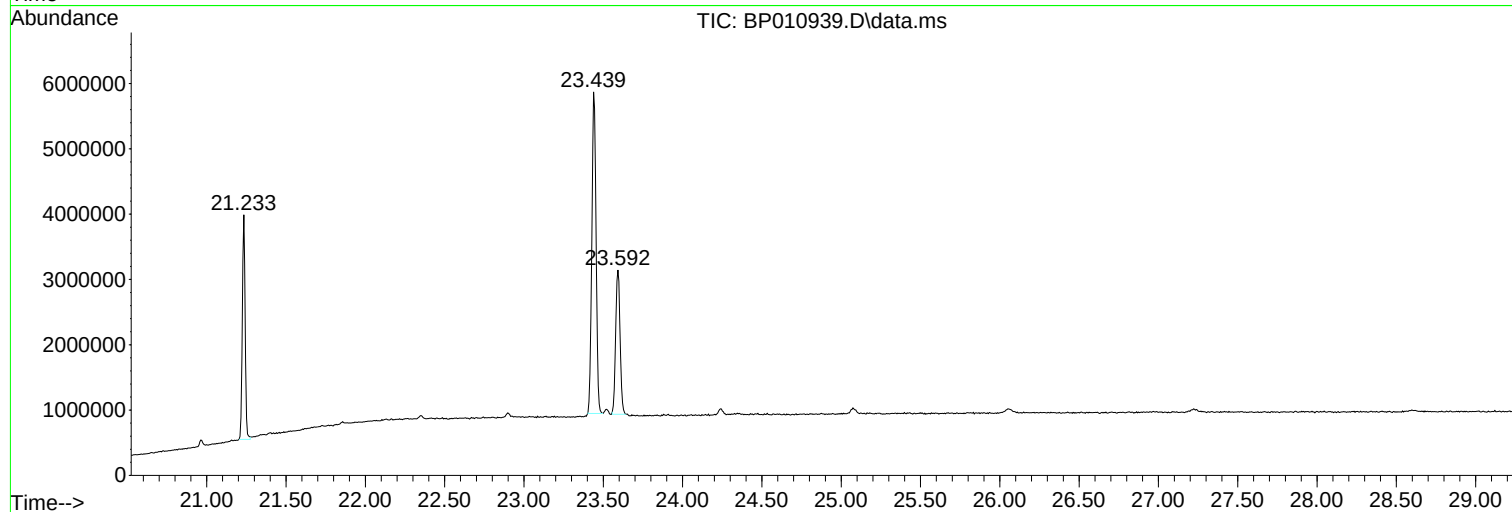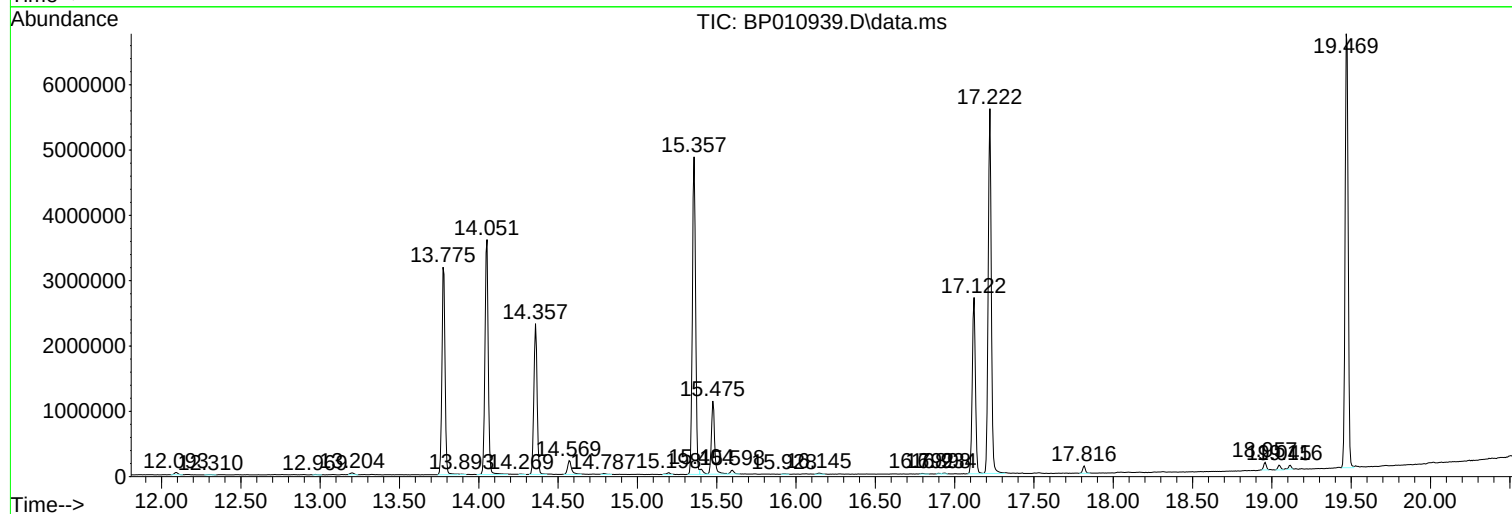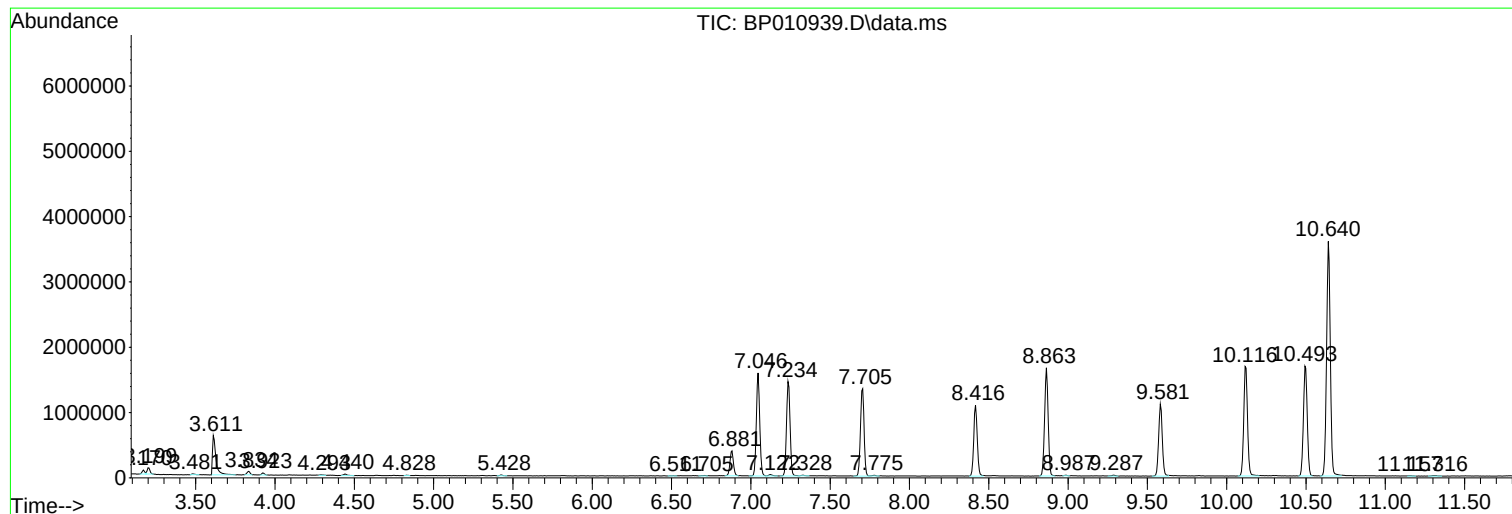

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010939.D
Acq On : 07 Jul 2022 14:34
Operator : CG/JU
Sample : N3577-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070722\
Data File : BP010939.D
Acq On : 07 Jul 2022 14:34
Operator : CG/JU
Sample : N3577-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc