

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071422\
 Data File : BP010969.D
 Acq On : 14 Jul 2022 12:40
 Operator : CG/JU
 Sample : SSTD01018
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010618

Quant Time: Jul 14 13:52:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 14 13:50:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	377692	20.000	ng/ul	0.00
20) Naphthalene-d8	10.481	136	1585819	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.351	164	912884	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	1815104	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.239	240	1812322	20.000	ng/ul	# 0.00
88) Perylene-d12	23.598	264	1792571	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	40194	4.026	ng/uL	0.00
4) Pyridine-d5	3.593	84	254836	9.588	ng/ul	0.00
7) Phenol-d5	6.864	99	283252	9.474	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	191244	9.781	ng/ul	0.00
11) 2-Chlorophenol-d4	7.217	132	233210	9.402	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	224780	9.510	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	106322	10.532	ng/ul	0.00
24) 2-Nitrophenol-d4	9.569	143	100556	12.040	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.105	165	194923	9.445	ng/ul	0.00
31) 4-Chloroaniline-d4	10.622	131	323862	9.614	ng/ul	0.00
46) Dimethylphthalate-d6	13.769	166	596207	9.534	ng/ul	0.00
49) Acenaphthylene-d8	14.040	160	690835	8.656	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	104797	10.729	ng/ul	0.00
60) Fluorene-d10	15.351	176	514902	9.595	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	65951	10.967	ng/ul	0.00
73) Anthracene-d10	17.216	188	745122	9.227	ng/ul	0.00
81) Pyrene-d10	19.475	212	910901	9.226	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.445	264	810335	9.148	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.217	88	42617	4.002	ng/uL#	84
5) Pyridine	3.617	79	264482	9.824	ng/ul#	74
6) Benzaldehyde	6.834	77	172742	10.950	ng/ul	96
8) Phenol	6.887	94	305262	9.546	ng/ul#	84
10) Bis(2-Chloroethyl)ether	7.122	93	251810	9.805	ng/ul	88
12) 2-Chlorophenol	7.252	128	246061	9.610	ng/ul	90
13) 2-Methylphenol	8.134	108	221815	9.317	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.158	45	227	0.007	ng/ul#	1
16) Acetophenone	8.511	105	365851	10.079	ng/ul#	89
17) N-Nitroso-di-n-propyla...	8.499	70	178958	9.750	ng/ul	91
18) 4-Methylphenol	8.464	108	239937	9.678	ng/ul	96
19) Hexachloroethane	8.758	117	97412	9.394	ng/ul#	81
22) Nitrobenzene	8.887	77	253586	10.066	ng/ul	92
23) Isophorone	9.416	82	472082	8.936	ng/ul	99
25) 2-Nitrophenol	9.599	139	115713	11.441	ng/ul#	82
26) 2,4-Dimethylphenol	9.663	107	254662	9.216	ng/ul	95
27) Bis(2-Chloroethoxy)met...	9.905	93	325026	9.752	ng/ul	98
29) 2,4-Dichlorophenol	10.128	162	204360	9.530	ng/ul	97
30) Naphthalene	10.528	128	786151	9.512	ng/ul	100
32) 4-Chloroaniline	10.646	127	324260	9.716	ng/ul	97
33) Hexachlorobutadiene	10.816	225	122624	8.951	ng/ul	95
34) Caprolactam	11.440	113	63260	9.391	ng/ul	95
35) 4-Chloro-3-methylphenol	11.781	107	227842	9.803	ng/ul	93
36) 2-Methylnaphthalene	12.152	142	506447	9.463	ng/ul	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071422\
 Data File : BP010969.D
 Acq On : 14 Jul 2022 12:40
 Operator : CG/JU
 Sample : SSTD01018
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010618

Quant Time: Jul 14 13:52:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 14 13:50:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.375	142	512060	9.630	ng/ul#	99
39) 1,2,4,5-Tetrachloroben...	12.522	216	232289	8.855	ng/ul#	98
40) Hexachlorocyclopentadiene	12.505	237	127386	7.663	ng/ul	96
41) 2,4,6-Trichlorophenol	12.769	196	147098	9.726	ng/ul	95
42) 2,4,5-Trichlorophenol	12.840	196	155895	9.605	ng/ul	100
43) 1,1'-Biphenyl	13.175	154	656699	9.138	ng/ul#	97
44) 2-Chloronaphthalene	13.216	162	491788	9.084	ng/ul	98
45) 2-Nitroaniline	13.428	65	130096	11.326	ng/ul#	84
47) Dimethylphthalate	13.816	163	606621	9.687	ng/ul	99
48) 2,6-Dinitrotoluene	13.934	165	96442	10.278	ng/ul	98
50) Acenaphthylene	14.069	152	790368	9.042	ng/ul	98
51) 3-Nitroaniline	14.263	138	118607	10.544	ng/ul	89
52) Acenaphthene	14.410	153	529275	9.385	ng/ul	99
53) 2,4-Dinitrophenol	14.463	184	44237	12.280	ng/ul	91
55) 4-Nitrophenol	14.575	109	85118	10.960	ng/ul#	72
56) Dibenzofuran	14.751	168	737680	9.549	ng/ul	96
57) 2,4-Dinitrotoluene	14.722	165	143238	11.424	ng/ul#	83
58) 2,3,4,6-Tetrachlorophenol	14.981	232	122914	10.575	ng/ul	91
59) Diethylphthalate	15.193	149	612581	9.839	ng/ul	98
61) Fluorene	15.404	166	594332	9.648	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.410	204	276040	9.573	ng/ul	98
63) 4-Nitroaniline	15.434	138	109847	10.561	ng/ul#	79
66) 4,6-Dinitro-2-methylph...	15.487	198	69413	10.682	ng/ul#	99
67) N-Nitrosodiphenylamine	15.622	169	500874	9.111	ng/ul	99
68) 4-Bromophenyl-phenylether	16.310	248	155502	8.548	ng/ul	97
69) Hexachlorobenzene	16.410	284	183101	8.690	ng/ul	93
70) Atrazine	16.593	200	168154	9.225	ng/ul	98
71) Pentachlorophenol	16.763	266	99873	9.206	ng/ul	94
72) Phenanthrene	17.157	178	926272	9.583	ng/ul	99
74) Anthracene	17.251	178	919838	9.462	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.134	216	249378	8.326	ng/uL	96
76) Pentachlorobenzene	14.663	250	223058	8.683	ng/uL	98
77) Carbazole	17.528	167	880265	10.059	ng/ul	99
78) Di-n-butylphthalate	18.104	149	1033522	9.911	ng/ul	99
80) Fluoranthene	19.145	202	1063619	8.759	ng/ul#	87
82) Pyrene	19.498	202	1118897	9.124	ng/ul#	82
83) Butylbenzylphthalate	20.398	149	467899	10.840	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.163	252	287345	7.678	ng/ul#	97
85) Benzo(a)anthracene	21.222	228	1076788	9.500	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.169	149	708569	10.366	ng/ul#	97
87) Chrysene	21.275	228	1076064	9.907	ng/ul	100
89) Di-n-octyl phthalate	22.080	149	1095239	10.293	ng/ul	100
90) Benzo(b)fluoranthene	22.875	252	1072844	9.624	ng/ul#	95
91) Benzo(k)fluoranthene	22.927	252	983341	9.280	ng/ul#	94
93) Benzo(a)pyrene	23.492	252	1017031	9.379	ng/ul#	94
94) Indeno(1,2,3-cd)pyrene	26.039	276	1173112	8.965	ng/ul#	88
95) Dibenzo(a,h)anthracene	26.063	278	1028289	9.162	ng/ul#	90
96) Benzo(g,h,i)perylene	26.786	276	997217	8.959	ng/ul#	88





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 4.002 ng/uL
RT: 3.217 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 88 Resp: 42617
Ion Ratio Lower Upper
88 100
43 33.1 35.8 53.6#
58 71.7 68.1 102.1

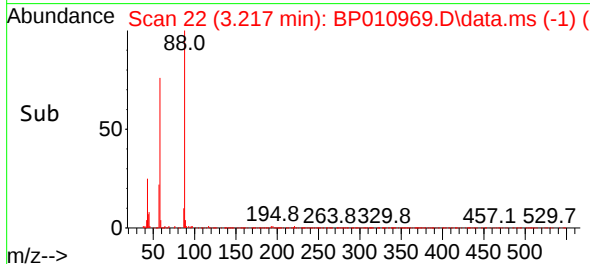

#5
Pyridine
Concen: 9.824 ng/uL
RT: 3.617 min Scan# 90
Delta R.T. 0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion: 79 Resp: 264482
Ion Ratio Lower Upper
79 100
52 74.9 83.8 125.8#
51 38.1 41.0 61.4#


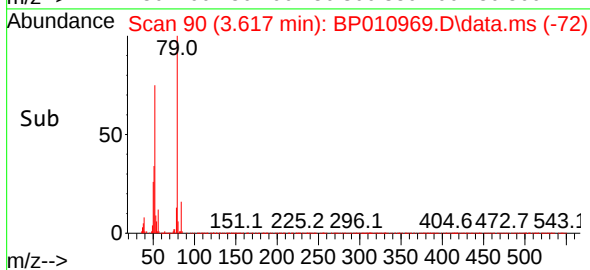

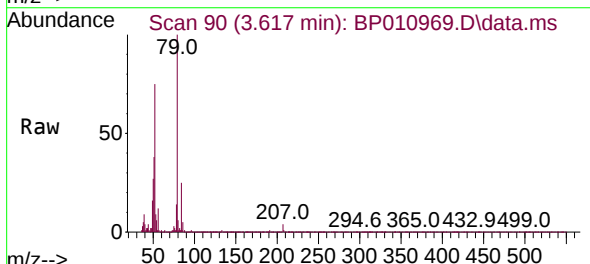


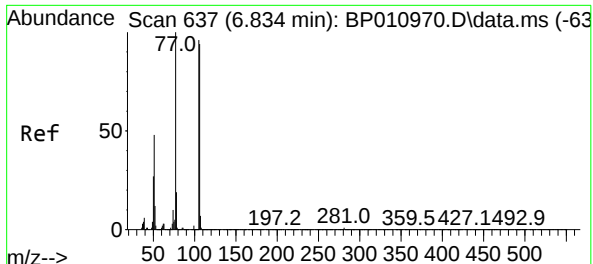

#6
Benzaldehyde
Concen: 10.950 ng/ul
RT: 6.834 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 77 Resp: 172742
Ion Ratio Lower Upper
77 100
105 101.7 76.0 114.0
106 92.8 73.2 109.8

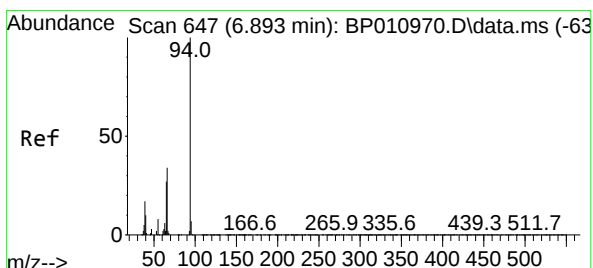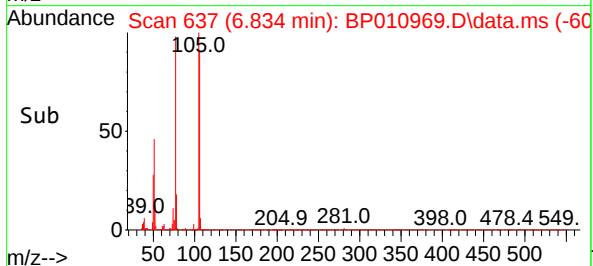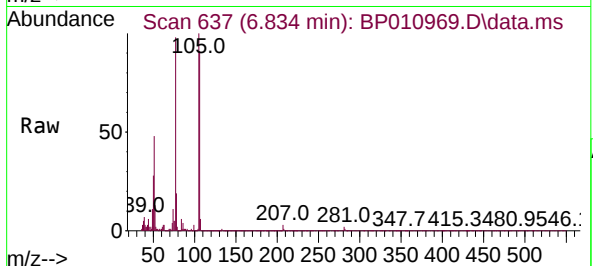

#8
Phenol
Concen: 9.546 ng/ul
RT: 6.887 min Scan# 646
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion: 94 Resp: 305262
Ion Ratio Lower Upper
94 100
65 27.0 27.4 41.2#
66 35.0 37.4 56.2#


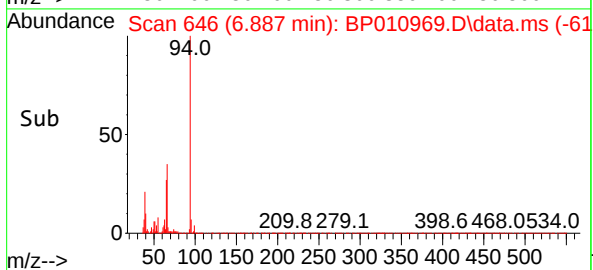

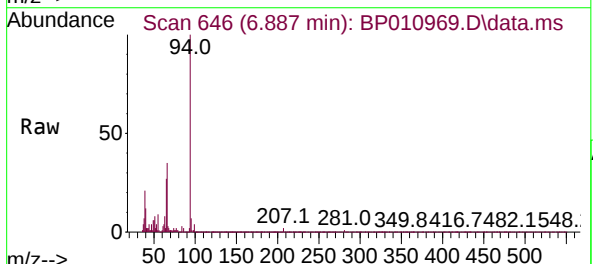




#10
Bis(2-Chloroethyl)ether
Concen: 9.805 ng/ul
RT: 7.122 min Scan# 686
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 93 Resp: 251810
Ion Ratio Lower Upper
93 100
63 77.0 72.4 108.6
95 31.5 27.3 40.9



#12
2-Chlorophenol
Concen: 9.610 ng/ul
RT: 7.252 min Scan# 708
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion: 128 Resp: 246061
Ion Ratio Lower Upper
128 100
64 45.1 44.8 67.2
130 31.3 25.8 38.6





#13

2-Methylphenol

Concen: 9.317 ng/ul

RT: 8.134 min Scan# 8

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :





SSTD010618

Tgt Ion:108 Resp: 221815

Ion Ratio Lower Upper

108 100

107 88.1 71.4 107.0

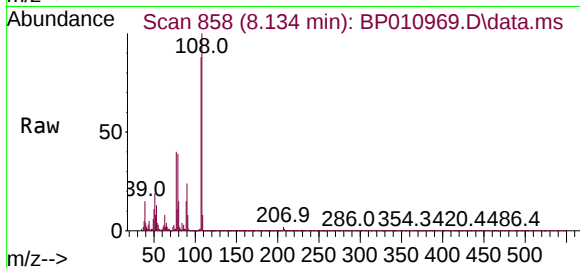

#14

2,2'-oxybis(1-Chloropropane)

Concen: 0.007 ng/ul

RT: 8.158 min Scan# 862

Delta R.T. -0.059 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion: 45 Resp: 227


Ion Ratio Lower Upper

45 100

77 370.5 11.2 16.8#

79 277.4 6.9 10.3#



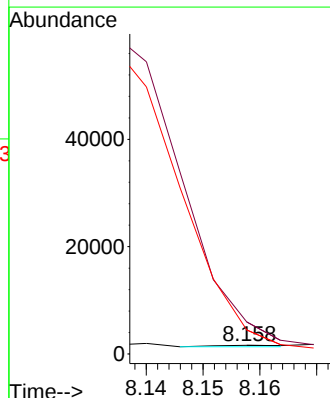
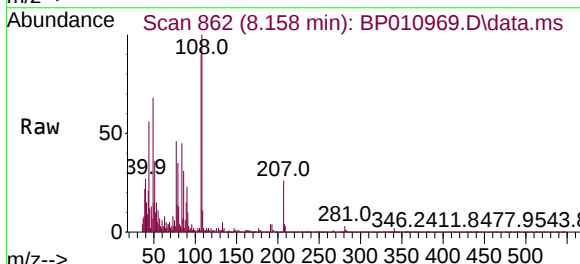




#16
Acetophenone
Concen: 10.079 ng/ul
RT: 8.511 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:105 Resp: 365851
Ion Ratio Lower Upper
105 100
77 76.4 67.5 101.3
51 27.1 29.6 44.4#

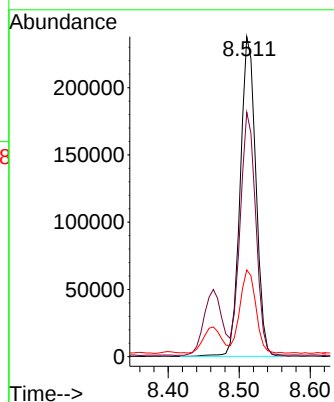

#17
N-Nitroso-di-n-propylamine
Concen: 9.750 ng/ul
RT: 8.499 min Scan# 920
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion: 70 Resp: 178958
Ion Ratio Lower Upper
70 100
42 58.8 53.8 80.8
101 10.1 7.8 11.6
130 22.5 15.4 23.2


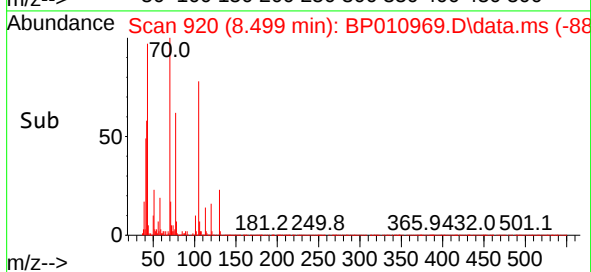
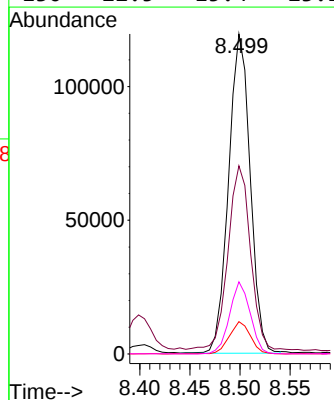





#18
4-Methylphenol
Concen: 9.678 ng/ul
RT: 8.464 min Scan# 914
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:108 Resp: 239937
Ion Ratio Lower Upper
108 100
107 114.4 88.3 132.5



#19
Hexachloroethane
Concen: 9.394 ng/ul
RT: 8.758 min Scan# 964
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:117 Resp: 97412
Ion Ratio Lower Upper
117 100
201 88.3 85.7 128.5
199 55.0 57.4 86.0#




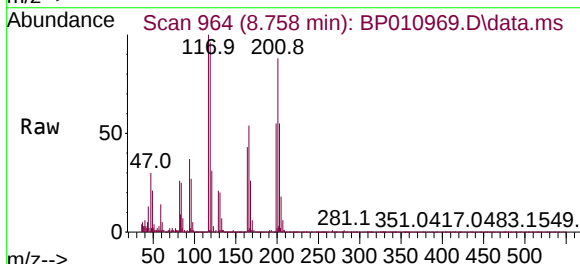




#22
Nitrobenzene
Concen: 10.066 ng/ul
RT: 8.887 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 77 Resp: 253586
Ion Ratio Lower Upper
77 100
123 45.3 31.5 47.3
65 13.4 11.4 17.2



#23
Isophorone
Concen: 8.936 ng/ul
RT: 9.416 min Scan# 1076
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion: 82 Resp: 472082
Ion Ratio Lower Upper
82 100
95 7.2 6.6 10.0
138 17.2 13.8 20.6









#25
2-Nitrophenol
Concen: 11.441 ng/ul
RT: 9.599 min Scan# 1107
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:139 Resp: 115713
Ion Ratio Lower Upper
139 100
65 51.9 54.2 81.4#
109 29.0 30.6 45.8#



#26
2,4-Dimethylphenol
Concen: 9.216 ng/ul
RT: 9.663 min Scan# 1118
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:107 Resp: 254662
Ion Ratio Lower Upper
107 100
121 53.3 39.1 58.7
122 86.9 66.1 99.1





#27

Bis(2-Chloroethoxy)methane

Concen: 9.752 ng/ul

RT: 9.905 min Scan# 1159

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion: 93 Resp: 325026

Ion Ratio Lower Upper

93 100

95 32.5 26.6 39.8

123 11.5 7.8 11.8



#29

2,4-Dichlorophenol

Concen: 9.530 ng/ul

RT: 10.128 min Scan# 1197

Delta R.T. -0.006 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion:162 Resp: 204360


Ion Ratio Lower Upper

162 100

164 63.5 52.5 78.7

98 37.7 31.4 47.0









#30
Naphthalene
Concen: 9.512 ng/ul
RT: 10.528 min Scan# 1265
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:128 Resp: 786151
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 12.7 10.2 15.4

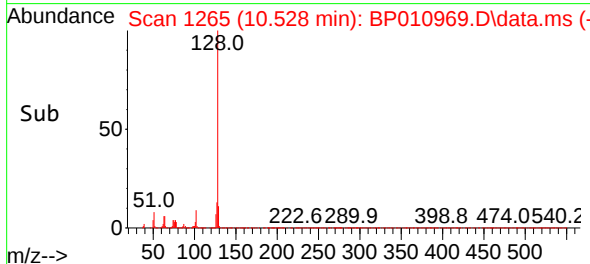

#32
4-Chloroaniline
Concen: 9.716 ng/ul
RT: 10.646 min Scan# 1285
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:127 Resp: 324260
Ion Ratio Lower Upper
127 100
129 31.0 26.2 39.2

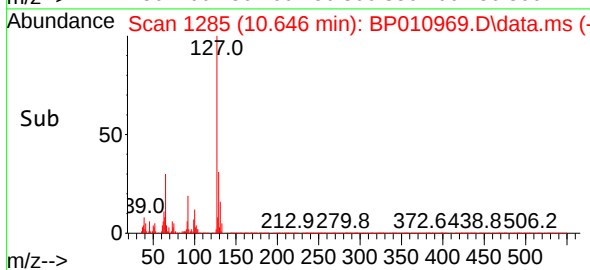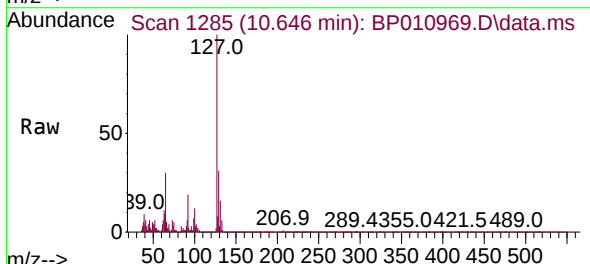



#33

Hexachlorobutadiene

Concen: 8.951 ng/ul

RT: 10.816 min Scan# 11

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:225 Resp: 122624

Ion Ratio Lower Upper

225 100

223 62.0 53.7 80.5

227 63.8 49.4 74.2

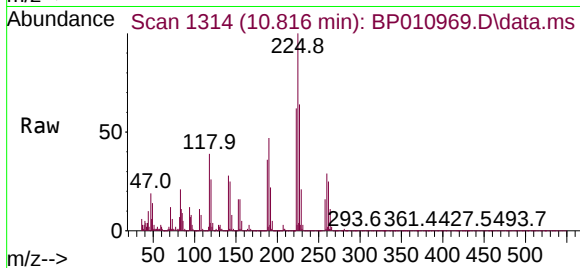

#34

Caprolactam

Concen: 9.391 ng/ul

RT: 11.440 min Scan# 1420

Delta R.T. -0.006 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion:113 Resp: 63260


Ion Ratio Lower Upper

113 100

55 182.6 153.8 230.8

56 133.2 110.2 165.4









#35
4-Chloro-3-methylphenol
Concen: 9.803 ng/ul
RT: 11.781 min Scan# 1479
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:107 Resp: 227842
Ion Ratio Lower Upper
107 100
144 25.1 18.6 27.8
142 81.7 59.6 89.4



#36
2-Methylnaphthalene
Concen: 9.463 ng/ul
RT: 12.152 min Scan# 1541
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:142 Resp: 506447
Ion Ratio Lower Upper
142 100
141 89.0 70.1 105.1


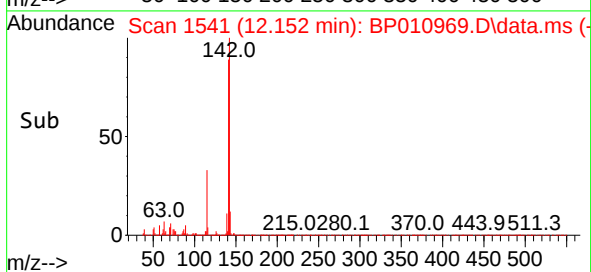






#37
1-Methylnaphthalene
Concen: 9.630 ng/ul
RT: 12.375 min Scan# 1579
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:142 Resp: 512060
Ion Ratio Lower Upper
142 100
141 90.6 73.3 109.9
116 3.4 4.0 6.0#



#39
1,2,4,5-Tetrachlorobenzene
Concen: 8.855 ng/ul
RT: 12.522 min Scan# 1604
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:216 Resp: 232289
Ion Ratio Lower Upper
216 100
214 78.3 63.0 94.6
179 22.4 18.1 27.1
108 20.4 13.6 20.4#

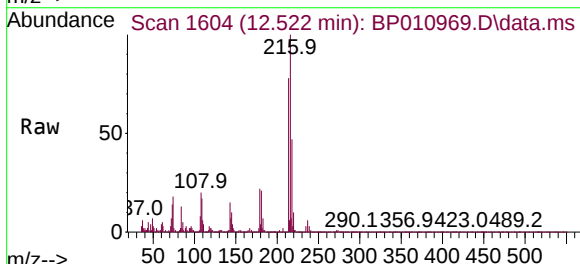



#40

Hexachlorocyclopentadiene

Concen: 7.663 ng/ul

RT: 12.505 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:237 Resp: 127386

Ion Ratio Lower Upper

237 100

235 62.9 52.8 79.2

272 12.6 11.5 17.3

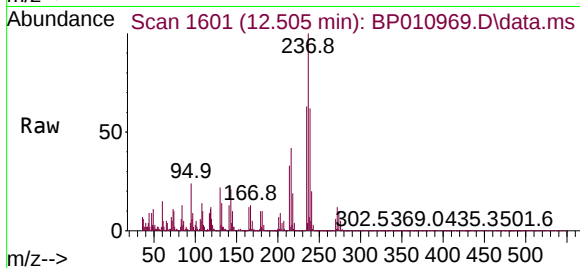

#41

2,4,6-Trichlorophenol

Concen: 9.726 ng/ul

RT: 12.769 min Scan# 1646

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion:196 Resp: 147098


Ion Ratio Lower Upper

196 100

198 91.8 78.2 117.4

200 30.2 25.0 37.6









#42
2,4,5-Trichlorophenol
Concen: 9.605 ng/ul
RT: 12.840 min Scan# 1
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:196 Resp: 155895
Ion Ratio Lower Upper
196 100
198 96.7 77.0 115.4
200 30.9 24.8 37.2



#43
1,1'-Biphenyl
Concen: 9.138 ng/ul
RT: 13.175 min Scan# 1715
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:154 Resp: 656699
Ion Ratio Lower Upper
154 100
153 40.9 31.9 47.9
76 14.5 9.2 13.8#



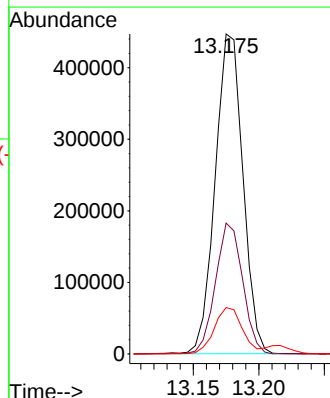





#44
2-Chloronaphthalene
Concen: 9.084 ng/ul
RT: 13.216 min Scan# 1722
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:162 Resp: 491788
Ion Ratio Lower Upper
162 100
164 32.9 25.5 38.3
127 41.0 31.9 47.9

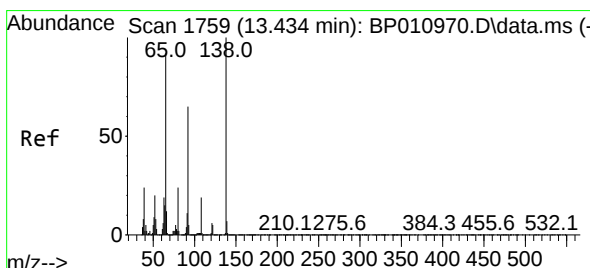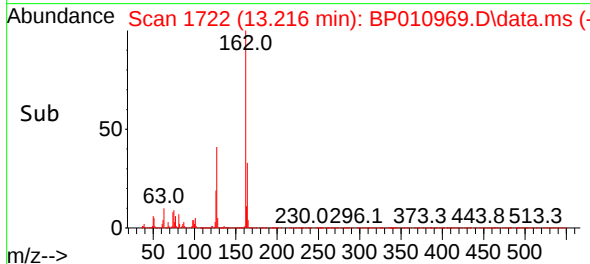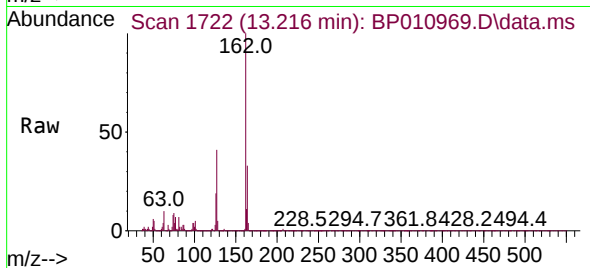

#45
2-Nitroaniline
Concen: 11.326 ng/ul
RT: 13.428 min Scan# 1758
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion: 65 Resp: 130096
Ion Ratio Lower Upper
65 100
92 70.0 49.0 73.6
138 100.9 66.4 99.6#


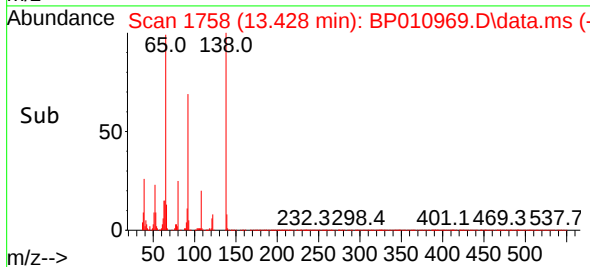

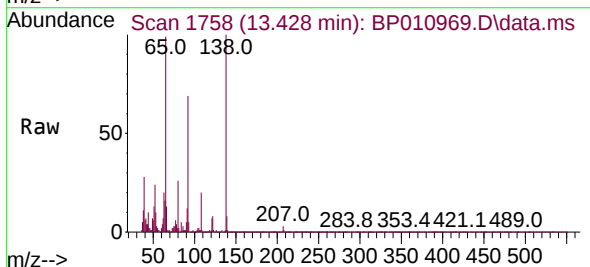




#47
Dimethylphthalate
Concen: 9.687 ng/ul
RT: 13.816 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:163 Resp: 606621
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.2
164 10.0 7.6 11.4

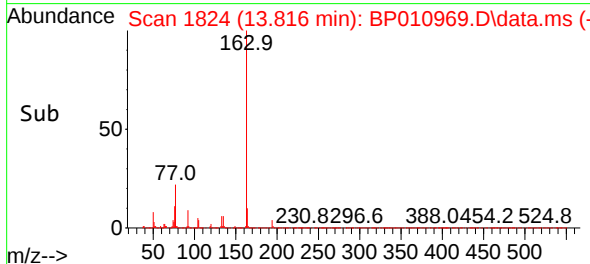

#48
2,6-Dinitrotoluene
Concen: 10.278 ng/ul
RT: 13.934 min Scan# 1844
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:165 Resp: 96442
Ion Ratio Lower Upper
165 100
89 66.5 52.9 79.3
121 28.0 19.4 29.2

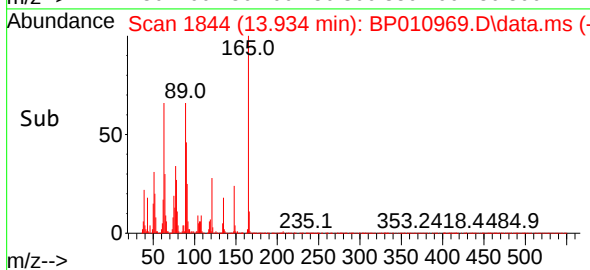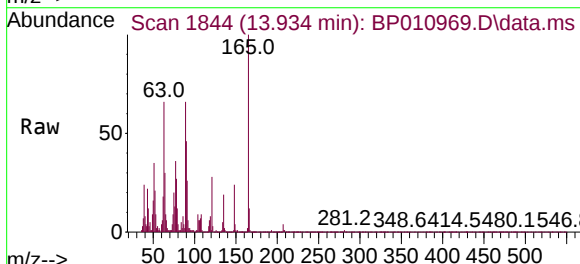



#50

Acenaphthylene

Concen: 9.042 ng/ul

RT: 14.069 min Scan# 1867

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:152 Resp: 790368

Ion Ratio Lower Upper

152 100

151 19.8 16.5 24.7

153 13.1 10.1 15.1

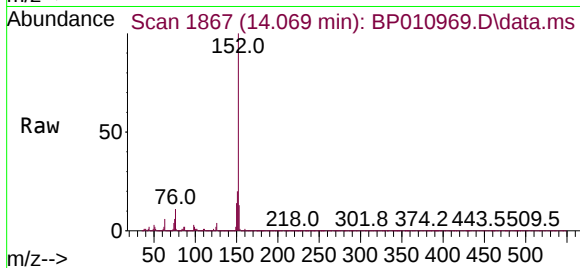

#51

3-Nitroaniline

Concen: 10.544 ng/ul

RT: 14.263 min Scan# 1900

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion:138 Resp: 118607


Ion Ratio Lower Upper

138 100

108 12.9 11.0 16.4

92 116.6 104.6 156.8


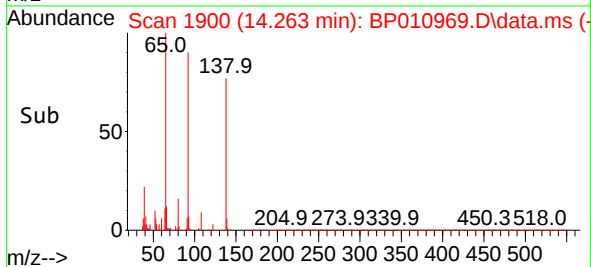

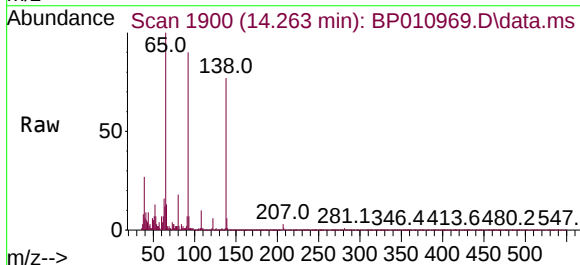




#52
Acenaphthene
Concen: 9.385 ng/ul
RT: 14.410 min Scan# 1925
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:153 Resp: 529275
Ion Ratio Lower Upper
153 100
152 47.2 36.2 54.2
154 89.0 70.8 106.2

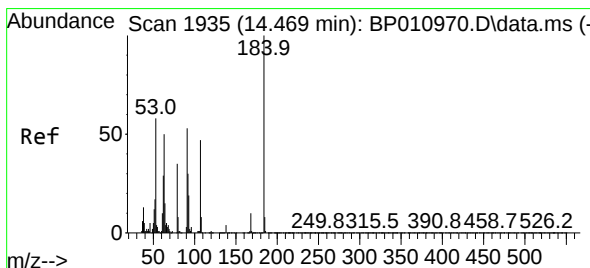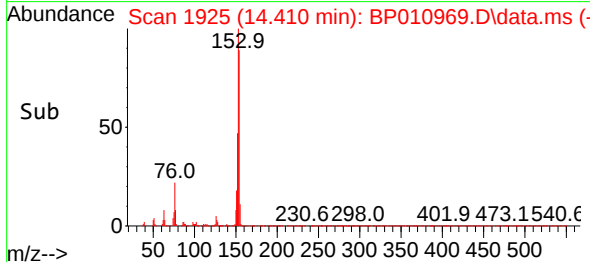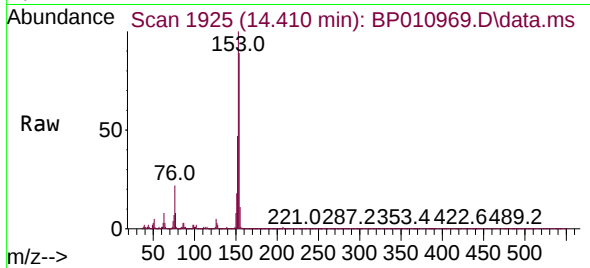

#53
2,4-Dinitrophenol
Concen: 12.280 ng/ul
RT: 14.463 min Scan# 1934
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:184 Resp: 44237
Ion Ratio Lower Upper
184 100
63 79.9 73.8 110.6
154 69.0 57.2 85.8


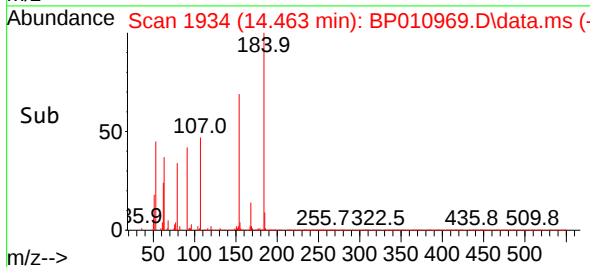

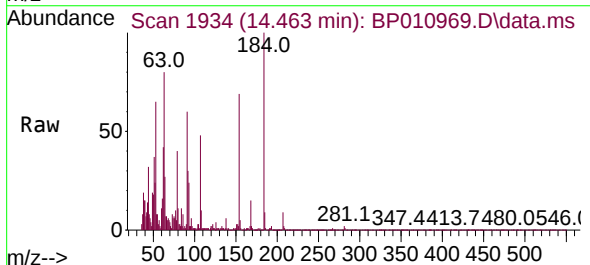




#55
4-Nitrophenol
Concen: 10.960 ng/ul
RT: 14.575 min Scan# 1953
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:109 Resp: 85118
Ion Ratio Lower Upper
109 100
139 143.4 75.6 113.4#
65 149.1 107.6 161.4



#56
Dibenzofuran
Concen: 9.549 ng/ul
RT: 14.751 min Scan# 1983
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:168 Resp: 737680
Ion Ratio Lower Upper
168 100
139 38.3 32.8 49.2









#57
2,4-Dinitrotoluene
Concen: 11.424 ng/ul
RT: 14.722 min Scan# 1978
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:165 Resp: 143238
Ion Ratio Lower Upper
165 100
63 45.3 47.0 70.6#
182 2.8 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 10.575 ng/ul
RT: 14.981 min Scan# 2022
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:232 Resp: 122914
Ion Ratio Lower Upper
232 100
131 51.4 35.8 53.8
130 2.7 1.8 2.8
166 33.9 23.7 35.5









#59
Diethylphthalate
Concen: 9.839 ng/ul
RT: 15.193 min Scan# 2058
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:149 Resp: 612581
Ion Ratio Lower Upper
149 100
177 21.2 17.6 26.4
150 12.2 10.3 15.5



#61
Fluorene
Concen: 9.648 ng/ul
RT: 15.404 min Scan# 2094
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:166 Resp: 594332
Ion Ratio Lower Upper
166 100
165 98.2 77.4 116.2
167 13.4 10.8 16.2




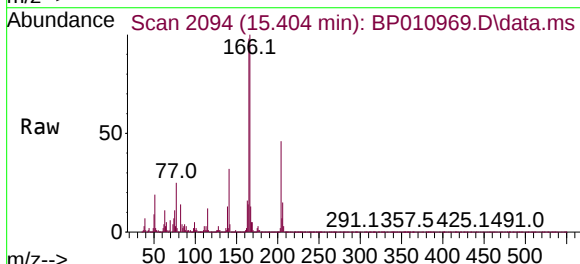




#62
4-Chlorophenyl-phenylether
Concen: 9.573 ng/ul
RT: 15.410 min Scan# 2095
Delta R.T. 0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:204 Resp: 276040
Ion Ratio Lower Upper
204 100
206 32.9 26.0 39.0
141 64.0 49.3 73.9



#63
4-Nitroaniline
Concen: 10.561 ng/ul
RT: 15.434 min Scan# 2099
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:138 Resp: 109847
Ion Ratio Lower Upper
138 100
92 55.5 46.2 69.2
108 76.0 85.8 128.8#


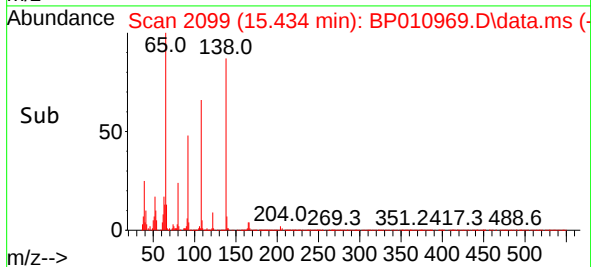

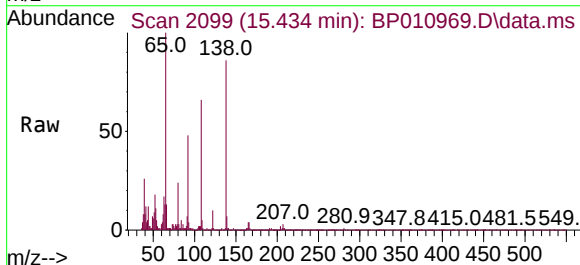




#66
4,6-Dinitro-2-methylphenol
Concen: 10.682 ng/ul
RT: 15.487 min Scan# 2108
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:198 Resp: 69413
Ion Ratio Lower Upper
198 100
182 7.5 4.3 6.5#
77 29.9 23.7 35.5

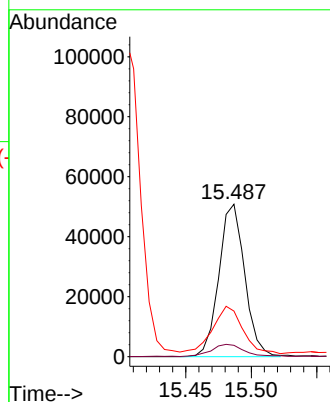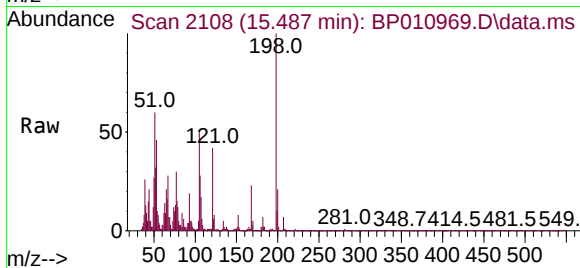

#67
N-Nitrosodiphenylamine
Concen: 9.111 ng/ul
RT: 15.622 min Scan# 2131
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:169 Resp: 500874
Ion Ratio Lower Upper
169 100
168 66.2 52.6 78.8
167 36.0 27.8 41.6



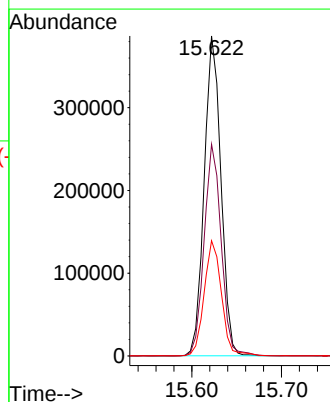





#68
4-Bromophenyl-phenylether
Concen: 8.548 ng/ul
RT: 16.310 min Scan# 2248
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:248 Resp: 155502
Ion Ratio Lower Upper
248 100
250 99.3 80.8 121.2
141 84.7 63.9 95.9



#69
Hexachlorobenzene
Concen: 8.690 ng/ul
RT: 16.410 min Scan# 2265
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:284 Resp: 183101
Ion Ratio Lower Upper
284 100
142 41.3 27.8 41.6
249 30.3 25.4 38.2





#70

Atrazine

Concen: 9.225 ng/ul

RT: 16.593 min Scan# 2296

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:200 Resp: 168154

Ion Ratio Lower Upper

200 100

173 27.0 20.7 31.1

215 47.3 38.6 57.8



#71

Pentachlorophenol

Concen: 9.206 ng/ul

RT: 16.763 min Scan# 2325

Delta R.T. 0.000 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion:266 Resp: 99873


Ion Ratio Lower Upper

266 100

264 60.0 51.4 77.2

268 60.9 53.5 80.3









#72
Phenanthrene
Concen: 9.583 ng/ul
RT: 17.157 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:178 Resp: 926272
Ion Ratio Lower Upper
178 100
179 15.5 12.7 19.1
176 19.0 14.6 22.0



#74
Anthracene
Concen: 9.462 ng/ul
RT: 17.251 min Scan# 2408
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:178 Resp: 919838
Ion Ratio Lower Upper
178 100
179 15.6 12.2 18.2
176 18.4 14.5 21.7




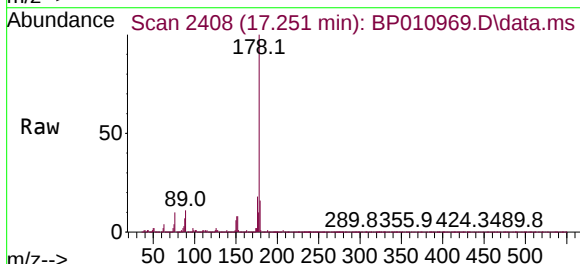




#75
1,2,3,4-Tetrachlorobenzene
Concen: 8.326 ng/uL
RT: 13.134 min Scan# 1708
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:216 Resp: 249378
Ion Ratio Lower Upper
216 100
214 77.6 65.0 97.4
218 46.0 39.1 58.7

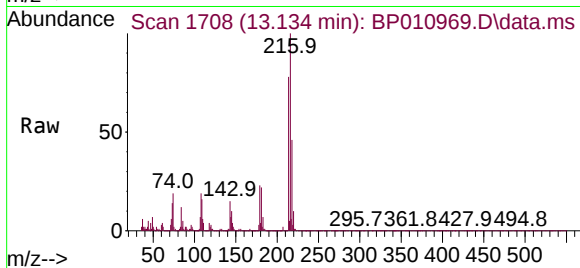

#76
Pentachlorobenzene
Concen: 8.683 ng/uL
RT: 14.663 min Scan# 1968
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:250 Resp: 223058
Ion Ratio Lower Upper
250 100
248 63.9 49.8 74.6
252 62.8 51.2 76.8


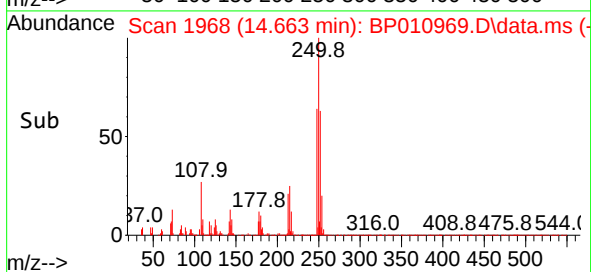






#77
Carbazole
Concen: 10.059 ng/ul
RT: 17.528 min Scan# 2455
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:167 Resp: 880265
Ion Ratio Lower Upper
167 100
166 21.6 16.9 25.3
139 14.1 10.6 16.0



#78
Di-n-butylphthalate
Concen: 9.911 ng/ul
RT: 18.104 min Scan# 2553
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:149 Resp: 1033522
Ion Ratio Lower Upper
149 100
150 8.7 7.1 10.7
104 4.9 4.6 6.8




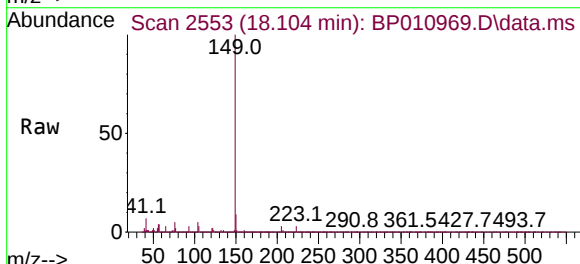




#80
Fluoranthene
Concen: 8.759 ng/ul
RT: 19.145 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:202 Resp: 1063619
Ion Ratio Lower Upper
202 100
101 14.5 7.1 10.7#
100 10.7 5.7 8.5#



#82
Pyrene
Concen: 9.124 ng/ul
RT: 19.498 min Scan# 2790
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:202 Resp: 1118897
Ion Ratio Lower Upper
202 100
101 17.1 7.9 11.9#
100 14.2 6.7 10.1#




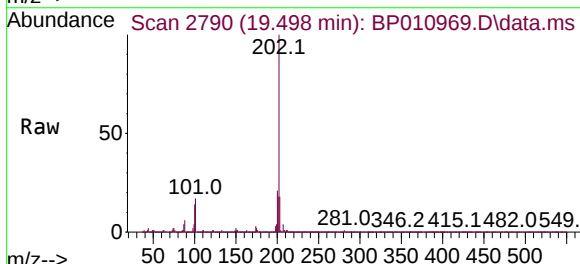




#83
Butylbenzylphthalate
Concen: 10.840 ng/ul
RT: 20.398 min Scan# 2944
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:149 Resp: 467899
Ion Ratio Lower Upper
149 100
91 75.0 60.0 90.0
206 19.1 17.4 26.2



#84
3,3'-Dichlorobenzidine
Concen: 7.678 ng/ul
RT: 21.163 min Scan# 3073
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:252 Resp: 287345
Ion Ratio Lower Upper
252 100
254 64.8 51.0 76.4
126 15.5 8.6 12.8









#85
Benzo(a)anthracene
Concen: 9.500 ng/ul
RT: 21.222 min Scan# 3084
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:228 Resp: 1076788
Ion Ratio Lower Upper
228 100
229 19.5 15.0 22.4
226 26.6 20.6 31.0

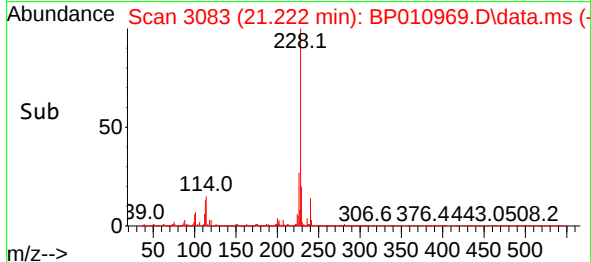

#86
Bis(2-ethylhexyl)phthalate
Concen: 10.366 ng/ul
RT: 21.169 min Scan# 3074
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:149 Resp: 708569
Ion Ratio Lower Upper
149 100
167 26.6 22.6 33.8
279 3.8 4.2 6.4

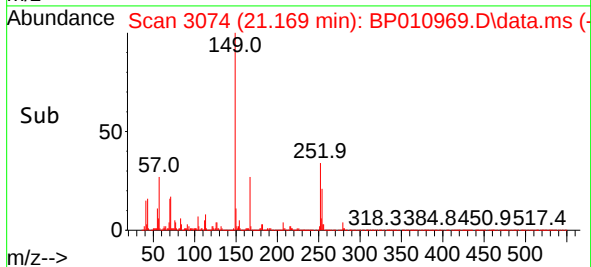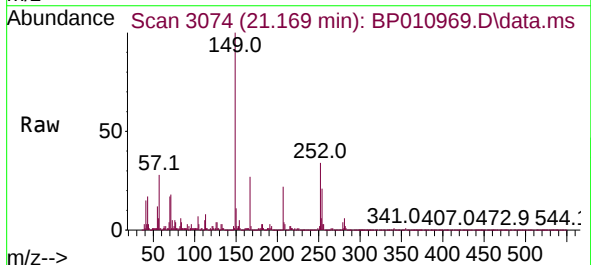



#87

Chrysene

Concen: 9.907 ng/ul

RT: 21.275 min Scan# 3093

Delta R.T. -0.006 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:228 Resp: 1076064

Ion Ratio Lower Upper

228 100

226 29.2 23.6 35.4

229 19.7 15.6 23.4

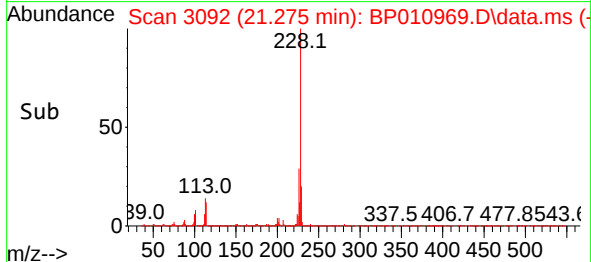

#89

Di-n-octyl phthalate

Concen: 10.293 ng/ul




RT: 22.080 min Scan# 3229


Delta R.T. -0.006 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Tgt Ion:149 Resp: 1095239


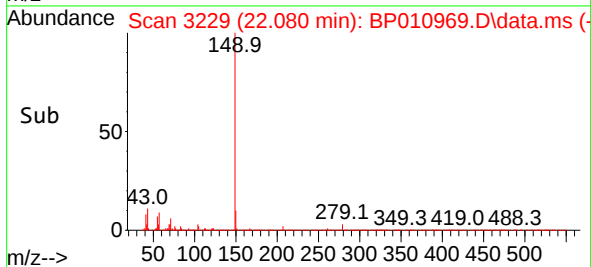

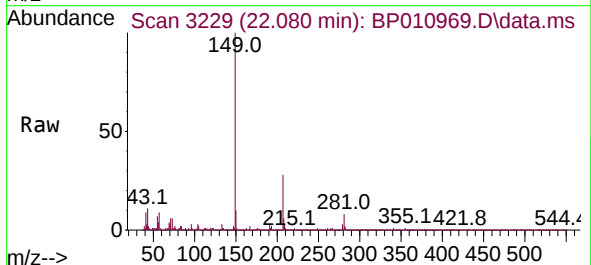




#90
Benzo(b)fluoranthene
Concen: 9.624 ng/ul
RT: 22.875 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:252 Resp: 1072844
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.6
125 13.9 6.2 9.2#

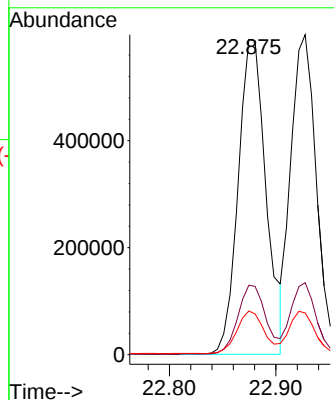

#91
Benzo(k)fluoranthene
Concen: 9.280 ng/ul
RT: 22.927 min Scan# 3373
Delta R.T. 0.000 min
Lab File: BP010969.D
Acq: 14 Jul 2022 12:40

Tgt Ion:252 Resp: 983341
Ion Ratio Lower Upper
252 100
253 22.5 17.0 25.4
125 13.0 6.2 9.4#

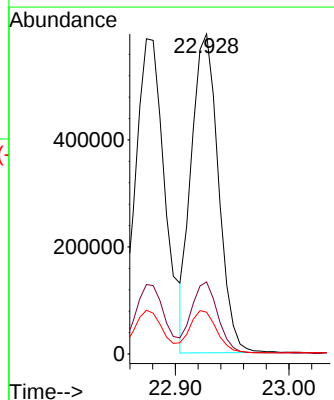



#93

Benzo(a)pyrene

Concen: 9.379 ng/ul

RT: 23.492 min Scan# 3470

Delta R.T. -0.006 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:252 Resp: 1017031

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.0

125 15.2 6.6 10.0#

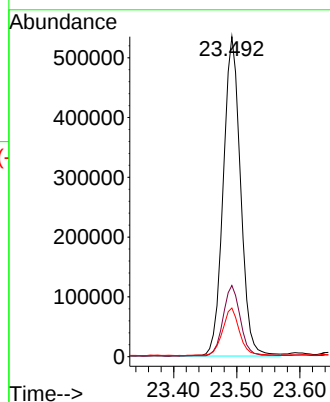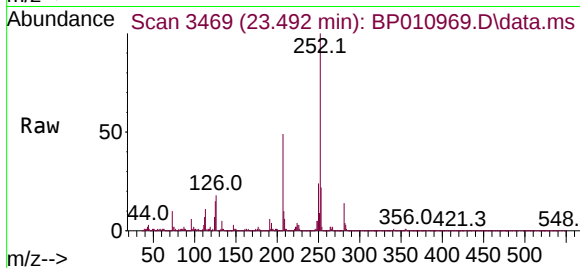

#94

Indeno(1,2,3-cd)pyrene

Concen: 8.965 ng/ul

RT: 26.039 min Scan# 3902

Delta R.T. -0.006 min

Lab File: BP010969.D

Acq: 14 Jul 2022 12:40




Tgt Ion:276 Resp: 1173112


Ion Ratio Lower Upper

276 100

138 29.3 14.6 22.0#

277 25.5 19.6 29.4









#95
 Dibenzo(a,h)anthracene
 Concen: 9.162 ng/ul
 RT: 26.063 min Scan# 3907
 Delta R.T. -0.006 min
 Lab File: BP010969.D
 Acq: 14 Jul 2022 12:40

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010618

Tgt Ion:278 Resp: 1028289
 Ion Ratio Lower Upper
 278 100
 139 20.8 9.4 14.2#
 279 24.9 18.9 28.3

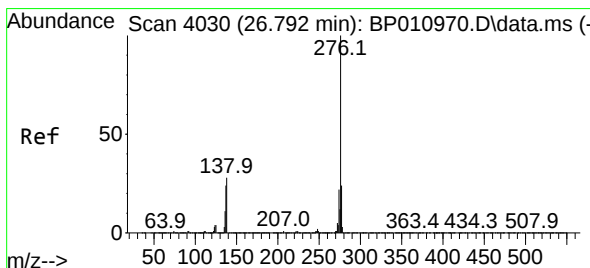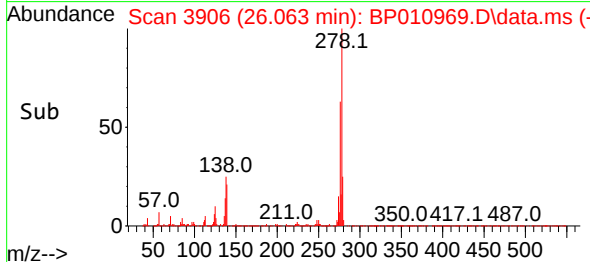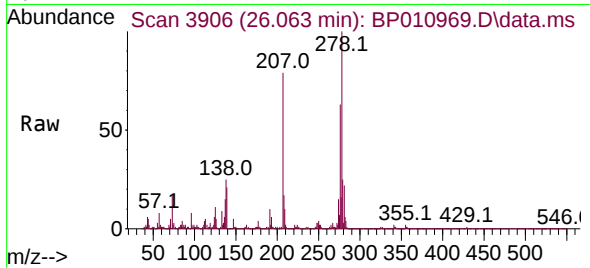

#96
 Benzo(g,h,i)perylene
 Concen: 8.959 ng/ul
 RT: 26.786 min Scan# 4029
 Delta R.T. -0.006 min
 Lab File: BP010969.D
 Acq: 14 Jul 2022 12:40

Tgt Ion:276 Resp: 997217
 Ion Ratio Lower Upper
 276 100
 138 26.8 12.7 19.1#
 277 23.7 18.2 27.4

